




INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<p>(51) International Patent Classification³ : A61M 5/00</p>	<p>A1</p>	<p>(11) International Publication Number: WO 84/ 01509 (43) International Publication Date: 26 April 1984 (26.04.84)</p>
<p>(21) International Application Number: PCT/US83/01619 (22) International Filing Date: 14 October 1983 (14.10.83) (31) Priority Application Number: 434,223 (32) Priority Date: 14 October 1982 (14.10.82) (33) Priority Country: US (71) Applicant: COLLAGEN CORPORATION [US/US]; 2500 Faber Place, Palo Alto, CA 94303 (US). (72) Inventors: SABELMAN, Eric, E. ; 711 Central Avenue, Menlo Park, CA 94025 (US). KOOGLE, Timothy, A. ; 924 6th Avenue, Redwood City, CA (US). KEN- NEDY, William ; 3043 Emerson Street, Palo Alto, CA 94306 (US). (74) Agents: CIOTTI, Thomas, E. et al.; Ciotti & Murashige, 800 Menlo Avenue, Suite 102, Menlo Park, CA 94025 (US).</p>		<p>(81) Designated States: AT (European patent), AU, BE (Eu- ropean patent), CH (European patent), DE (Euro- pean patent), FR (European patent), GB (European patent), JP, LU (European patent), NL (European pa- tent), SE (European patent). Published <i>With international search report.</i></p>

(54) Title: SYRINGE FORCE AMPLIFICATION DEVICE

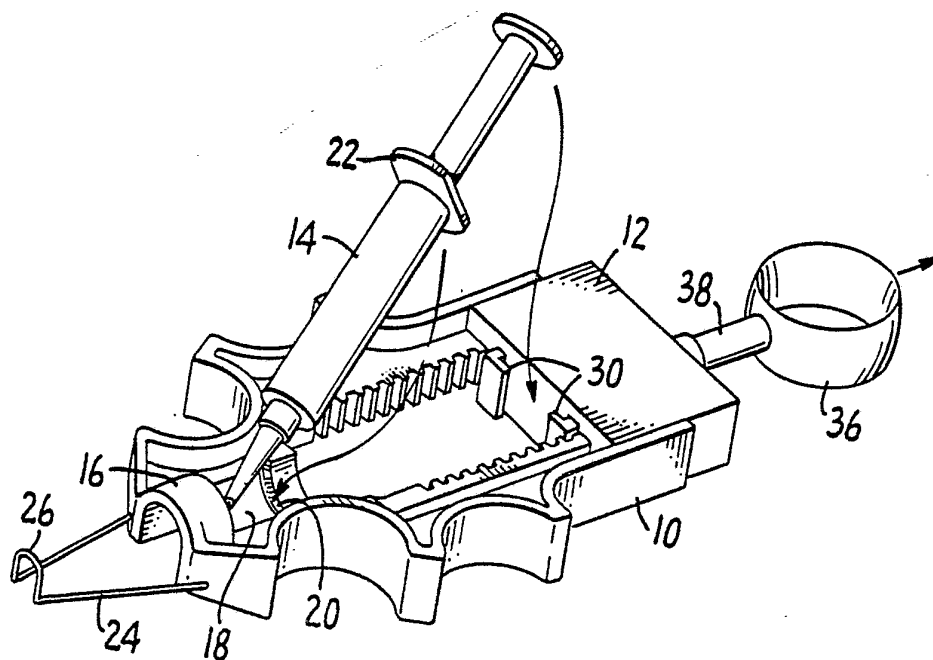

(57) Abstract

A syringe assist device including a frame (10) and moveable carriage (12) that are respectively attached to a conventional syringe (14) and its plunger. The frame has a toothed rack (44) and the carriage contains a force amplifying gear (48) and lever mechanism (52). A thumb ring (36) transmits the force applied by the user's thumb to the lever (52) to rotate the gear (48) and move the carriage (12) along the frame (10). This action in turn applies amplified compression to the syringe plunger. A ratchet connection between the lever (52) and the gear (48) enables the movement of the carriage (12) to be continued without force amplification when the lever (52) has reached the end of its stroke.

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	LI	Liechtenstein
AU	Australia	LK	Sri Lanka
BE	Belgium	LU	Luxembourg
BR	Brazil	MC	Monaco
CF	Central African Republic	MG	Madagascar
CG	Congo	MR	Mauritania
CH	Switzerland	MW	Malawi
CM	Cameroon	NL	Netherlands
DE	Germany, Federal Republic of	NO	Norway
DK	Denmark	RO	Romania
FI	Finland	SE	Sweden
FR	France	SN	Senegal
GA	Gabon	SU	Soviet Union
GB	United Kingdom	TD	Chad
HU	Hungary	TG	Togo
JP	Japan	US	United States of America
KP	Democratic People's Republic of Korea		

SYRINGE FORCE AMPLIFICATION DEVICEDescriptionTechnical Field

The present invention is directed to a device for amplifying the mechanical force applied to a syringe to compress the plunger into the barrel of the syringe with a fine degree of control.

Background Art

Most liquid medicines and the like that are typically injected with a syringe have a sufficiently low viscosity that the plunger of the syringe can be manually compressed into its barrel, to expel the liquid therefrom, with relatively little effort. However, when a high viscosity material is to be injected, particularly through a hypodermic needle having a small opening, difficulties are presented. As the force required to move the plunger increases, the degree of control that can be exercised over the rate of injection is lessened. For materials having extremely high viscosity, such as a collagen implant for example, the force required to move the plunger approaches the maximum force available to finger and thumb muscles that is consistent with fine motor control.

In the past, most devices for assisting the compression of a syringe have been relatively complex and often obstruct the view of the needle or otherwise pose difficulties relative to conventional injection techniques. One type of device comprises a pistol-grip pawl and ratchet mechanism. A drawback associated with this type of device is that the advance of the plunger is limited to steps of a fixed size, as determined by the ratchet mechanism. Consequently,



-2-

the degree of control that is available is limited. In addition, most commercially available devices of this type are adapted for relatively large syringes, and are not suited for use with smaller syringes
5 having a capacity of 1-3 cc., for example.

Other types of devices are not suited for use with conventional syringes. For example, one pneumatic syringe assist device requires a syringe that does not have a plunger, so that the compressed
10 air can act directly on the material to be injected.

Objects of the Invention

Accordingly it is a general object of the present invention to provide a novel device for amplifying the manual force that is applied to the
15 plunger of a syringe during injection of a liquid material.

It is a more specific object of the present invention to provide a novel device that utilizes a mechanical advantage to amplify the force applied to a
20 syringe plunger.

It is another object of the present invention to provide such a device that does not obstruct the view of the needle, to possibly limit injection sites, or otherwise interfere with the injection
25 process.

It is a further object of the present invention to provide such a device that retains, and possibly even enhances, the tactile feedback that is provided to the person operating the syringe.

30 It is yet another object of the invention to provide a novel syringe force amplifying device that retains the ability to operate the syringe with the familiar and comfortable hand position that is normally utilized.



It is still a further object of the invention to provide such a device that can accommodate variations in hand size, strength and holding style.

Still another object of the invention is to provide a novel syringe force amplifying device that is both rugged and simple to construct.

Yet a further object of the invention is to provide a force amplification device that can be readily used with conventional syringes.

10 Disclosure of the Invention

In accordance with the present invention, these and other objects are achieved, and their attendant advantages are provided, by a syringe assist device including a frame and moveable carriage that are respectively attached to a conventional syringe and its plunger. The frame has a toothed rack and the carriage contains a force amplifying gear and lever mechanism. A thumb ring transmits the force applied by the user's thumb to the lever to rotate the gear and move the carriage along the frame. This action in turn applies amplified compression to the syringe plunger. A ratchet connection between the lever and the gear enables the movement of the carriage to be continued when the lever has reached the end of its stroke.

Further features and advantages of the invention are described in greater detail hereinafter with particular reference to a preferred embodiment of the invention illustrated in the accompanying drawings.



Brief Description of the Drawings

Figure 1 is a perspective view of the syringe assist device, illustrating the manner that a syringe is inserted to be connected thereto;

5 Figure 2 is a top view of the device with a syringe inserted;

Figure 3 is a side view of the device with a syringe inserted;

10 Figure 4 is an enlarged top view of the frame and carriage with the top half of the carriage removed to illustrate the gear and lever mechanism; and

15 Figure 5 is a cross-sectional end view of the frame and carriage, taken along the section line 5-5 of Figure 4.

Modes for Carrying Out the Invention

Referring to Figures 1-3, a syringe assist device constructed in accordance with the present invention basically comprises a frame 10 and a carriage 12 that is moveable along the frame. The forward end of the frame has a bore that accomodates the barrel 14 of a syringe. This bore is defined by an upper arc-shaped bridge 16 at the forwardmost end of the frame, and a lower arc-shaped bridge 18 disposed 25 behind the upper bridge 16. The spacing of the bridges in this manner allows the syringe to be inserted into the bore at an angle, as depicted in Figure 1. The lower bridge 18 is provided with a slot 20 to accomodate the flange 22 that is typically located at 30 the top of the barrel, and thereby holds the syringe in place on the frame.

A spring clip 24 projects from the front of the frame, and includes an arcuate portion 26 at its



-5-

forwardmost end that is snapped in place around the
needle luer hub 28 of the syringe once it is inserted
into the frame. The spring clip not only serves to
secure the attachment of the syringe to the frame, but
5 it also retains the needle in place and prevents its
detachment, for example due to needle hub or syringe
failure under high internal pressure.

The carriage 12 includes a pair of clips 30
that accomodate the disk-type flange 32 at the end of
10 the syringe plunger 34, to thereby secure the plunger
to the carriage. Thus, when the syringe is inserted
into the frame with its flange 22 disposed in the slot
20 and the plunger is engaged in the clip 30, any
movement of the carriage 12 relative to the frame will
15 induce corresponding movement of the plunger relative
to the barrel 14 of the syringe.

To enable the syringe assist device to be
operated with the same one-handed holding style that
is typically utilized with syringes, a thumb ring 36
20 is disposed on the end of a plunger 38 that projects
from the rear of the carriage 12. Two pairs of finger
grips 40 and 42 are provided on the frame. The two
pairs of grips are displaced along the length of the
frame to thereby accomodate different hand sizes and
25 different holding styles. Thus the device can be held
by placing the index and middle fingers of the hand in
one of the pairs of grips and placing the thumb in the
ring 36. The plunger 38 is translated into and out of
the carriage with the thumb ring, utilizing the same
30 motion as is employed with a syringe by itself.

The manner in which the device operates to
amplify the force that is manually applied to the
thumb ring is explained with reference to the detailed
diagrams of Figures 4 and 5. For ease of manufacture



-6-

and assembly of the device, the carriage 12 can be made of two halves that are fitted together. The carriage is shown with the top half removed in Figure 4.

The frame 12 is provided with two opposed
5 parallel racks 44 having teeth 46. Two pinion gears 48 rotate about shafts 50 within the carriage, and their teeth respectively mesh with those of the racks 44. A lever 52 is disposed on each shaft 50 for limited pivotal movement. As best illustrated in Figure
10 5, each lever 52 is engaged with its associated pinion gear 48 by means of ratchet teeth 54 disposed on the opposing faces of the lever and the gear. These teeth have one face that is parallel to the axis of the shafts 50, and another face that is disposed approxi-
15 mately 45° relative thereto. Thus, when the levers are pivoted in one direction, the pinion gears will be forced to rotate therewith. The ratchet teeth are set up so that this occurs when the levers are moved forward, i.e., the lower lever in Figure 4 pivots in a
20 counterclockwise direction and the upper lever moves in a clockwise direction. However, in the other direction of movement, relative rotation is allowed to take place between each lever and pinion gear by the slanted surfaces of the ratchet teeth. The levers 52
25 are biased in an axial direction into normal engagement with the pinion gears by means of springs 56, for example spring washers.

The ends of the levers 52 that are remote
from the shafts 50 include slots 58 that accommodate a
30 shaft 60. The shaft 60 is parallel to the gear shafts 50, and is translatable in a transverse direction within two recesses 62 in the carriage 12. Translation of the shaft 60, and hence pivoting of the levers 52, is provided by the plunger 38, which is rigidly
35 connected to the shaft.



The moment arm, or operative length, of each lever 52, i.e., the distance between the axes of the shafts 50 and 60, is greater than that of the gear which it engages, i.e., greater than the distance
5 between the axis of the shaft 50 and the point of engagement between the gear teeth and the rack teeth 46. Thus, the gear and lever arrangement provides a mechanical advantage with respect to force applied through the plunger 38. Preferably, the levers and
10 gears are dimensioned so that the carriage moves along the frame with a force that is four times greater than that applied to the thumb ring 36 and plunger 38.

In operation, the thumb ring 36 is pulled to move the carriage to the right (as viewed in
15 Figure 4), and a syringe is inserted in the device in the manner illustrated in Figure 1. The plunger flange 32 is engaged in the clips 30 of the carriage, and the retainer 26 snapped in place around the needle hub, to attach the syringe to the device as
20 shown in Figures 2 and 3. Thereafter, as the thumb ring is pushed into the carriage, the levers 52 and gears 48 will be pivoted about the shafts 50, causing the carriage to move forward along the frame and compress the plunger into the barrel 14 with a greater
25 force than that applied by the thumb to the ring. Conversely, the carriage will move a proportionately shorter distance than the thumb ring.

At the end of travel of the thumb ring, i.e., when the levers 52 contact the front wall 64 of
30 the carriage, the carriage can continue to move forward under direct pressure from the thumb if no mechanical advantage is required. In this case, the ratchet teeth 54 will enable the pinion gears 48 to continue turning as the carriage moves along the
35 frame, even though the levers are stationary.



-8-

Alternatively, if force amplification is required to continue the movement of the plunger, the thumb ring is retracted to pull the plunger out of the carriage. In this case, the carriage will remain
5 stationary due to the dampening effect provided by the syringe, i.e., the plunger will resist being pulled from the barrel. Again, the ratchet teeth will allow relative rotation between the levers and the gears,
10 enabling the levers to be pivoted rearwardly while the gears remain motionless. The thumb ring can then be pressed towards the carriage again, providing continued forward movement of the carriage with force amplification.

In order to enable the carriage to be
15 retracted, a pair of cam surfaces 66 are provided on each lever 52. These cam surfaces are disposed at an appropriate angle, e.g., 45°, relative to the axis of the shafts 50. A pair of corresponding cams 68 are provided on the carriage adjacent each lever (only two
20 of which are illustrated in Figure 4 adjacent the upper lever). As the levers 52 approach the limit of their travel when the thumb ring is pulled away from the carriage, the cam surfaces 66 will engage and ride up on the cams 68, causing the levers to move axially
25 against the bias of the springs 56. Consequently, the ratchet mechanisms will be disengaged, enabling the pinion gears to rotate freely. Thus, the entire carriage will be retracted if the thumb ring continues to be pulled outwardly.

30 From the foregoing, it can be seen that the present invention provides a device that amplifies the manual force applied to a syringe while retaining the ability to operate the syringe in a conventional fashion and without obstruction. Precise control over the



-9-

amount and rate of compression of the syringe is afforded, along with tactile feedback as to the resistance offered by the syringe.

It will be appreciated by those of ordinary skill in the art that the present invention can be embodied in other specific forms without departing from the spirit or essential characteristics thereof. The presently disclosed embodiment is therefore considered in all respects to be illustrative and not restrictive. The scope of the invention is indicated by the appended claims rather than the foregoing description, and all changes that come within the meaning and range of equivalents thereof are intended to be embraced therein.



Claims

1. Apparatus for amplifying the manual force applied to compress the plunger of a syringe into its barrel, comprising:

5 a frame having means for attachment to the barrel of a syringe;

a carriage mounted on said frame so as to be moveable relative thereto along the longitudinal axis of a syringe attached to the frame, said carriage including means for engaging the plunger of a syringe;

10 a gear rotatably mounted on said carriage and operatively engaging said frame such that rotation of said gear induces movement of said carriage along said axis; and

15 manually actuatable means for rotating said gear with a mechanical advantage such that the linear force applied to the plunger of a syringe connected to said carriage is greater than the force that is manually applied to rotate said gear.

2. The apparatus of claim 1 wherein said manually actuatable means includes a pivotable lever operatively engaged for rotation with said gear, and means for applying a linear force to the end of said 5 lever that is remote from its pivot axis, said lever having a greater moment arm than said gear.

3. The apparatus of claim 2 wherein said lever is engaged with said gear by means of a ratchet arrangement that enables relative rotation between said lever and said gear in one direction.



-11-

4. The apparatus of claim 3 further including means for disengaging said lever from said gear near one end of the pivot stroke of said lever, to thereby permit relative rotation of said lever and
5 said gear in the other direction.

5. The apparatus of claim 1 wherein said frame includes finger grips for grasping by at least two fingers of a person operating a syringe, and said manually actuatable means includes a thumb ring to
5 accomodate the thumb of the person.

6. The apparatus of claim 5 wherein two pairs of finger grips are provided on said frame at different locations along its length to accomodate different hand sizes and holding styles.

7. The apparatus of claim 1 wherein said frame further includes a retainer for attachment to the needle of a syringe.

8. A device for increasing the compressive force that is manually applied to a syringe, comprising:

a frame having means for attachment to the
5 barrel of a syringe and including a pair of opposed racks of teeth;

a carriage mounted for movement between said racks of teeth along a path of travel parallel thereto, said carriage having means for engaging the
10 plunger of a syringe attached to said frame;

a pair of pinion gears rotatably disposed on said carriage and respectively engaging said racks of teeth;



-12-

a pair of levers respectively engaged for
15 rotation with said pinion gears, each of said levers
having an operative length greater than the radius of
its associated pinion gear to thereby provide a
mechanical advantage; and

a plunger connected to said levers and
20 adapted to be manually translated to pivot said levers
and thereby move said carriage relative to said frame
due to the interaction between the rotating gears and
the rack teeth.

9. The device of claim 8 wherein said
levers are engaged with their respective pinion gears
by means of ratchet arrangements that enable relative
rotation to take place between said levers and their
5 respective gears in one direction.

10. The device of claim 9 further including
means for disengaging said levers from said gears near
one end of the pivot stroke of said levers, to thereby
permit relative rotation of said levers and said gears
5 in the other direction.

11. The device of claim 8 wherein said
plunger includes a ring disposed at the end thereof
that is remote from its connection to said levers,
said ring being adapted to accommodate the thumb of a
5 user.

12. The device of claim 11 wherein two
pairs of finger grips are provided on said frame at
different locations along its length to accommodate
different hand sizes and holding styles.



13. The device of claim 8 wherein said frame further includes a retainer for attachment to the needle of a syringe.

14. Apparatus for amplifying the manual force applied to compress the plunger of a syringe into its cylinder, comprising:

a frame having means for attachment to the
5 barrel of a syringe;

a carriage mounted on said frame so as to be moveable relative thereto and including means for engaging the plunger of a syringe attached to said frame;

10 means adapted to be manually translated along a path of travel coaxial with that of the plunger to apply a linear force to said carriage; and

means operatively disposed between said
15 force applying means and said frame for moving said carriage along said frame with a mechanical advantage such that the force applied to the plunger of a syringe by said carriage is greater than the manual force applied to said force applying means.



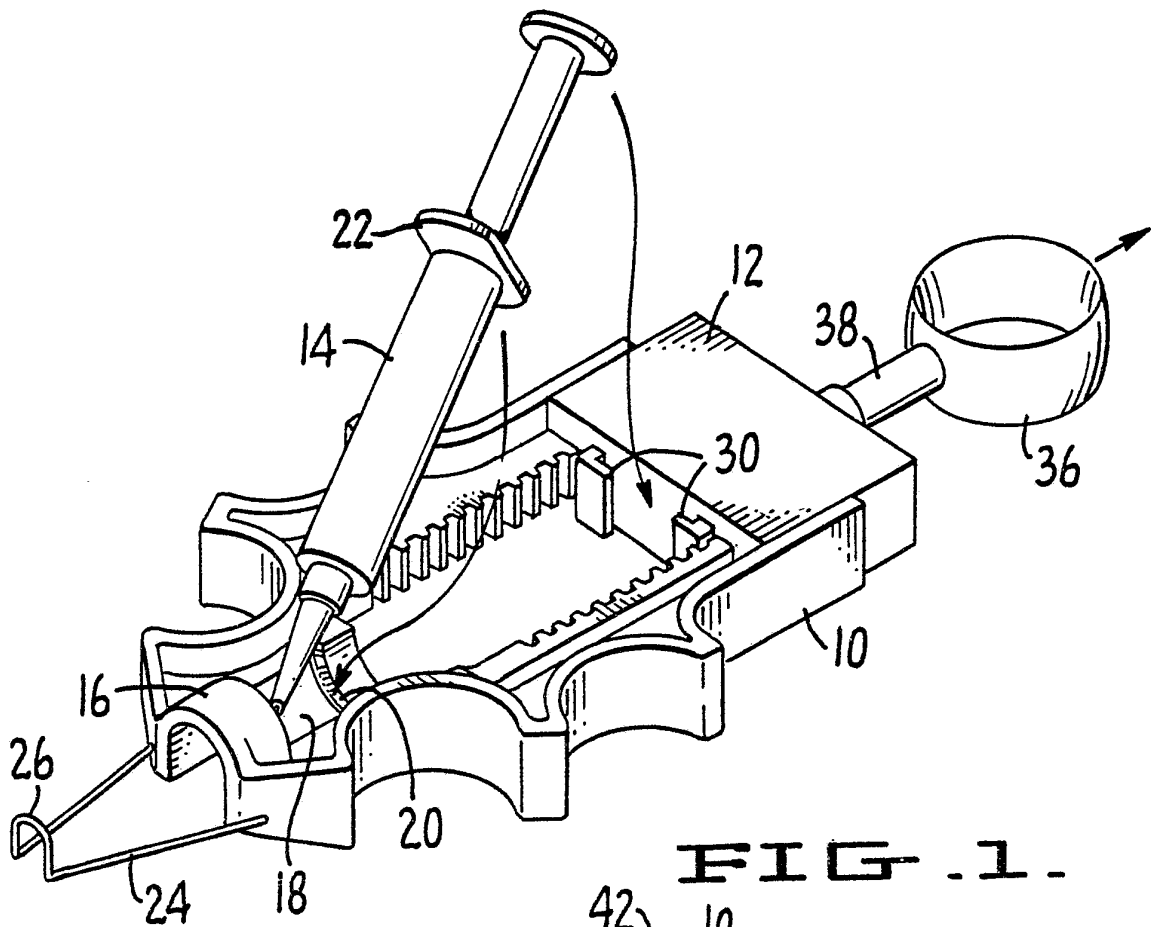


FIG. 1.

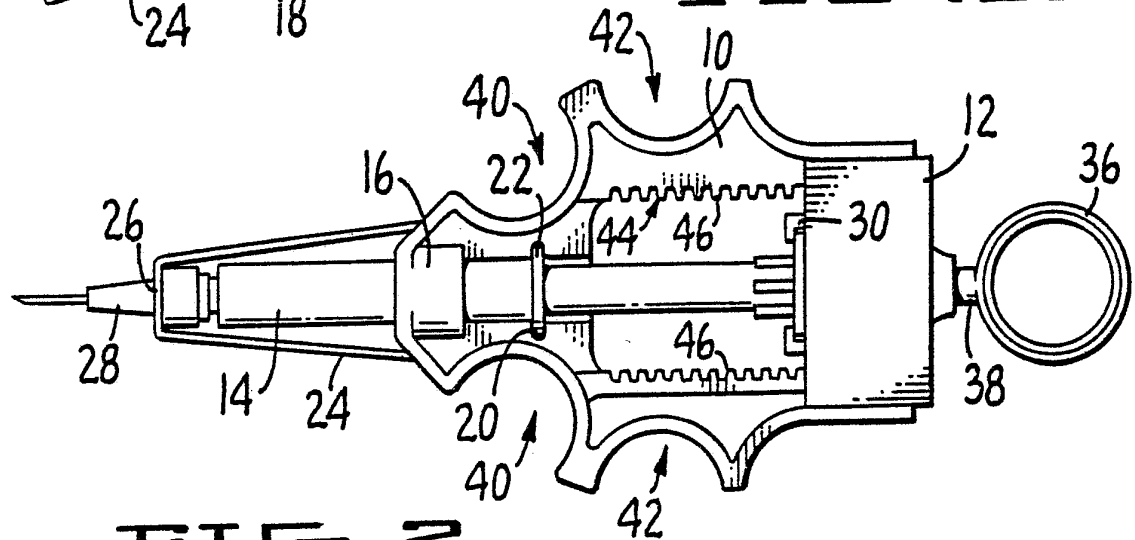


FIG. 2.


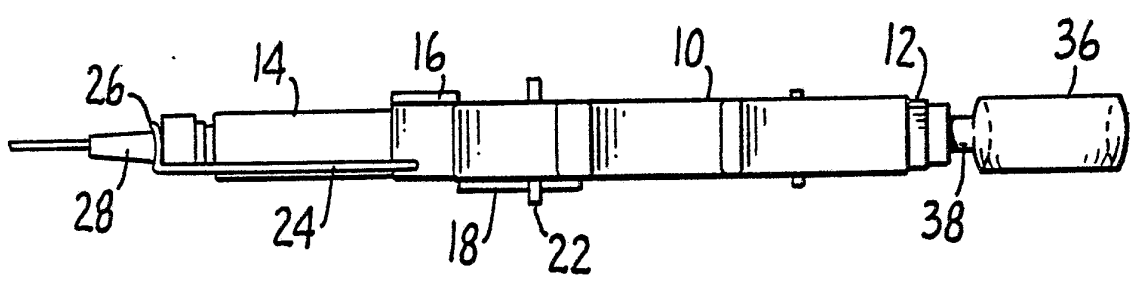


FIG. 3.



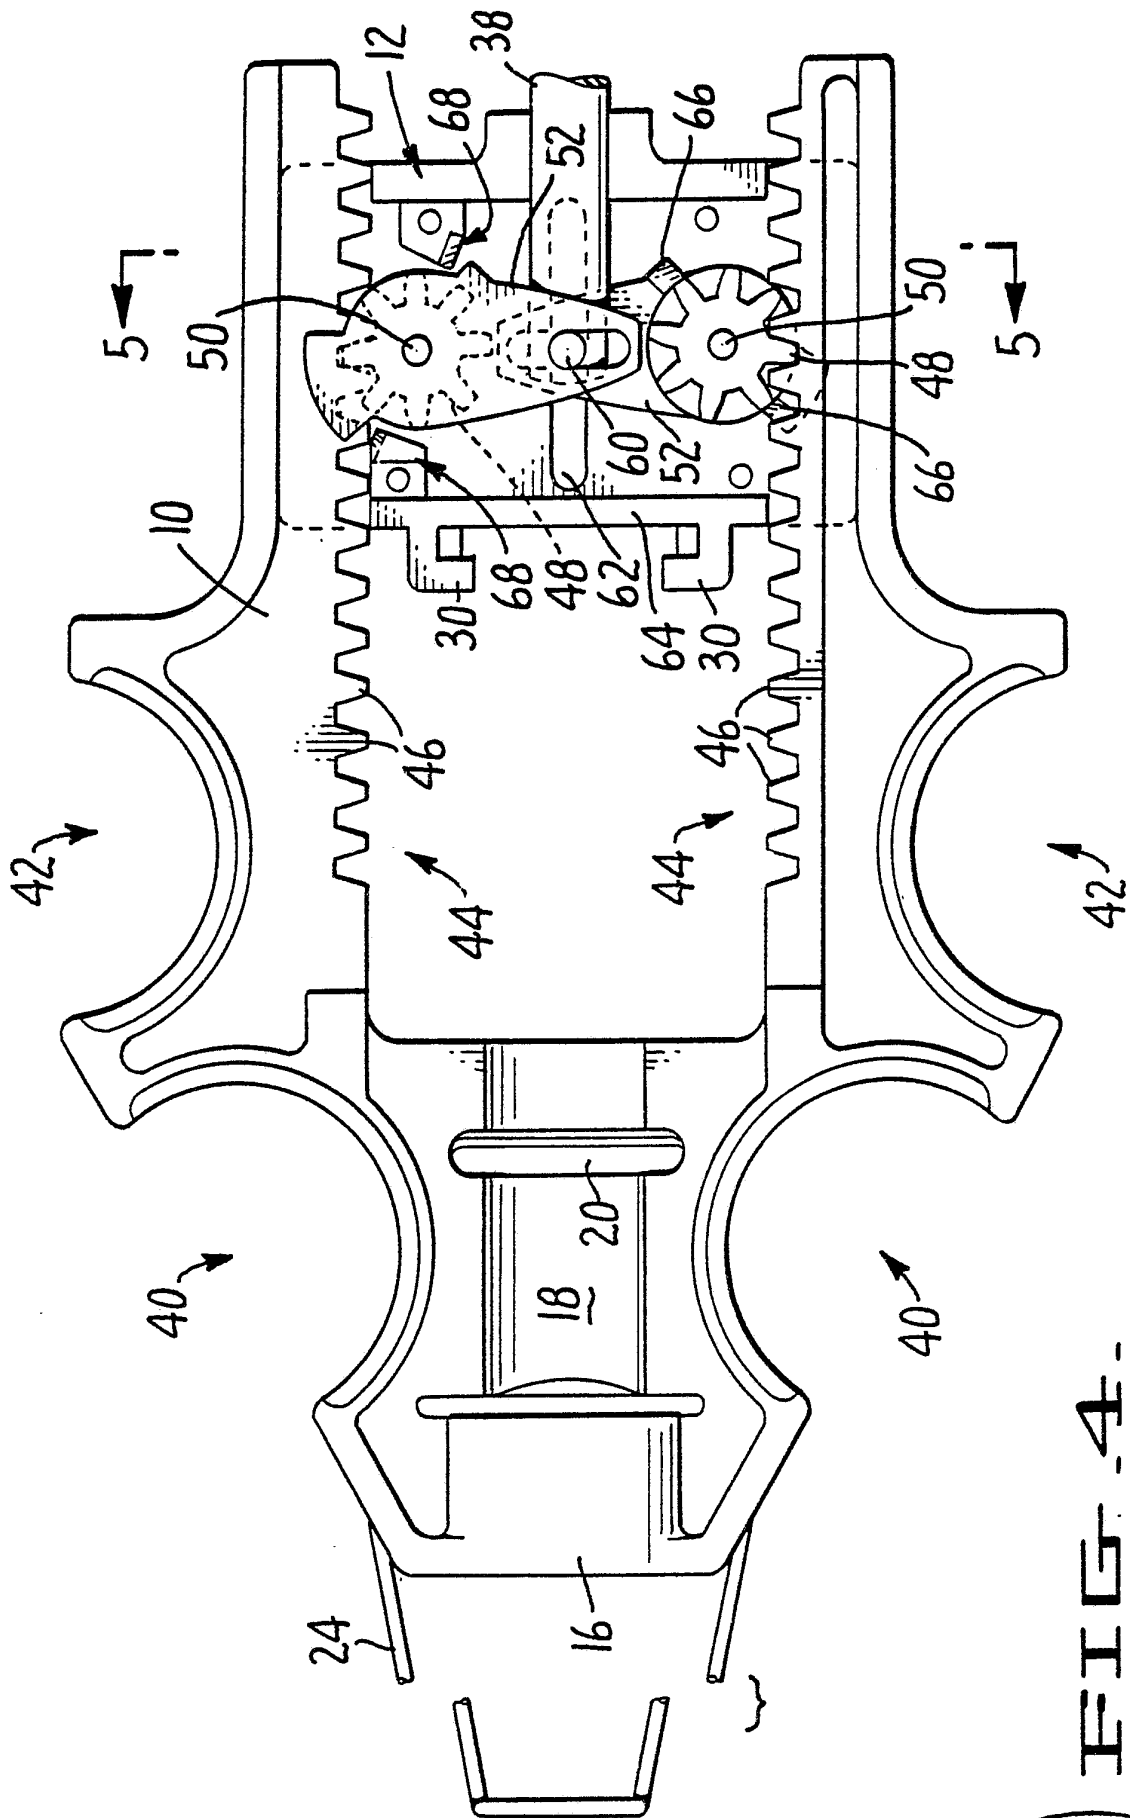

SUBSTITUTE SHEET

FIG. 4



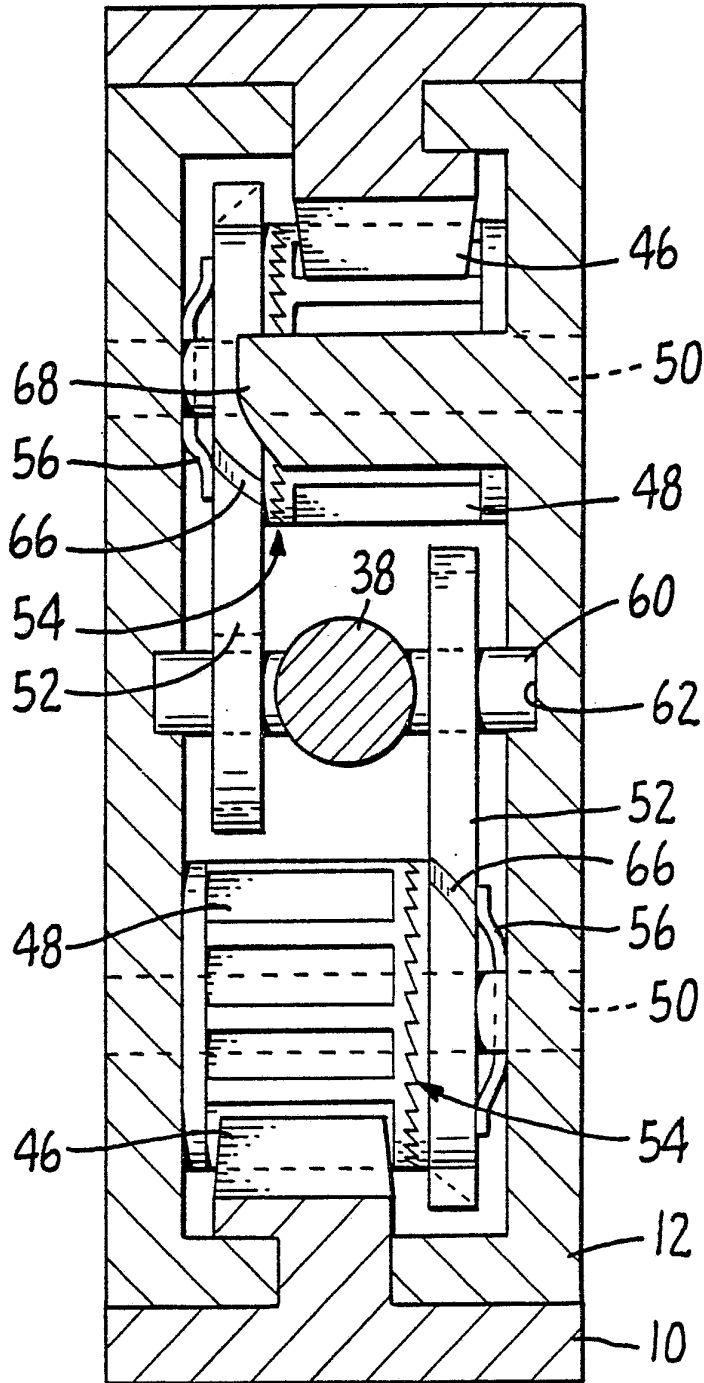



FIG. 5.

SUBSTITUTE SHEET



INTERNATIONAL SEARCH REPORT

International Application No PCT/US83/01619

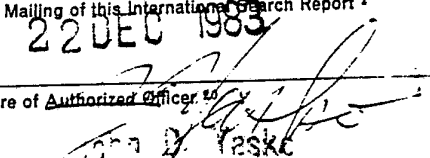I. CLASSIFICATION OF SUBJECT MATTER (if several classification symbols apply, indicate all) ³		
According to International Patent Classification (IPC) or to both National Classification and IPC		
INT. CL. ³ A61M 5/00		
US. CL. 604/224		
II. FIELDS SEARCHED		
Minimum Documentation Searched ⁴		
Classification System	Classification Symbols	
US	604/224, 220, 218, 209 222/386, 390, 391	
Documentation Searched other than Minimum Documentation to the Extent that such Documents are Included in the Fields Searched ⁵		
III. DOCUMENTS CONSIDERED TO BE RELEVANT ¹⁴		
Category [*]	Citation of Document, ¹⁶ with indication, where appropriate, of the relevant passages ¹⁷	Relevant to Claim No. ¹⁸
X	US, A, 780,147 17 January 1905 WILCOX et al	1-3,14
X	US, A, 4,231,368 04 November 1980 BECKER	1-4,7,14
Y	US, A, 854,399 21 May 1907 BRIDGE	5,6
Y	US, A, 1,798,116 24 March 1931 BROCKWAY	5,6
<p>[*] Special categories of cited documents: ¹⁵</p> <p>"A" document defining the general state of the art which is not considered to be of particular relevance</p> <p>"E" earlier document but published on or after the international filing date</p> <p>"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)</p> <p>"O" document referring to an oral disclosure, use, exhibition or other means</p> <p>"P" document published prior to the international filing date but later than the priority date claimed</p> <p>"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention</p> <p>"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step</p> <p>"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.</p> <p>"&" document member of the same patent family</p>		
IV. CERTIFICATION		
Date of the Actual Completion of the International Search ²	Date of Mailing of this International Search Report ²	
13 December 1983	22 DEC 1983	
International Searching Authority ¹	Signature of Authorized Officer ¹⁹	
ISA/US	 JOHN D. TOSKE	