



US00D893547S

(12) **United States Design Patent**
Dumas et al.

(10) **Patent No.:** **US D893,547 S**

(45) **Date of Patent:** **** Aug. 18, 2020**

(54) **SURGICAL PUMP DISPLAY SCREEN OR PORTION THEREOF WITH GRAPHICAL USER INTERFACE**

5,830,180 A 11/1998 Chandler et al.
6,024,720 A 2/2000 Chandler et al.
6,176,847 B1 1/2001 Humphreys, Jr. et al.
6,394,974 B1 5/2002 Kadziauskas et al.
7,010,369 B2 3/2006 Borders et al.
D572,724 S * 7/2008 Guimaraes D14/495

(Continued)

(71) Applicant: **DePuy Synthes Products, Inc.**,
Raynham, MA (US)

FOREIGN PATENT DOCUMENTS

(72) Inventors: **Oliver Dumas**, East Sandwich, MA (US); **Eduard Grinberg**, Sharon, MA (US)

WO 2019/046560 A1 3/2019

(73) Assignee: **DePuy Synthes Products, Inc.**,
Raynham, MA (US)

OTHER PUBLICATIONS

(**) Term: **15 Years**

“Fluid Management System” Nov. 28, 2018, posted at a1medtech.com, [site visited Dec. 2, 2019]. https://www.a1medtech.com/Fluid-Management-System_c_115.html.*

(Continued)

(21) Appl. No.: **29/661,431**

Primary Examiner — Jack Reickel

Assistant Examiner — John M Otte

(22) Filed: **Aug. 28, 2018**

(51) **LOC (12) Cl.** **14-04**

(52) **U.S. Cl.**

USPC **D14/495**

(58) **Field of Classification Search**

USPC D14/485–495; D20/11; D21/324, 325
CPC G06F 3/048; G06F 3/0481; G06F 3/04817;
G06F 3/0482; G06F 3/0483; G06F
3/04842; G06F 3/0485; G06F 3/04855;
G06F 3/486; G06F 3/0488; G06F
3/04886; G06F 9/4443; G06F 17/211;
G06F 17/212; F16M 11/08; A61B 5/1115;
A61B 5/7445; A61B 5/6892; G06Q
50/24; G06Q 50/22; H04W 4/90; A61M
1/0027; G16H 20/13; A61G 7/002
See application file for complete search history.

(57)

CLAIM

The ornamental design for a surgical pump display screen or portion thereof with graphical user interface, as shown and described.

DESCRIPTION

FIG. 1 is a first view of a display screen or portion thereof with graphical user interface, showing our new design; FIG. 2 is a second image thereof; and, FIG. 3 is a third image thereof.

The broken line showing of a display screen or portion thereof with graphical user interface is included for the purpose of showing portions of the article which form no part of the claim.


The appearance of the transitional image sequentially transitions between the images shown in FIGS. 1-3. The process or period in which one image transitions to another image forms no part of the claimed design.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D276,819 S * 12/1984 James D14/494
D278,804 S * 5/1985 Tanikawa D10/125
D281,081 S * 10/1985 Zwissler D14/488
5,315,530 A 5/1994 Gerhardt et al.
5,520,638 A 5/1996 O’Quinn et al.

1 Claim, 2 Drawing Sheets

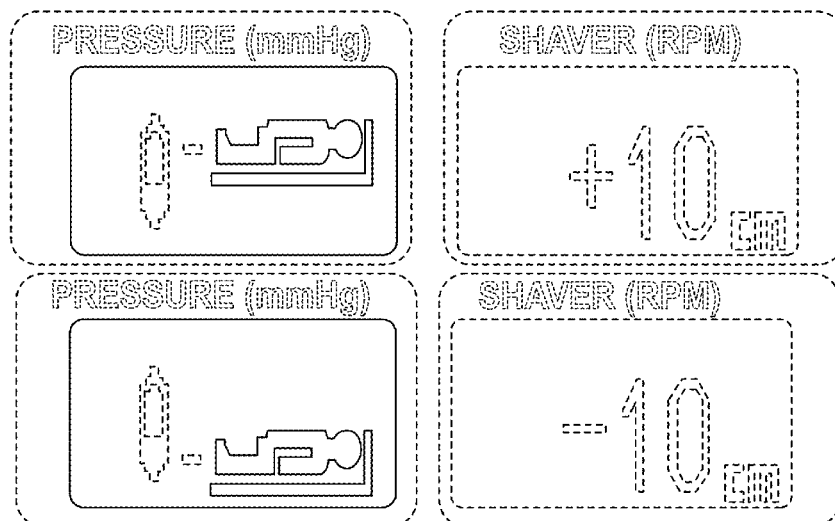

(56)

References Cited

U.S. PATENT DOCUMENTS

- | | | | | | | | | | |
|--------------|------|---------|--------------------|-------------------------|--------------|------|---------|----------------|-----------------------|
| D572,725 | S * | 7/2008 | Guimaraes | D14/495 | 2014/0026322 | A1 * | 1/2014 | Bell | A61G 7/002
5/600 |
| 7,421,316 | B2 | 9/2008 | Gray et al. | | 2014/0171959 | A1 | 6/2014 | Yacono | |
| 7,510,542 | B2 | 3/2009 | Blight | | 2014/0278524 | A1 * | 9/2014 | Vaglio | G06Q 50/24
705/3 |
| 7,604,610 | B2 | 10/2009 | Shener et al. | | 2015/0025450 | A1 | 1/2015 | King et al. | |
| 7,628,054 | B2 | 12/2009 | Hajishah et al. | | 2015/0057774 | A1 | 2/2015 | Boukhny et al. | |
| D611,498 | S * | 3/2010 | Alvarez | D14/488 | 2015/0133895 | A1 | 5/2015 | Klomp | |
| 8,424,362 | B2 | 4/2013 | Hajishah et al. | | 2015/0277703 | A1 * | 10/2015 | Davis | G06F 3/04817
705/2 |
| 9,089,367 | B2 | 7/2015 | Thoe et al. | | 2015/0290387 | A1 | 10/2015 | Mollstam | |
| D738,928 | S * | 9/2015 | Mahaffey | D14/495 | 2016/0030668 | A1 | 2/2016 | Barnes et al. | |
| D738,929 | S * | 9/2015 | Mahaffey | D14/495 | 2016/0346443 | A1 | 12/2016 | Woolford | |
| 9,162,023 | B2 | 10/2015 | Barnes et al. | | 2016/0346454 | A1 | 12/2016 | Woolford | |
| D742,917 | S * | 11/2015 | Perez | D14/492 | 2017/0157312 | A1 | 6/2017 | Woolford | |
| 9,205,186 | B2 | 12/2015 | Tarkeshian et al. | | 2017/0209639 | A1 | 7/2017 | Wolter | |
| 9,211,096 | B2 | 12/2015 | Tremper et al. | | 2018/0184984 | A1 * | 7/2018 | Zerhusen | A61B 5/6892 |
| 9,289,110 | B2 | 3/2016 | Woolford et al. | | 2019/0070343 | A1 * | 3/2019 | Dumas | A61M 1/0027 |
| 9,289,541 | B2 | 3/2016 | Norman et al. | | | | | | |
| 9,295,582 | B2 | 3/2016 | Rockley et al. | | | | | | |
| D759,063 | S * | 6/2016 | Chen | D14/486 | | | | | |
| 9,433,723 | B2 | 9/2016 | Steen et al. | | | | | | |
| D772,905 | S * | 11/2016 | Ingenlath | D14/486 | | | | | |
| 9,597,445 | B2 | 3/2017 | Ha et al. | | | | | | |
| D800,162 | S * | 10/2017 | Havranek, Jr. | D14/492 | | | | | |
| 9,830,424 | B2 * | 11/2017 | Dixon | G06Q 50/22 | | | | | |
| D835,151 | S * | 12/2018 | Martin | H04W 4/90
D14/488 | | | | | |
| D877,755 | S * | 3/2020 | Iida | D14/485 | | | | | |
| D881,237 | S * | 4/2020 | Arima | D14/495 | | | | | |
| 2003/0052787 | A1 * | 3/2003 | Zerhusen | G16H 20/13
340/573.1 | | | | | |
| 2005/0092523 | A1 | 5/2005 | McCaskill et al. | | | | | | |
| 2006/0290515 | A1 * | 12/2006 | Kankkunen | F16M 11/08
340/572.8 | | | | | |
| 2007/0078370 | A1 | 4/2007 | Shener et al. | | | | | | |
| 2010/0010584 | A1 * | 1/2010 | Skelton | A61B 5/7445
607/62 | | | | | |
| 2010/0050085 | A1 | 2/2010 | Blike et al. | | | | | | |
| 2010/0069937 | A1 | 3/2010 | Seto et al. | | | | | | |
| 2012/0089419 | A1 * | 4/2012 | Huster | A61B 5/1115
705/3 | | | | | |
| 2012/0130308 | A1 | 5/2012 | Silkaitis et al. | | | | | | |
| 2012/0138533 | A1 | 6/2012 | Curtis et al. | | | | | | |
| 2012/0302941 | A1 | 11/2012 | Teodorescu et al. | | | | | | |
| 2013/0317417 | A1 | 11/2013 | Claus et al. | | | | | | |

OTHER PUBLICATIONS

- “Bed, hospital, medical, patient, sick, treatment icon” Feb. 11, 2017, posted at iconfinder.com, [site visited Apr. 14, 2020]. <https://www.iconfinder.com/iconsets/medical-health-care-blue-series-set-1> (Year: 2017).*
- “Hospital Bed Remote Control Panel stock photo” Jun. 11, 2012, posted at istockphoto.com, [site visited Apr. 14, 2020]. <https://www.istockphoto.com/photo/hospital-bed-remote-control-panel-gm182153618-18921428> (Year: 2012).*
- “Arthrex Continuous Wave III Arthroscopy Pump User’s Guide”, 2013, 52 pages.
- “Arthrex Dual Wave Arthroscopy Pump User’s Guide”, 2015, 60 pages.
- “Arthrex Dual Wave Quick Reference, brochure”, 2015, 10 pages.
- “Arthrex Fluid Management, brochure”, 2016, 8 pages.
- “Con Med 24k Pump”, Product Overview, Aug. 29, 2017, 3 pages.
- “Con Med 24k Quick Set Up Guide, brochure”, 2010, 4 pages.
- “DePuy Mitek K130169 501 (k) Summary, dated prepared Jan. 22, 2013”, May 1, 2013, 8 pages.
- “International Search Report and Written Opinion for International App. No. PCT/US18/48814”, dated Nov. 15, 2018, 9 pages.
- “PowerPump System Operator’s Manual”, 2010, 32 pages.

* cited by examiner

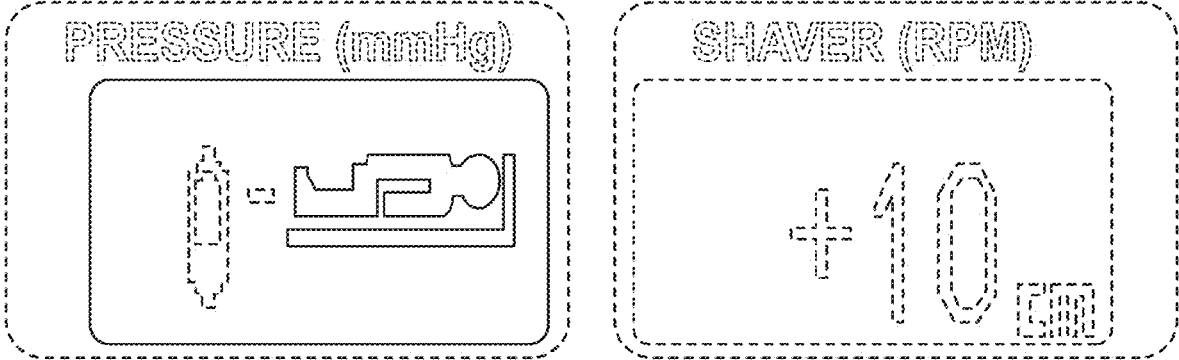


FIG. 1

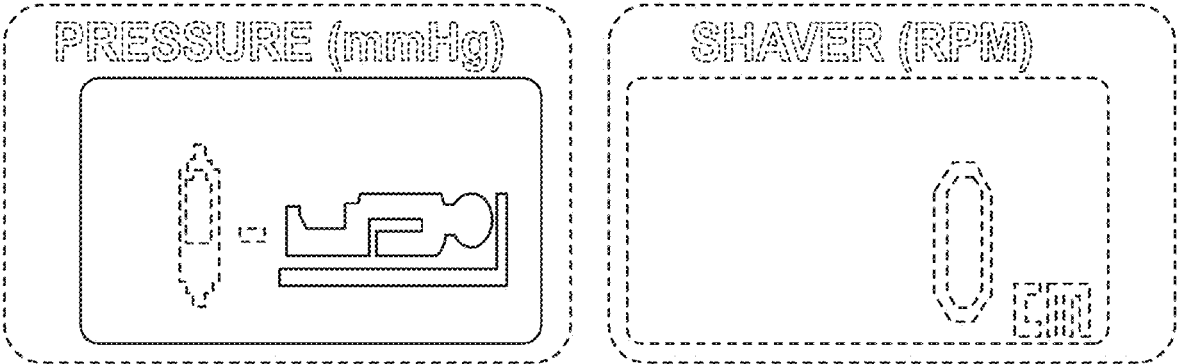


FIG. 2

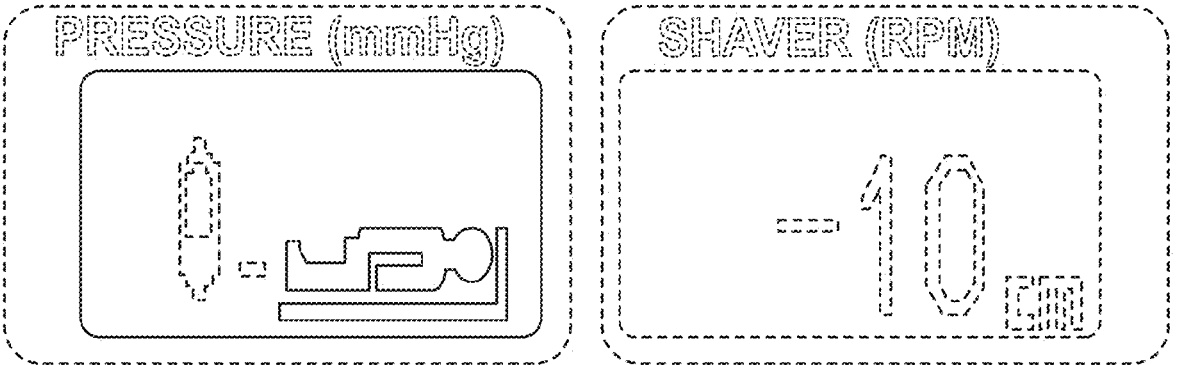


FIG. 3