



US 20120191174A1

(19) **United States**

(12) **Patent Application Publication**
Vinluan et al.

(10) **Pub. No.: US 2012/0191174 A1**

(43) **Pub. Date: Jul. 26, 2012**

(54) **ADVANCED ENDOVASCULAR GRAFT AND DELIVERY SYSTEM**

(21) Appl. No.: **13/297,219**

(22) Filed: **Nov. 15, 2011**

(75) Inventors: **Jenine S. Vinluan**, Petaluma, CA (US); **Mark Eugene Purter**, Windsor, CA (US); **William Patrick Stephens**, Santa Rosa, CA (US); **Mark Geusen**, Santa Rosa, CA (US); **Carl Hermann Poppe**, Danville, CA (US); **Christopher Lynn Staudenmayer**, Santa Rosa, CA (US); **Diego Aristizabal**, Santa Rosa, CA (US); **Michael V. Chobotov**, Santa Rosa, CA (US); **James R. Watson**, Santa Rosa, CA (US); **Teresa Woodson**, Santa Rosa, CA (US); **Riley King**, Santa Rosa, CA (US)

Related U.S. Application Data

(60) Provisional application No. 61/414,375, filed on Nov. 16, 2010.


Publication Classification

(51) **Int. Cl.**
A61F 2/06 (2006.01)
A61F 2/84 (2006.01)
(52) **U.S. Cl.** **623/1.12; 623/1.13; 623/1.11**

(57) **ABSTRACT**

Embodiments are directed in part to endovascular prostheses and methods of deploying same. Embodiments may be directed more specifically to stent grafts and methods of positioning and deploying such devices within the body of a patient.

(73) Assignee: **TRIVASCULAR, INC.**, Santa Rosa, CA (US)

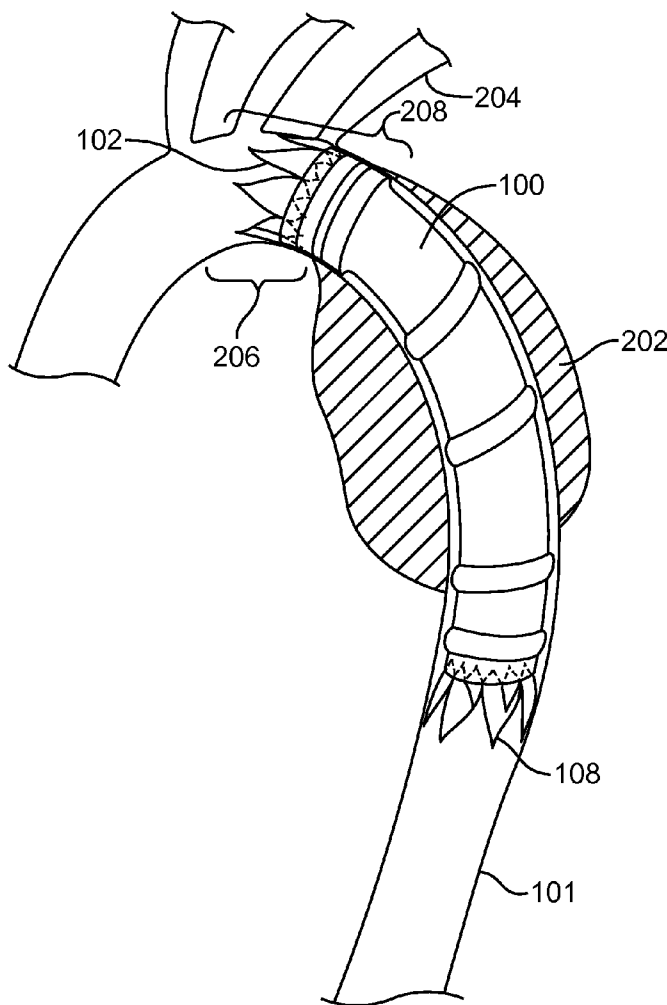

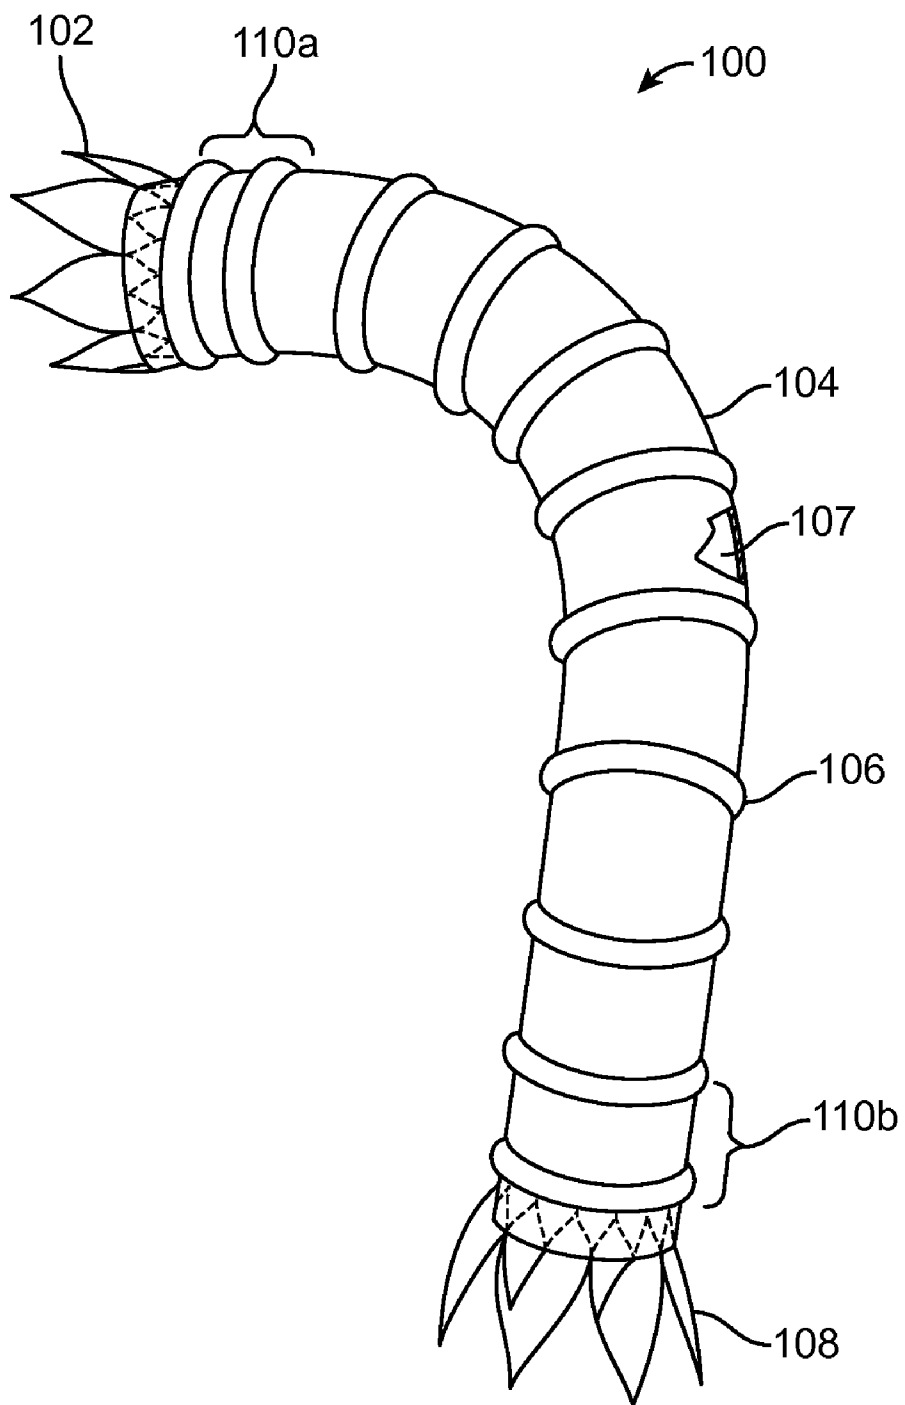


FIG. 1

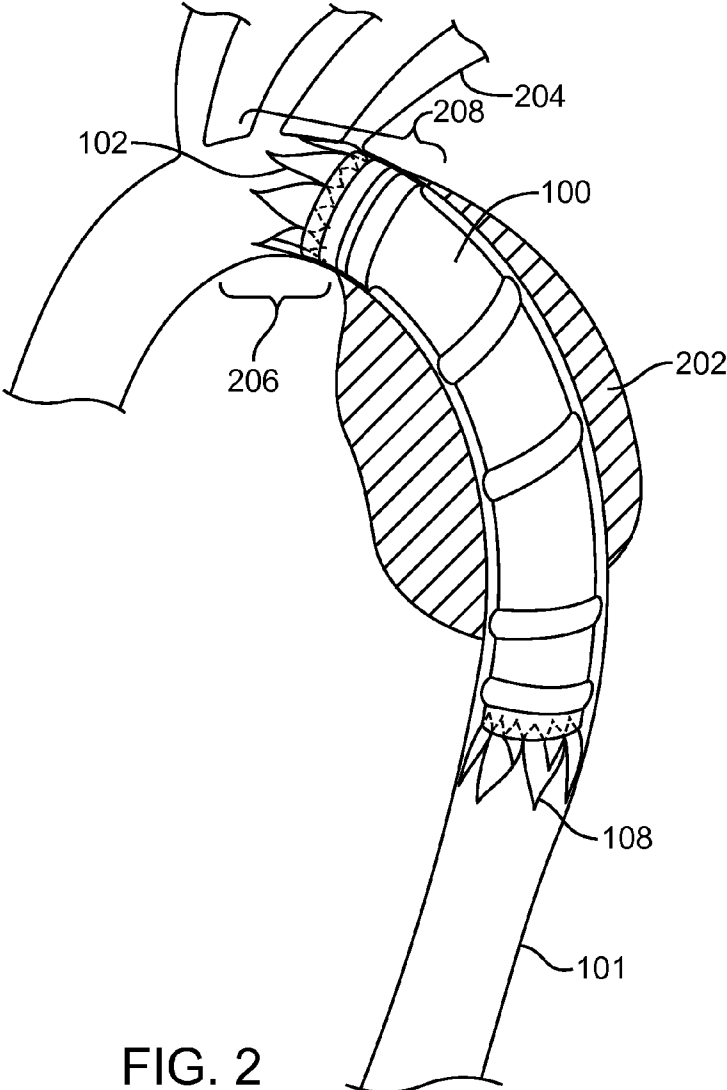


FIG. 2

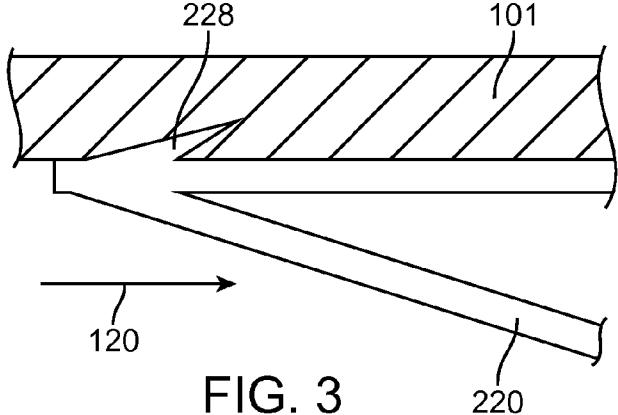


FIG. 3

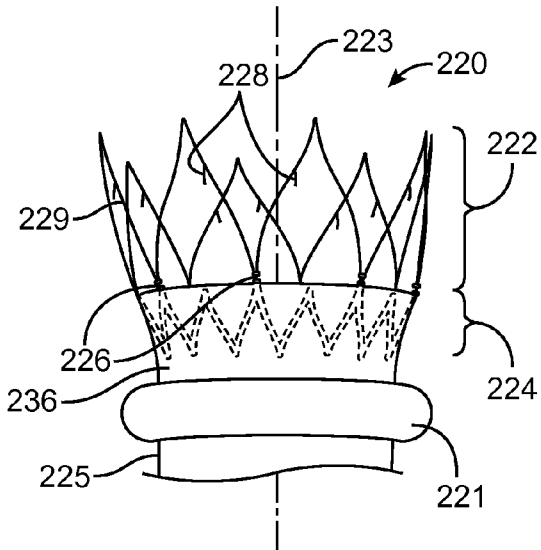


FIG. 4




FIG. 5

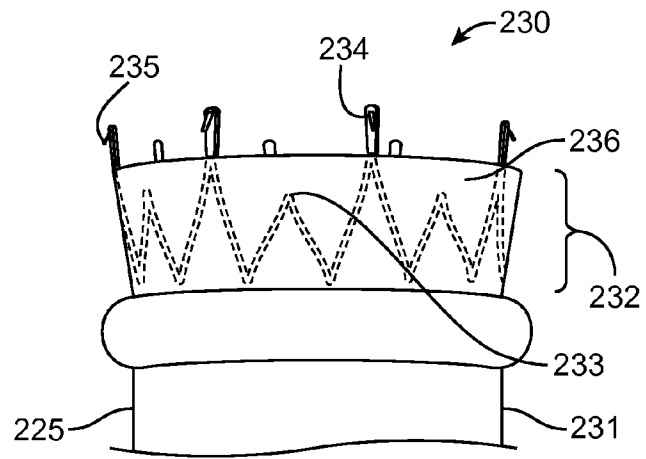


FIG. 6

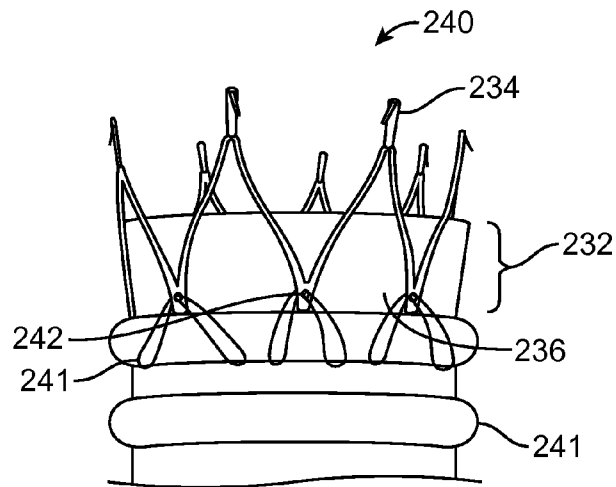


FIG. 7

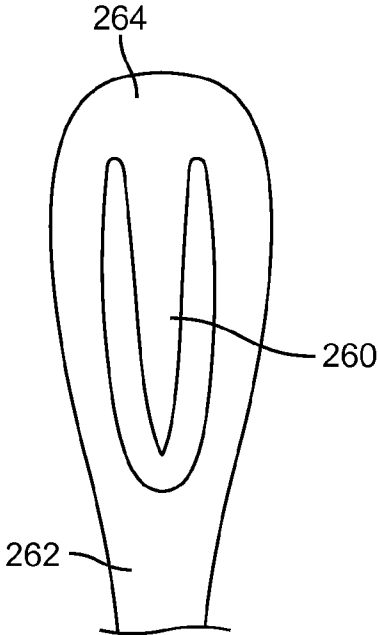


FIG. 8

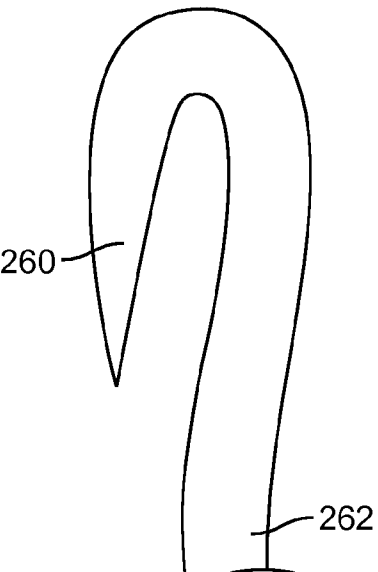


FIG. 9

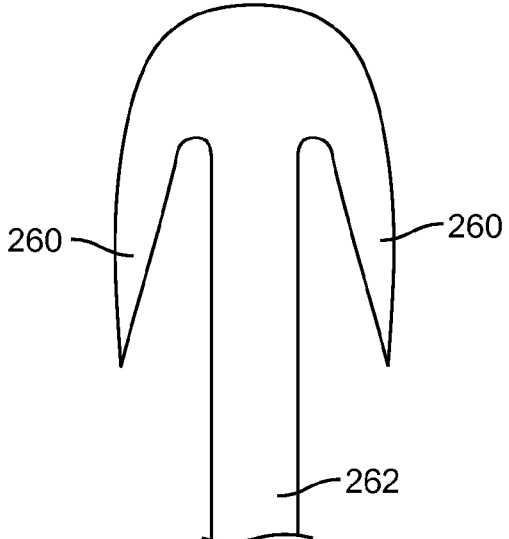


FIG. 10

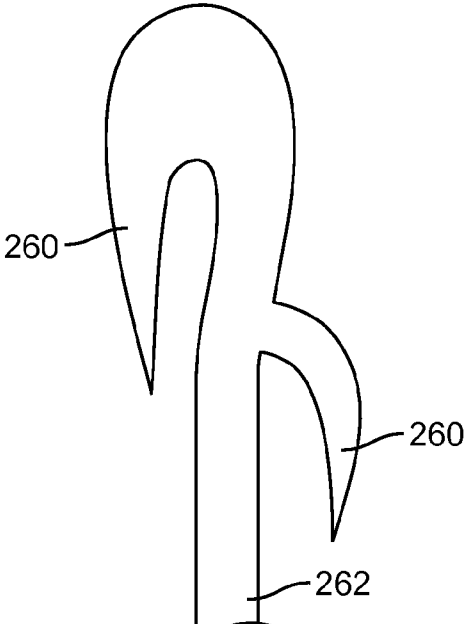


FIG. 11

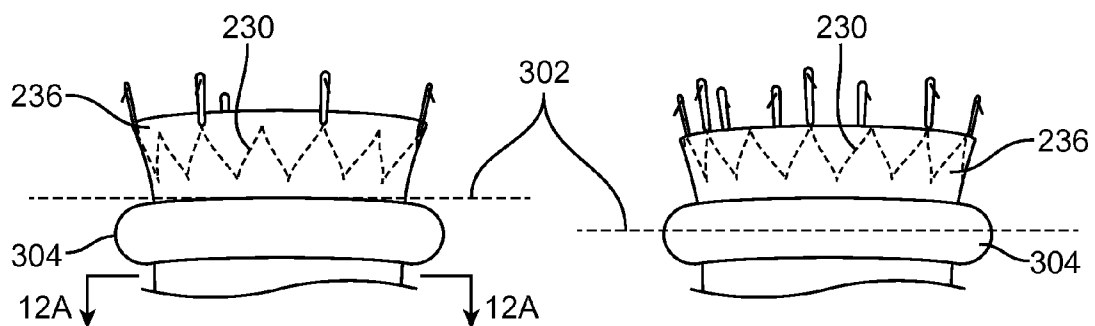


FIG. 12

FIG. 13




FIG. 12A

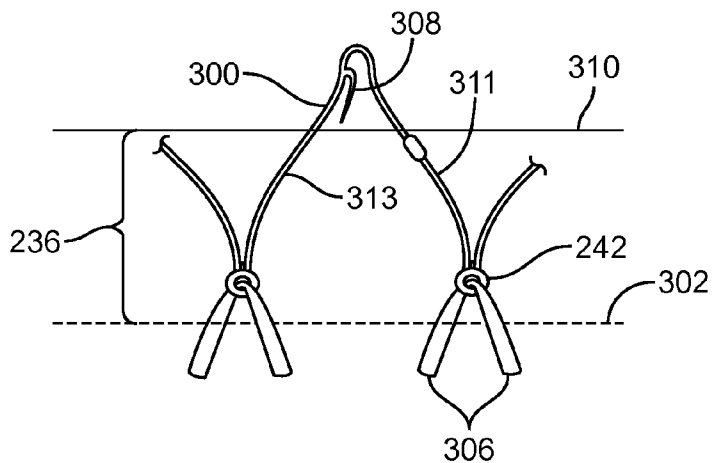


FIG. 14

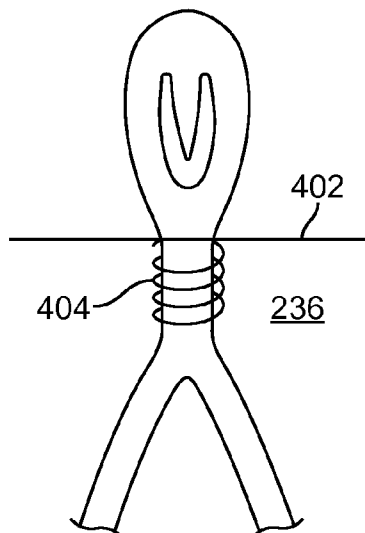


FIG. 15

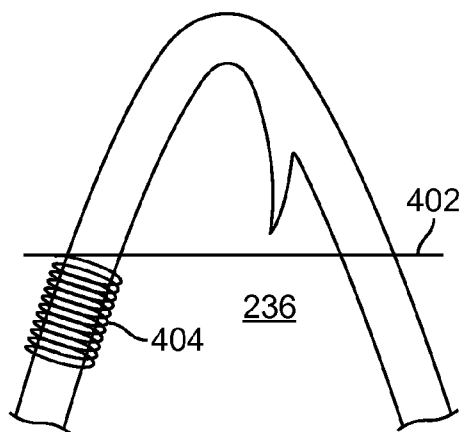


FIG. 16

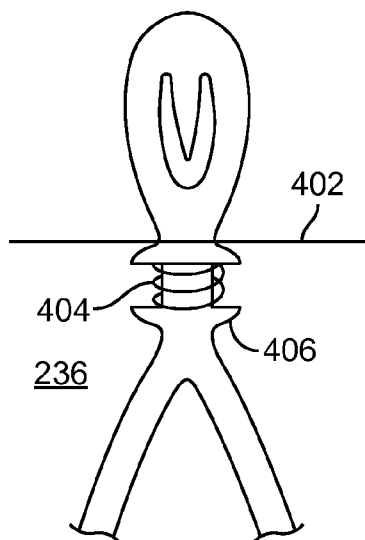


FIG. 17

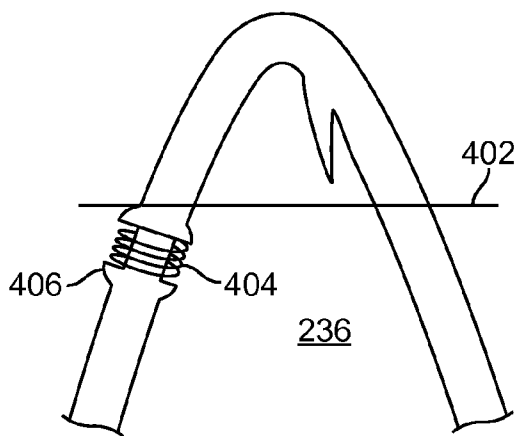
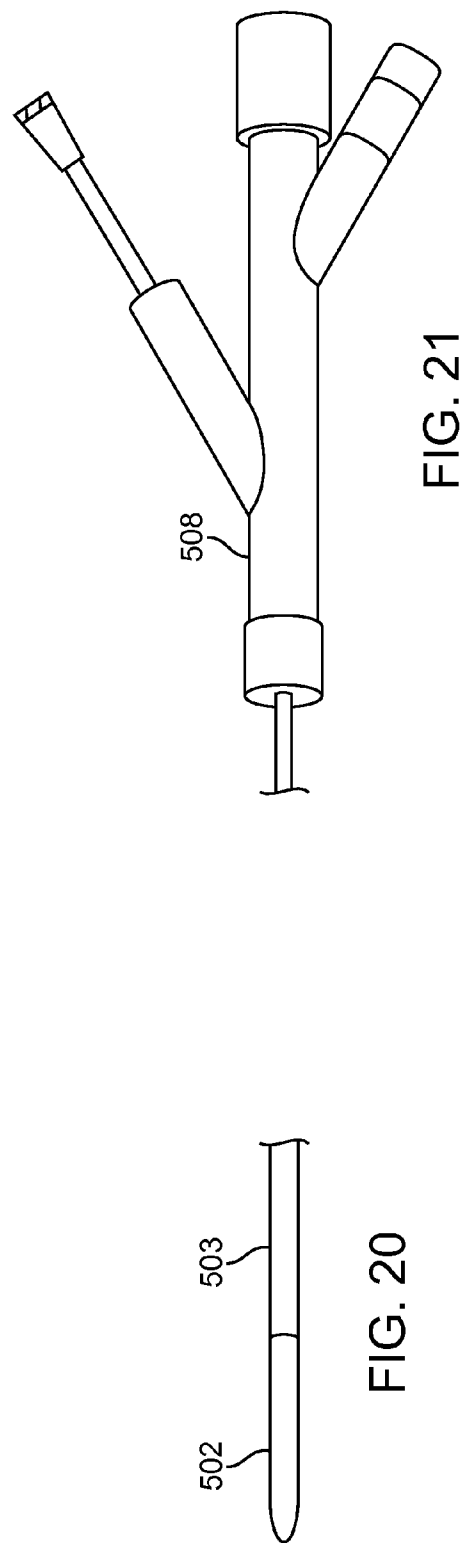
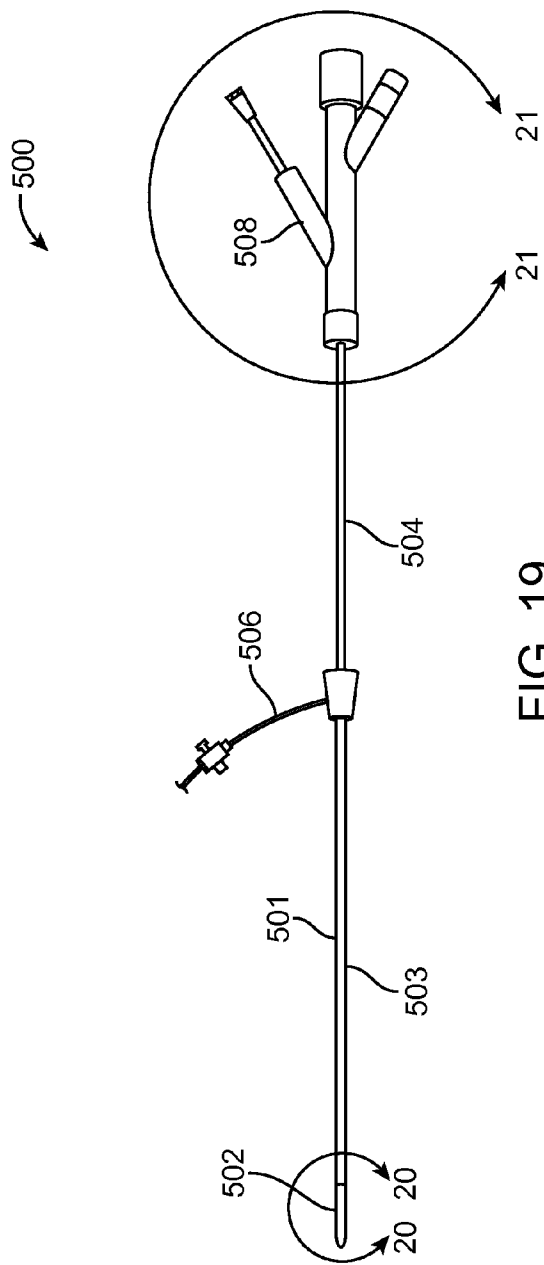


FIG. 18



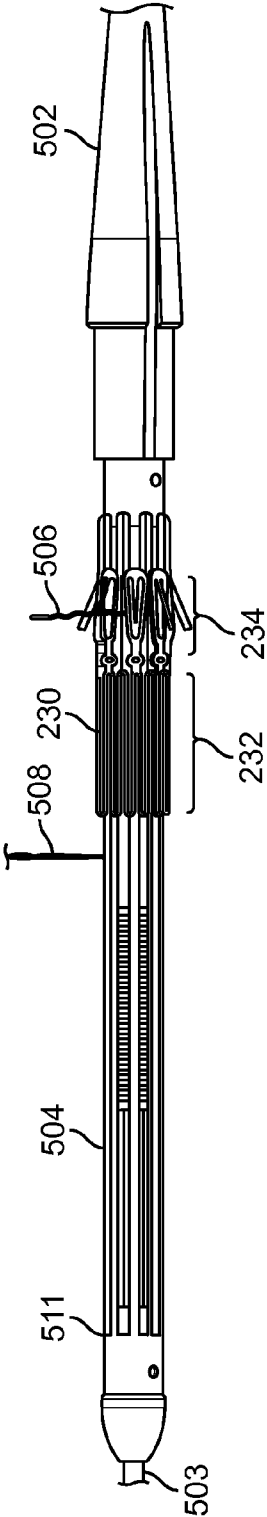


FIG. 22

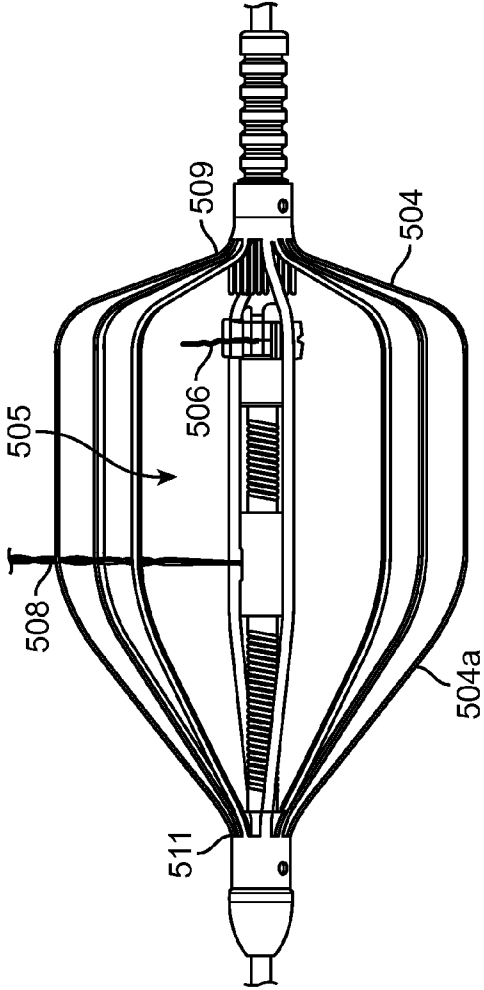


FIG. 23

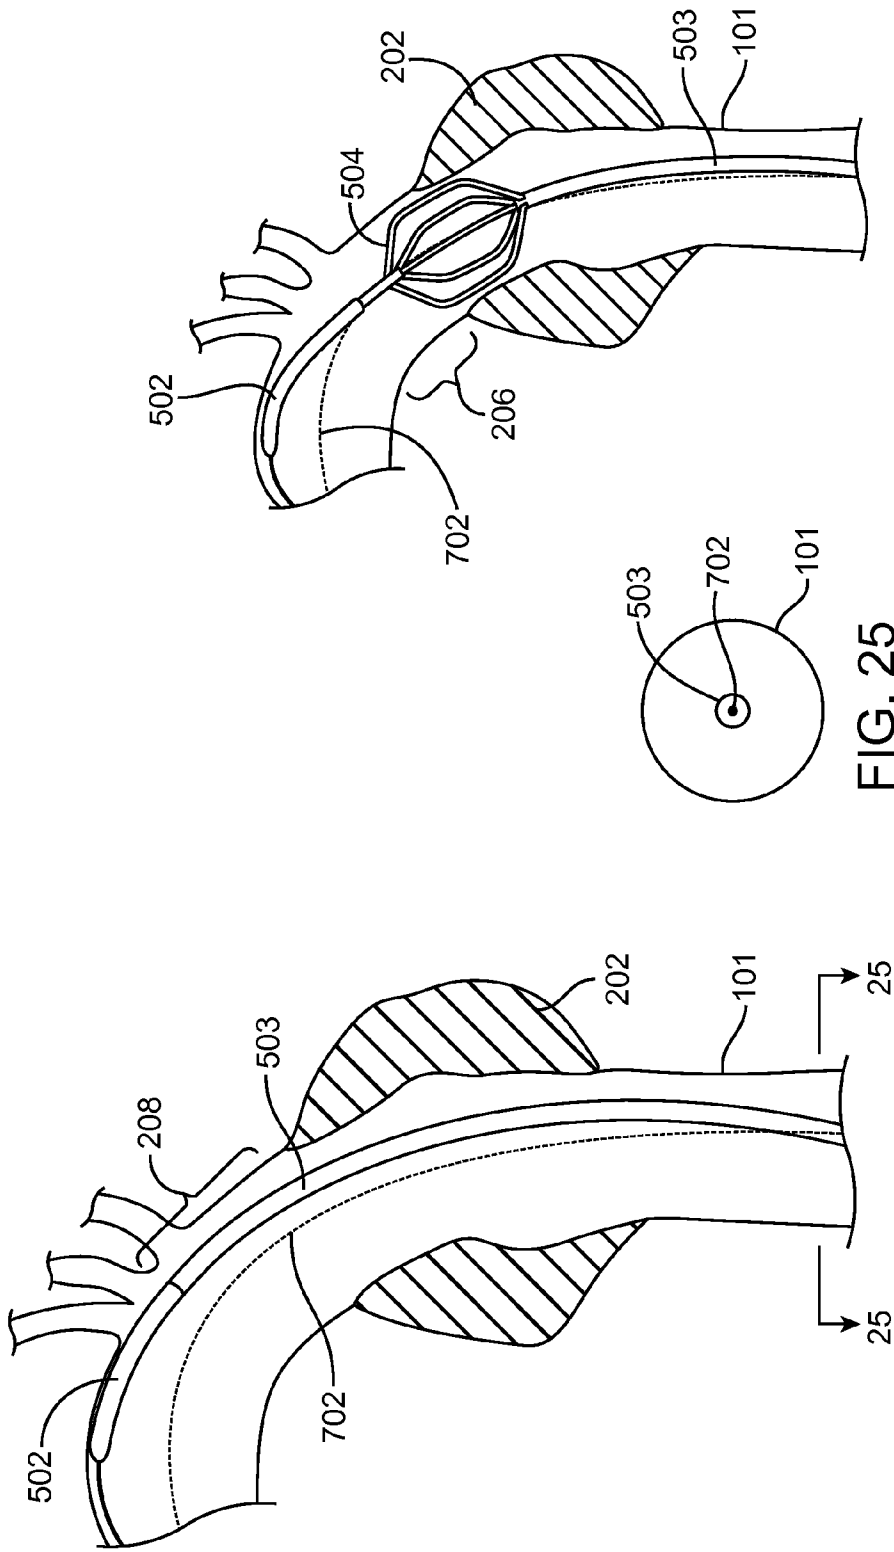


FIG. 26

FIG. 25

FIG. 24

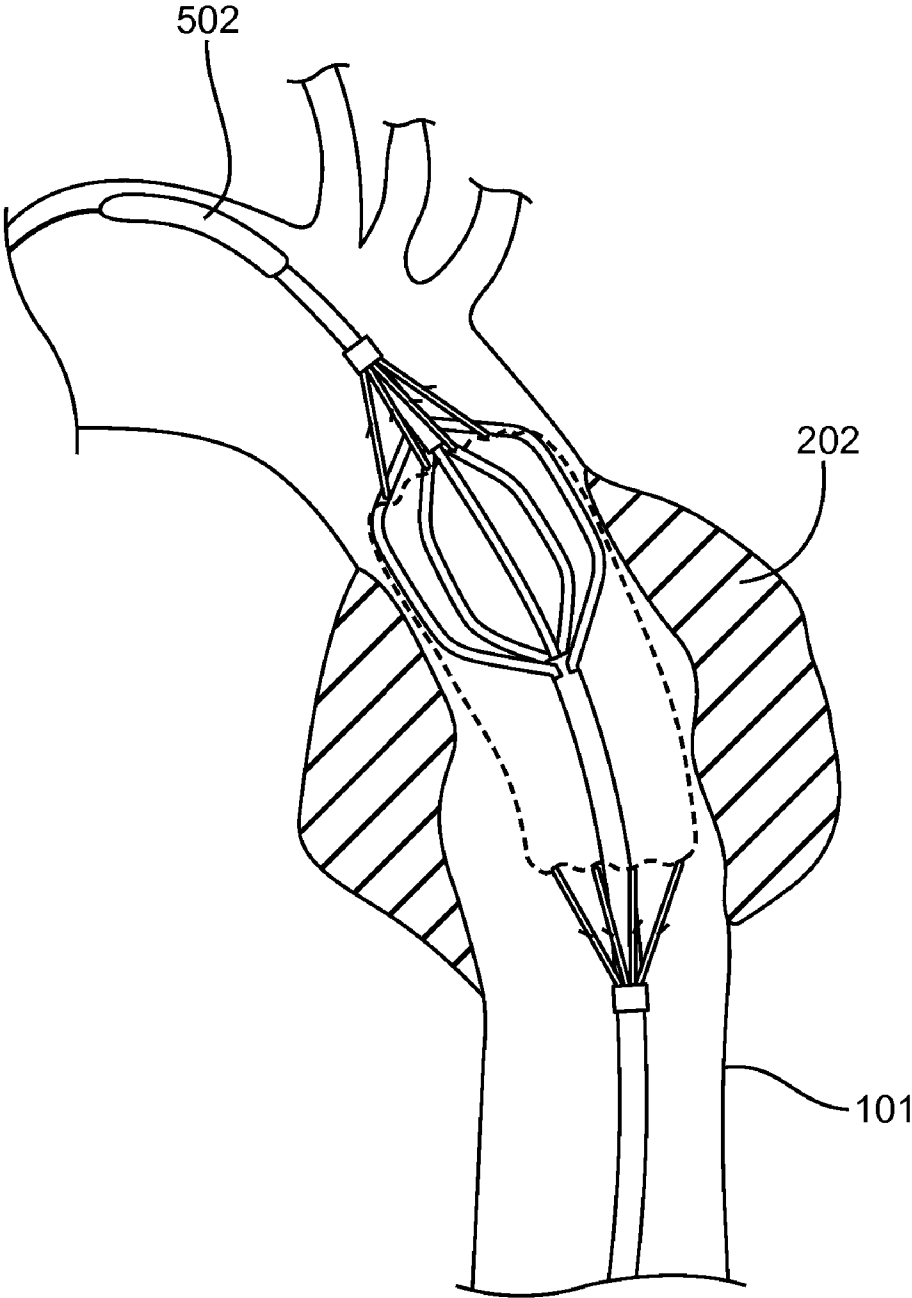


FIG. 27

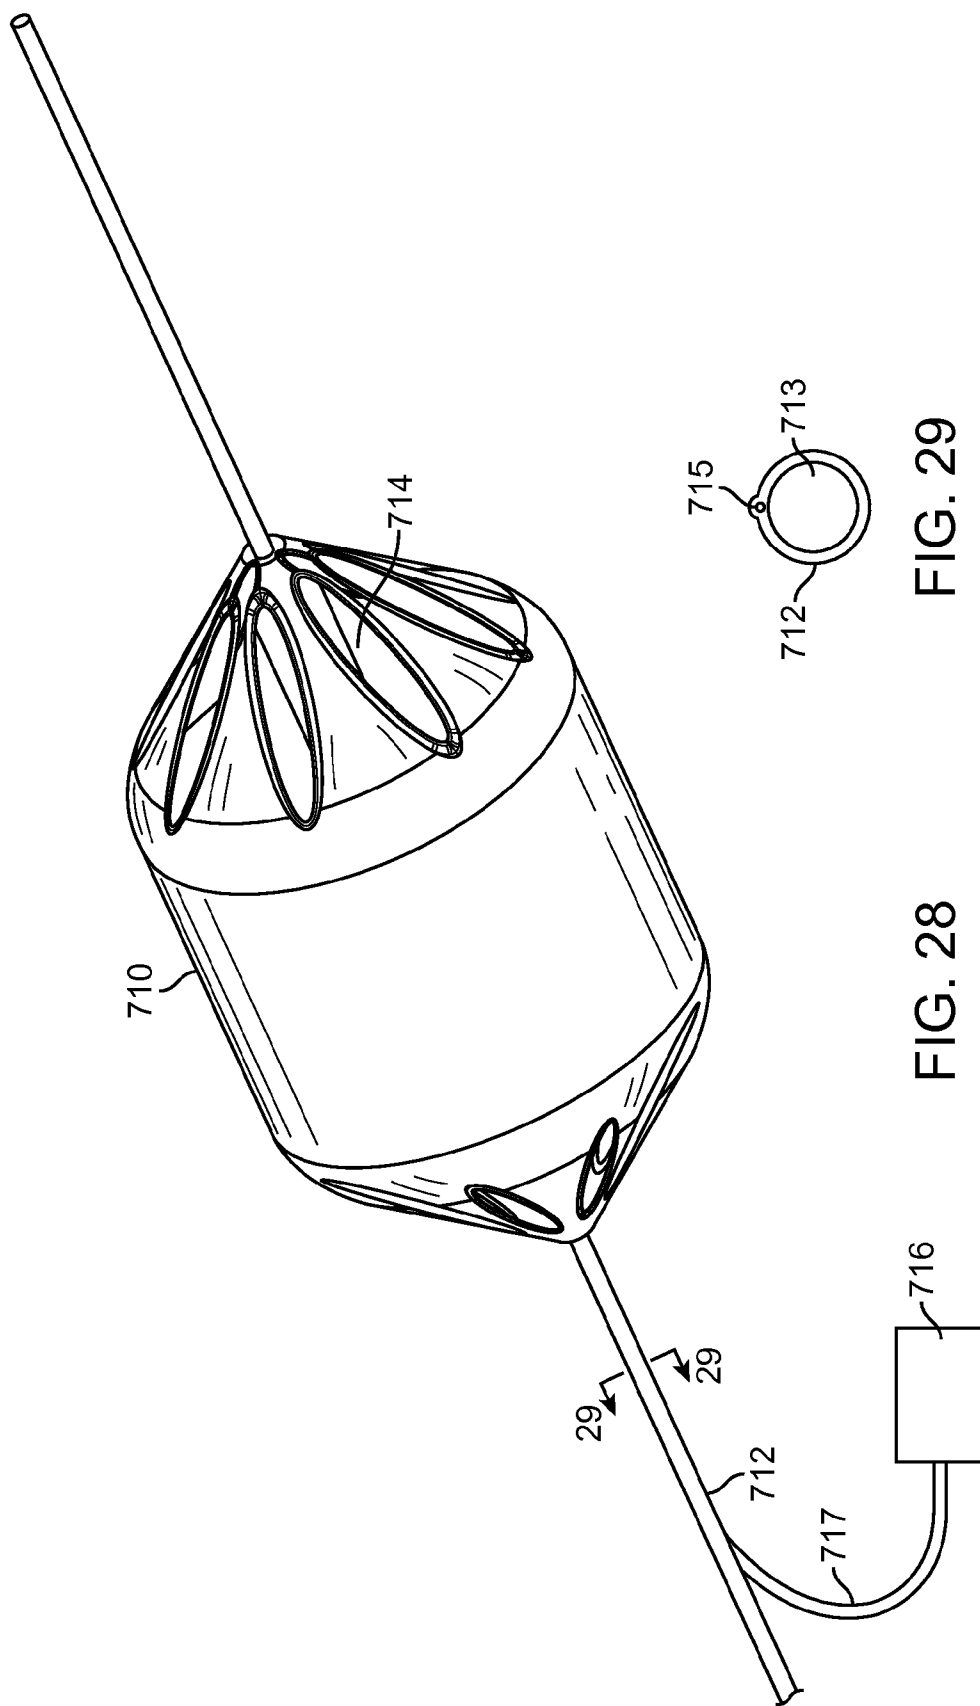


FIG. 29

FIG. 28

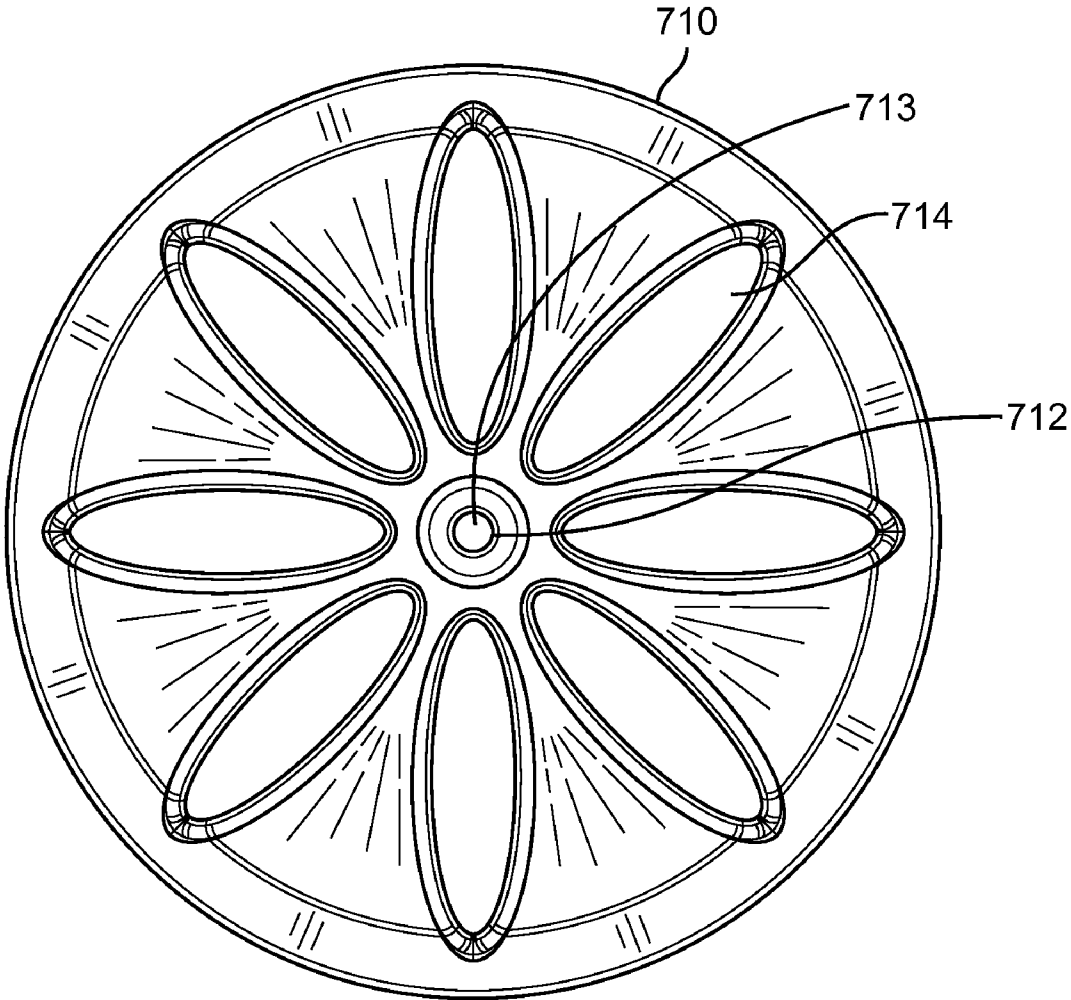


FIG. 30

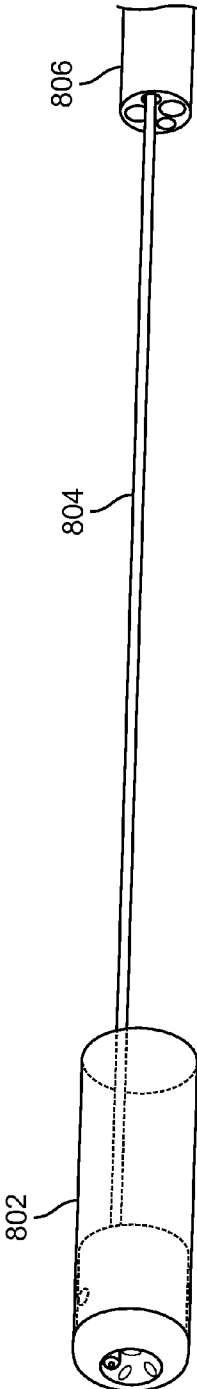


FIG. 31

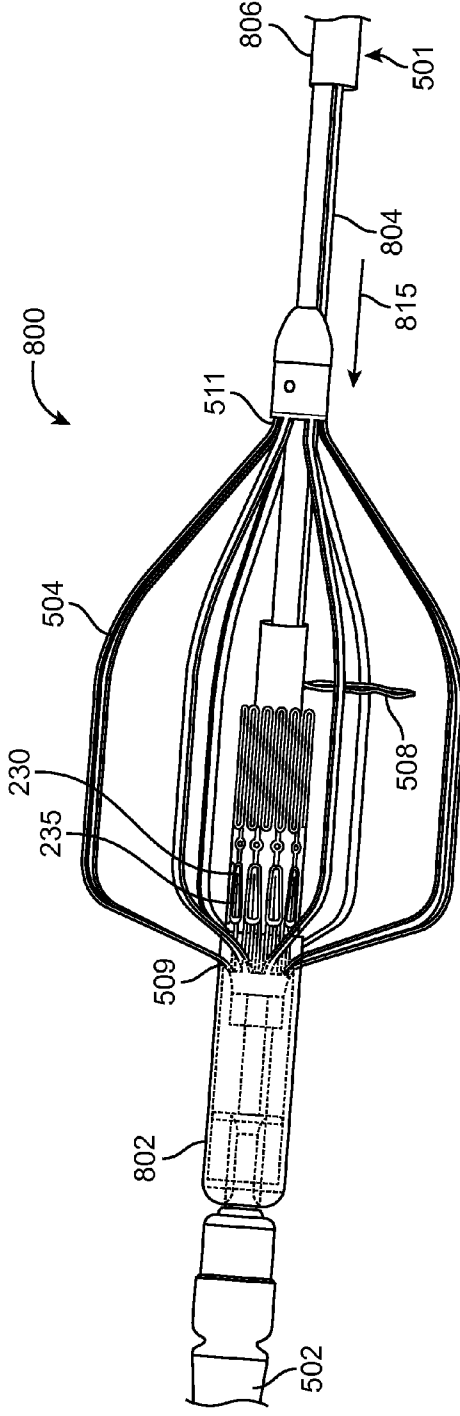


FIG. 32

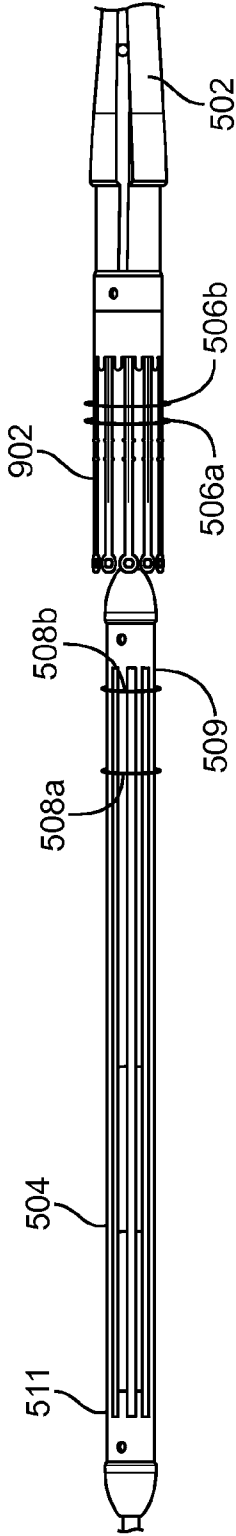


FIG. 33

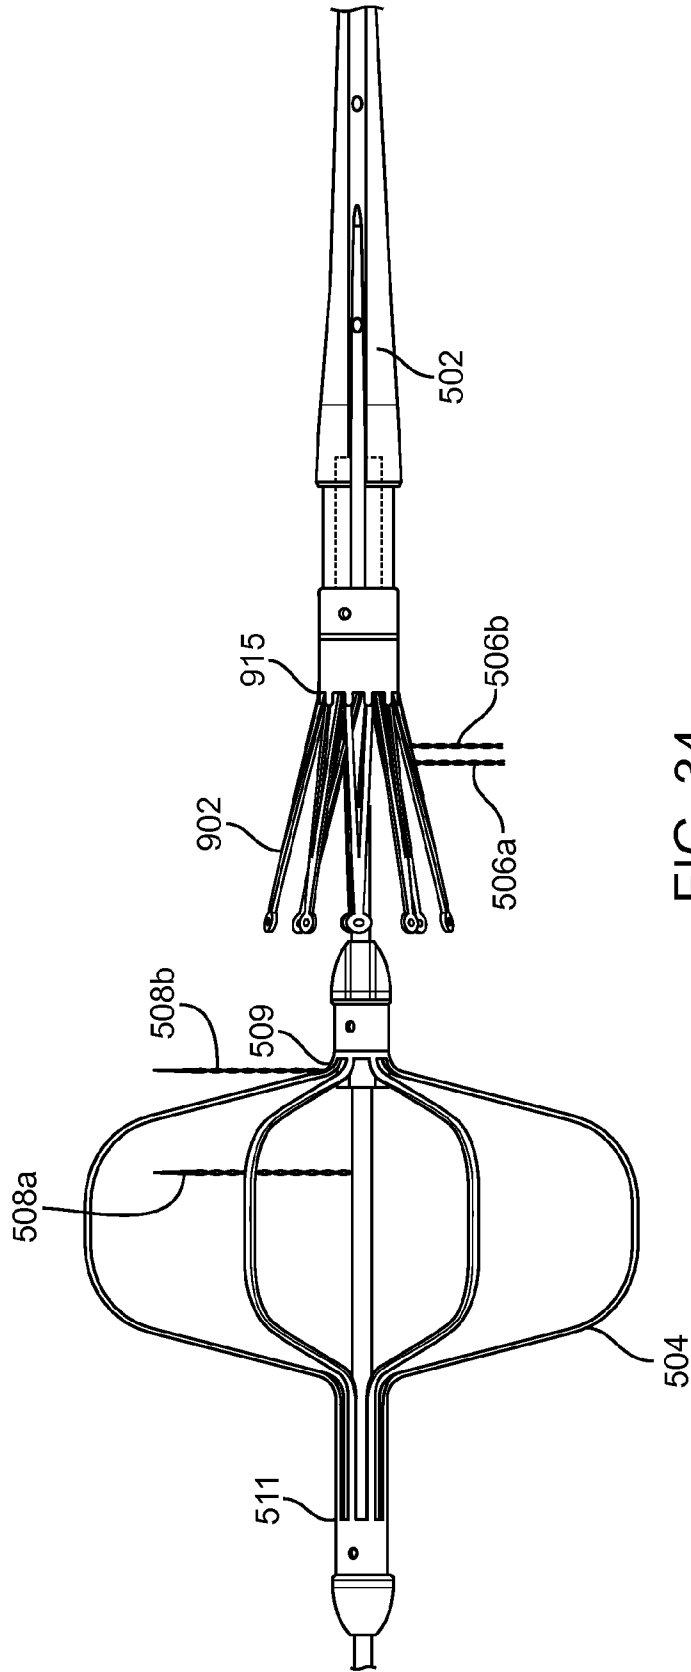


FIG. 34

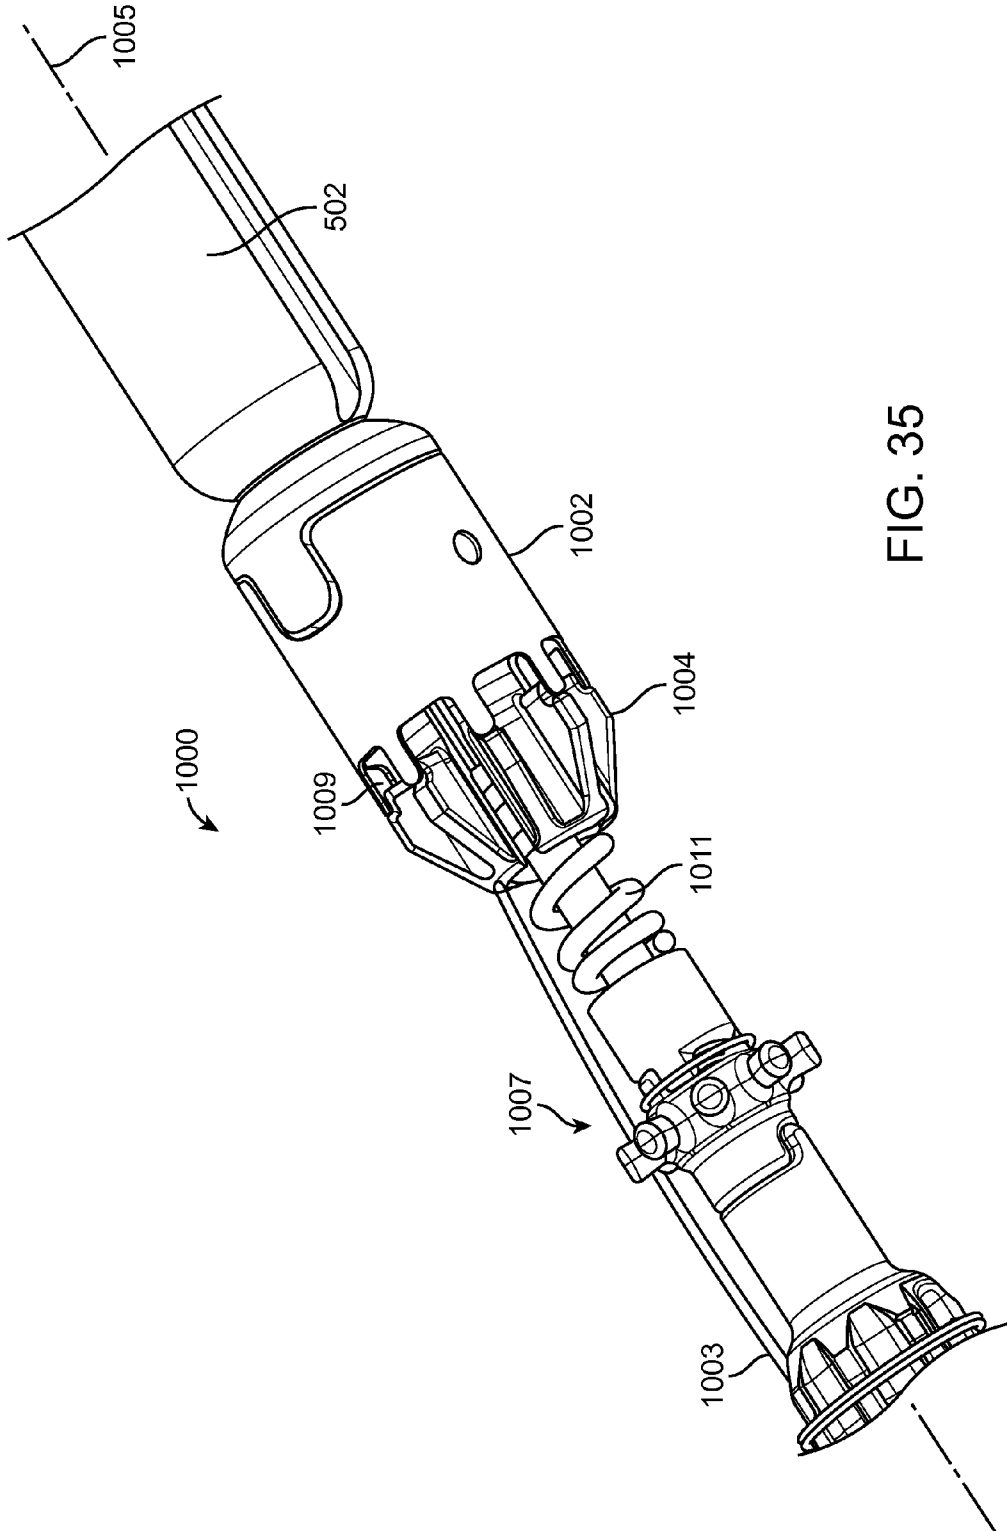


FIG. 35

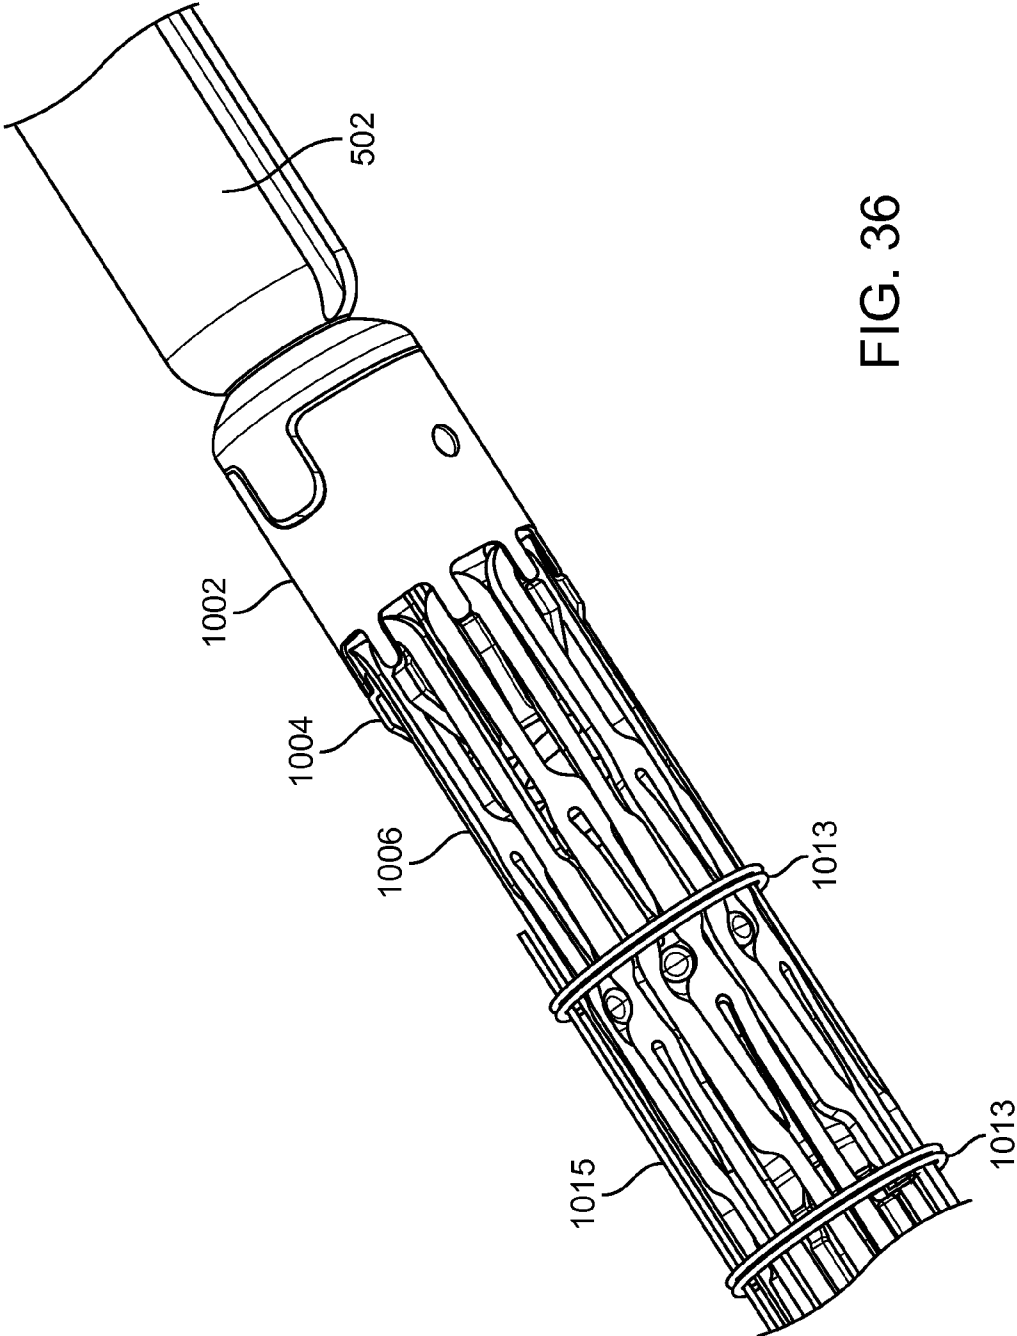


FIG. 36

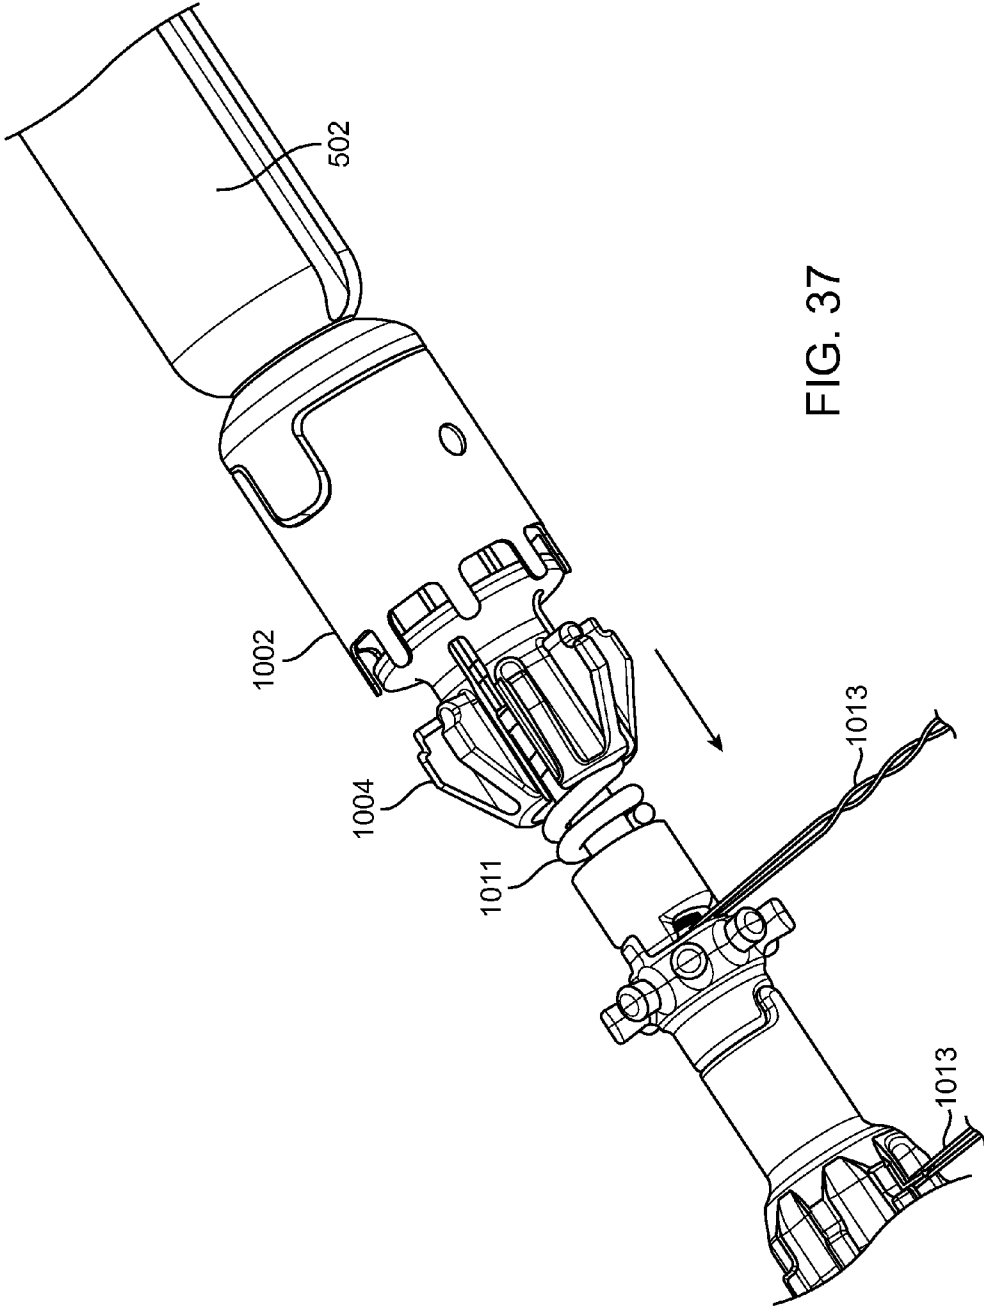


FIG. 37

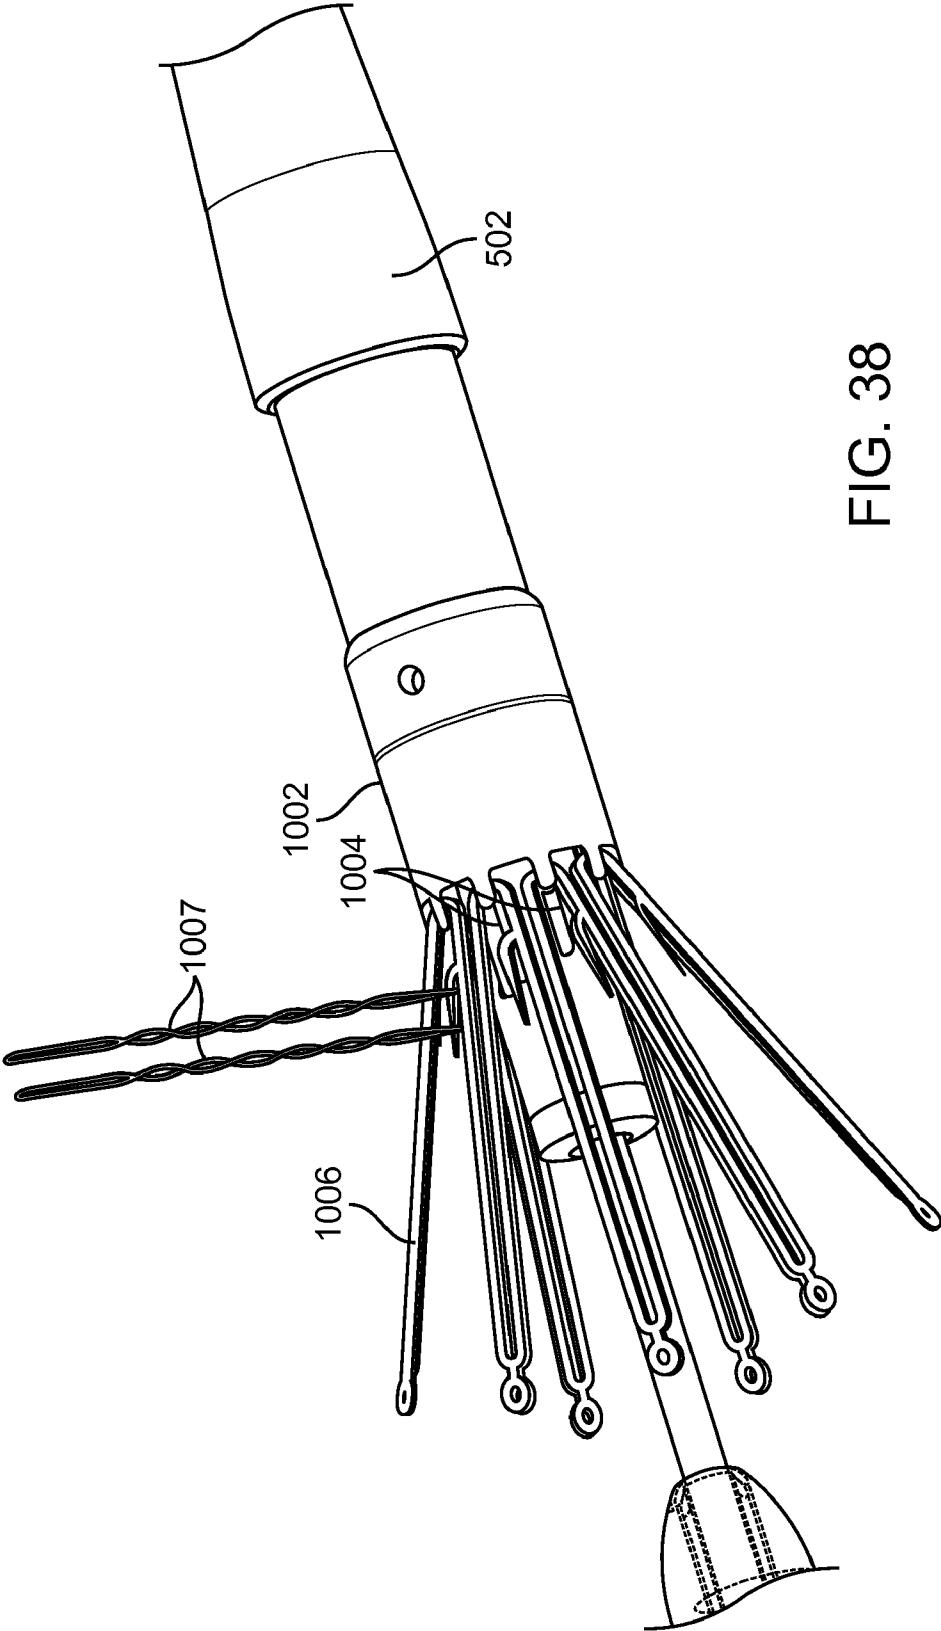


FIG. 38

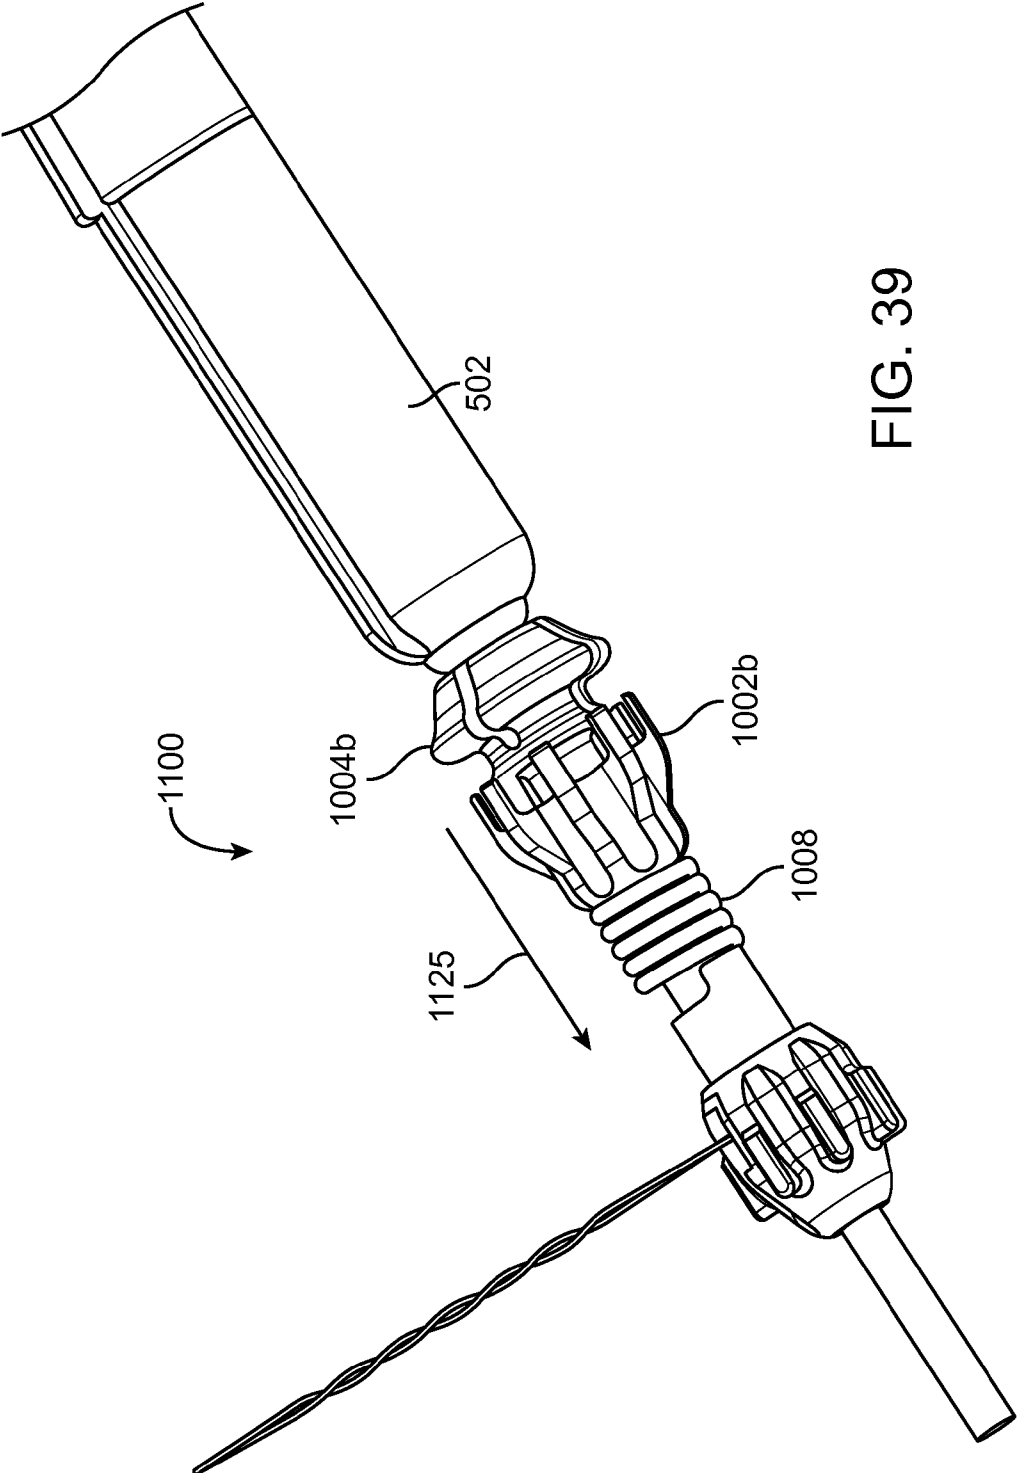


FIG. 39

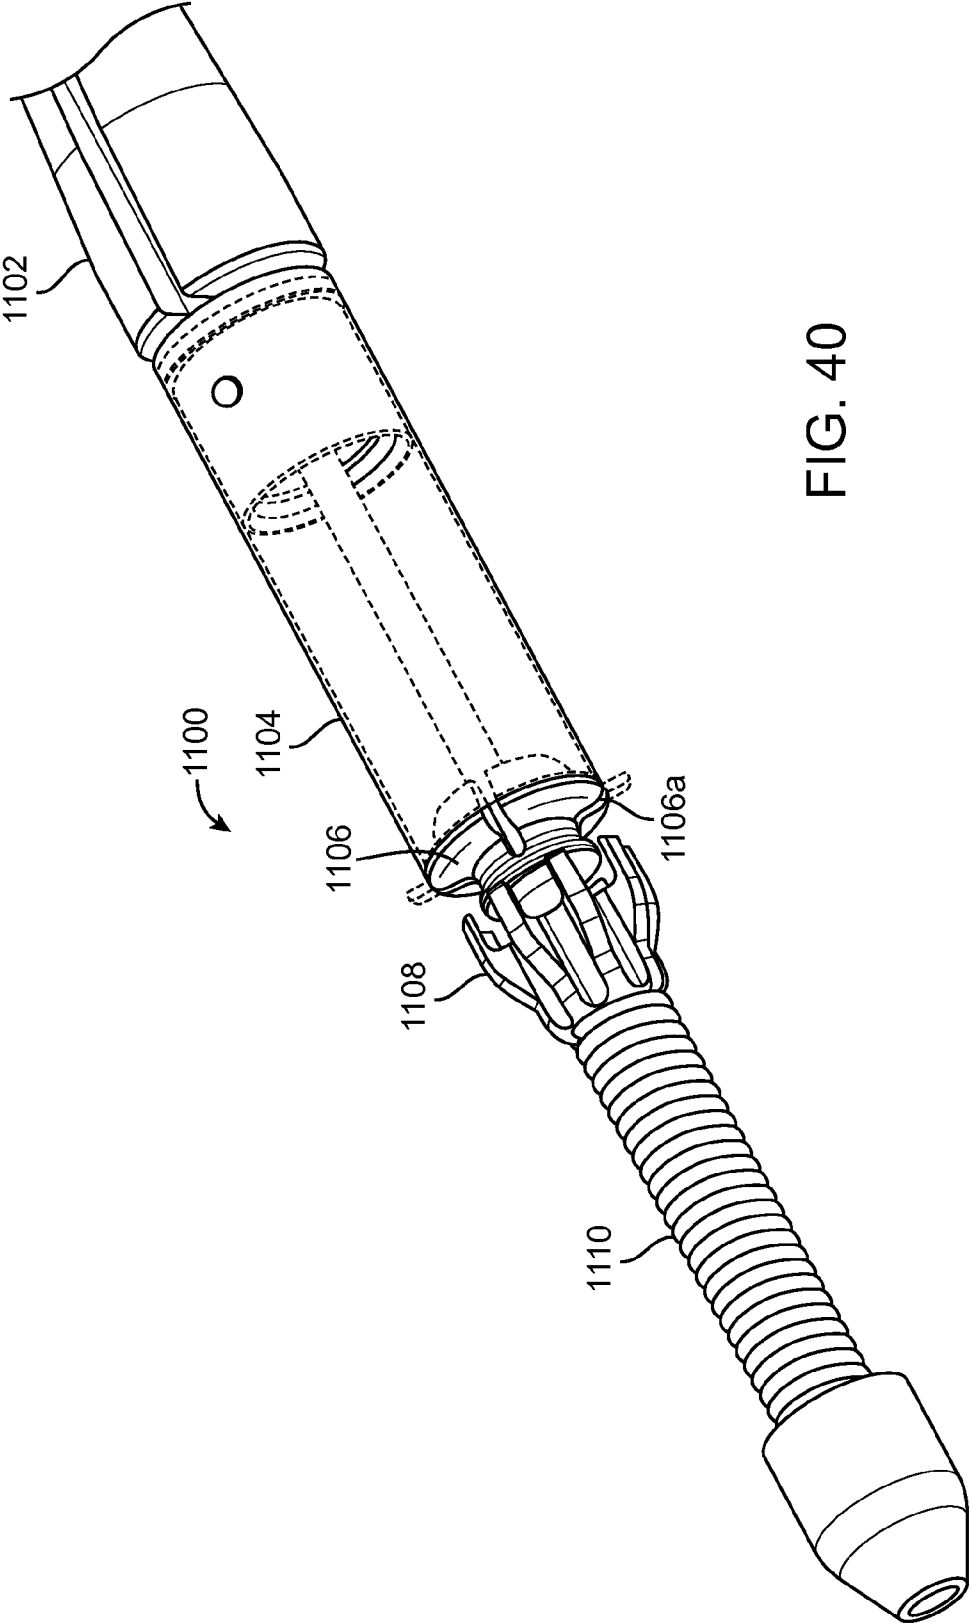


FIG. 40

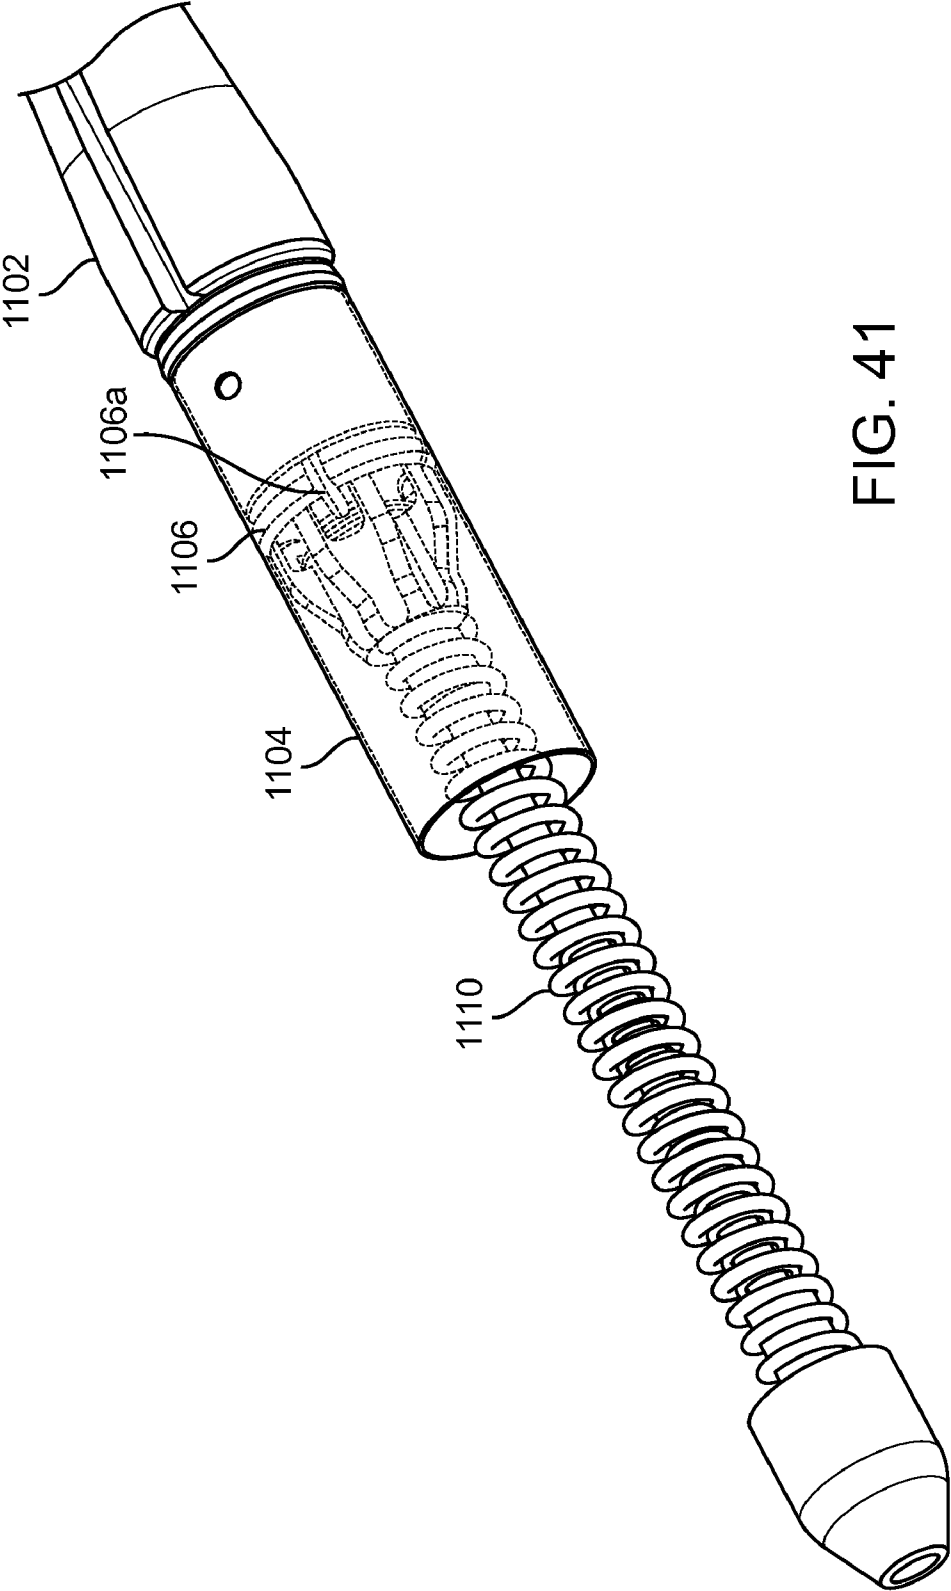


FIG. 41

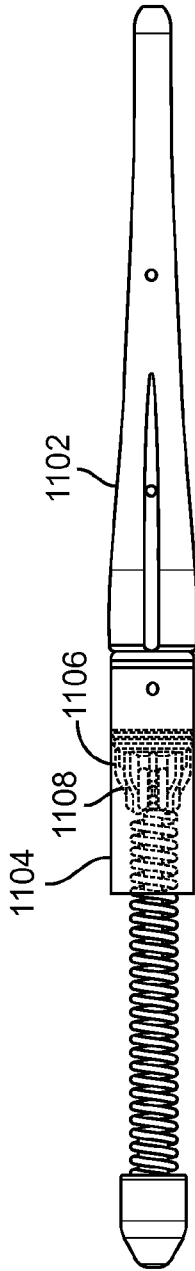


FIG. 42

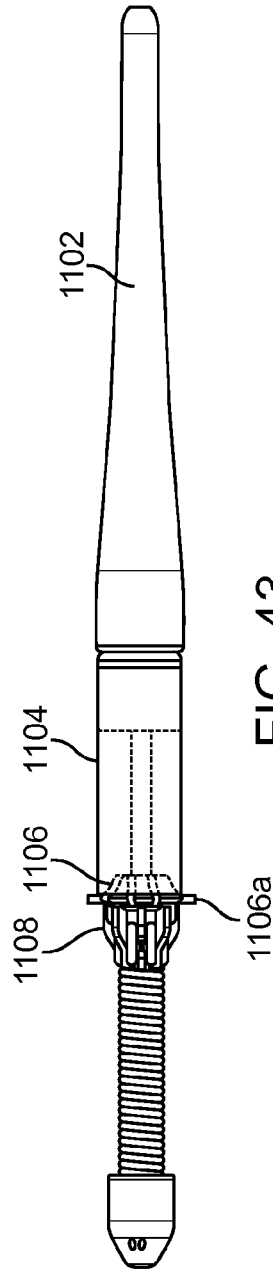


FIG. 43

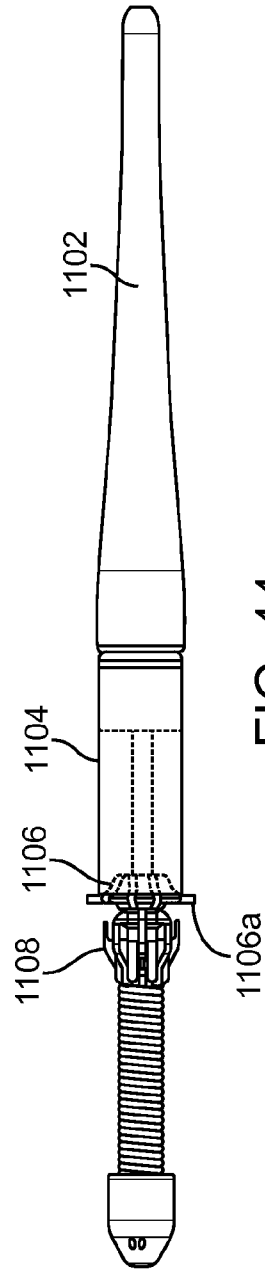


FIG. 44

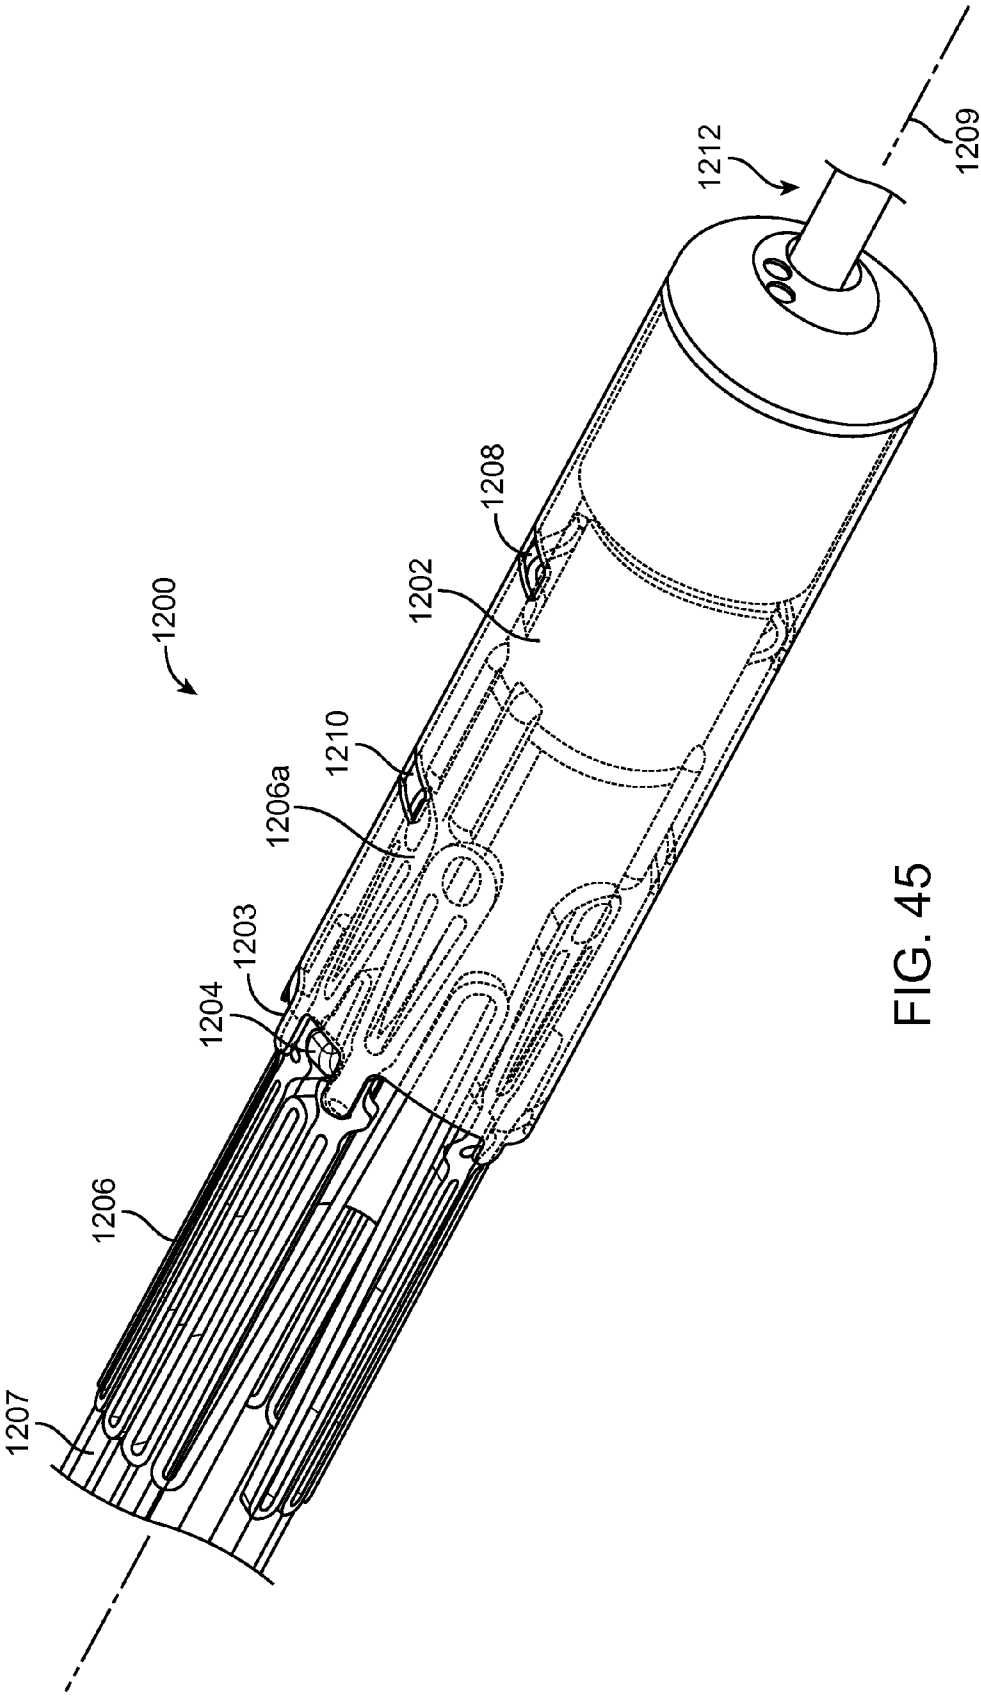


FIG. 45

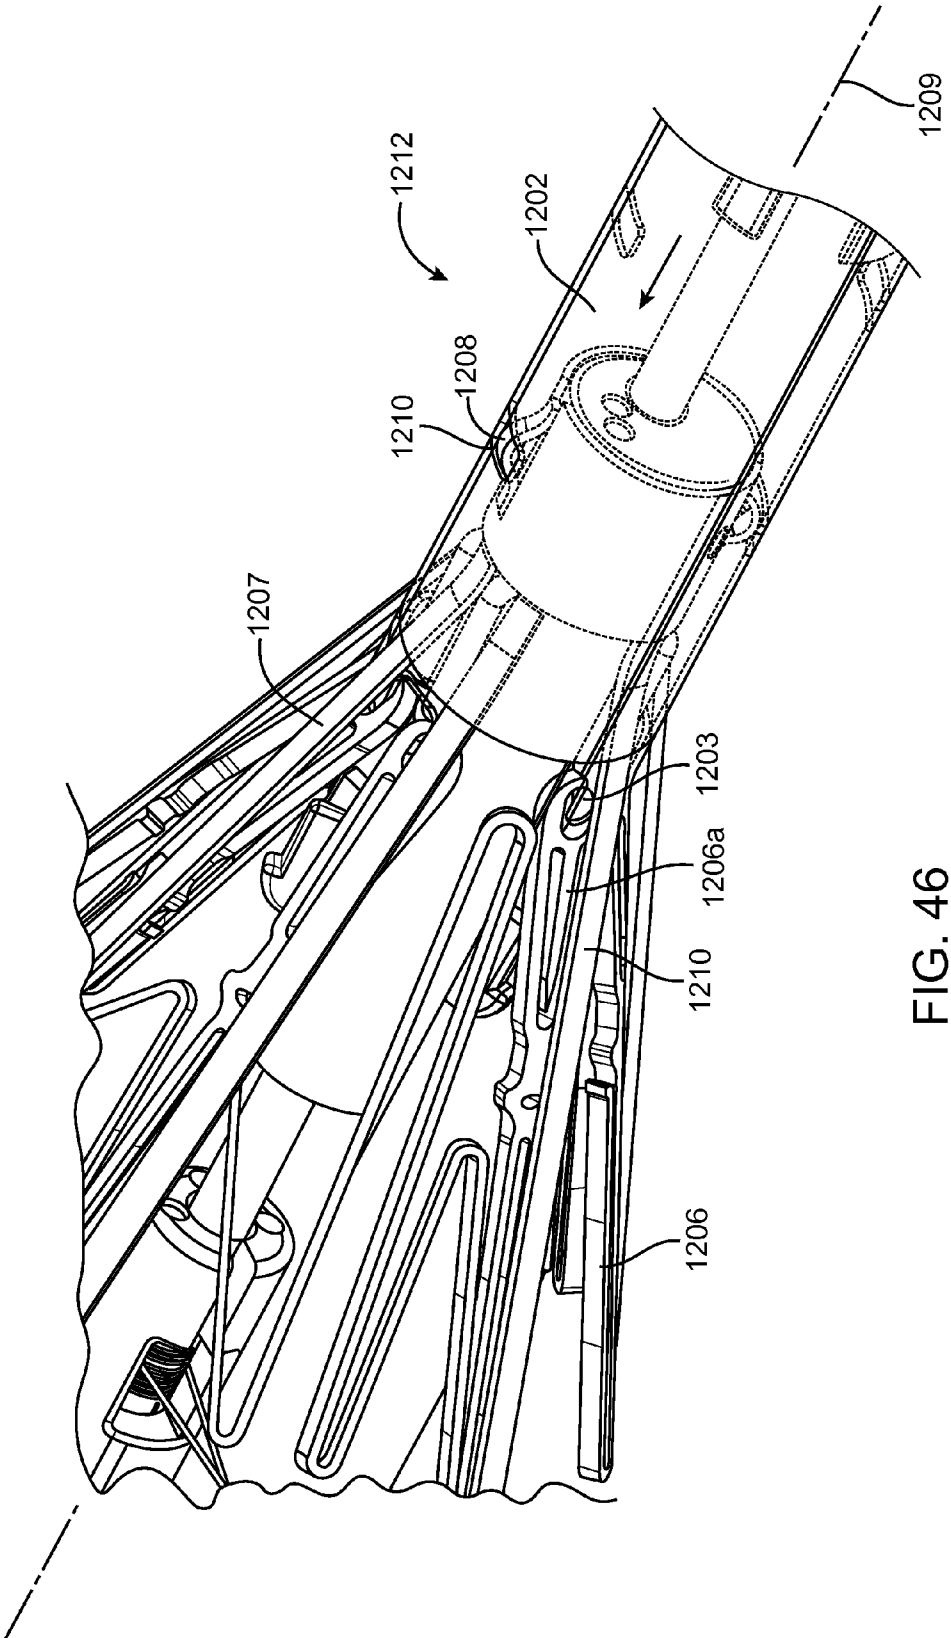


FIG. 46

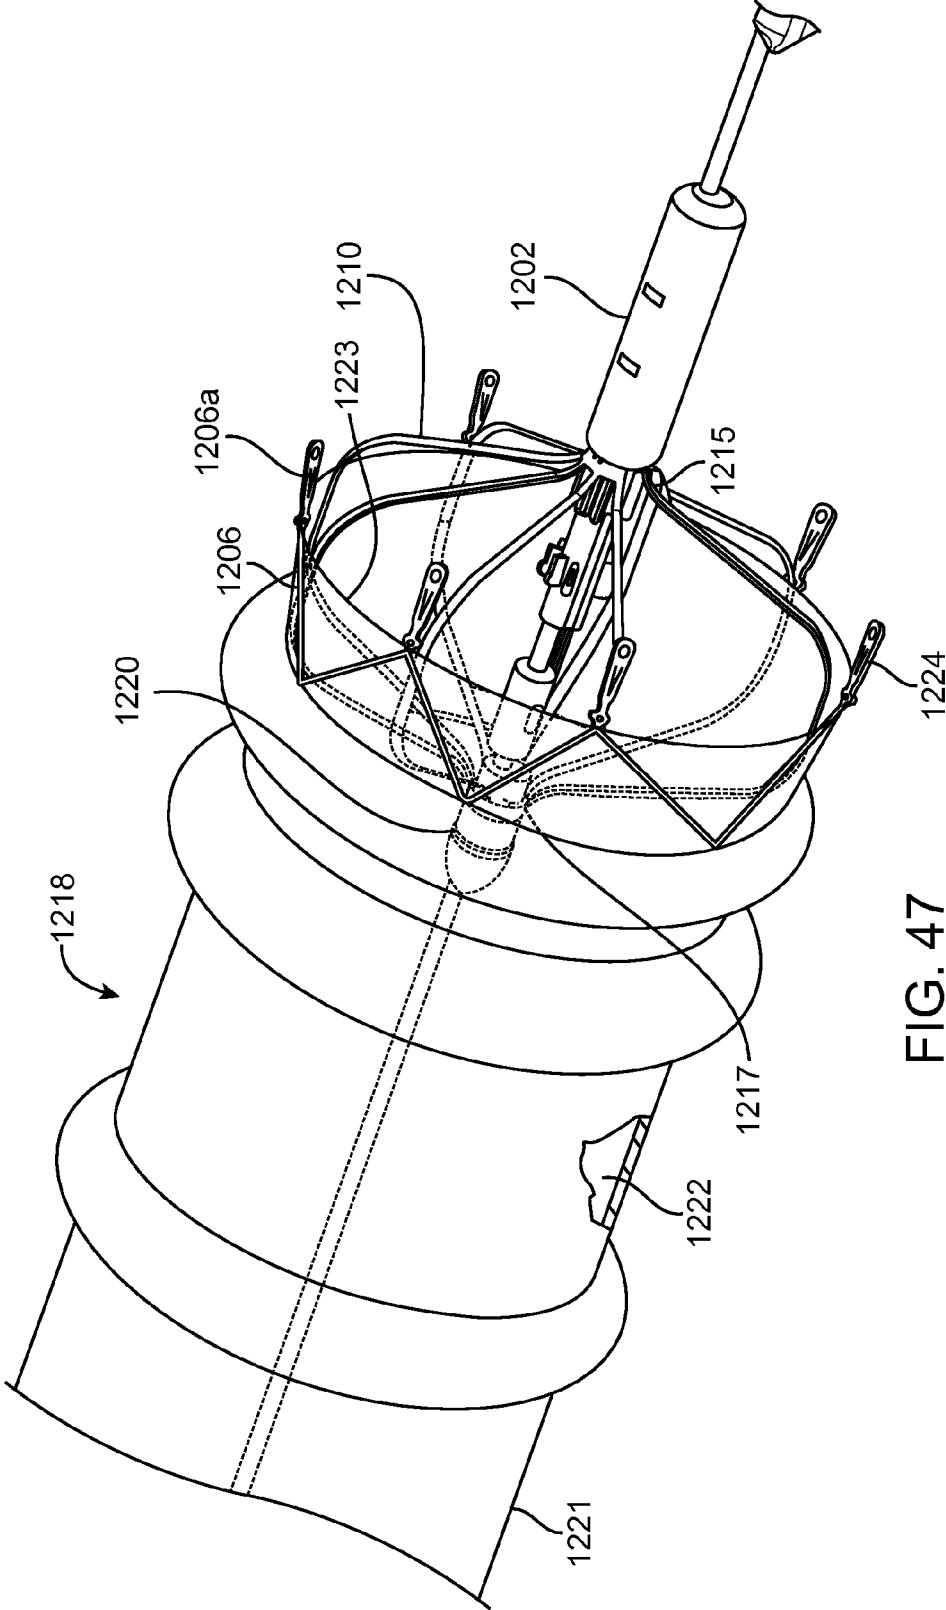


FIG. 47

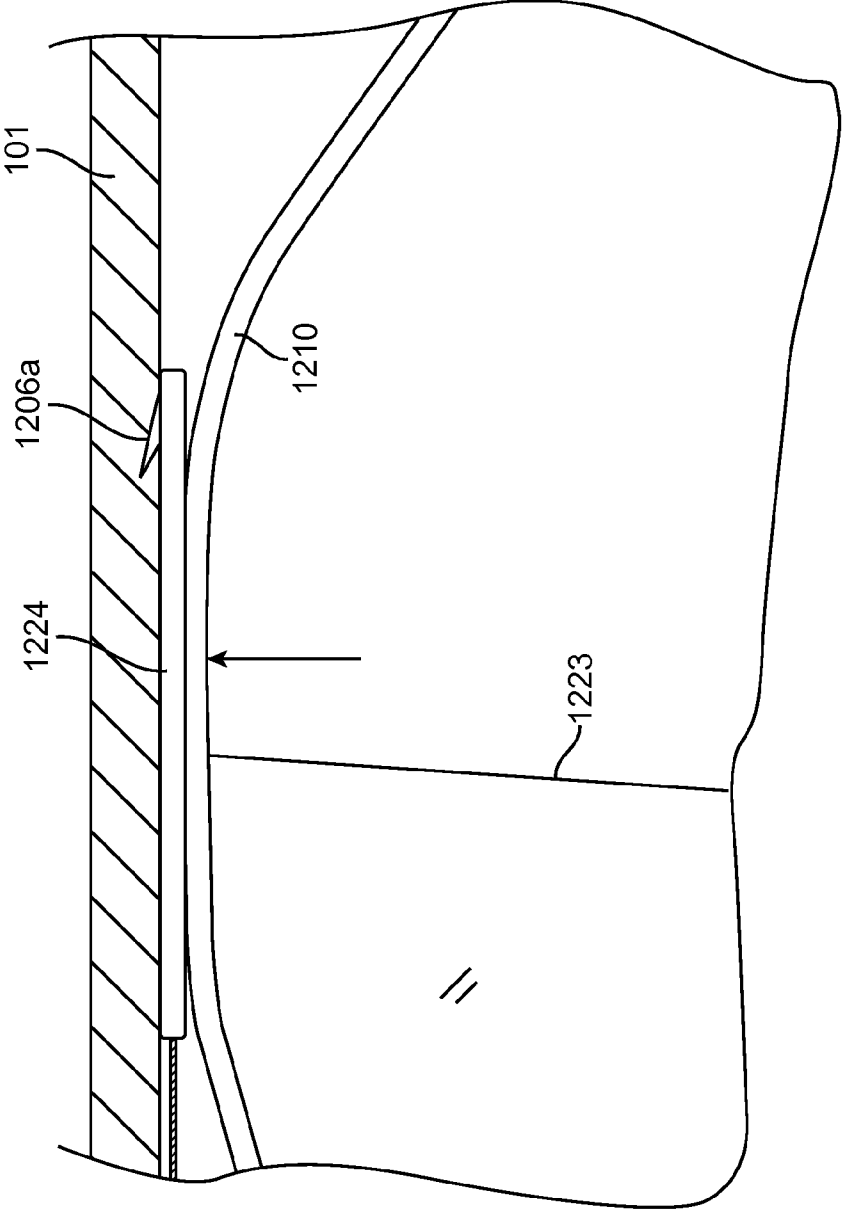


FIG. 48

ADVANCED ENDOVASCULAR GRAFT AND DELIVERY SYSTEM

RELATED APPLICATIONS

[0001] This application claims priority under 35 U.S.C. section 119(e) from U.S. Provisional Patent Application Ser. No. 61/414,375, filed Nov. 16, 2010, by J. Vinluan et al., titled "Advanced Endovascular Graft and Delivery System", which is incorporated by reference herein in its entirety.

FIELD OF THE INVENTION

[0002] Some embodiments relate in part to endovascular prostheses and methods of deploying same. Embodiments may be directed more specifically to stent grafts and methods of making and deploying same within the body of a patient.

BACKGROUND

[0003] An aneurysm is a medical condition indicated generally by an expansion and weakening of the wall of an artery of a patient. Aneurysms can develop at various sites within a patient's body. Thoracic aortic aneurysms (TAAs) or abdominal aortic aneurysms (AAAs) are manifested by an expansion and weakening of the aorta which may be a serious and life threatening condition for which intervention is generally indicated. Existing methods of treating aneurysms include invasive surgical procedures with graft replacement of the affected vessel or body lumen or reinforcement of the vessel with a graft.

[0004] Surgical procedures to treat aortic aneurysms can have relatively high morbidity and mortality rates due to the risk factors inherent to surgical repair of this disease as well as long hospital stays and painful recoveries. This is especially true for surgical repair of TAAs, which is generally regarded as involving higher risk and more difficulty when compared to surgical repair of AAAs. An example of a surgical procedure involving repair of an AAA is described in a book titled *Surgical Treatment of Aortic Aneurysms* by Denton A. Cooley, M.D., published in 1986 by W. B. Saunders Company.

[0005] Due to the inherent risks and complexities of surgical repair of aortic aneurysms, endovascular repair has become a widely-used alternative therapy, most notably in treating AAAs. Early work in this field is exemplified by Lawrence, Jr. et al. in "Percutaneous Endovascular Graft: Experimental Evaluation", *Radiology* (May 1987) and by Mirich et al. in "Percutaneously Placed Endovascular Grafts for Aortic Aneurysms: Feasibility Study," *Radiology* (March 1989).

[0006] When deploying devices by catheter or other suitable instrument, it may be advantageous to have a flexible and low profile stent graft and delivery system for passage through the various guiding catheters as well as the patient's sometimes tortuous anatomy. Many of the existing endovascular devices and methods for treatment of aneurysms, while representing significant advancement over previous devices and methods, use systems having relatively large transverse profiles, often up to 24 French. Also, such existing systems have greater than desired lateral stiffness, which can complicate the delivery process.

[0007] In addition, the sizing of stent grafts may be important to achieve a favorable clinical result. In order to properly size a stent graft, the treating facility typically must maintain a large and expensive inventory of stent grafts in order to

accommodate the varied sizes of patient vessels due to varied patient sizes and vessel morphologies. Alternatively, intervention may be delayed while awaiting custom size stent grafts to be manufactured and sent to the treating facility. As such, minimally invasive endovascular treatment of aneurysms is not available for many patients that would benefit from such a procedure and can be more difficult to carry out for those patients for whom the procedure is indicated.

[0008] In addition to low profile, other features may be desirable as well. For example, it is well known that the AAA and TAA patient population presents a wide variety of anatomy for treatment. One particular challenge is providing stent-graft treatment to patients with either tortuous anatomies and/or small landing zones for stent-graft that have barbed stents to engage the luminal surface of the aorta or other vascular.

[0009] What have been needed are stent graft systems and methods that are adaptable to a wide range of patient anatomies and that can be safely and reliably deployed using a flexible low profile system.

SUMMARY

[0010] Some embodiments include advanced stent graft systems comprising, either singularly or in combination, a number of features. In some embodiments, a stent graft may include a short or no proximal stent portions. In other embodiments, proximal stent portions may include one or a plurality of barb structures. Other embodiments include various radiopaque marker embodiments.

[0011] Some embodiments may include advanced delivery systems having a centering device, such as a basket or an inflatable structure. Other embodiments show various constraints for loading of stent grafts within catheters. Other embodiments show various constraints in combination with centering devices.

[0012] Some embodiments of a stent graft may include a graft body including a flexible tubular main body having an inner lumen configured to confine a flow of fluid therethrough and a graft collar disposed at a proximal end of the main body. The stent graft may also include a stent having a distal stent portion which is disposed distally of a proximal edge of the graft collar. The distal stent portion may be at least partially secured to the graft collar. The stent may also have a proximal stent portion which is disposed proximally of the graft collar, includes at least one barb extending radially outward therefrom and includes an axial length of about 1 mm to about 5 mm.

[0013] Some embodiments of a method of deploying a stent graft in a patient's vessel include providing a stent graft having a graft body including a flexible tubular main body with an inner lumen configured to confine a flow of fluid therethrough and a graft collar disposed at a proximal end of the main body. The stent graft may also include a stent having a distal stent portion which is disposed distally of a proximal edge of the graft collar and which is at least partially secured to the graft collar. The stent may also have a proximal stent portion which is disposed proximally of the graft collar, includes at least one barb extending radially outward therefrom and includes an axial length of about 1 mm to about 5 mm. Thereafter, the stent graft may be axially positioned at a desired site within the patient's vessel with the at least one barb disposed axially coextensive with a viable landing zone of the patient's vessel. The stent may then be deployed so as

to engage the tissue of the viable landing zone of an inner luminal wall of the patient's vessel.

[0014] Some embodiments of a delivery system for delivering a stent graft include a delivery catheter having an elongate shaft with a proximal section and a distal section. The system may also include a stent graft having a main graft body with an inner lumen configured for confining a flow of blood therethrough. The stent graft may be loaded on the proximal section of the delivery catheter with the elongate shaft disposed within the inner lumen. In addition, the delivery system may also include an expandable centering device disposed on the elongate shaft within the inner lumen of the stent graft. The centering device may be configured to expand from a radially contracted state to a radially expanded state for centering the elongate shaft and stent graft of the delivery system toward a midline or longitudinal axis of a patient's vessel when introduced into the patient's vessel. In some cases, the centering device includes an expanding basket, the basket having elongate tines that extend substantially parallel to the elongate shaft of the delivery catheter in the radially contracted configuration. The elongate tines may also be configured to bow radially outwardly from the elongate shaft in a substantially concentric arrangement in the radially expanded configuration. The centering device may also include an inflatable structure having a collapsed deflated state and an enlarged inflated state. In some cases, in the enlarged inflated state, the centering device may have a substantially cylindrical configuration including vias that extend from ports in a proximal surface of the centering device to respective ports in a distal surface of the centering device. The vias may be configured to provide for continuous flow of blood through the inflatable centering device and delivery system during inflation of the centering device and deployment of the stent graft.

[0015] Some embodiments of a method of centering a delivery system during deployment of a stent graft include providing a delivery system for delivering a stent graft. Such a delivery system may include a delivery catheter having an elongate shaft with a proximal section and a distal section. The delivery system may also include a stent graft having a main graft body with an inner lumen configured for confining a flow of blood therethrough and a stent secured to the main graft body, the stent graft being loaded on the proximal section of the delivery catheter with the elongate shaft disposed within the inner lumen. The delivery system may further include an expandable centering device disposed on the elongate shaft within the inner lumen. The centering device may be configured to expand from a radially contracted state to a radially expanded state for centering the elongate shaft and stent graft of the delivery system toward a midline longitudinal axis of a patient's vessel when introduced into the patient's vessel. Thereafter, the delivery catheter may be positioned within a patient's vessel such that the stent graft is axially positioned at a desired site within the patient's vessel. The expandable centering device may be in the radially contracted state during the positioning process in some cases. The expandable centering device may then be expanded to the radially expanded state to center the elongate shaft and stent graft of the delivery system toward the longitudinal axis of the patient's vessel. In addition, the stent of the stent graft may then be deployed so as to engage an inner luminal wall of the patient's vessel.

[0016] Some embodiments of a delivery system for delivering a stent graft include a delivery catheter having an elongate shaft with a proximal section and a distal section. The

delivery catheter may also include a releasable stent constraint system disposed on the proximal section elongate shaft. In some cases, the stent constraint system may include a crown constraint sleeve having a rigid tubular structure disposed about the elongate shaft with a plurality of crown restraint extensions extending distally from the crown constraint sleeve. The crown restraint extensions may generally be circumferentially spaced from each other. The catheter may also have a strut support assembly which is slidably disposed about the elongate shaft distally adjacent the crown constraint sleeve. The strut support assembly includes a plurality of strut supports which are circumferentially aligned with respective crown restraint extensions of the crown constraint sleeve and which extend radially away from a longitudinal axis of the elongate shaft. The constraint system has a docked state wherein the strut supports form closed but openable crown constraint passages between the strut supports and respective crown constraint extensions of the crown constraint sleeve. The constraint system also includes an open state wherein the strut support assembly is spaced axially away from the crown constraint sleeve and the crown restraint passages are opened to allow radial expansion of stent crowns disposed therein. The delivery system may also include a stent graft including a self-expanding stent secured to a proximal end of a main graft body. In some cases, the main graft body may have an inner lumen configured for confining a flow of blood therethrough. The stent graft is loaded on the proximal section of the delivery catheter with the elongate shaft disposed within the inner lumen and a plurality of proximal stent crowns disposed within closed crown restraint passages of the stent constraint system. So configured, the strut support assembly is in a docked state.

[0017] Some embodiments of a method of deploying a stent graft include providing a delivery system for delivering a stent graft. The delivery system may include a delivery catheter having an elongate shaft with a proximal section and a distal section and a releasable stent constraint system disposed on the proximal section elongate shaft. In some cases, the stent constraint system may include a crown constraint sleeve including a rigid tubular structure disposed about the elongate shaft with a plurality of crown restraint extensions extending distally from the crown constraint sleeve. Generally, the crown restraint extensions may be circumferentially spaced from each other. The stent constraint system may also include a strut support assembly which is disposed about the elongate shaft distally adjacent the crown constraint sleeve. The strut support assembly may include a plurality of strut supports which are circumferentially aligned with respective crown restraint extensions of the crown constraint sleeve and which extend radially away from a longitudinal axis of the elongate shaft. The constraint system is configured to have a docked state wherein the strut supports form closed but openable crown constraint passages between the strut supports and respective crown constraint extensions of the crown constraint sleeve. There is also an open state of the constraint system wherein the strut support assembly is spaced axially away from the crown constraint sleeve and the crown restraint passages are opened to allow radial expansion of stent crowns disposed therein. The delivery system further includes a stent graft having a self-expanding stent secured to a proximal end of a main graft body. The main graft body may have an inner lumen configured for confining a flow of blood therethrough. In some instances, the stent graft may be loaded on the proximal

mal section of the elongate shaft with the elongate shaft disposed within the inner lumen and a plurality of proximal stent crowns disposed within closed crown restraint passages of the stent constraint system with the strut support assembly in a docket state. Such a stent graft may be axially positioning at a desired site within the patient's vessel. Thereafter, the crown restraint sleeve may be axially separated from the strut support assembly so as to open the crown restraint passages allowing crowns of the stent contained within the crown restraint passages to radially expand. In some instances, the crown constraint sleeve may be secured to elongate shaft and the strut support assembly may be slidingly disposed about elongate shaft distally adjacent the crown constraint sleeve. In such a case, axially separating the crown restraint sleeve from the strut support assembly so as to open the crown restraint passages allowing crowns of the stent contained within the crown restraint passages to radially expand may include displacing the strut support assembly in an axial direction relative to the crown constraint sleeve and the elongate shaft. In some cases, the strut support assembly is secured to the elongate shaft and the crown constraint sleeve is slidingly disposed about elongate shaft proximally adjacent the crown constraint sleeve. In such an embodiment, axially separating the crown restraint sleeve from the strut support assembly so as to open the crown restraint passages allowing crowns of the stent contained within the crown restraint passages may include displacing the crown constraint sleeve in a proximal direction relative to the strut support assembly and the elongate shaft.

[0018] Some embodiments of a delivery system for delivering a stent graft include a delivery catheter having an elongate shaft with a proximal section and a distal section. The delivery catheter may also include a releasable stent constraint system disposed on the proximal section elongate shaft. The stent constraint system may include a stent constraint sleeve which has a rigid tubular structure slidably disposed about the elongate shaft between a distal position and a proximal position. The stent constraint sleeve may also include a plurality of crown sections that extend distally from the crown constraint sleeve and are circumferentially spaced from each other. The constraint system may further include a plurality of strut supports which are secured to the elongate shaft distally adjacent the stent constraint sleeve, which are circumferentially spaced from each other and which extend radially away from a longitudinal axis of the elongate shaft. Such a constraint system may have a constraint state wherein the stent constraint sleeve is disposed in the distal position and a deployment state wherein the stent constraint sleeve is in the proximal position. The delivery catheter may also include an expandable basket having a plurality of elongate tines which are disposed in a substantially tubular configuration, which extend axially along the elongate shaft of the delivery catheter in a position distally adjacent the stent constraint sleeve, and which are configured to bow radially outward upon reduction of a separation between proximal ends of the elongate tines and distal ends of the elongate tines. In addition, the delivery system may have a stent graft including a flexible main graft body and a self-expanding stent. The main graft body portion may include an inner lumen configured for confining a flow of blood therethrough, a proximal end and a distal end. The self-expanding stent may have a proximal end, a distal end secured to the proximal end of the main graft body, and a plurality of proximal stent crowns which include at least one barb. For such a configuration, the

stent graft may be loaded on the proximal section of the elongate shaft with the elongate shaft disposed within the inner lumen. The plurality of proximal stent crowns which include at least one barb may be disposed within and radially constrained by the stent constraint sleeve with the stent constraint sleeve in the distal position. In addition, at least one elongate tine of the expandable basket may be disposed beneath a stent crown that includes a barb, the at least one elongate tine being configured to apply outward radial force on the stent crown upon deployment of the stent and expansion of the expandable basket.

[0019] Some embodiments of a method of deploying a stent graft include providing a delivery system for delivering a stent graft. In some cases, such a delivery system may include a delivery catheter having an elongate shaft with a proximal section and a distal section. The delivery catheter may also include a releasable stent constraint system disposed on the proximal section elongate shaft. The stent constraint system may include a stent constraint sleeve which has a rigid tubular structure slidably disposed about the elongate shaft between a distal position and a proximal position. The stent constraint sleeve may also include a plurality of crown sections that extend distally from the crown constraint sleeve and are circumferentially spaced from each other. The constraint system may further include a plurality of strut supports which are secured to the elongate shaft distally adjacent the stent constraint sleeve, which are circumferentially spaced from each other and which extend radially away from a longitudinal axis of the elongate shaft. Such a constraint system may have a constraint state wherein the stent constraint sleeve is disposed in the distal position and a deployment state wherein the stent constraint sleeve is in the proximal position. The delivery catheter may also include an expandable basket having a plurality of elongate tines which are disposed in a substantially tubular configuration, which extend axially along the elongate shaft of the delivery catheter in a position distally adjacent the stent constraint sleeve, and which are configured to bow radially outward upon reduction of a separation between proximal ends of the elongate tines and distal ends of the elongate tines. In addition, the delivery system may have a stent graft including a flexible main graft body and a self-expanding stent. The main graft body portion may include an inner lumen configured for confining a flow of blood therethrough, a proximal end and a distal end. The self-expanding stent may have a proximal end, a distal end secured to the proximal end of the main graft body, and a plurality of proximal stent crowns which include at least one barb. For such a configuration, the stent graft may be loaded on the proximal section of the elongate shaft with the elongate shaft disposed within the inner lumen. The plurality of proximal stent crowns which include at least one barb may be disposed within and radially constrained by the stent constraint sleeve with the stent constraint sleeve in the distal position. In addition, at least one elongate tine of the expandable basket may be disposed beneath a stent crown that includes a barb, the at least one elongate tine being configured to apply outward radial force on the stent crown upon deployment of the stent and expansion of the expandable basket. For such a system the stent graft may be axially positioned at a desired site within the patient's vessel and the stent constraint sleeve axially displaced in a proximal direction from the distal position to the proximal position to release the crowns of the stent to radially expand. In addition, the expandable basket may be radially expanded such that at least one elongate tine of the

expandable basket which is disposed beneath a corresponding crown having a barb extends radially outward and applies an outward radial force to the corresponding crown so as to facilitate engagement of the barb with tissue of the patient's vessel at the desired site.

[0020] Certain embodiments are described further in the following description, examples, claims and drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

[0021] FIG. 1 is a perspective view of an embodiment of an inflatable stent graft.

[0022] FIG. 2 shows the stent graft of FIG. 1 as placed in a vessel lumen of a patient having a TAA condition in partial section.

[0023] FIG. 3 shows an enlarged view in partial section of a barb of a proximal stent of the stent graft of FIG. 1 penetrating and engaged with tissue of the patient's vessel.

[0024] FIG. 4 shows an embodiment of a stent portion of a stent graft.

[0025] FIG. 5 shows an enlarged view of a connection between a proximal stent portion and distal stent portion.

[0026] FIG. 6 shows an embodiment of a stent portion of a stent graft.

[0027] FIG. 7 shows an embodiment of a stent portion of a stent graft.

[0028] FIG. 8 shows an embodiment of a barb structure of a stent.

[0029] FIG. 9 shows an embodiment of a barb structure of a stent.

[0030] FIG. 10 shows an embodiment of a barb structure of a stent.

[0031] FIG. 11 shows an embodiment of a barb structure of a stent.

[0032] FIG. 12 shows an embodiment of stent structure formed onto a graft collar.

[0033] FIG. 12A is a transverse cross section view of the graft of FIG. 12 taken along lines 12A-12A of FIG. 12.

[0034] FIG. 13 shows an embodiment of stent structure formed onto a graft collar.

[0035] FIG. 14 shows an embodiment of stent structure formed onto a graft collar.

[0036] FIG. 15 shows an embodiment of a barb structure as positioned with respect to a graft collar or proximal edge thereof and an embodiment of a radiopaque marker.

[0037] FIG. 16 shows an embodiment of a barb structure as positioned with respect to a graft collar or proximal edge thereof and an embodiment of a radiopaque marker.

[0038] FIG. 17 shows an embodiment of a barb structure as positioned with respect to a graft collar or proximal edge thereof and an embodiment of a radiopaque marker.

[0039] FIG. 18 shows an embodiment of a barb structure as positioned with respect to a graft collar or proximal edge thereof and an embodiment of a radiopaque marker.

[0040] FIG. 19 shows an exemplary catheter delivery system embodiment.

[0041] FIG. 20 shows an enlarged view of the nosecone of the delivery catheter of FIG. 5.

[0042] FIG. 21 shows an enlarged view of a handle portion of the delivery catheter of FIG. 5.

[0043] FIG. 22 shows an embodiment of a delivery system including an expandable basket arrangement in a radially constrained state.

[0044] FIG. 23 shows the expandable basket arrangement of FIG. 22 in a radially expanded state with closer spacing between distal and proximal ends of the basket than in FIG. 22.

[0045] FIG. 24 depicts a delivery catheter being positioned inside a patient's aorta.

[0046] FIG. 25 shows a transverse cross section view of the delivery catheter within the patient's aorta of FIG. 24 taken along lines 25-25 of FIG. 24.

[0047] FIG. 26 shows the delivery catheter of FIG. 24 with a centering basket deployed.

[0048] FIG. 27 shows the delivery catheter of FIG. 24 with the centering basket deployed within an inner lumen of a graft body section of a stent graft with proximal and distal stents partially deployed.

[0049] FIG. 28 is a perspective view of an embodiment of a centering device including an inflatable structure.

[0050] FIG. 29 is a transverse cross section view of a dual lumen elongate tubular member that includes a lumen for a guidewire and an inflation lumen for the inflatable structure.

[0051] FIG. 30 is an end view of the inflatable structure of FIG. 28.

[0052] FIG. 31 shows a perspective view of a portion of an embodiment of a delivery catheter that includes a sleeve coupled to a multi-lumen shaft by a push rod.

[0053] FIG. 32 is an elevation view of a section of a delivery catheter that includes an expandable member having a basket configuration with the basket in a shortened and radially expanded state.

[0054] FIG. 33 shows an embodiment of a basket configuration of a delivery catheter with the basket and a stent of the stent graft loaded thereon in a radially constrained state.

[0055] FIG. 34 shows the delivery catheter and stent graft of FIG. 33 with the stent partially deployed and the basket in a radially expanded state.

[0056] FIG. 35 is a perspective view of a portion of an embodiment of a stent constraint system with the stent of a stent graft not shown for purposes of illustration.

[0057] FIG. 36 is a perspective view of the stent constraint system of FIG. 35 with the stent shown in a radially constrained state loaded onto the delivery catheter and held in place by the constraint system.

[0058] FIG. 37 is an elevation view of the constraint system of FIG. 36 with the stent deployed from the constraint system.

[0059] FIG. 38 is a perspective view of a portion of an embodiment of a stent constraint system with a stent in a partially deployed state and a graft body of the stent graft not shown for purposes of illustration.

[0060] FIG. 39 is a perspective view of the stent constraint system of FIG. 38 with the stent fully deployed.

[0061] FIG. 40 is a perspective view of a portion of an embodiment of a stent constraint system with a sleeve thereof in a proximal position.

[0062] FIG. 41 is a perspective view of the constraint system of FIG. 40 with the sleeve displaced distally relative to the position of a support and crown constraint assembly shown in FIG. 40.

[0063] FIG. 42 is an elevation view of the constraint system of FIG. 40 crown constraint assembly and support disposed in a proximal position configured to constrain a stent which is not shown for purposes of clarity of illustration.

[0064] FIG. 43 is an elevation view of the constraint system as shown in FIG. 42 but with the crown constraint assembly disposed distally of the proximal edge of the sleeve but still engaged with the support.

[0065] FIG. 44 shows the constraint system of FIG. 43 with the crown constraint assembly disposed distally of the sleeve and distally disengaged from the support so as to fully release a previously constrained stent.

[0066] FIG. 45 shows a perspective view of an embodiment of a stent constraint system including an expandable basket and stent in a radially constrained configuration.

[0067] FIG. 46 is a perspective view of the constraint system of FIG. 45 with a sleeve displaced proximally relative to the stent and basket so as to partially release the stent and allow the expandable basket to radially expand.

[0068] FIG. 47 is a perspective view of the constraint system of FIG. 46 wherein the stent graft previously constrained by the constraint system has been deployed and the tines of the expandable basket are applying an outward radial force against respective struts and barbs of the stent in order to more fully engage target tissue of a patient's vessel.

[0069] FIG. 48 is an enlarged elevation view in partial section of a tine disposed adjacent a strut and barb of a stent and applying an outward radial force against the barb towards tissue of the patient's vessel wall.

[0070] The drawings illustrate embodiments of the invention and are not limiting. For clarity and ease of illustration, the drawings are not made to scale and, in some instances, various aspects may be shown exaggerated or enlarged to facilitate an understanding of particular embodiments.

DETAILED DESCRIPTION

[0071] Embodiments may be directed generally to methods and devices for treatment of fluid flow vessels with the body of a patient. Treatment of blood vessels is specifically indicated for some embodiments, and, more specifically, treatment of aneurysms, such as thoracic aortic aneurysms and abdominal aortic aneurysms. Prosthetic devices used for the treatment of fluid flow vessels within a patient's body are typically subjected to a variety of forces such as pulsatile expansion and contraction of a patient's vessels as well as significant hemodynamic forces resulting from a high rate of flow of blood through the vessels. Often diseased vessels that require treatment are tortuous and narrow making percutaneous delivery of the prosthetic to the treatment site difficult. As such, it may be important for a prosthetic such as a stent graft to be configured to securely anchor to an inner luminal surface of the patient's vessel to prevent axial slippage or movement of the device after deployment. Such anchoring may be necessarily carried out in a short axial section of relatively healthy vessel tissue in order to properly secure the device. As such, some stent graft embodiments may require a configuration that may be securely anchored within such constraints. It may also be important for the stent graft to establish a good seal between an outside surface of the stent graft and the inner luminal surface of the patient's vessel in order to effectively isolate the vascular defect such as an aneurysm from the hemodynamic forces of blood flow. Proper placement of the prosthetic at deployment may also be a challenge and thus some delivery system embodiments used to deploy a prosthetic for treatment of a patient's aneurysm may be configured to accurately position the stent graft as well as allow for partial deployment and repositioning of the stent graft prior to full deployment.

[0072] FIG. 1 is a perspective view of an inflatable stent graft 100 made particularly for TAA. Such a stent graft 100 may have features which are similar to or the same as those of the Ovation™ Stent Graft System of TriVascular Inc. Stent graft 100 may include a proximal stent 102 having a substantially tubular overall configuration, a main graft body 104 also having a substantially tubular overall configuration, inflation channels 106 disposed on the flexible main graft body 104 and distal stent 108 having a substantially tubular configuration. Stents 102 and 108 may be made from any suitable material. For example, self-expanding stent embodiments 102 and 108 may be made from superelastic materials such as NiTi alloy or the like or any other suitable high strength material. Stent embodiments 102 and 108 that are configured to be balloon expandable may be made from other high strength materials such as stainless steel, MP35N, Elgiloy® or the like. Inflation sealing rings 110a and 110b may be included to provide a better sealing between an outside surface of the stent graft 100 and an inner luminal surface of the patient's vessel. Such an improved seal may be helpful in reducing or preventing the possibility of endoleaks that might occur around the fabric or layers of the main graft body 104 stent graft. The inflation sealing rings or expandable cuffs 110a and 110b may have an interior volume that is in fluid communication with an interior volume of the inflation channels 106.

[0073] The distal end of the proximal stent 102 is secured to a connection ring or sealing ring disposed within a proximal end of the main graft body 104. A proximal end of the distal stent 108 is secured to a connection ring or sealing ring disposed in a distal end of the main graft body 104. The stents 102 and 108 may be secured by any suitable method or device discussed or incorporated herein such as the "dogbone" type connection discussed below with regard to FIG. 5.

[0074] Main graft body 104 may be made from any suitable flexible biocompatible material for constructing such stent grafts. For example, body 104 might be made from a fabric such as Dacron®, from a polymer such as a fluoropolymer like polytetrafluorethylene (PTFE) or expanded PTFE (ePTFE) or any other suitable material. In some instances, it may be desirable for the material of the main graft body to be configured to be thin and flexible in order to pack tightly for a reduced profile during delivery and be configured to confine a flow of blood through a tubular structure made of the material. In cases, the type of material used for the main graft body and whether the main graft body includes inflation channels and inflation sealing rings may be of less importance. Some embodiments may, however, include a main graft body made of PTFE and have inflation channels and sealing rings. In some cases the main graft body 104 may have an axial length of about 50 mm to about 400 mm, more specifically, about 100 mm to about 300 mm. In some cases, an inner lumen 107 configured to confine a flow of blood or other bodily fluid therethrough of the main graft body 104 may have a transverse diameter or dimension of about 15 mm to about 39 mm, more specifically, about 30 mm to about 36 mm. The proximal and distal stents 102 and 108 may have dimensions commensurate with those of the main graft body 104. The stents 102 and 108 may have any suitable number of crowns or apices depending on the transverse expanded dimension or diameter and axial length of the stents 102 and 104. In some cases, the sinusoidal structure of the stents 102 and 104 may have about 3 to about 16 apices per side.

[0075] Embodiments having such construction which may be substituted into or included with any of the suitable embodiments discussed here are generally disclosed in commonly-owned U.S. Pat. Nos. 6,331,191, filed Nov. 25, 1998, by Chobotov, titled “Layered Endovascular Graft”; 6,395,019 filed Aug. 14, 1998, by Chobotov, titled “Endovascular Graft”; 6,602,280 filed Jan. 31, 2001, by Chobotov, titled “Delivery System and Method for Expandable Intracorporeal Device”; 6,733,521 filed Apr. 11, 2001, by Chobotov, et al., titled “Delivery System and Method for Endovascular Graft”; 6,761,733 filed Jul. 27, 2001, by Chobotov et al., titled “Delivery System and Method for Bifurcated Endovascular Graft”; 6,776,604 filed Dec. 20, 2001, by Chobotov et al., titled “Method and Apparatus for Shape Forming Endovascular Graft Material”; 7,066,951 filed Apr. 17, 2003, by Chobotov, titled “Delivery System and Method for Expandable Intracorporeal Device”; 7,081,129 filed Apr. 24, 2002, by Chobotov, titled “Endovascular Graft”; 7,147,660 filed Dec. 20, 2002, by Chobotov et al., titled “Advanced Endovascular Graft”; 7,147,661 filed Dec. 20, 2001, by Chobotov et al., titled “Radially Expandable Stent” and 7,150,758 filed Mar. 6, 2003, by Kari et al., titled “Kink Resistant Endovascular Graft”; and in United States Published Patent Application Numbers 2005/0027347, Aug. 13, 2003, by Chobotov et al., titled “Endovascular Graft Joint and Method for Manufacturing”; **2006/0222596** filed Apr. 1, 2005, by Askari et al., titled “Non-Degradable, Low Swelling, Water Soluble Radiopaque Hydrogel Polymer”; **2006/0233990** filed Apr. 13, 2005, by Humphrey et al., titled “PTFE Layers and Methods of Manufacturing”; **2006/0233991** filed Apr. 13, 2005, by Humphrey et al., titled “PTFE Layers and Methods of Manufacturing”; **2009/0082845** filed Sep. 26, 2007, by Chobotov, titled “Alignment Stent Apparatus and Method”; **2009/0082846** filed Sep. 26, 2007, by Chobotov, titled “Asymmetric Stent Apparatus and Method” and 2009/0099649 filed Oct. 3, 2008, by Chobotov et al., titled “Modular Vascular Graft for Low Profile Percutaneous Delivery”—all such patents and patent applications are fully incorporated by reference in their entirety herein. In addition, any suitable stent graft, delivery system or components thereof disclosed in these incorporated patent and patent applications may be substituted for embodiments of same discussed herein.

[0076] FIG. 2 shows an elevation view in partial section of the stent graft embodiment **100** of FIG. 1 as implanted and deployed in an aorta **101** of a patient having a TAA condition **202**. As shown, stent graft **100** is implanted in such a manner so as to establish a good hemostatic seal between an outside surface of the stent graft **100** at the inflation seals **110a** and the proximal stent deployed at a suitable landing zone so as not to occlude the left subclavian artery **204** with the fabric or other flexible layers of the stent graft **100**. In this case, the aneurysm **202** has been effectively isolated from the nominal blood flow through the vessel **101**. The nominal blood may flow pass through the inner lumen of the main graft body **104** and stents **102** and **108** after such deployment of the stent graft **100**. In some cases, proximal stent **102** may be deployed proximally of the left subclavian artery **204** of the patient and optional barbs shown in FIG. 3 may be used to better fixate the stent grafts **102** and **108** by engaging with the luminal surface of the aorta **101**. Stent graft **100** as well as others discussed herein may also be deployed such that the left subclavian artery **204** is covered by the fabric or layers of the main graft

portion **104**—up to the left common carotid artery with a trans-graft between the left subclavian and one of the adjoining arteries.

[0077] As mentioned above, patient anatomy may be widely varied—with some patients having extreme neck angulation and curvature of the aorta (as depicted in vessel element or section **206** and vessel element or section **208** of FIG. 2. Vessel section **206** may be described as being the lesser-curve side of the aorta and vessel section **208** may be described as the greater-curve section of the patient’s aorta **101**. Vessel section of the greater curve **208** may also have a short axial length section or “landing zone” for securing a proximal stent **102** of a stent graft **100**. In some cases, such extreme conditions of short landing zones may rule out a particular patient for treatment by any known endograft because the risk of certain failure modes may be too great. Such failure modes might include stent breakage (because of extreme hemodynamic conditions in the thoracic aorta); insufficient sealing or the like. It will be appreciated that such extreme conditions of neck angulation and curvature and short landing zones may also appear in AAA conditions and, therefore, the devices and techniques of the present disclosure may also be desirable in the treatment of AAA conditions—or anywhere in a patient’s body where such conditions may exist.

[0078] FIG. 3 is an elevation view in partial section of a proximal portion of a proximal stent **220** of a stent graft such as stent graft **100** discussed above. An optional barb **228** of the stent **220** is extending from a strut of the stent **220** at an angle pointing substantially in a distal direction along a direction of a flow of blood in the vessel **101** of the deployment. The barb **228** is also angled slightly radially outward towards the vessel wall **101** in order to penetrate and mechanically engage the tissue of the patient’s vessel **101**. Such a barb arrangement may be incorporated in to any suitable stent embodiment discussed herein. In addition, although FIG. 3 depicts the engagement of a proximal stent with a patient’s vessel **101**, a similar arrangement and deployment configuration may be used for distal stents, such as distal stent **108** and the like but with the directions of the stent and barb **228** reversed relative to the direction of blood flow as indicated by arrow **120**.

[0079] Several embodiments of stents that might serve as either proximal stents or distal (if any) stents on a stent graft are discussed herein. If a stent graft is destined to be placed into an area of challenging anatomy, short landing zones or in an area where the hemodynamics are challenging (e.g. high pressure and blood velocity, such as found near the heart in the thoracic aorta), then it may be desirable to have a stent that is not susceptible to failure (e.g. stent fractures) or to damaging the patient’s vasculature (in the case of movement of the stent in vivo due to blood flow).

[0080] FIG. 4 shows an embodiment of a stent **220** of a stent graft **221** which includes a proximal portion **222** of the stent **220** and a distal portion **224** of the stent **220**. Distal portion **224** in this case may be mechanically mated to a graft collar **236** of a graft body portion **225** of the stent graft **221** in any known manner or fashion—such as overlaying a layer of graft material and mating (as shown herein via sintering or the like), or by sewing the distal portion **224** onto the fabric material of the body portion of the stent graft. The material of the graft body portion **225** may be the same as discussed above with regard to stent graft **100**. The graft body portion **225** may have a generally tubular configuration that extends along a longitudinal axis **223** of the stent graft **221**. The stent

graft **221** may also share other suitable materials, dimensions and features of stent graft **100** such as inflatable channels **106** and inflation sealing rings or cuffs **110** etc.

[0081] Proximal portion **222** of the stent **220** may be mated to the distal portion **224** via connection **226** (e.g. a dogbone structure) or may be made integrally with the distal portion. Optional barbs **228** may be constructed on the proximal portion **222** of the stent **220**—the barbs **228** may be either welded or otherwise mechanically mated to the proximal portion **222**. In other embodiments, barbs **228** may be made integrally with the proximal portion **222** of the stent **220** and may also be located on a strut **229** of the proximal portion **222** (as shown), or may be made at the apices of the proximal portion **222**. The stents disclosed herein generally may be constructed out of any material suitable for this application—e.g. stainless steel, self-expanding metal such as superelastic alloys (NiTi or the like), etc.

[0082] Distal portion **224** of stent **220** may have a first axial length and proximal portion **222** of stent **220** may have a second axial length. As shown, the axial length of the proximal portion **222** is longer than the axial length of the distal portion **224**. This may be advantageous in some cases where a patient has a challenging landing zone in the vessel **101**—but in other cases, it may not be desirable from the standpoint of the stent's dynamic behavior in vivo. For example, in the case of a TAA, a stent graft **221** having a long proximal portion **222** might be subject to movement or hemodynamic forces that may cause injury to the patient's aorta due to movement of the proximal portion **222** against the patient's vasculature **101**. In some embodiments, an axial length of proximal portion **222** may be about 20 mm to about 30 mm and an axial length of the distal portion **224** may be about 10 mm to about 15 mm. The proximal portion **222** may be secured to the distal portion **224** of the stent graft **221** by any suitable device or method. In some cases the attachment **226** may be an integral attachment, in some cases there may be a linked or mechanical attachment such as the dogbone type attachment shown in more detail in FIG. 5.

[0083] FIG. 6 shows another embodiment of a stent **230** of a stent graft **231** that may have desirable characteristics for providing good clinical performance in difficult anatomical conditions such as the anatomical conditions noted above including a highly angulated vessel configuration or difficult landing zone. For example, stent **230**, which may be a self-expanding stent embodiment with a generally sinusoidal zig-zag configuration, may be configured to have an overall axial length that is less than an overall axial length of the stent **220** shown in FIG. 4. In addition, it may be possible to use either a short proximal portion or extension **234** extending proximally out from the graft collar **236** and distal portion **232**—or no proximal portion **234** at all. In such cases, the barbs **235** of the stent might be substantially located at the top of graft collar **236**. As shown in FIG. 6, it may be desirable for the number of proximal portions **234** to be some fractional proportion to the number of apices **233** of distal portion **232** (e.g. one half). In other embodiments, stent proximal portion or extension **234** may include different fractional proportions. In some embodiments, the short proximal portion or extension **234** may have an axial length on order of about 1 mm to about 14 mm, more specifically, about 1 mm to about 5 mm. The distal portion **232** may have an axial length on the order of about 10 mm to about 15 mm in some cases. In the case where the proximal portion **232** is about 1 mm or less in axial length, it may be considered that the proximal portion **234** may be

just a barb **235** that sits atop the apices **233** of the distal portion **232** and may be just even with a top or proximal end of the graft collar **236**.

[0084] In some embodiments of the stent graft **231**, the stent graft **231** may include a graft body **225** including a flexible tubular main body having an inner lumen configured to confine a flow of fluid therethrough as shown in FIG. 6. The graft collar **236** may be disposed at a proximal end of the main body. The stent graft **231** may also include the stent **230** having a distal stent portion **232** which is disposed distally of a proximal edge of the graft collar **236**. The distal stent portion **232** may be at least partially secured to the graft collar **236**. In some cases, the entire distal stent portion **232** may be secured to the graft body at a position such as the graft collar **236**. The distal stent portion **232** may be secured by any suitable means, including disposing the distal portion **232** between adjacent layers of material of the graft collar **236** or of the graft body **225** generally. The stent **230** may also include the proximal stent portion **234** which is disposed proximally of the graft collar **236** and may include at least one barb **235**. The barb **235** may be extending generally in a distal direction and also extend somewhat radially outward from the proximal stent portion **234** and may have an axial length of about 1 mm to about 5 mm. In some instances, the proximal stent portion **234** includes a plurality of barbs **235** disposed proximally of the proximal edge of the graft collar **236**. Self-expanding embodiments of the stent **230** and barbs **235** may include superelastic materials such as superelastic alloys including NiTi alloys and the like. In some cases, the stent graft **231** may have a stent **230** with a proximal portion **234** wherein no barbs are disposed more than about 5 mm from the proximal edge of the graft collar **236**.

[0085] In some cases, the distal stent portion **232** may include a continuous sinusoidal configuration and the at least one barb **235** is disposed on a strut or extension of the proximal stent portion **234** that extends proximally from an apex of the sinusoidal configuration of the distal stent portion **232** as shown in FIG. 6. In other cases, the distal stent portion **232** may include a distal portion of a continuous sinusoidal configuration and the at least one barb may be disposed on a strut of a proximal portion **234** of the sinusoidal configuration that extends proximally from the proximal edge of the graft collar **236** and forms the proximal stent portion of the stent as shown in FIG. 14. In some instances, the stent **230** may include a balloon expandable stent that is made of a high strength biocompatible material that is subject to elastic deformation during radial expansion from a radially constrained state suitable for percutaneous delivery to an expanded deployed state suitable for engaging an inner luminal wall of a patient's vessel. Such high strength materials for balloon expandable stent construction may include high strength alloys such as stainless steel. Such stent embodiments, such as stent **230** or any other suitable stent embodiment discussed herein may include at least one eyelet on a distal portion of the stent and the distal portion of such a stent may be secured to a graft collar **236** or any other suitable portion of a graft body portion of a stent graft with a flap of flexible material that may be disposed through the eyelet and secured to the graft collar. Such a flap of material (as shown in FIGS. 7 and 14) may be secured to the graft collar or graft body by adhesive bonding, welding, sintering or the like.

[0086] Some embodiments of a method of deploying such a stent graft in a patient's vessel **101** may include providing the stent graft **231** above. Thereafter, the stent graft **231** may

be axially positioned at a desired site within the patient's vessel **101** (as shown in FIG. 27 and discussed below) with the at least one barb **235** disposed axially coextensive with a viable landing zone of the patient's vessel **101**. The stent **230** may then be deployed so as to radially expand and physically engage the tissue of the viable landing zone of an inner luminal wall of the patient's vessel **101**. In some cases, deploying the stent **230** may include deploying the stent disposed at a proximal end of the stent graft **231** disposed towards a source of blood flow in the patient's vessel **101**, such as the patient's heart (not shown). In some instances wherein the stent **230** includes a self-expanding stent, deploying the stent **230** includes releasing a radial constraint from the stent **230** in a radially constrained state. In some embodiments wherein the stent **230** includes a balloon expandable stent, deploying the stent **230** includes expanding the stent **230** radially outward with an expandable member (not shown) disposed within an inner lumen of the stent **230**. In some such cases, the expandable member may include an inflatable balloon and deploying the stent may include expanding the stent radially outward by inflating the inflatable balloon with a source of pressurized fluid.

[0087] In some embodiments, it may be desirable to have a stent of a stent graft (such as stent graft **100**, stent graft **221**, stent graft **231** or any other suitable stent graft discussed herein) that includes barbs (such as barbs **228**, **235** or the like) that are disproportionately positioned and/or populated on one side of the stent. For example, in a highly angulated aorta **101**, the top side of a stent graft may tend to take the brunt of the hemodynamic forces and pressures (being on the greater curve **208** of the aorta as shown in FIG. 2) than the side of the stent graft that lies along the lesser curve **206** of the aorta **101**. In such a case, it may be desirable to configure a stent such that the top side portion of the stent includes more barbs (e.g. along every apices) and a lesser number or density of barbs along the low portion of the stent (e.g. to have barbs at every other apices).

[0088] In some cases, distal portion **232** of the stent **230** may be mated to the graft mechanically by encapsulating the metallic stent in between two or more layers of graft material and the graft layers mated or otherwise bonded together—e.g. between two layers of PTFE and sintered into place. The distal portion **232** could also be mated by sewing the distal portion to the graft materials of the graft body **225** or in any other known manner of mating or bonding layers.

[0089] FIG. 7 shows an embodiment of a stent graft **241** that may have similar features, dimensions and material with respect to stent graft **231**, where a distal portion **232** of a stent **240** is mated to the graft collar **236** by using flaps of material **241** (e.g. PTFE) that are placed through eyelet **242**. Fluorinated ethylene propylene (FEP) may be incorporated around eyelet **242** to improve the mating of the stent **240** to the graft collar **236**. One advantage of using flaps of materials may be to improve the tensile strength of the retention of the stent **240** to the graft. The use of flaps may also reduce the amount of graft collar needed to anchor the stent **240**. In some embodiments, the proximal portion **234** may have a length on order of about 5-15 mm and the distal portion **232** may have a length on order of about 5-15 mm.

[0090] FIGS. 8-11 show various embodiments of barbs that may be used for any suitable stent graft embodiment discussed in the present application. Barbs **260** may be placed at the apices of proximal portions (such as proximal portion **234** or distal portions **232**, if there is no proximal portion **234**) of

stents or at the end of a strut or extension **262**. The barb embodiments **260** and struts or extensions **262** may be disposed at either the proximal end or distal end of any suitable stent graft upon which they are used. Barbs **260** may be biased outward towards the tissue of an inner luminal surface of a patient's vessel **101** as shown in FIG. 3 to better engage the luminal surface of the patient's vessel **101**, such as the aorta. In some embodiments, the barbs **260** may have a length extending from the strut of about 1 mm to about 5 mm.

[0091] FIG. 8 shows a barb **260** that extends along a center line or longitudinal axis of strut **262** which has support legs extending to each side of the barb to a proximal most section or apex **264** from which the barb **260** extends. FIG. 9 illustrates a barb **260** that has a substantially hook shaped configuration wherein the barb is formed from an extension of the strut **262** which bends around in a u-turn and has a sharpened tip. In some cases, the strut **262** may be bent around in a u-turn at an angle of about 150 degrees to about 190 degrees. FIG. 10 illustrates a double-barb configuration wherein a strut **262** hooks around on two sides disposed opposite each other to form two barbs **260**. Each barb **260** is formed by a u-shaped type pattern or configuration similar to the barb configuration shown in FIG. 9 but on two opposed sides of the strut. The barbs may extend distally along the strut **262** over a length of about 1 mm to about 5 mm, in some embodiments. FIG. 11 shows a double barb configuration similar to that of FIG. 10 with a first barb **260** on one side of the strut and a second barb **260** on an opposite side of the strut **262**. However, in the embodiment of FIG. 11, a first barb **260** extends from a proximal apex of the strut and a second barb **260** extends from a position distal to the apex of the strut **262**. In the embodiment shown, the second barb **260** extends from a position on the strut **262** that is substantially axially coextensive with the sharpened tissue penetrating point or tip of the first barb **260**.

[0092] FIGS. 12 and 13 show embodiments of incorporation of the stent structure **230** within the graft material and configurations for securing the stent structure to the graft body. Dashed line **302** shown in FIGS. 12 and 13 represents a proximal boundary of a portion of the main graft where the inner lumen **107** defined by the main body of the stent graft is substantially cylindrical. Proximal of line or axial position represented by line **302** the inner lumen may begin to flare in a proximal direction to a larger inner luminal transverse dimension. In particular, graft collar **236** which is proximal of line **302**, may be constructed to flare outwardly from line **302** in a proximal direction. This flared configuration may be advantageous to help create a proper sealing of the aneurysm from the blood flow. This may be particularly the case when there is sufficient radial force provides by the stent to hold graft collar **236** against the luminal surface. FIG. 12 shown a stent graft embodiment having a configuration wherein a proximal sealing ring **304** (for example, sealing ring **304** could be an inflatable portion filled with a gel capable of hardening to provide a seal against blood flow) is distal of line **302**. FIG. 13 depicts a similar sealing ring **304** that is configured to be proximal of, or straddling, line **302**. It may be desirable in some cases to include a sealing ring **304** which is disposed proximal of line **302** because it may tend to allow for a shortening of the edge of graft collar **236**. This may be useful for the treatment of patient having a shortened landing zone or area for securing mechanical attachment or fixation members of a stent, such as barbs or the like.

[0093] FIG. 14 depicts a somewhat flattened rendition of an embodiment of a stent portion **311**. Although only a portion

311 of the stent is shown in the flattened illustration, the stent portion may be representative of a complete stent **300** having a typical configuration of the stents discussed herein generally with a substantially tubular or cylindrical shape with a stent element of high strength material extending about a longitudinal axis of the stent in a somewhat sinusoidal undulating pattern. For the embodiment shown in FIG. **14**, anchoring of the stent **300** to a graft body section may be provided at least in part by flap material **306** threaded through eyelet **242** in a manner similar to that shown in the embodiment of FIG. **7**. The flap material **306** may be selected to have a high tensile strength and bonding compatibility with the material of the graft body. In some cases, the flap **306** may include the same material as that of the main graft body. In some instances, such material may include Dacron®, PTFE or any other suitable material. Flap material **306** may be secured to the main graft body of the stent by adhesive bonding, such as with the use of FEP or the like, welding, sintering or any other suitable method. The flaps **306** may have a somewhat ribbon like configuration with a width that is substantially greater than the thickness of the flaps **306** in order to spread the tensile load imposed on the eyelet **242** over a greater area of the graft collar **236** or graft body generally. Barb **308** of stent **300**, as shown, may be integrally constructed with the strut **311** such that there is no joint between the strut **313** and the barb **308** and the material of the strut extends continuously into the barb **308**. Graft collar **236**, after trimming excess material, may be defined by lines **302** to **310** in FIG. **14**.

[**0094**] FIGS. **15-18** show various embodiments of radiopaque (RO) markers placed upon stent portions which may be used for any suitable stent embodiment discussed herein. As shown, the various RO markers may be placed as close to, straddling or proximal to, the top edge or proximal edge **402** of the graft collar **236** in order to better orient the device for the physician during implantation procedures. The RO markers **404** may be constructed of a wound or clipped elongate element or strand of NiTi, Pt, composite NiTi/Pt—Ir or NiTi/Au, Au or any other known biocompatible radiopaque materials. Markers **404** may be constructed in coil configuration made from coiled radiopaque wire or clip or any other known fashion. Markers **404** may be placed in an optional small transverse section of a dogbone structure **406** formed into the strut of a stent as shown in FIGS. **17** and **18** to maintain the position of the marker during manufacturing and loading into a delivery catheter. The dogbone structure includes a pair of opposed enlarged portions or shoulder portions of the strut of the stent with a reduced section therebetween. The elongate element may be wound or clipped to the reduced section so as to be mechanically captured between the shoulder portions of the dogbone **406**. Any of the stent, barb, radiopaque marker, graft body section, inflatable channel, inflatable sealing ring embodiments or the like discussed herein may be included together in any suitable desired combination in an appropriate structure or configuration. In particular, any of the RO marker embodiments of FIGS. **15-18** may be used on any of the stent embodiments discussed herein. Any of the stent connection methods such as the use of flaps **306** as shown in FIGS. **7** and **14** may be used to connect any of the stent embodiments discussed herein to any suitable stent graft body section.

[**0095**] Various embodiments of delivery systems are discussed herein that may be adapted for the deployment of the stent graft systems discussed herein. FIG. **19** shows a catheter delivery system **500** which includes a delivery catheter **501** having a nosecone **502** which is placed initially into the

patient percutaneously or by any other known vascular surgical technique. Nosecone **502** is at a proximal end of integral outer sheath **503** which may house any of the stent graft system embodiments discussed herein as well as any other suitable stent graft embodiment. Other parts of system **500** include a flush port **506** and handle **508** for the physician-operator to effect the deployment of the stent graft.

[**0096**] FIG. **22** shows an elevation view of a stent graft embodiment loaded onto delivery catheter system **500** with the graft portion of the stent graft not shown for clarity of illustration. Nosecone **502** is disposed at the proximal end of an elongate shaft **505** of the delivery catheter and is secured to a tubular member including a lumen (e.g. guide wire lumen **503**). The stent **230** is shown having distal portion **232** and proximal portion **234** (without the graft material shown) loaded on the catheter and placed in proximity over an optional basket **504** which is coaxially disposed within the stent **230**. Basket **504** may be constructed out of a self-expanding or super elastic metal e.g. NiTi (Nitinol) or the like. The basket **504** may include a plurality of struts or tines **504a**.

[**0097**] Tines **504a** may be shape set in any manner that is desirable to aid in the deployment of the stent graft. It will be appreciated that tines **504a** may have one or more “humps” (e.g. camel hump feature, not shown) or the tines may be constructed to have helical or otherwise twisted orientation to each other. In some embodiments, both the stent **230** and the basket **504** may be loaded and secured via belts **506** and **508** respectively. Belts **506** and **508** may be actuated or deployed by the physician-operator via control means on the handle **508**. The basket **504** and the stent **230** may also be constrained and loaded in any other suitable manner or fashion.

[**0098**] FIG. **23** depicts basket **504** after belt **508** has been released (or has otherwise been released from constraint). Basket **504**, as deployed, defines a substantially symmetric opened configuration having a larger outer transverse dimension or diameter than the basket **504** in a constrained state as shown in FIG. **22**. Not shown in FIG. **23** is that basket **504** is forcing the graft material of the stent graft in an opening biased position which is shown in FIG. **27**. At this point, the physician-operator may release the belt **506** (or any other known restraining means or devices for the stent); thus allowing the stent **230** (if self-expanding) to expand and have the barbs (if any) engage the luminal surface of the patient's vessel **101**.

[**0099**] Some embodiments of a delivery system for delivering a stent graft may include the delivery catheter **501** with an elongate shaft having a proximal section and a distal section. The system may also include a stent graft having a main graft body with an inner lumen configured for confining a flow of blood therethrough. The stent graft may be loaded on the proximal section of the delivery catheter **501** with the elongate shaft disposed within the inner lumen. In addition, the delivery system may also include the expandable centering device or basket **504** disposed on the elongate shaft within the inner lumen of the stent graft. The centering device **504** may be configured to expand from a radially contracted state as shown in FIG. **22** to a radially expanded state as shown in FIG. **23** for centering the elongate shaft and stent graft of the delivery system toward a midline or longitudinal axis **702** of a patient's vessel **101** when introduced into the patient's vessel **101**. In some cases, the centering device may include and expanding basket such as expanding basket **504**.

[**0100**] In some cases, the basket may include the elongate tines **504a** that extend substantially parallel to the elongate

shaft of the delivery catheter in the radially contracted configuration as shown in FIG. 22. The elongate tines 504a may also be configured to bow radially outwardly from the elongate shaft in a substantially concentric arrangement in the radially expanded configuration as shown in FIG. 23. In some cases, the elongate tines are configured to self-expand to the radially expanded configuration and in some cases the elongate tines are configured to expand to the radially expanded configuration due to axial compressive force applied to at least one end of the tines. For the self-expanding embodiments, the elongate tines may include a self-expanding or superelastic metal such as a NiTi alloy. Some embodiments of the centering device may have an outer transverse dimension of about 50 mm to about 80 mm in the radially expanded state and may be configured to expand to an outer transverse dimension that is at least as large as an inner transverse dimension of the inner lumen of the patient's vessel 101.

[0101] FIGS. 24-26 show a dynamic operation and deployment of basket 504 during a deployment sequence of the stent graft. In some instances, the delivery catheter 501 may be positioned within a patient's vessel 101 such that the stent graft is axially positioned at a desired site within the patient's vessel 101 as shown in FIG. 27. The expandable centering device may be in the radially contracted state during the positioning process in some cases. The expandable centering device may then be expanded to the radially expanded state to center the elongate shaft and stent graft of the delivery system toward the longitudinal axis 702 of the patient's vessel 101. In addition, the stent 230 of the stent graft may then be deployed so as to engage an inner luminal wall of the patient's vessel. FIG. 24 shows the catheter 501 inserted into a vessel 101 of a patient having a TAA condition 202. As shown, the delivery catheter 501 would tend to lie along the greater-curve 208 of the aorta because of the mechanical stiffness of the catheter. It will be appreciated, however, that due to variations in patient anatomy and geometry that the delivery catheter 501 might also tend to lie along the lesser-curve, instead of the greater-curve. In some cases however, it may be desirable to have the catheter move and lie more along the midline or longitudinal axis 702 of the aorta prior to device deployment of the stent graft from the delivery catheter 501.

[0102] Nosecone 502 is shown also along greater-curve 208. Midline 702 shows the middle of the thoracic region of the aorta 101 itself. If the stent graft were to be deployed with the catheter as shown in FIG. 24, there is a possibility that the stent and the graft portions of the stent graft may not deploy in a desirable manner. For example, the stent portion might miss the desired landing zone and there may be some undesirable positioning of graft material due to an asymmetric deployment which might compromise the integrity of the later-filled sealing rings in producing an sufficient seal and exclusion of the aneurysm 202 from blood flow.

[0103] FIG. 26 shows how an expandable basket 504 may alleviate some of these undesirable conditions. Basket 504, as deployed, may help to center the stent graft along midline 702 prior to deployment of the stent portion and subsequent filling of inflation rings in the graft material. In some instances, deploying the stent may include deploying a stent disposed at a proximal end of the stent graft disposed towards a source of blood flow in the patient's vessel 101. In some embodiments wherein the expandable centering device includes a basket 504, expanding the expandable centering device may include allowing self-expanding elongate tines 504a of the basket 504 to self-expand to the radially expanded state. In some

embodiments expanding the expandable centering device includes axially compressing at least one end of elongate tines 504a of the basket 504 to shorten a separation of the proximal ends and distal ends of the elongate tines 504a of the basket 504 and expand a center portion of the tines 504a to the radially expanded state. In some cases, expanding the expandable centering device to the radially expanded state to center the elongate shaft and stent graft of the delivery system toward the longitudinal axis of the patient's vessel 101 may include expanding the expandable centering device, such as basket 504, or balloon 710 discussed below, to an outer transverse dimension which is about the same as a transverse dimension of an inner lumen of the patient's vessel 101 at a position of the expandable centering device.

[0104] Some centering device embodiments may also include an inflatable structure such as the inflatable structure 710 shown in FIG. 28. The inflatable structure 710 may have a collapsed deflated state (not shown) and an enlarged inflated state as shown in FIG. 28. In some cases, in the enlarged inflated state, the centering device 710 may have a substantially cylindrical configuration including vias that extend from ports 714 in a proximal surface of the centering device 710 to respective ports in a distal surface of the centering device. The vias 714 may be configured to provide for continuous flow of blood through the inflatable centering device and delivery system during inflation of the centering device and deployment of the stent graft. In some cases, the expandable vias have a cumulative cross section that is at least about 5 percent to about 10 percent of the total cross section of the centering device in an expanded state. In some instances, the expandable centering device may include a configuration that is radially concentric with the elongate shaft in the enlarged inflated state.

[0105] FIG. 28 shows an embodiment of an inflatable balloon 710 which may be used in place of or in addition to basket 504 and which serves to aid the catheter to tend toward midline 702 of the patient's vessel 101 prior to deployment. Balloon 710 includes a plurality of films or layers of flexible material that may be hermetically sealed together or otherwise joined to form a fluid tight interior volume that once inflated may assume an annular or circular shape. The balloon 710 may also include a structure or structures that allow blood to flow therethrough. For some embodiments, via holes or vias 714 may pass from a proximal end of the balloon 710 to a distal end of the balloon 710 at a radial position disposed inwardly of the outer radial surface of the balloon 710. The vias 714 may extend from a port on a proximal surface of the balloon 710 to a respective port on a distal surface of the balloon 710. Balloon 710 may be mated to an elongated tubular member 712 by any suitable method or means, in particular, via adhesives or the like. The elongated tubular member 712 may have an inner lumen 713 that may be used to accommodate a guidewire or the like as shown in FIG. 29.

[0106] Ports (not shown on elongated tubular member 712) in fluid communication with an interior volume of the balloon 710 and with an inflation lumen 715 may be used to inflate balloon 710 with air, gas or liquid or the like. The inflation of balloon 710 may be carried out by injection of an inflation fluid from a source of pressurized fluid 716, through supply lumen 717, through inflation lumen 715 and into the interior volume of the balloon 710. FIG. 30 is an end view of balloon 710 once inflated illustrating the vias. There may be other devices to effect the centering of the delivery catheter 501 prior to deployment and embodiments of the present inven-

tion encompass all such known means and devices. It may be merely desirable that the delivery catheter **501** be induced to lie more along the midline or longitudinal axis **702** of the aorta prior to device deployment. In some cases, expanding the expandable centering device may include inflating an interior volume of the inflatable structure with a biocompatible fluid to expand the inflatable structure to the radially expanded state. For some embodiments, the interior volume of the inflatable structure may be inflated through an inflation lumen with a fluid from a source of pressurized fluid. The source of pressurized fluid may include a syringe for some embodiments and inflating the interior volume of the inflatable structure may include injecting fluid from an interior volume of the syringe through the inflation lumen and into the interior volume of the inflatable structure. Any suitable inflation fluid may be used for inflating the interior volume of the inflatable structure including biocompatible fluids such as saline solution.

[0107] FIGS. **31** and **32** illustrate an embodiment of a deployment structure **800** for the stent **230** or any other suitable stent of a stent graft discussed herein which may be incorporated into a delivery system having a delivery catheter such as delivery catheter **501**. The main graft body of the stent graft loaded onto the delivery catheter is not shown in FIG. **32** for purposes of clarity of illustration. The delivery catheter **501** shown in FIG. **32** may include many of the same features, dimensions and materials as those of the delivery catheter embodiments **501** discussed herein. As shown in FIGS. **31** and **32**, sleeve **802** is slidably disposed over the elongate shaft of the delivery catheter **501** and may be configured to surround and constrain barbs **235** once the stent **230** is loaded into delivery catheter **501** and the sleeve is disposed in a distal position covering the barbs **235** of the stent **230**. The physician-operator may deploy basket **504** as described herein by shortening the separation of the proximal ends **509** of the tines of the expandable basket relative to the distal ends **511** of the tines of the elongate basket **504**. Thereafter, an axial force may be applied to push rod **804** which may be slidably disposed within or adjacent an elongate multi-lumen structure or shaft **806**. Once sleeve **802** is pushed proximally beyond mechanical mating with or radial constraint of barbs **235**, the stent portion would deploy in an outward radial direction.

[0108] FIGS. **33** and **34** show yet another embodiment of the delivery system **500** which is configured to deploy stent graft embodiments discussed herein. FIGS. **33** and **34** do not show the main graft body of the stent graft for purposes of clarity of illustration. FIG. **33** shows the stent graft as loaded onto the delivery catheter **501** in a radially constrained state suitable for percutaneous delivery through the vessels **101** of a patient's body. In this embodiment, there are shown multiple belt/constraints for both stent **902** and basket **504**—with belts **506a** and **506b** being disposed about and radially constraining self-expanding stent **902** and belts **508a** and **508b** disposed about and radially constraining basket **504**. FIG. **34** shows the belts **508a** and **508b** released from constraint of the basket **504** which is shown in a radially expanded state with a shorter axial separation between proximal and distal ends **509** and **511** relative to the axial separation shown in FIG. **33**. The belts **508a** and **508b** may be held or locked into a constraining configuration by a trigger wire (not shown) and deployed by retraction of the trigger wire as shown in FIG. **36** and discussed below. In some cases, a physician-operator may deploy basket **504** in stages via belts **508a** and **508b** for a more accurate and controlled deployment.

[0109] In some cases, an operator may also wish to deploy stent **902** in stages for a more accurate placement or better control of the stent deployment. In particular, FIG. **34** shows the partial deployment of stent **902** wherein a first belt **508a** and a second or final constraint or belt **508b** has been released from a constraining configuration with the retraction of a trigger wire or any other suitable means. However, a stent crown constraint **915** which may have features and/or mode of operation similar to those of constraint **1000** shown in FIG. **35** and discussed below, has yet to be actuated or released—which may allow for repositioning of the stent graft by the physician under fluoroscopy. Thereafter, an operator may deploy constraint **915** to completely deploy stent **902**. The belts **508a**, **508b**, **506a** and **506b** may also be deployed or released in any desired order or sequence in order to achieve a desired partially deployed state of either the basket **504** or the stent **902**.

[0110] FIGS. **35-37** depict an embodiment of loading a stent of a stent graft onto a delivery catheter of a delivery system. Constraint system **1000** comprises a crown constraint sleeve **1002** and strut support assembly **1004**. In FIG. **35**, both crown constraint **1002** and stent support assembly **1004** are shown as they would be configured in a docket position, constraining a stent (without the stent shown for purposes of illustration). FIG. **36** shows the same configuration but with stent **1006** loaded and constrained by constraint system **1000**. FIG. **37** shows the configuration of constraint system **1000** upon removing the constraint imposed by the constraint system **1000** on the stent **1006** and deploying the stent in a vessel lumen **101** of the patient. It may be seen that strut support assembly **1004** has moved distally with respect to crown constraint sleeve **1002** via a pull wire **1003**, push rod, spring action or any other known manner of effecting slidable coupling. After deployment, it is desirable that crown constraint **1002** and strut support assembly **1004** reconnect, so as to not capture or engage with the tissue of a patient's vessel **101**. Belts are also shown released and extending radially from delivery catheter.

[0111] Some embodiments of a delivery system for delivering a stent graft include the delivery catheter **501** having an elongate shaft with a proximal section and a distal section. The delivery catheter **501** may also include the releasable stent constraint system **1000** disposed on the proximal section elongate shaft. In some cases, the stent constraint system **1000** may include the crown constraint sleeve **1002** having a rigid tubular structure disposed about the elongate shaft with a plurality of crown restraint extensions extending distally from the crown constraint sleeve **1002**. The crown restraint extensions may generally be circumferentially spaced from each other. The catheter **501** may also include the strut support assembly **1004** which is slidably disposed about the elongate shaft distally adjacent the crown constraint sleeve **1002**. The strut support assembly **1004** may include a plurality of the strut supports which are circumferentially aligned with respective crown restraint extensions of the crown constraint sleeve **1002** and which extend radially away from a longitudinal axis **1005** of the elongate shaft **1007**.

[0112] The constraint system has a docked state wherein the strut supports form closed but openable crown constraint passages **1009** between the strut supports and respective crown constraint extensions of the crown constraint sleeve **1002**. The constraint system also includes an open state wherein the strut support assembly **1004** is spaced axially away from the crown constraint sleeve **1002** and the crown

restraint passages are opened to allow radial expansion of stent crowns disposed therein. The delivery system may also include a stent graft including a self-expanding stent **230** secured to a proximal end of a main graft body. In some cases, the main graft body may have an inner lumen configured for confining a flow of blood therethrough. The stent graft is loaded on the proximal section of the delivery catheter **501** with the elongate shaft **1007** disposed within the inner lumen and a plurality of proximal stent crowns disposed within closed crown restraint passages **1009** of the stent constraint system **1000**. So configured, the strut support assembly **1004** is in a docket state.

[0113] In some cases, the crown constraint sleeve **1002** may be secured to the elongate shaft **1007** and the strut support assembly **1004** may be slidably disposed about the elongate shaft **1007** distally adjacent the crown constraint sleeve **1002**. In addition, such a strut support assembly **1004** may be resiliently biased towards the crown constraint sleeve **1002** in an axial direction. In some instances, the strut support assembly **1004** may be resiliently biased towards the crown constraint sleeve **1002** in an axial direction by an axially oriented spring **1011** disposed between the strut support assembly **1004** and the elongate shaft **1007**. For some other embodiments, the strut support assembly **1004** may be secured to the elongate shaft **1007** and the crown constraint sleeve **1002** may be slidably disposed about the elongate shaft **1007** proximally adjacent the crown constraint sleeve **1002**. In some cases, the delivery system may also include at least one releasable belt **1013** disposed about the stent **1006** of the stent graft. The at least one releasable belt **1013** may be locked in a constrained configuration about the stent **1006** with a removable trigger wire **1015** that may be axially retracted in order to release the constrained belts which are mechanically captured in a constraining configuration by the trigger wire **1015**.

[0114] In use, a stent graft loaded on a delivery catheter having such a constraint system **1000** may be axially positioning at a desired site within the patient's vessel **101** as shown in FIG. 27. Thereafter, the crown restraint sleeve **1002** may be axially separated from the strut support assembly **1004** so as to open the crown restraint passages **1009** allowing crowns of the stent **1006** contained within the crown restraint passages **1009** to radially expand. In some instances, the crown constraint sleeve **1002** may be secured to elongate shaft **1007** and the strut support member **1004** may be slidably disposed about elongate shaft **1007** distally adjacent the crown constraint sleeve **1002**. In such a case, axially separating the crown restraint sleeve **1002** from the strut support assembly **1004** so as to open the crown restraint passages **1009** allowing crowns of the stent **1006** contained within the crown restraint passages **1009** to radially expand may include displacing the strut support member **1004** in an axial direction relative to the crown constraint sleeve **1002** and the elongate shaft **1007**. In some cases, the strut support assembly **1004** may be secured to the elongate shaft **1007** and the crown constraint sleeve **1002** is slidably disposed about elongate shaft **1007** proximally adjacent the crown constraint sleeve **1002**. In such an embodiment, axially separating the crown restraint sleeve **1002** from the strut support assembly **1004** so as to open the crown restraint passages **1009** allowing crowns of the stent **1006** contained within the crown restraint passages **1009** may include displacing the crown constraint sleeve **1002** in a proximal direction relative to the strut support assembly **1004** and the elongate shaft **1007**.

[0115] In some cases, the crown constraint sleeve **1002** may be secured to the elongate shaft **1007** and the strut support member **1004** may be slidably disposed about elongate shaft **1007** distally adjacent the crown constraint sleeve **1002**. In such a case, axially separating the crown restraint sleeve **1002** from the strut support assembly **1004** so as to open the crown restraint passages **1009** allowing crowns of the stent **1006** contained within the crown restraint passages **1009** to radially expand may include displacing the strut support member **1004** in an axial direction relative to the crown constraint sleeve **1002** and the elongate shaft **1007**. For such embodiments, the strut support assembly **1004** may be resiliently biased towards the crown constraint sleeve **1002** in an axial direction and displacing the strut support assembly **1004** in an axial direction relative to the crown constraint sleeve **1002** and the elongate shaft **1007** may include retracting the strut support assembly **1004** by applying axial displacement in a distal direction on a pull rod or pull wire **1003** that is secured to the strut support assembly **1004** and extends distally to a distal end of the elongate shaft **1007**.

[0116] In some cases (not shown), the strut support assembly **1004** may be secured to the elongate shaft **1007** and the crown constraint sleeve **1002** may be slidably disposed about elongate shaft **1007** proximally adjacent the crown constraint sleeve **1002**. For such an embodiment, axially separating the crown restraint sleeve **1002** from the strut support assembly **1004** so as to open the crown restraint passages **1009** allowing crowns of the stent **1006** contained within the crown restraint passages **1009** may include displacing the crown constraint sleeve **1002** in a proximal direction relative to the strut support assembly **1004** and the elongate shaft **1007**. In such a case, the crown constraint sleeve **1002** may be resiliently biased towards the strut support assembly **1004** in an axial direction and displacing the crown constraint sleeve **1002** in an axial direction relative to the strut support member **1004** and the elongate shaft **1007** may include displacing the crown constraint sleeve **1002** by applying axial displacement in a proximal direction on a push rod (not shown) that is secured to the crown constraint sleeve **1002** and extends distally to a distal end of the elongate shaft **1007**.

[0117] FIG. 38 illustrates an embodiment of loading the constraint system **1000** shown in FIGS. 35-37 which may be incorporated into any suitable delivery system discussed herein. In this embodiment, strut support **1004** is held rigidly with respect to the delivery catheter **501** and crown constraint sleeve **1002** is slidably attached to the delivery catheter **501** and, upon removing of the constraint of the stent, crown constraint sleeve **1002** is moved proximally with respect to the catheter. Additionally, stent **1006** is shown flared out in the distal portion due to release of a first belt constraint **1007**. The slidable movement of crown constraint sleeve **1002** may be accomplished after physician-operator has an opportunity to reposition the delivery catheter **501** within the vessel **101** of the patient with the aid of visualization such as by fluoroscopy.

[0118] FIG. 39 shows an embodiment of a constraint system **1100** for loading any suitable stent discussed herein and which may be incorporated into any suitable delivery system discussed herein. FIG. 39 shows a constraint configuration after release and deployment of the stent. Crown constraint assembly **1002b** has been moved slidably in a distal direction as shown by arrow **1125** relative to support structure **1004b**. Return spring **1008** is used to dock crown constraint assembly **1002b** to support **1004b** to radially constrain the proximal

stent crowns of the stent graft. The crown constraint assembly may be axially displaced as shown by a pull wire **1003** as shown in FIG. **35** and discussed above. The crown constraint assembly **1002b** includes proximally extending crown elements which are circumferentially spaced from each other and configured to form openable constraint apertures similar to apertures **1009** shown in FIG. **35** when the assembly **1002b** is axially engaged with support structure **1004b**.

[0119] FIGS. **40-44** show an embodiment of a constraint system for loading a stent of a stent graft, including any suitable stent or stent graft embodiments discussed herein. The constraint system may also be incorporated into any suitable delivery system discussed herein. Nosecone **1102** is the proximal most portion of the delivery catheter and is mated to sleeve **1104**. Sleeve **1104** provides the constraint for the stent and the barbs, together with support **1106** and crown constraint assembly **1108**. Spring **1110** provides a mechanism for the mating/de-mating of crown constraint assembly **1108** and support **1106**. FIG. **40** shows the configuration of the constraint system immediately after the stent has been fully deployed into the patient.

[0120] FIG. **41** shows the constraint in a configuration such as would be the case with the stent loaded (stent not shown) and prior to release of any constraint. It should be noted that support **1106** has cantilevered portions **1106a** that may be spring loaded so that when support **1106** is inside sleeve **1104** the cantilevered portions are compressed to a smaller dimension and when support **1106** is moved distally from sleeve **1104** (as shown in FIG. **35**), then the cantilevered portions expand as shown by the dashed lines of **1106a** in FIG. **35**; thus not allowing the support **1106** to return inside sleeve **1104**.

[0121] FIGS. **42** through **44** show a sequence of figures whereby the stent is released from a constrained configuration. FIG. **42** shows the configuration where the stent is fully loaded prior to deployment. FIG. **43** shows the configuration where the support **1106** and crown **1108** have been moved relative with respect to sleeve **1104**. In this configuration, stent (not shown) has its distal portion flared outward; but the apices of the stent and barbs are still constrained by crown **1108** and support **1106** which are axially pushed together to confine the proximal crowns of the stent. FIG. **44** shows the configuration immediately after full deployment of the stent wherein the crown **1108** has been moved distally relative with respect to support **1106** to open a gap between the support **1106** and the crown constraint assembly **1108** to allow the stent to self-expand.

[0122] FIGS. **45-47** show an embodiment of a constraint system **1200** for use on a delivery catheter of a delivery system wherein a stent may be partially deployed and have barbs which are disposed on the stent mechanically pushed radially outward to aid the engagement of the barbs with the patient's vessel. FIG. **45** shows sleeve **1202** locked in a first position with lock **1208** (which in this case is constructed on one of the tines of an expandable basket **1207**). Lock **1208** is shown poking through a first hole **1209** in sleeve **1202** and will be allowed to move to a second hole **1210** disposed on a different axial position of sleeve **1202**. Stent **1206** and barbs **1206a** are shown to be fully constrained by a crown section **1203** of sleeve **1202** disposed adjacent to support **1204**.

[0123] FIG. **46** depicts a configuration when lock **1208** has been axially displaced to the second hole position **1210**. In this configuration, stent **1206** has its distal portion in a flared

position while the barbs **1206a** are still constrained by crowns of crown section **1203**. Tines **1210** of the basket **1207** are shown as deployed.

[0124] FIG. **47** shows a configuration with barbs **1206a** released from all constraint and tines **1210** of the basket **1207** as deployed. It may be desirable to have first housing section **1220** to be slidably connected to sleeve **1202** so that moving sleeve **1202** towards housing section **1220** may further expand tines **1210** of the basket. By doing so, tines **1210** may push against stent struts or the graft material (not shown) with greater radial force. This may allow some of all of barbs **1206a** to better engage the luminal surface of the patient's vessel **101**.

[0125] Some embodiments of a delivery system for delivering a stent graft may include a delivery catheter **501** having an elongate shaft **1212** with a proximal section and a distal section. The delivery catheter **501** may also include the releasable stent constraint system **1200** disposed on the proximal section of elongate shaft **1212** as shown in FIG. **45**. The stent constraint system **1200** may include the stent constraint sleeve **1202** which may have a rigid tubular structure slidably disposed about the elongate shaft **1212**. The stent constraint sleeve **1202** may be axially translatable between a distal position as shown in FIG. **45** and a proximal position as shown in FIG. **46**. The stent constraint sleeve **1202** may also include a plurality of the crown sections **1203** that extend distally from the crown constraint sleeve **1202** and are circumferentially spaced from each other. The constraint system **1200** may further include the plurality of strut supports **1204** which are secured to the elongate shaft **1212** distally adjacent the stent constraint sleeve **1202**. The strut supports **1204** may be circumferentially spaced from each other and extend radially outward or away from a longitudinal axis **1209** of the elongate shaft **1212**.

[0126] Such a constraint system **1200** may have a constraint state wherein the stent constraint sleeve **1202** is disposed in the distal position as shown in FIG. **45** and a deployment state wherein the stent constraint sleeve **1202** is in the proximal position as shown in FIG. **46**. The delivery catheter **501** may also include the expandable basket **1207** having a plurality of elongate tines **1210** which are disposed in a substantially tubular configuration, which extend axially along the elongate shaft **1212** of the delivery catheter **501** in a position distally adjacent the stent constraint sleeve **1202**, and which are configured to bow radially outward upon reduction of a separation between proximal ends **1215** of the elongate tines **1210** and distal ends **1217** of the elongate tines **1210**. In addition, the delivery system **501** may have a stent graft **1218** including a flexible main graft body **1221** and a self-expanding stent, such as self-expanding stent **1206**. The main graft body portion **1221** may include an inner lumen **1222** configured for confining a flow of blood therethrough, a proximal end **1223** and a distal end. The self-expanding stent **1206** may have a proximal end, a distal end secured to the proximal end of the main graft body **1221**, and a plurality of proximal stent crowns **1223** which include at least one barb **1206a**.

[0127] For such a configuration, the stent graft **1218** may be loaded on the proximal section of the elongate shaft **1212** with the elongate shaft disposed within the inner lumen of the graft body **1222**. The plurality of proximal stent crowns **1223** which include at least one barb **1206a** may be disposed within and radially constrained by the stent constraint sleeve **1202** with the stent constraint sleeve **1202** in the distal position. In addition, at least one elongate tine **1210** of the expandable

basket **1207** may be disposed beneath a stent crown **1223** that includes a barb **1206a**, the at least one elongate tine **1210** being configured to apply outward radial force on the stent crown **1223** upon deployment of the stent **1206** and expansion of the expandable basket **1207**.

[0128] The entirety of each patent, patent application, publication and document referenced herein hereby is incorporated by reference. Citation of the above patents, patent applications, publications and documents is not an admission that any of the foregoing is pertinent prior art, nor does it constitute any admission as to the contents or date of these publications or documents.

[0129] Modifications may be made to the foregoing without departing from the basic aspects of the invention. Although embodiments of the invention have been described in substantial detail with reference to one or more specific embodiments, those of ordinary skill in the art will recognize that changes may be made to the embodiments specifically disclosed in this application, yet these modifications and improvements are within the scope and spirit of the invention.

[0130] Embodiments illustratively described herein suitably may be practiced in the absence of any element(s) not specifically disclosed herein. Thus, for example, in each instance herein any of the terms “comprising,” “consisting essentially of,” and “consisting of” may be replaced with either of the other two terms. The terms and expressions which have been employed are used as terms of description and not of limitation and use of such terms and expressions do not exclude any equivalents of the features shown and described or portions thereof and various modifications are possible within the scope of the invention claimed. The term “a” or “an” can refer to one of or a plurality of the elements it modifies (e.g., “a reagent” can mean one or more reagents) unless it is contextually clear either one of the elements or more than one of the elements is described. Thus, it should be understood that although embodiments have been specifically disclosed by representative embodiments and optional features, modification and variation of the concepts herein disclosed may be resorted to by those skilled in the art, and such modifications and variations are considered within the scope of this invention.

[0131] Certain embodiments of the invention are set forth in the claim(s) that follow(s).

What is claimed is:

1. A stent graft comprising:
 - a graft body comprising a flexible tubular main body having an inner lumen configured to confine a flow of fluid therethrough and a graft collar disposed at a proximal end of the main body; and
 - a stent including a distal stent portion which is disposed distally of a proximal edge of the graft collar and which is at least partially secured to the graft collar and a proximal stent portion which is disposed proximally of the graft collar, includes at least one barb extending radially outward therefrom and includes an axial length of about 1 mm to about 5 mm.
2. The stent graft of claim 1 wherein the distal stent portion comprises an axial length of about 10 mm to about 15 mm.
3. The stent graft of claim 2 wherein the proximal stent portion includes a plurality of barbs disposed proximally of a proximal edge of the graft collar.
4. The stent graft of claim 1 wherein the entire distal stent portion is secured to graft collar.

5. The stent graft of claim 4 wherein the distal stent portion is disposed between adjacent layers of material of the graft collar.

6. The stent graft of claim 1 wherein the stent comprises a self-expanding stent.

7. The stent graft of claim 6 wherein the self-expanding stent comprises a superelastic alloy.

8. The stent graft of claim 7 wherein the superelastic alloy comprises NiTi alloy.

9. The stent graft of claim 1 wherein the at least one barb is oriented in a distal direction.

10. The stent graft of claim 1 wherein no barbs are disposed more than about 5 mm from the proximal edge of the graft collar.

11. The stent graft of claim 1 wherein the distal stent portion comprises a continuous sinusoidal configuration and the at least one barb is disposed on a strut that extends proximally from an apex of a sinusoidal configuration of the distal stent portion.

12. The stent graft of claim 1 wherein the distal stent portion comprises a distal portion of a continuous sinusoidal configuration and the at least one barb is disposed on a strut of a proximal portion of the sinusoidal configuration that extends proximally from the proximal edge of the graft collar and forms the proximal stent portion of the stent.

13. The stent graft of claim 1 wherein the stent comprises a balloon expandable stent.

14. The stent graft of claim 13 wherein the balloon expandable stent comprises a high strength alloy.

15. The stent graft of claim 14 wherein the high strength alloy comprises a stainless steel alloy.

16. The stent graft of claim 1 wherein the distal stent portion comprises at least one eyelet and the distal stent portion is secured to the graft collar with flap of material disposed through the eyelet and secured to the graft collar.

17. A method of deploying a stent graft in a patient's vessel, comprising:

- a. providing a stent graft comprising:
 - a graft body comprising a flexible tubular main body having an inner lumen configured to confine a flow of fluid therethrough and a graft collar disposed at a proximal end of the main body, and
 - a stent including a distal stent portion which is disposed distally of a proximal edge of the graft collar and which is at least partially secured to the graft collar and a proximal stent portion which is disposed proximally of the graft collar, includes at least one barb extending radially outward therefrom and includes an axial length of about 1 mm to about 5 mm;
- b. axially positioning the stent graft at a desired site within the patient's vessel with the at least one barb disposed axially coextensive with a viable landing zone of the patient's vessel; and
- c. deploying the stent of the stent graft so as to engage the tissue of the viable landing zone of an inner luminal wall of the patient's vessel.

18. The method of claim 17 wherein deploying the stent comprises deploying the stent disposed at a proximal end of the stent graft disposed towards a source of blood flow in the patient's vessel.

19. The method of claim 17 wherein the stent comprises a self-expanding stent and deploying the stent comprises releasing a radial constraint from the stent in a radially constrained state.

20. The method of claim **17** wherein the stent comprises a balloon expandable stent and deploying the stent comprises expanding the stent radially outward with an expandable member disposed within an inner lumen of the stent.

21. The method of claim **20** wherein the expandable member comprises an inflatable balloon and deploying the stent comprises expanding the stent radially outward by inflating the inflatable balloon with a source of pressurized fluid.

22. A delivery system for delivering a stent graft, the delivery system comprising:

a delivery catheter comprising an elongate shaft with a proximal section and a distal section;

a stent graft having a main graft body with an inner lumen configured for confining a flow of blood therethrough, the stent graft being loaded on the proximal section of the delivery catheter with the elongate shaft disposed within the inner lumen; and

an expandable centering device disposed on the elongate shaft within the inner lumen, the centering device being configured to expand from a radially contracted state to a radially expanded state for centering the elongate shaft and stent graft of the delivery system toward a midline longitudinal axis of a patient's vessel when introduced into the patient's vessel.

23. The delivery system of claim **22** wherein said centering device comprises an expanding basket, the basket including elongate tines that extend substantially parallel to the elongate shaft of the delivery catheter in the radially contracted configuration and are configured to bow radially outwardly from the elongate shaft in a substantially concentric arrangement in the radially expanded configuration.

24. The delivery system of claim **23** wherein the elongate tines are configured to self-expand to the radially expanded configuration.

25. The delivery system of claim **23** wherein the elongate tines are configured to expand to the radially expanded configuration due to axial compressive force applied to at least one end of the tines.

26. The delivery system of claim **24** wherein the elongate tines comprise of a self-expanding metal.

27. The delivery system of claim **26** wherein the self-expanding metal comprises NiTi alloy.

28. The delivery system of claim **24** wherein the elongate tines comprise of a superelastic metal.

29. The delivery system of claim **28** wherein the superelastic metal comprises NiTi alloy.

30. The delivery system of claim **22** wherein said centering device comprises an inflatable structure including:

a collapsed deflated state, and

an enlarged inflated state with a substantially cylindrical configuration including vias that extend from ports in a proximal surface of the centering device to respective ports in a distal surface of the centering device for continuous flow of blood through the centering device and delivery system during inflation of the centering device and deployment of the stent graft.

31. The delivery system of claim **30** wherein the expandable vias have a cumulative cross section that is at least about 5 percent to about 10 percent of the total cross section of the centering device in an expanded state.

32. The delivery system of claim **30** wherein the expandable centering device comprises a configuration that is radially concentric with the elongate shaft in the enlarged inflated state.

33. The delivery system of claim **22** wherein the centering device has an outer transverse dimension of about 50 mm to about 80 mm in the radially expanded state.

34. The delivery system of claim **22** wherein the centering device is configured to expand to an outer transverse dimension that is at least as large as an inner transverse dimension of the inner lumen of the patient's vessel.

35. A method of centering a delivery system during deployment of a stent graft, comprising:

a. providing a delivery system for delivering a stent graft, the delivery system comprising:

a delivery catheter comprising an elongate shaft with a proximal section and a distal section,

a stent graft having a main graft body with an inner lumen configured for confining a flow of blood therethrough and a stent secured to the main graft body, the stent graft being loaded on the proximal section of the delivery catheter with the elongate shaft disposed within the inner lumen, and

an expandable centering device disposed on the elongate shaft within the inner lumen, the centering device being configured to expand from a radially contracted state to a radially expanded state for centering the elongate shaft and stent graft of the delivery system toward a midline longitudinal axis of a patient's vessel when introduced into the patient's vessel;

b. positioning the delivery catheter within a patient's vessel such that the stent graft is axially positioned at a desired site within the patient's vessel with the expandable centering device in the radially contracted state;

c. expanding the expandable centering device to the radially expanded state to center the elongate shaft and stent graft of the delivery system toward the longitudinal axis of the patient's vessel; and

d. deploying the stent of the stent graft so as to engage an inner luminal wall of the patient's vessel.

36. The method of claim **35** wherein deploying the stent comprises deploying a stent disposed at a proximal end of the stent graft disposed towards a source of blood flow in the patient's vessel.

37. The method of claim **35** wherein the expandable centering device comprises a basket and wherein expanding the expandable centering device comprises allowing self-expanding elongate tines of the basket to self-expand to the radially expanded state.

38. The method of claim **35** wherein the expandable centering device comprises a basket and wherein expanding the expandable centering device comprises axially compressing at least one end of elongate tines of the basket to shorten a separation of the proximal ends and distal ends of the elongate tines of the basket and expand a center portion of the tines to the radially expanded state.

39. The method of claim **35** wherein the expandable centering device comprises an inflatable structure and wherein expanding the expandable centering device comprises inflating an interior volume of the inflatable structure with a biocompatible fluid to expand the inflatable structure to the radially expanded state.

40. The method of claim **39** wherein the interior volume of the inflatable structure is inflated through an inflation lumen with a fluid from a source of pressurized fluid.

41. The method of claim **40** wherein the source of pressurized fluid comprises a syringe and inflating the interior volume of the inflatable structure comprises injecting fluid from

an interior volume of the syringe through the inflation lumen and into the interior volume of the inflatable structure.

42. The method of claim **39** wherein the biocompatible fluid comprises saline solution and inflating an interior volume of the inflatable structure comprises inflating the interior volume with saline solution.

43. The method of claim **35** wherein expanding the expandable centering device to the radially expanded state to center the elongate shaft and stent graft of the delivery system toward the longitudinal axis of the patient's vessel comprises expanding the expandable centering device to an outer transverse dimension which is about the same as a transverse dimension of an inner lumen of the patient's vessel at a position of the expandable centering device.

44. A delivery system for delivering a stent graft, the delivery system comprising:

- (1) a delivery catheter comprising an elongate shaft with a proximal section and a distal section;
- (2) a releasable stent constraint system disposed on the proximal section elongate shaft, the stent constraint system comprising:
 - (a) a crown constraint sleeve including a rigid tubular structure disposed about the elongate shaft with a plurality of crown restraint extensions extending distally from the crown constraint sleeve, the crown restraint extensions being circumferentially spaced from each other, and
 - (b) a strut support assembly which is slidingly disposed about the elongate shaft distally adjacent the crown constraint sleeve, and which includes a plurality of strut supports which are circumferentially aligned with respective crown restraint extensions of the crown constraint sleeve and which extend radially away from a longitudinal axis of the elongate shaft,
 - (c) a docked state wherein the strut supports form openable crown constraint passages between the strut supports and respective crown constraint extensions of the crown constraint sleeve, and
 - (d) an open state wherein the strut support assembly is spaced axially away from the crown constraint sleeve and the crown restraint passages are opened to allow radial expansion of stent crowns disposed therein; and
- (3) a stent graft including a self-expanding stent secured to a proximal end of a main graft body, the main graft body having an inner lumen configured for confining a flow of blood therethrough, the stent graft being loaded on the proximal section of the delivery catheter with the elongate shaft disposed within the inner lumen and a plurality of proximal stent crowns disposed within closed crown restraint passages of the stent constraint system with the strut support assembly in a docket state.

45. The delivery system of claim **44** wherein the crown constraint sleeve is secured to elongate shaft and the strut support assembly is slidingly disposed about elongate shaft distally adjacent the crown constraint sleeve.

46. The delivery system of claim **45** wherein the strut support assembly is resiliently biased towards the crown constraint sleeve in an axial direction.

47. The delivery system of claim **46** wherein the strut support assembly is resiliently biased towards the crown constraint sleeve in an axial direction by an axially oriented spring disposed between the strut support assembly and the elongate shaft.

48. The delivery system of claim **44** wherein the strut support assembly is secured to the elongate shaft and the crown constraint sleeve is slidingly disposed about elongate shaft proximally adjacent the crown constraint sleeve.

49. The delivery system of claim **44** further comprising at least one releasable belt disposed about the stent of the stent graft.

50. The delivery system of claim **49** wherein the at least one releasable belt is locked in a constrained configuration about the stent with a removable trigger wire.

51. A method of deploying a stent graft, comprising:

providing a delivery system for delivering a stent graft, the delivery system comprising:

- (1) a delivery catheter comprising an elongate shaft with a proximal section and a distal section;
- (2) a releasable stent constraint system disposed on the proximal section elongate shaft, the stent constraint system comprising:
 - (a) a crown constraint sleeve including a rigid tubular structure disposed about the elongate shaft with a plurality of crown restraint extensions extending distally from the crown constraint sleeve, the crown restraint extensions being circumferentially spaced from each other,
 - (b) a strut support assembly which is disposed about the elongate shaft distally adjacent the crown constraint sleeve, and which includes a plurality of strut supports which are circumferentially aligned with respective crown restraint extensions of the crown constraint sleeve and which extend radially away from a longitudinal axis of the elongate shaft,
 - (c) a docked state wherein the strut supports form openable crown constraint passages between the strut supports and respective crown constraint extensions of the crown constraint sleeve, and
 - (d) an open state wherein the strut support assembly is spaced axially away from the crown constraint sleeve and the crown restraint passages are opened to allow radial expansion of stent crowns disposed therein; and
- (3) a stent graft including a self-expanding stent secured to a proximal end of a main graft body, the main graft body having an inner lumen configured for confining a flow of blood therethrough, the stent graft being loaded on the proximal section of the elongate shaft with the elongate shaft disposed within the inner lumen and a plurality of proximal stent crowns disposed within closed crown restraint passages of the stent constraint system with the strut support assembly in a docket state;

axially positioning the stent graft at a desired site within the patient's vessel; and

axially separating the crown restraint sleeve from the strut support assembly so as to open the crown restraint passages allowing crowns of the stent contained within the crown restraint passages to radially expand.

52. The method of claim **51** wherein the crown constraint sleeve is secured to elongate shaft and the strut support assembly is slidingly disposed about elongate shaft distally adjacent the crown constraint sleeve and wherein axially separating the crown restraint sleeve from the strut support assembly so as to open the crown restraint passages allowing crowns of the stent contained within the crown restraint passages to radially

expand comprises displacing the strut support assembly in an axial direction relative to the crown constraint sleeve and the elongate shaft.

53. The method of claim **52** wherein the strut support assembly is resiliently biased towards the crown constraint sleeve in an axial direction and displacing the strut support assembly in an axial direction relative to the crown constraint sleeve and the elongate shaft comprises retracting the strut support assembly applying axial displacement in a distal direction on a pull rod that is secured to the strut support assembly and extends distally to a distal end of the elongate shaft.

54. The method of claim **51** wherein the strut support assembly is secured to the elongate shaft and the crown constraint sleeve is slidably disposed about elongate shaft proximally adjacent the crown constraint sleeve and wherein axially separating the crown restraint sleeve from the strut support assembly so as to open the crown restraint passages allowing crowns of the stent contained within the crown restraint passages comprises displacing the crown constraint sleeve in a proximal direction relative to the strut support assembly and the elongate shaft.

55. The method of claim **54** wherein the crown constraint sleeve is resiliently biased towards the strut support assembly in an axial direction and displacing the crown constraint sleeve in an axial direction relative to the strut support assembly and the elongate shaft comprises displacing the crown constraint sleeve by applying axial displacement in a proximal direction on a push rod that is secured to the crown constraint sleeve and extends distally to a distal end of the elongate shaft.

56. The method of claim **51** wherein the stent constraint system further comprises at least one releasable belt disposed about and constraining the stent of the stent graft and further comprising releasing the releasable belt to at least partially deploy the stent.

57. The method of claim **56** wherein the at least one releasable belt is locked in a constrained configuration about the stent with a removable trigger wire and wherein releasing the releasable belt comprises withdrawing the trigger wire from the releasable belt.

58. A delivery system for delivering a stent graft, the delivery system comprising:

- (1) a delivery catheter comprising an elongate shaft with a proximal section and a distal section;
- (2) a releasable stent constraint system disposed on the proximal section elongate shaft, the stent constraint system comprising:
 - (a) a stent constraint sleeve which includes a rigid tubular structure slidably disposed about the elongate shaft between a distal position and a proximal position and which includes a plurality of crown sections that extend distally from the crown constraint sleeve and that are circumferentially spaced from each other,
 - (b) a plurality of strut supports which are secured to the elongate shaft distally adjacent the stent constraint sleeve, which are circumferentially spaced from each other and which extend radially away from a longitudinal axis of the elongate shaft,
 - (c) a constraint state wherein the stent constraint sleeve is disposed in the distal position, and
 - (d) a deployment state wherein the stent constraint sleeve is in the proximal position;

- (3) an expandable basket including a plurality of elongate tines which are disposed in a substantially tubular configuration, which extend axially along the elongate shaft of the delivery catheter in a position distally adjacent the stent constraint sleeve, and which are configured to bow radially outward upon reduction of a separation between proximal ends of the elongate tines and distal ends of the elongate tines; and

(4) a stent graft including:

- (a) a flexible main graft body having an inner lumen configured for confining a flow of blood therethrough, a proximal end and a distal end, and
- (b) a self-expanding stent with a proximal end, a distal end secured to the proximal end of the main graft body, a plurality of proximal stent crowns which include at least one barb; and

wherein the stent graft is loaded on the proximal section of the elongate shaft with the elongate shaft disposed within the inner lumen, the plurality of proximal stent crowns which include at least one barb are disposed within and radially constrained by the stent constraint sleeve with the stent constraint sleeve in the distal position, and with at least one elongate tine of the expandable basket disposed beneath a stent crown that includes a barb, the at least one elongate tine being configured to apply outward radial force on the stent crown upon deployment of the stent and expansion of the expandable basket.

59. The system of claim **58** wherein the delivery system further comprises a lock member which is axially fixed relative to the elongate shaft, which engages a first hole in the stent constraint sleeve when the stent constraint sleeve is in the distal position, which engages a second hole disposed distally of the first hole when the stent constraint sleeve is in a proximal position.

60. A method of deploying a stent graft, comprising:

- (A) providing a delivery system for delivering a stent graft, the delivery system comprising:
 - (1) a delivery catheter comprising an elongate shaft with a proximal section and a distal section;
 - (2) a releasable stent constraint system disposed on the proximal section elongate shaft, the stent constraint system comprising:
 - (a) a stent constraint sleeve which includes a rigid tubular structure slidably disposed about the elongate shaft between a distal position and a proximal position and which includes a plurality of crown sections that extend distally from the crown constraint sleeve and that are circumferentially spaced from each other,
 - (b) a plurality of strut supports which are secured to the elongate shaft distally adjacent the stent constraint sleeve, which are circumferentially spaced from each other and which extend radially away from a longitudinal axis of the elongate shaft,
 - (c) a constraint state wherein the stent constraint sleeve is disposed in the distal position, and
 - (d) a deployment state wherein the stent constraint sleeve is in the proximal position;
- (3) an expandable basket including a plurality of elongate tines which are disposed in a substantially tubular configuration, which extend axially along the elongate shaft of the delivery catheter in a position distally adjacent the stent constraint sleeve, and which are configured to bow

radially outward upon reduction of a separation between proximal ends of the elongate tines and distal ends of the elongate tines; and

(4) a stent graft including:

(a) a flexible main graft body having an inner lumen configured for confining a flow of blood therethrough, a proximal end and a distal end, and

(b) a self-expanding stent with a proximal end, a distal end secured to the proximal end of the main graft body, a plurality of proximal stent crowns which include at least one barb; and

wherein the stent graft is loaded on the proximal section of the elongate shaft with the elongate shaft disposed within the inner lumen, the plurality of proximal stent crowns which include at least one barb are disposed within and radially constrained by the stent constraint sleeve with the stent constraint sleeve in the distal position, and with at least one elongate tine of the expandable basket disposed beneath a stent crown that includes a barb, the at least one elongate tine being configured to apply outward radial force on the stent crown upon deployment of the stent and expansion of the expandable basket;

(B) axially positioning the stent graft at a desired site within the patient's vessel;

(C) axially displacing the stent constraint sleeve in a proximal direction from the distal position to the proximal position to release the crowns of the stent to radially expand; and

(D) radially expanding the expandable basket such that at least one elongate tine of the expandable basket which is disposed beneath a corresponding crown having a barb extends radially outward and applies an outward radial force to the corresponding crown so as to facilitate engagement of the barb with tissue of the patient's vessel at the desired site.

61. The method of claim 60 wherein the delivery system further comprises a lock member which is axially fixed relative to the elongate shaft, which engages a first hole in the stent constraint sleeve when the stent constraint sleeve is in the distal position, which engages a second hole disposed distally of the first hole when the stent constraint sleeve is in a proximal position and wherein axially displacing the stent constraint sleeve in a proximal direction from the distal position to the proximal position comprises disengaging the lock from the first hole and engaging the lock in the second hole.

* * * * *