

(19) **DANMARK**

(10) **DK/EP 1404403 T4**



(12) **Oversættelse af ændret
europæisk patentskrift**

Patent- og
Varemærkestyrelsen

-
- (51) Int.Cl.: **A 61 M 25/01 (2006.01)** **A 61 M 25/00 (2006.01)**
- (45) Oversættelsen bekendtgjort den: **2017-01-30**
- (80) Dato for Den Europæiske Patentmyndigheds bekendtgørelse om opretholdelse af patentet i ændret form: **2016-10-19**
- (86) Europæisk ansøgning nr.: **02748637.2**
- (86) Europæisk indleveringsdag: **2002-06-28**
- (87) Den europæiske ansøgnings publiceringsdag: **2004-04-07**
- (86) International ansøgning nr.: **DK2002000450**
- (87) Internationalt publikationsnr.: **WO2003002179**
- (30) Prioritet: **2001-06-29 DK 200101041** **2001-06-29 US 893514**
2001-09-24 DK 200101386 **2001-12-13 DK 200101870**
2001-12-13 DK 200101869 **2001-12-27 US 26819**
2002-04-17 DK 200200569 **2002-04-17 DK 200200570**
2002-06-13 DK 200200895
- (84) Designerede stater: **AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU MC NL PT SE TR**
- (73) Patenthaver: **COLOPLAST A/S, Holtedam 1, 3050 Humlebæk, Danmark**
- (72) Opfinder: **JENSEN, Lars, Boegelund, Daemningen 65, 1, 2610 Rødovre, Danmark**
TANGHOJ, Allan, Jellerod Have 59, 2980 Kokkedal, Danmark
- (54) Benævnelse: **Kateterindretning**
- (56) Fremdragne publikationer:
EP-A- 1 023 882
WO-A-00/30575
DE-A- 2 462 537
DE-A- 3 816 906
FR-A- 2 293 948
GB-A- 2 230 702
GB-A- 2 278 285
US-A- 3 769 981
US-A- 3 867 945
US-A- 3 894 540
US-A- 4 284 459
US-A- 5 354 263
US-A- 5 391 155
US-A- 5 409 469
EP-A1- 1 023 882
WO-A1-00/30575
WO-A1-91/05577

Fortsættes ...

DE-A1- 2 462 537

DE-A1- 3 816 906

FR-A1- 2 293 948

US-A- 4 583 967

US-A- 4 652 259

BERSTEN A.D. ET AL: 'Central Venous Catheter Stiffness and its Relation to Vascular Perforation'

ANAESTHESIS AND INTENSIVE CARE vol. 16, 1988, pages 342 - 357

ECKMANN D.M. PH.D.: 'Variations in Epidural Catheter Manufacture: Implications for Bending and Stiffness'

REGIONAL ANESTHESIA AND PAIN MEDICINE vol. 28, no. 1, 01 January 2003, pages 37 - 42

Colorite Polymers "Clear Injection Molding Compounds"

CAFIERI S. ET AL: 'Modeling the mechanical properties of pasta cooked at different times' JOURNAL OF FOOD

ENGINEERING vol. 100, 2010, pages 336 - 342

GORDON J.E.: 'The science of structures and materials', 1913, SCIENTIFIC AMERICAN BOOKS, INC., NEW YORK page 31

DESCRIPTION

[0001] The present invention relates to an elongated tubular catheter member for draining bodily fluids, e.g. from the bladder.

[0002] Catheters for draining the bladder are increasingly used for intermittent as well as indwelling or permanent catheterisation. Typically catheters are used by patients suffering from urinary incontinence or by disabled individuals like paraplegics who may have no control permitting voluntary urination and for whom catheterisation may be the way of urinating.

[0003] Catheterisation is thus increasingly becoming a daily-life procedure significantly improving quality of life for a large group of patients.

[0004] Typically, catheters are designed for one-time use and accordingly the costs for producing, packing and sterilising a catheter is an important issue. Existing catheters are made from a single piece of a continuous catheter tube. Typically, the thickness of the catheter tube is constant throughout its length.

[0005] The length of the catheter enables insertion of a certain length into the urethra until urine starts to flow. At this point, a certain over-length of the catheter should be available. The over-length supports for the user to firmly hold the catheter and to guide the urine to a place of disposal and to withdraw the catheter safely and without any risk of the catheter disappearing into the urethra.

[0006] Existing catheters are designed to minimise the risk of sores in the mucous membrane and to give substantially no sensation of pain during insertion. Accordingly known catheters are typically provided with a smooth and slippery surface optimised for safe and comfortable insertion into the urethra. Therefore, it may often be difficult, not least for the disabled user, to handle the catheter by manipulation of the slippery over-length.

[0007] It is important that the tubular member does not collapse or kink and thereby blocks the passage for the urine to drain through the catheter. Existing catheters are therefore typically made from a form stable and relatively hard but still bendable tube e.g. made from PVC, PU or PE. Since the hardness of the tubes is selected relatively high with the view to avoid kinking, the catheters may collapse if they are bent with a too small radius of curvature.

[0008] Accordingly, existing catheters not only have a considerable length but they are also typically packed in an elongate condition. Therefore the existing catheters may be troublesome to handle and to bring along, not least for the individuals for whom catheterisation is a daily-life procedure, wherein catheterisation takes place several times a day and wherein the used catheters must be disposed via the garbage collection.

[0009] GB-A-2 278 285 discloses a catheter comprising two catheter sections joined by a flexion portion or, alternatively, a ball-and socket joint. In view of the embodiments of GB-2 278 285, it is an aim of the present invention to provide catheter which is more compact, at least in its storage configuration.

Description of the invention

[0010] The invention provides a kit for preparing a catheter for draining a bodily cavity according to claim 1. Accordingly a catheter is provided which may be adapted at least for one configuration wherein the catheter can be inserted into urethra or into an artificial urinary canal and one configuration wherein the length of the catheter is reduced. As an example, the length may be reduced to a length in the range of one half, one third, one fourth or even to one fifth of the normal required length including the required over-length for manipulation of the catheter.

[0011] The catheter section could be provided in the form of oblong tubular, hollow sections wherein the passage is defined inside the sections or the sections may comprise an oblong solid kernel with one or more vanes extending radially from the kernel and along the entire length thereof. The vanes thus defines a number of draining passages for draining urine between the kernel and a bodily draining passage, e.g. the urethra. The advantage of using a passage defined between a solid kernel and a wall of the urethra is that the flow of bodily fluid cleans the urethra and thus reduces the risk of infection compared with a traditional catheter, wherein the bodily fluid is drained inside the catheter isolated from the body canal.

[0012] A rigidity of substantially the full length of the catheter allows for manipulation of the catheter as one uniform catheter

tube. Thereby, insertion of the proximal end of the catheter may be performed without touching the part of the catheter which is going to be inserted into the urethra. Preferably the catheter is provided with a bending moment defined as the product between E-modulus and moment of inertia of at least 1 MPamm^4 . Since the proximal (inserted) end of the catheter, for male individuals, must pass prostate in a curved passage, the proximal end portion of the catheter, e.g. the first 10-50 mm., such as 20-40 mm., such as 25-35 mm, such as the first 30 mm of the catheter may be provided with an even lower bending moment defined as the product between E-modulus and moment of inertia of less than e.g. $0,6 \text{ MPaMM}^4$ or even less than $0,3 \text{ MPamm}^4$. Other parts of the catheter, e.g. a distal end portion where the urine is drained into the lavatory, a bag or similar place of disposal, may similarly be provided with a reduced bending moment.

[0013] The cross-sectional flow area or the hydraulic radius defined as the ratio of the cross-sectional flow area to the wetted perimeter, may be selected independently upon the length, e.g. on the basis of the size of the urethra, which size depends on the individual using the catheter. Each of the sections may have either the same cross-sectional flow area or hydraulic radius or each section may have individual cross-sectional flow areas or hydraulic radiuses. However, at least one part of one section should have a cross-sectional shape and size adapted for the size of urethra or an artificial urinary canal. Similarly one section should preferably have a length selected on the basis of the length of the urethra or the urinary canal. Thereby it may be achieved that only one section is to be inserted and therefore no transition between sections needs to be inserted. However, especially for male individuals where urethra is particularly long, a catheter having an inserted length divided in two sections or more may be provided. In this specific case it will be appropriate to provide a transition between the sections which at least on the outer surface of the catheter have substantially no recess or sharp edge.

[0014] Preferably, at least one of the catheter sections is provided in a length in the range of 50-90 mm., such as in the range of 55-85 mm., such as in the range of 60-80 mm such as with a length in the size of 70 mm which length has been found to be a suitable insertable length for most female individuals. For male individuals, catheter sections may preferably be provided in a length in the range of 180-250 mm., such as in the range of 190-240 mm., such as in the range of 200-230 mm such as in the size of 220 mm. For the male individuals it may further be preferred to provide at least a part of the inserted end of the catheter in a material or in dimensions so that a the tube becomes very flexible, without kinking. This will easy the passage of the catheter past prostate.

[0015] The outer cross-sectional shape of at least one of the sections should preferably be substantially circular with a cross-sectional area in the range of $0,5 \text{ mm}^2 - 30 \text{ mm}^2$.

[0016] Even more preferred is to provide at least one of the sections with a hydraulic radius ("cross-sectional area"/"circumferential length") in the size of 0,2-1,5 mm.. Alternatively, at least one of the sections should have a cross-sectional shape matching the shape of urethra or an artificial urinary canal, still with a cross-sectional area in the range of $0,5 \text{ mm}^2 - 30 \text{ mm}^2$ or a hydraulic radius in the size of 0,2-1,5 mm. However, the other of the sections does not necessarily have to have the same cross-sectional shape, nor the same hydraulic radius. The wall thickness of the catheter should preferably be in the range between 0,5-1,5 mm.

[0017] The catheter or at least a part of the catheter could be made from a thermoplastic elastomeric material, other thermoplastic materials, curable elastomeric materials, polyamide resins or elastomers or any mixture thereof, i.e. the group may comprise materials like, PVC, PU, PE, latex, and/or Kraton™.

[0018] According to a preferred embodiment, the present invention relates to a urinary catheter divided into completely separated catheter sections. Each catheter section has at least one end provided with means for connecting the section with another section corresponding to an adjacent part of the catheter. As an example the catheter may be divided into two tubular connectable pieces connected by connecting means.

[0019] Preferably, the connecting means are provided with a rigidity allowing for manipulation of at least one of the catheter sections by manipulation of one of the other catheter sections. At least the connection between each of the pieces should provide sufficient rigidity to allow one proximal section to be inserted into the urethra by manipulation of one of the other sections. Therefore, the connection is preferably provided so that at least the part of the catheter extending the connection zone, has a bending moment defined as the product between E-modulus and moment of inertia of at least $0,6 \text{ MPamm}^4$ such as at least 1 MPamm^4 . In order not to have the individual sections falling apart during use, the connection should preferably be adapted to take up an axial force of at least 0,5 Newton or at least to take up an axial force larger than the axial force required for withdrawal of the catheter from the urethra or artificial urinary canal.

[0020] The pieces are telescopically connected. It is appreciated that the sections are in fixed engagement so that they do not disconnect during use of the catheter, while urine is drained through the catheter. However, since the urine is always drained in one direction, the connection does not necessarily have to be liquid-tight. As an example a telescopic connection may be established by inserting the section adapted for insertion into urethra into a distal section. The flow direction of the urine will at least substantially prevent the connection from leaking even though the connection as such is not completely liquid tight. However, a completely sealed connection may provide an even safer catheter with a reduced risk of contaminating hands etc.

[0021] In one embodiment wherein the two catheter sections are arranged in a telescopic fashion, a first one of the catheter sections may be intended for insertion into the human urethra, whereas a second one of the catheter sections is usually intended for forming a prolongation of the catheter outside the human urethra during use of the catheter. In use, that is in the first mutual configuration of the two catheter sections, the second catheter section preferably coextends with the first catheter section away from a distal end of the first catheter section. In the second mutual configuration, which usually is the configuration in which the telescopic kit is stored and transported, at least a portion of the first catheter section may be surrounded by the second catheter section. In the second mutual configuration, a tubular protective member may be provided between an outer surface of the first catheter section and an inner wall of the second catheter section. The dimensions of the tubular protective member and the catheter sections may be such that, in the second mutual configuration, a substantially annular and longitudinally extending cavity is formed between an outer surface of the first catheter section and an inner wall of the second catheter section. The first catheter section may have a hydrophilic surface, and a liquid swelling medium may be provided in the annular cavity, so as to swell the hydrophilic surface of the first catheter section, whereby the first catheter section being encapsulated in the tightly sealed annular cavity may be preserved in its wet, swelled condition for a period of 1-5 years, such as 3-5 years, or more. A tight sealing of the annular cavity is desired for all kinds of catheter surfaces, including hydrophilic and hydrophobic catheter surfaces, in order to prevent contamination to enter into the cavity. Thus, in the second mutual condition, the telescopic joint may serve to define a liquid and contamination tight seal between the second catheter section and an ambient atmosphere.

[0022] A distal end of the second catheter section is preferably provided with a tight seal which may be tight to both liquids and contamination, and which may be removable, so that when a distal end of the second catheter section is inserted into, e.g., a urine collection bag, a passage for urine is formed at the location from which the seal has been removed. The tubular protective member is preferably removable when the first and second catheter sections are in the first mutual position, so that, when the tubular protective member is removed, the proximal end portion of the first catheter section is exposed and ready for insertion into the human urethra. The distal end of the second catheter section may as an alternative be provided into one piece with a collection bag. As an example, the second catheter section may be provided with a plastic welding-flange for adhesively bonding a plastic collection bag to the second catheter section.

[0023] In general, the problems of introducing a catheter into urethra depend not only of the size of the introduced part of the catheter but also on the slipperiness of the introduced part. The catheter section or at least a part of the catheter section or sections adapted for insertion into urethra or an artificial urinary canal may provide a surface slipperiness for easy and safe insertion. However, it has been found that lubricated or slippery surfaces, are difficult to handle, not least for a user having reduced dexterity. It is therefore an object of the present invention to provide a catheter with an inserted part being treated so as to provide a slippery surface and another part not being treated, so as to provide a surface which may easily be handled. The division of the catheter into one part being treated and one part not being treated may preferably follow the aforementioned division of the catheter with the purpose of making the catheter collapsible or separable. According to an alternative embodiment, the parts may be provided in the form of one part being smooth and another part being provided with a rough surface.

[0024] According to a preferred embodiment, at least one of the sections is provided with gripping means easing a firm grip in the catheter. Not least for the disabled user, the gripping means will improve the value of the catheter considerably. Gripping means may be provided as a radially extending flange or flanges or as a zone having a large outer cross sectional diameter. The catheter, or at least one of the catheter sections, may also be provided with means for engaging an external handle. As an example, one of the tubular catheter tubes may be provided with a ring-shaped bulge for attaching a handle. The ring-shaped bulge could be provided as a short tubular piece of plastic with a larger radial size than the catheter, the catheter being inserted and glued into the short piece of plastic.

[0025] A section provided with a hydrophilic surface treated with a liquid swelling medium may provide an excellent lubrication for the insertion and also provide compatibility with the body tissue. It is therefore a further preferred embodiment of the invention to provide at least one of the sections with a hydrophilic surface layer.

[0026] One of the catheter sections could be used as a sterile package for the other sections, e.g. by arranging the sections in a telescopic manner inside one section, closing and sealing that section in both ends, e.g. by a peelable and optionally a metallised foil e.g. made from a thermoplastic elastomeric material, other thermoplastic materials, curable elastomeric materials, polyamide

resins or elastomers or any mixture thereof, i.e. the group may comprise materials like, PVC, PU, PE, latex, and/or Kraton™, thereby allowing for sterilising the assembly by radiation.

[0027] The liquid swelling medium for the hydrophilic surface may be provided in the package for initiation of the low friction character already when the catheter is being packed. The liquid swelling medium may simply be a saline solution, a bactericidal solution capable of swelling the hydrophilic surface and capable of keeping the surface in a sterile condition or it may be pure water. The swelling may also be initiated already before packaging of the catheter, the catheter then being packed in a substantially gas impermeable package for conservation of the moistened surface. Furthermore, the liquid swelling medium may be provided in a capsule or container packed together with the catheter for swelling of the hydrophilic material immediately prior to the insertion.

[0028] Embodiments of the present invention may comprise :

- a flexible elongated tube with an inner cross-sectional shape and size defining a first conduit for draining urine, said tube having an insertion end and a discharge end, and
- a supporting member being introduced into the first conduit and provided with an outer cross-sectional shape and radial size substantially equal to the inner cross-sectional shape and size of the elongate tube so as to support said tube against collapsing during bending of the tube, the supporting member having a flexibility allowing curling.

[0029] The flexible elongated tube could have the shape of a regular catheter of the known kind. Preferably, the tube or at least a part of the tube is made from a thermoplastic elastomeric material, other thermoplastic materials, curable elastomeric materials, polyamide resins or elastomers or any mixture thereof, i.e. the group may comprise materials like, PVC, PU, PE, latex, and/or Kraton™.

[0030] The supporting member supports the catheter to avoid collapsing when the catheter is bent, e.g. for the purpose of packing the catheter in user friendly short packages. The supporting member may be either solid or the supporting member may be hollow and thus defining a second conduit. The solid supporting member should be adapted for removal prior to draining of the bladder, whereas a hollow supporting member may remain inside the tube while the bladder is emptied through the first and second conduit.

[0031] The supporting member may as an example be glued inside the elongated tube or the supporting member may even be moulded into the tube during the process of producing the tube. The supporting member may even be completely integrated in the elongated tube.

[0032] The supporting member could be made from any suitable material such as e.g. plastic, steel, aluminium, a thermoplastic elastomeric material, other thermoplastic materials, curable elastomeric materials, polyamide resins or elastomers or any mixture thereof. As an example, the supporting member may be a helical spring provided in a length in the range of 20-60 mm, such as in the range of 30-50 mm., such as in the range of 35-45 mm. The spring should be positioned inside the elongated tube in the zone where it is desired to bend the catheter, e.g. midway along the longitudinal axis of the elongated tube. During use, the urine is drained through the first conduit of the elongated tube and past the supporting member through the second conduit.

[0033] According to a preferred embodiment, the supporting member is provided in a length in the range of 60-120 mm, such as in the range of 70-110 mm., such as in the range of 80-100 mm and the supporting member may even be extending out of the discharge end of the elongated tube. This will enable the user to remove the supporting member during the process of inserting the catheter into urethra.

[0034] According to a further preferred embodiment, the supporting member is provided with gripping means for easing withdrawal of the supporting member from the discharge end during insertion of the catheter.

[0035] In further embodiments, the at least two catheter sections are arranged in a coextending fashion with a tubular protective member surrounding a first, proximal one of said catheter sections, the kit further comprising a joint for interconnecting the first and the second catheter section, the joint defining a liquid tight seal at a proximal end of a substantially annular and longitudinally extending cavity provided between the proximal end portion of the first catheter section and an inner wall of the tubular protective member, the tubular protective member being removably connected to the joint and/or to the second catheter section, so that, when the tubular protective member is removed, the proximal end portion of the first catheter section is exposed and ready for insertion into the human urethra.

The passage may be defined either inside the hollow, tubular catheter sections or between a solid kernel and the wall of the urethra or similar bodily channel.

[0036] Such embodiments of the kit may be regarded as modifications of telescopic embodiments of the kit according to the invention, the modification comprising that a longitudinal movement of the two catheter sections relative to each other is usually not intended and that only one mutual configuration is usually intended.

[0037] In particular, the catheter may be provided so that the sections are adapted to be moved between at least two positions with respect to each other. One position being a position wherein the second section surrounds the first section and the other position being a position wherein the second section forms an extension for the first section.

[0038] Preferably, the joint between the first section and the second section is a telescopic joint providing a liquid tight seal between the sections while they are moved between the first position and the second position. As an example, the first section may be provided with a piston seal adapted to slide along the inner surface of the second section while the first section is being pulled out of second section between the first and second position.

[0039] In order to allow the user to insert the first section into a body canal, it will be appreciated to have a locking arrangement of the first and/or the second catheter section for locking the position of the first section with respect to the second section, when the sections are in the second position, i.e. when the catheter is in a configuration ready for insertion into the body canal.

In order to allow the user to pull the first catheter section out of the second catheter section without touching the insertable part of the catheter, the tubular protective member may preferably be provided to engage the first catheter section in a locking engagement. Thereby, it will be allowed to use the tubular protective member to pull the first catheter section out of the second catheter section.

[0040] When the first catheter section has been pulled out of the first catheter section, i.e. when the sections are in the second position, i.e. in the position wherein the second catheter section forms an extension for the first catheter section, the tubular protective member should be allowed to disengage the first catheter section. When the tubular protective member has been removed, the catheter is in a "ready to insert" state.

[0041] In order to use the second catheter section as a sealing envelope or package for the first catheter section, i.e. for the insertable catheter section, the distal end of the first catheter section may preferably be adapted to seal an opening in a distal end of the second catheter section while the sections are in the first position and not to seal set opening when the sections are in the second position. When the sections are brought into the second position, i.e. when the catheter is "ready for insertion", the opening in the distal end of the second section may be used for draining the bodily liquids, e.g. urine out of the catheter.

[0042] In order to allow the annular cavity to be used e.g. for carrying a frictional reducing substance, e.g. a water or saline solution for a hydrophilic catheter, a hydrogel or similar lubricating substance, the kit may preferably be provided with a sealing engagement between the tubular protective member and the first catheter section when the tubular protective member is engaging the first catheter section. When the tubular protective member is disengaged from the first catheter section, i.e. after the catheter has reached its "ready for insertion state", the annular cavity is open to the ambient atmosphere thus exposing the insertable tip of the first catheter section and allowing the user to drain surplus friction reducing substances.

[0043] According to a preferred embodiment, the first catheter section is provided with a hydrophilic surface and the friction reducing substance provided in the annular cavity is a liquid swelling medium, e.g. water or a saline solution.

[0044] The catheter may further comprise a connector part for connecting the proximal insertion section to a further catheter section or to a urinary collection bag. The connector part may be made from the same material as the proximal insertion section, whereby, at the step of forming the proximal insertion section, the proximal insertion section and the connector part may be formed substantially simultaneously. Alternatively, the connector part may be made from a material different from the material of the proximal insertion section, whereby the connector part and the proximal insertion section are formed in distinct process steps, for example in a multi-component injection moulding process.

Brief description of the drawings

[0045] Preferred embodiments of the invention will now be described in details with reference to the drawing in which:

Fig. 1 shows an embodiment of the kit, wherein one catheter part is inserted for storage into another of the catheter parts thus

substituting a catheter package,

Fig. 2 shows the embodiment of Fig. 1, wherein the inserted catheter part is partially withdrawn from one end of the package,

Fig. 3 shows the embodiment of Figs. 1 and 2, wherein the inserted catheter part is completely withdrawn from the package and then attached to the other end of the package, the package thus functions as a handle for manipulation of the catheter,

Fig. 4 shows a folded telescopic catheter kit,

Fig. 5 shows the catheter kit of Fig. 4, in an extended configuration,

Fig. 6 shows the catheter kit of Fig. 4, unfolded and after withdrawal of the combined closure and withdrawal cap,

Fig. 7, shows a preferred embodiment of a combined closure and withdrawal cap for the kit shown in Figs. 5 and 6,

Fig. 8 shows yet another preferred embodiment of a combined closure and withdrawal cap for the kit shown in Figs. 5 and 6,

Figs. 9-12 illustrate an embodiment of a kit according to the invention, wherein the catheter sections are arranged in a telescopic fashion,

Figs. 13-16 show a further embodiment, wherein the catheter sections are arranged in a telescopic fashion,

Fig. 17 shows a catheter part provided with gripping means for easing the handling of the catheter,

Fig. 18 shows a preferred cross-sectional shape of a catheter part adapted for insertion into the urethra,

Detailed description of the drawings

[0046] Fig. 1 shows an embodiment of the catheter kit according to the present invention, wherein the first catheter section, not shown in Fig. 7, is sterilely packed inside the second catheter section 21, the second catheter section being sealed in both ends with sealing caps or foils 22,23.

[0047] Preferably the first section is coated with a hydrophilic coating, providing a low friction surface of the first catheter section when treated with a liquid swelling medium. The coating could be of the kind which sustains being activated with the liquid swelling medium for longer time, e.g. for several month. Thereby the liquid swelling medium could be provided in the catheter package from the time of packaging so as to provide a ready-to-use catheter. Hydrophilic coatings are known per se, see e.g. the published patent applications WO 98/58988, WO 98/58989, WO 98/58990 or EP 0570370. For this purpose, the sealing caps or foils should preferably be provided in a gas impermeable material for conservation of the humidity and thus the lubricity of the catheter for longer time, e.g. for several month. As an example, the second catheter section and/or the sealing caps may be made from a thermoplastic elastomeric material, other thermoplastic materials, curable elastomeric materials, polyamide resins or elastomers or any mixture thereof, i.e. the group may comprise materials like, PVC, PU, PE, latex, and/or Kraton™. The caps may be provided with a thickness allowing for sufficient gas impermeability. As an alternative, they may be made from metallised foils.

[0048] As seen in Fig. 2, the first catheter section is easily withdrawn from the second catheter section by pulling the cap or foil 23 which cap or foil engages the distal end of the first catheter section.

[0049] Fig. 3 shows the assembled catheter after the first catheter section has been attached to the second catheter section. The foil or cap 23 can either be removed completely as shown in Fig. 3 or can at least be penetrated by the connecting means 24 of the second catheter section.

[0050] Fig. 4 shows an embodiment of the catheter kit wherein the first and the second catheter sections are connected telescopically. The first catheter section is sterilely packed inside the second catheter section 26. The second catheter section being sealed by a first sealing closure 27 and a second sealing closure 28. Prior to use, the first sealing closure is removed. If the first catheter section is provided with a hydrophilic surface layer, and if the catheter section is packed with a liquid swelling medium, the liquid medium may be emptied through the passage opened by the first sealing closure. As best seen in Fig. 5, the second sealing closure engages the first catheter section 30 for easy withdrawal of the first catheter section. When the first catheter section has been completely withdrawn, the distal part of the first catheter section engages the proximal end of the second catheter section in the connecting zone 31 and the second sealing closure easily disengages the first catheter section.

The catheter is then in a configuration for use.

[0051] Fig. 7 shows a preferred embodiment of the second sealing closure 28, wherein the closure is provided with internal and radially inwardly extending projections 33 adapted for engaging the hole 32 shown in Fig. 6.

[0052] Fig. 8 shows another embodiment of the second sealing closure 28, wherein flexible gripping flanges 34 softly grips the proximal (inserted) end of the first catheter section for easy withdrawal of the first catheter section from the second catheter section upon removal of the second sealing closure.

[0053] The telescopic embodiment of the catheter kit, disclosed in Figs. 4-8, should preferably be provided so that the internal diameter of the second catheter section is slightly larger than the external diameter of the first catheter section. This is an advantage, e.g. in the case where the first catheter section is coated with a hydrophilic surface coating and in order not to scrape off the coating when sliding the first catheter section out of the second catheter section. On the other hand, it is an important aspect to provide a connecting zone wherein the first catheter section and the second catheter section firmly engages. Thereby, insertion and orientation of the first section is possible merely by manipulation of the second section and without the sections mutually sliding in the telescopic connection. It is furthermore important to assure that the first catheter section does not slip out of the second section in which case the first catheter section might disappear into the urethra. For this purpose, the distal end (opposite the inserted end) of the first catheter section may be provided with a radially outwardly extending flange disallowing the first catheter section to slip out of the second catheter section.

[0054] Figs. 9-12 illustrate a second embodiment of a catheter kit wherein the first and second sections 42, 44 are telescopically interconnected. A tubular protective member 46 surrounds a portion of the first catheter section 42 and forms a substantially annular cavity 48 around the first catheter section. In the second mutual configuration, shown in Fig. 16, in which the kit is intended to be stored and shipped, the first catheter section 42 and the tubular protective member 46 are inserted as far as possible into the second catheter section 44. A hydrophilic swelling medium, such as water, may be provided in the cavity 48, so that a hydrophilic surface coating optionally provided at the surface of the first catheter section 42 is stored in its swelled, i.e. wet condition. A surplus of hydrophilic swelling medium may be present in the cavity 48 in order to prevent the hydrophilic surface coating from drying out. A liquid-tight seal so is provided at the distal end of the first catheter section 42. A liquid-tight closing member 52 closes the distal end of the second catheter section 44. In one embodiment, the closing member 52 is removable so that a passage is provided between the second catheter section 44 and a urine collection bag, or another device for accumulating or conveying urine, mounted to the distal end of the section catheter section 44, when the closing member 52 is removed. In another embodiment, the closing member 52 is an integrated part of the second catheter section 44, in which case a wall 53 of the closing member 52 may be perforated in order to provide a passage between the second catheter section 44 and a urine collection bag, or other device for accumulating or conveying urine, mounted to the distal end of the section catheter section 44. In yet another embodiment, the closing member 52 may be substituted by a perforated end wall, e.g. a wall made from a central plate connected to the outer wall of the second catheter section 44 at its distal end by means of radially extending ribs or spokes. In such an embodiment, the first catheter section 42 and the seal 50 may be formed as a single, integrated piece.

[0055] As shown in Fig. 10, an outer wall of the second catheter section 44 forms a handle, the tubular protective member 46 being arranged so that it extends out of the handle at the proximal end thereof. The tubular protective member 46 may form a flange at its proximal end, so as to facilitate a user's extraction of the first catheter section 42 and the tubular protective member 46 out of the handle/second catheter section 44. When extracted, the tubular protective member 46 and thus the first catheter section 42 surrounded thereby coextend with the handle or second catheter section 44, as illustrated in Fig. 11. A protrusion 47 at the distal end of the tubular protective member 46 releasably secures the tubular protective member 46 to the seal 50, see Figs. 9, 11 and 12. The seal 50 may be designed so that it engages the proximal end portion of the second catheter section 44 by a snap action once the seal 50 and the tubular protective member 46 have reached the fully extracted position shown in Fig. 11. In the example shown in Fig. 9, the seal 50 has a groove 51 which, in the extracted position shown in Figs. 11 and 12 engages a flange 45 at the proximal end of the second catheter section 44. Immediately prior to use of the catheter, the tubular protective member 46 is removed, so that the first catheter section 42 is exposed, as shown in Fig. 12.

[0056] Figs. 13-16 illustrate a further embodiment of a catheter kit, wherein the catheter sections are arranged in a telescopic fashion. As shown in the exploded view in Fig. 16, the kit comprises the following parts: a first catheter section 62, a second catheter section 64 with one or more inner flange portions 65, a guide member 66 with protrusions 67, a joint 69 with a collar portion 70 and slits 71 for the guide member 66, as well as a distal closure member 72 and a proximal closure member 73. The kit is stored and transported in the configuration shown in Fig. 13, wherein the second catheter section surrounds the first catheter section 62 and the guide member 66. Prior to use of the catheter, the distal closure member 72 is removed, and the guide member 66 is extracted, as shown in Fig. 14. The guide member 66 is extracted as far as possible, i.e. until the protrusions 67, due to their elasticity, engage respective grooves (not shown) provided in the slits 71 of the joint 69, see Fig. 16. The joint 69 is

secured from sliding out of the second catheter section 64 by means of the inner flange portions 65 of the second catheter section 64. The proximal closure member 73 is also removed. Next, the guide member 66 is pushed back into the second catheter section 64. As the guide member engages the joint which is firmly connected to the distal end of the first catheter section, the joint 69 and the first catheter section 62 are pushed out of the distal end of the second catheter section 64 as the guide member 66 is pushed in the second catheter section 62. When the collar portion 70 of the joint 69 engages an inner flange or protrusion provided at the proximal end of the second catheter section 64, the kit is ready for use, and the first catheter section 62 may be introduced into the urethra of a human. A urine collection bag or other means for accumulating or conveying urine may be mounted to the proximal end of the second catheter section 64.

[0057] Fig. 17 shows a handle 40 for easy manipulation of the catheter. The handle may be highly appreciated not least for disabled users of the catheter e.g. for people having a reduced dexterity.

[0058] Fig. 18 shows a preferred cross-sectional shape of the insertable part of the catheter. As the inserted part has an oval cross-sectional shape, the bending moment around the x-axis (indicated in Fig. 18) will be different from the bending moment around the y-axis. The relatively low bending moment around the y-axis will enhance the ability of the catheter to bend in one direction, and thereby easy the insertion of the catheter past prostate. The relatively high bending moment around the x - axis will enhance the general stiffness of the catheter thereby easing manipulation of the inserted part of the catheter from the part of the catheter not being inserted.

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- [GB2278285A \[0009\] \[0009\]](#)
- [WO9858988A \[0047\]](#)
- [WO9858989A \[0047\]](#)
- [WO9858990A \[0047\]](#)
- [EP0570370A \[0047\]](#)

EP1404403

Patentkrav

1. Kit til fremstilling af et kateter til udtømning af en menneskelig blære via urinrøret, hvor kittet omfatter mindst to kateterafsnit (20; 21; 26; 30; 42; 44; 5 62; 64), der definerer en passage deri, hvor afsnittene er indrettet til at blive anbragt i en første indbyrdes konfiguration, hvor passagerne føres sammen til en passage, og afsnittene sammen udgør et kateter med en længde, der er større end længden af hvert individuelle kateterafsnit og med en sådan stivhed, at kateteret kan manøvreres til indføring af et 10 proximalt afsnit af kateterets afsnit (20; 30; 42; 62) i urinrøret ved håndtering af et andet af kateterets afsnit (21; 26; 44; 64) og en anden indbyrdes konfiguration, hvor kittet er kortere, end når afsnittene er indrettet i den første indbyrdes konfiguration, kendetegnet ved at nævnte afsnit (20; 21; 26; 30; 42; 44; 62; 64) omfatter et par separate afsnit 15 forbundet ved hjælp af et teleskopisk led (24; 31; 50; 69), og ved at mindst den del af kateteret, der udstrækker en forbindelseszone mellem kateterafsnittene, har et bøjningsmoment på mindst $0,6 \text{ MPamm}^4$, hvor bøjningsmomentet er defineret som produktet mellem E-modulus og inertimomentet.
- 20 2. Kit ifølge et hvilket som helst af de foregåede krav, hvor det teleskopiske led (24; 31; 50; 63) tilvejebringer en stivhed, der muliggør manøvrering af mindst et af kateterafsnittene (20; 21; 26; 30; 42; 44; 62; 64) ved hjælp af håndtering af et af de andre kateterafsnit (20; 21; 26; 30; 42; 44; 62; 64).
- 25 3. Kit ifølge krav 1 eller 2, hvor mindst et afsnit af det første af kateterafsnittene (20; 30; 42; 62) er omgivet af et andet af kateterafsnittene (21; 26; 44; 64) i den anden indbyrdes konfiguration.

EP1404403

4. Kit ifølge krav 3, hvor en proximal endedel af det første kateterafsnit (42) er tiltænkt til indføring i det menneskelige urinrør, og hvor mindst det proximale endefsnit af det første kateterafsnit (42) i den anden indbyrdes konfiguration er omgivet af et rørformet beskyttelseselement (46).
- 5 5. Kit ifølge krav 4, hvor teleskopledet (24; 31; 50; 69) definerer en væsketæt tætning (50; 69) ved en proximal ende af et i det væsentlige ringformet og sig i længderetningen strækkende hulrum (48) tilvejebragt mellem det proximale endefsnit af det første kateterafsnit (42) og en indvendig væg af det rørformede beskyttelseselement (46).
- 10 6. Kit ifølge krav 5, hvor der i det ringformede hulrum (48) er tilvejebragt et flydende svulmemiddel til en hydrofil kateteroverflade.
7. Kit ifølge et hvilket som helst af de foregående krav, hvor mindst et af kateterafsnittene (20; 21; 26; 30; 42; 44; 62; 64) er forsynet med en hydrofil overflade af i det mindste en del af sin overflade tiltænkt til at
- 15 tilvejebringe en lavfriktionsoverfladeegenskab af den del af kateteret ved hjælp af behandling med et flydende svulmemiddel inden brug af kateteret.
8. Kit ifølge et hvilket som helst af de foregående krav, hvor afsnittene (20; 21; 26; 30; 42; 44; 62; 64) er indrettet i den anden konfiguration inden i en
- 20 pakke.
9. Kit ifølge krav 8, hvor pakken i det mindste delvist er dannet af mindst et af afsnittene (21; 26; 44; 64).
10. Kit ifølge krav 8 eller 9, hvor pakken indbefatter en mængde flydende svulmemiddel, der er tilstrækkelig til behandlingen af den hydrofile

EP1404403

overfladedel for at tilvejebringe en lavfriktionsoverfladeegenskab af den del.

11. Kit ifølge et hvilket som helst af de foregående krav, hvor mindst et af afsnittene (20; 30; 42; 62) er belagt med et smøremiddel.

DRAWINGS

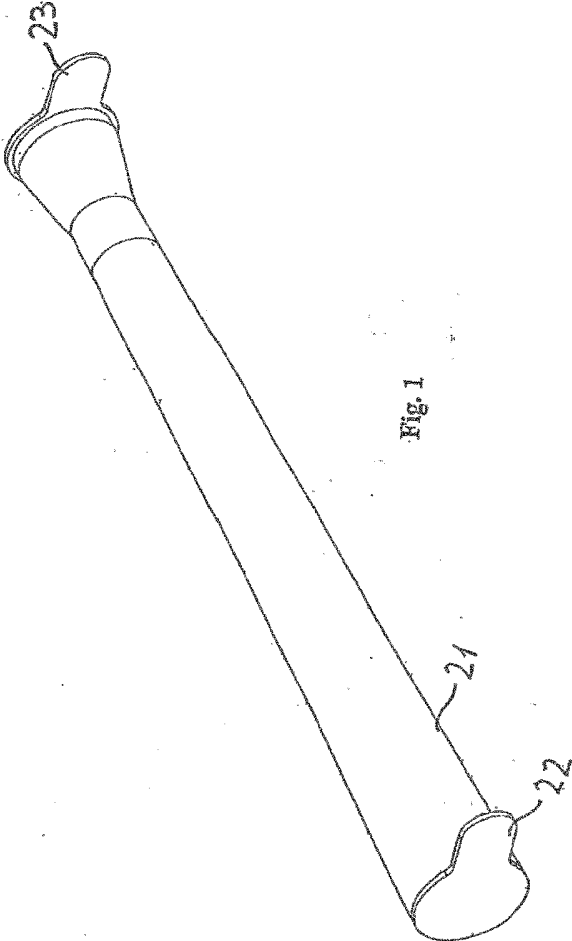


Fig. 1

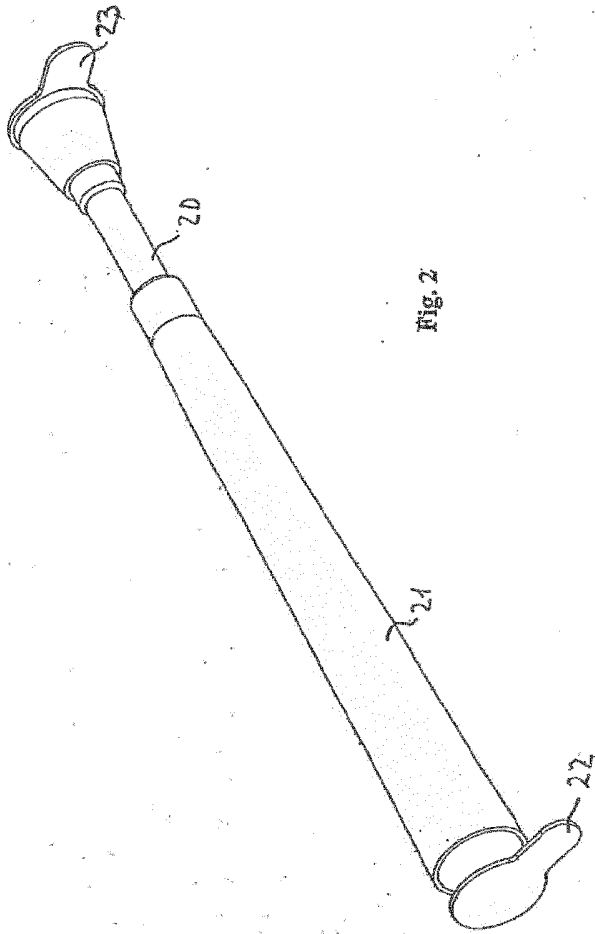


Fig. 2

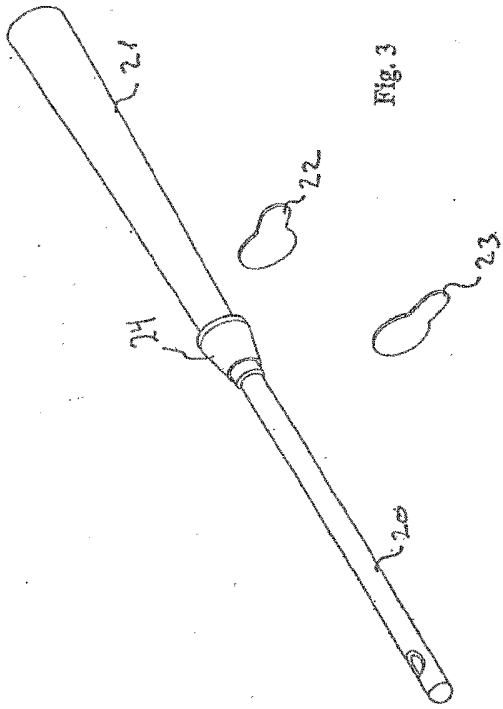


Fig. 3

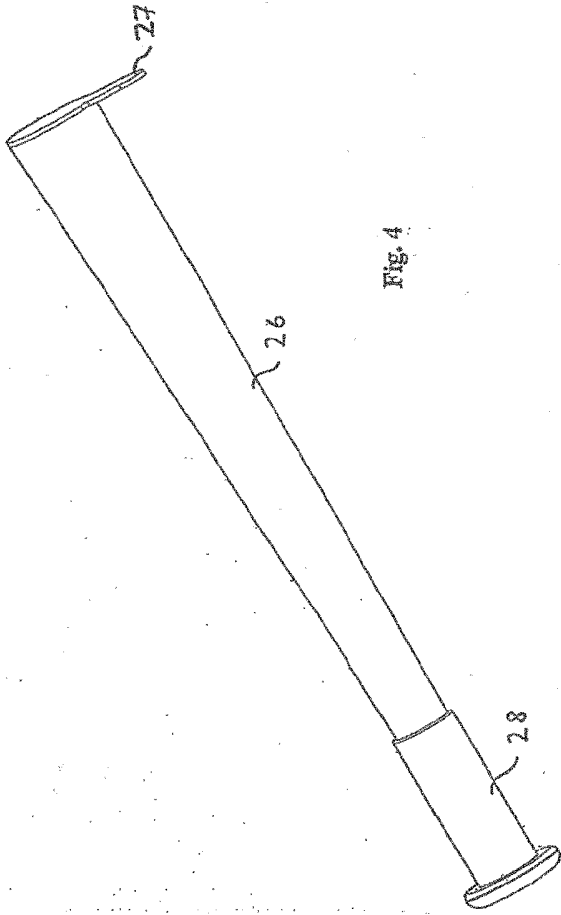


Fig. 4

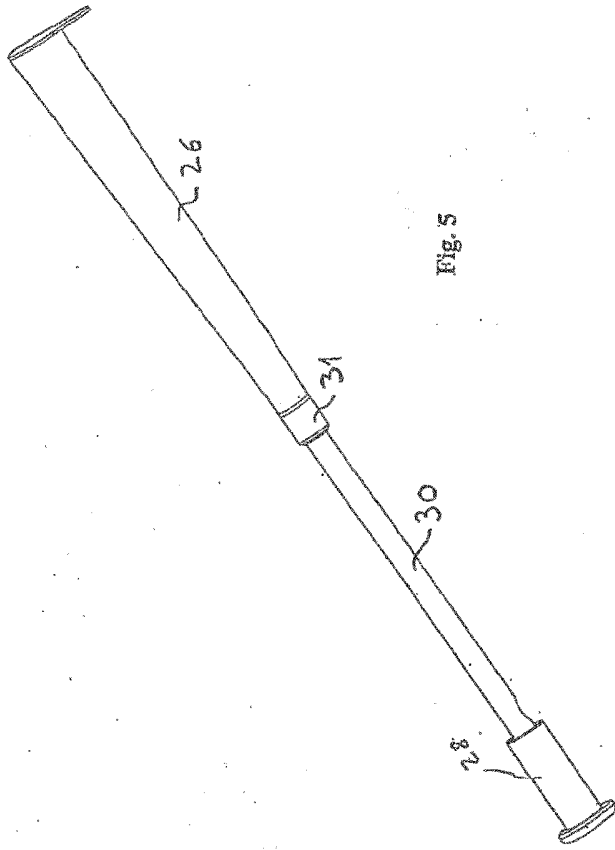


Fig. 5

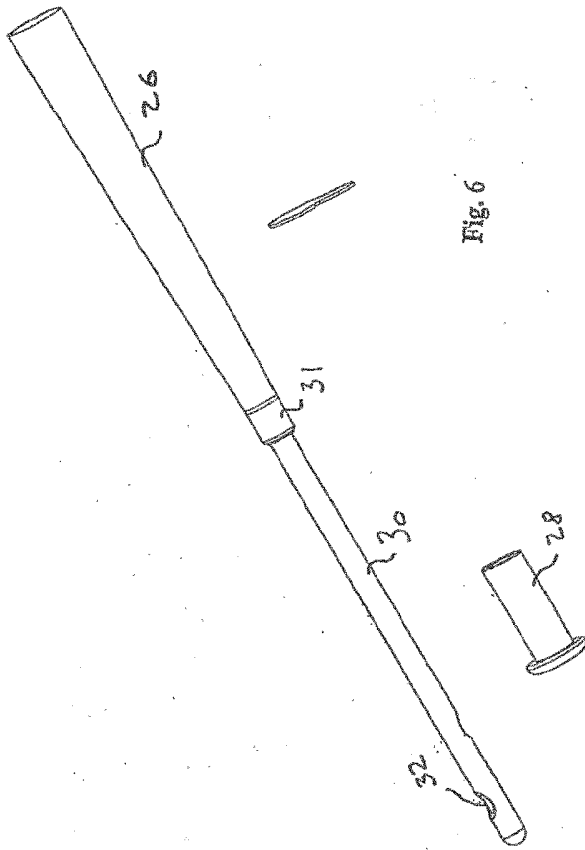


Fig. 6

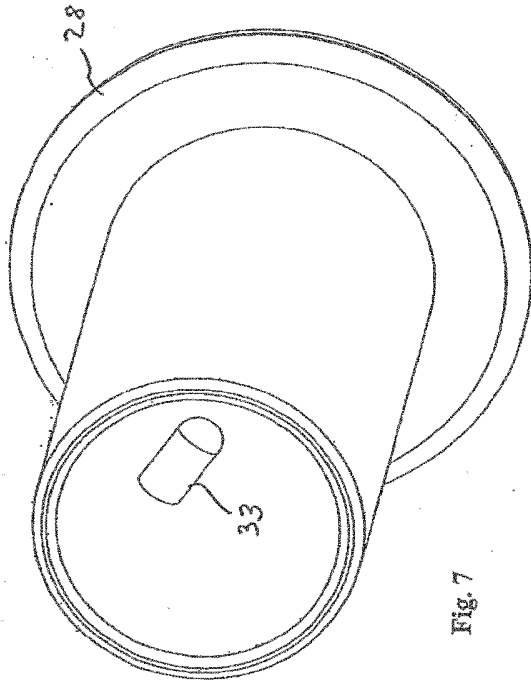


Fig. 7

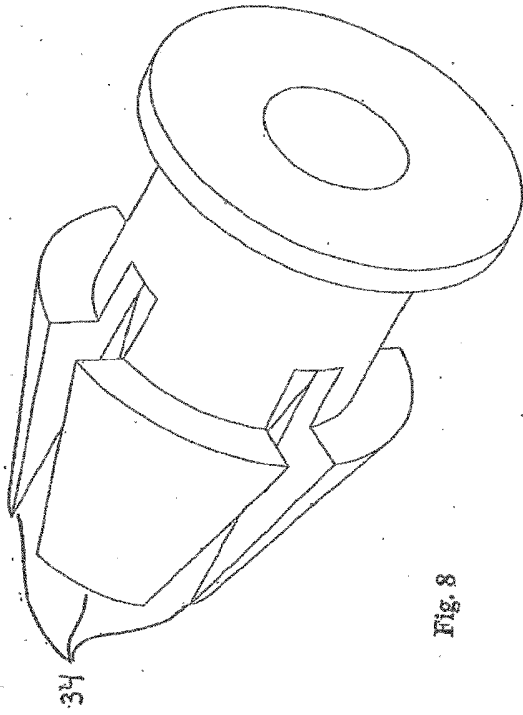


Fig. 8

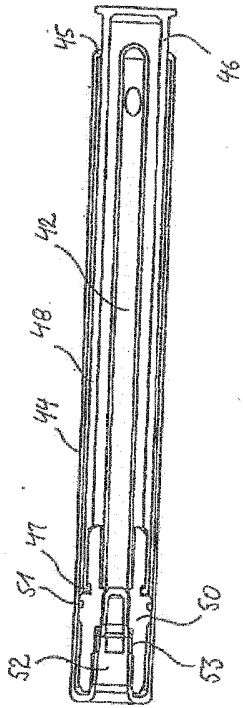


Fig. 9

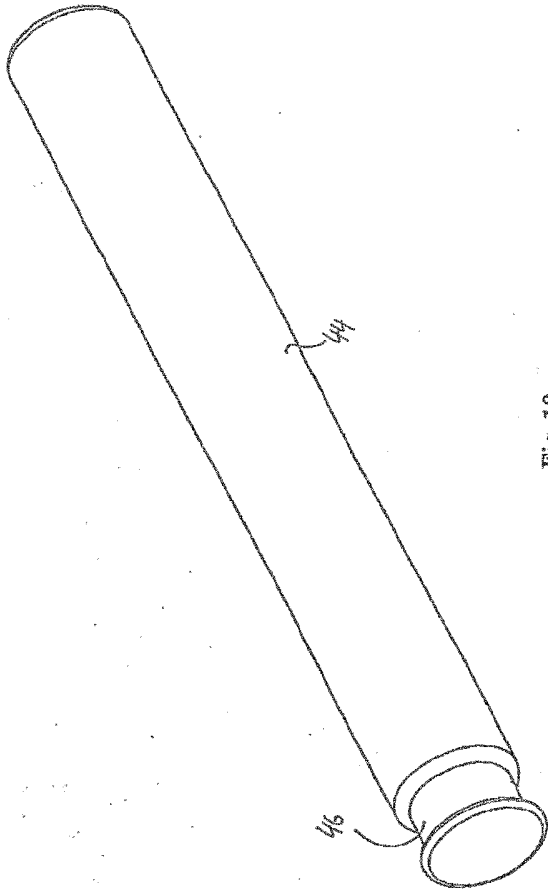


Fig. 10

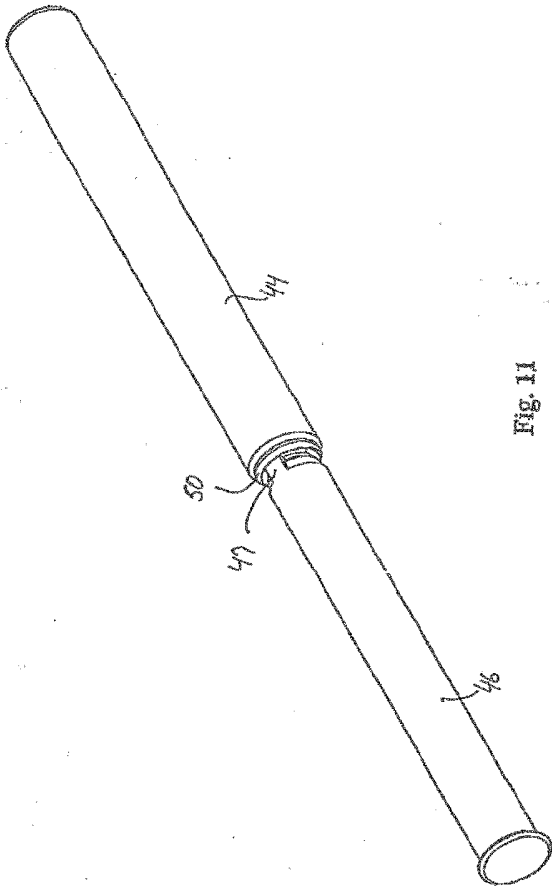


Fig. 11

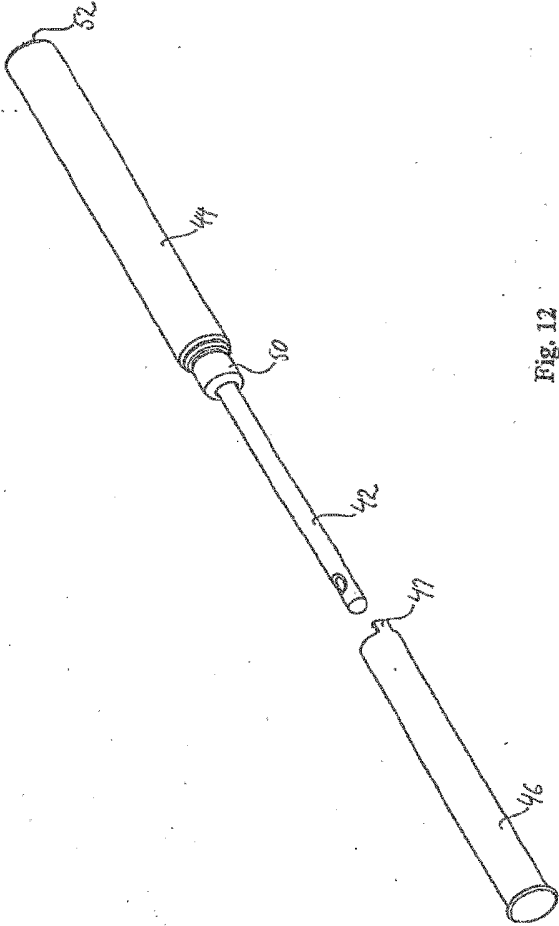


Fig. 12

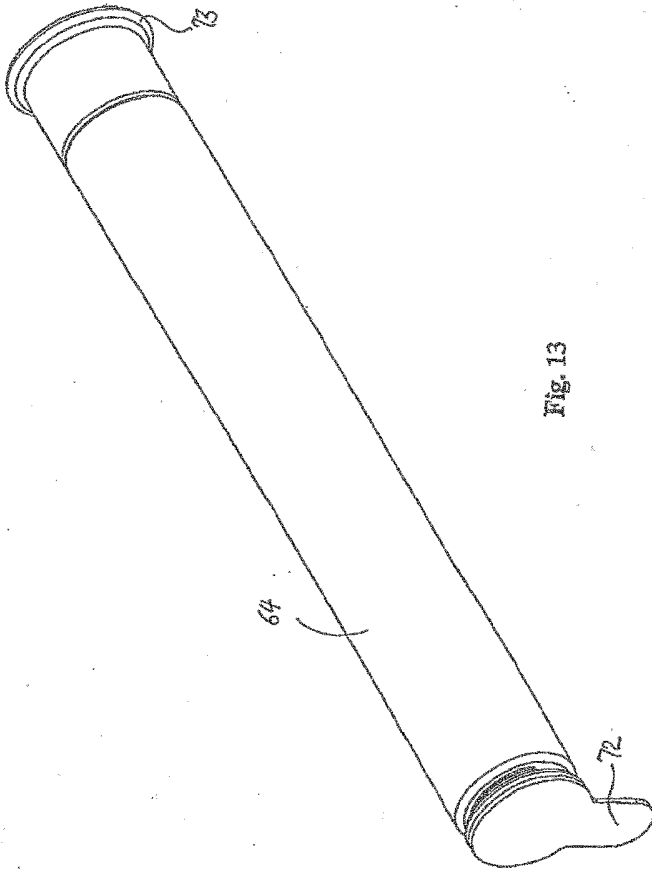


Fig. 13

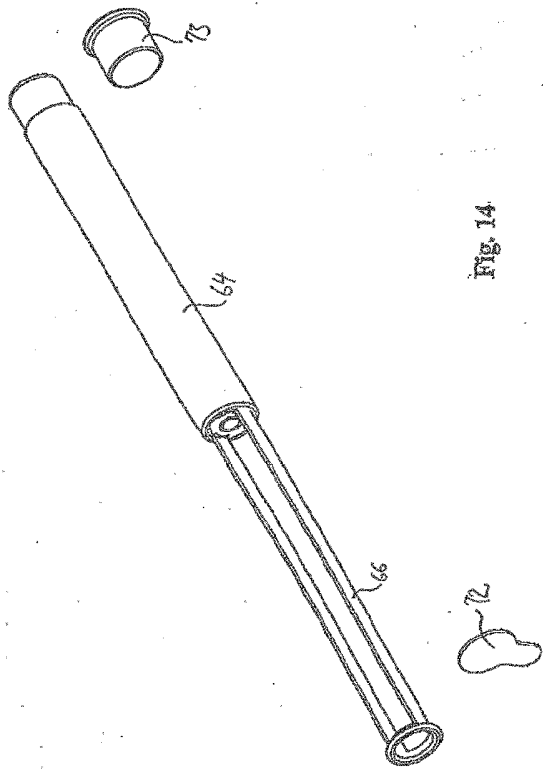


Fig. 14

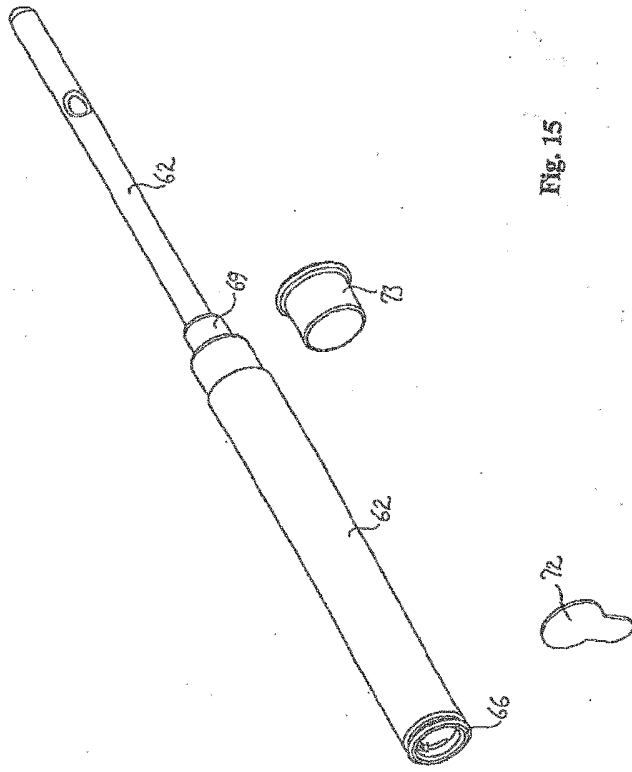


Fig. 15

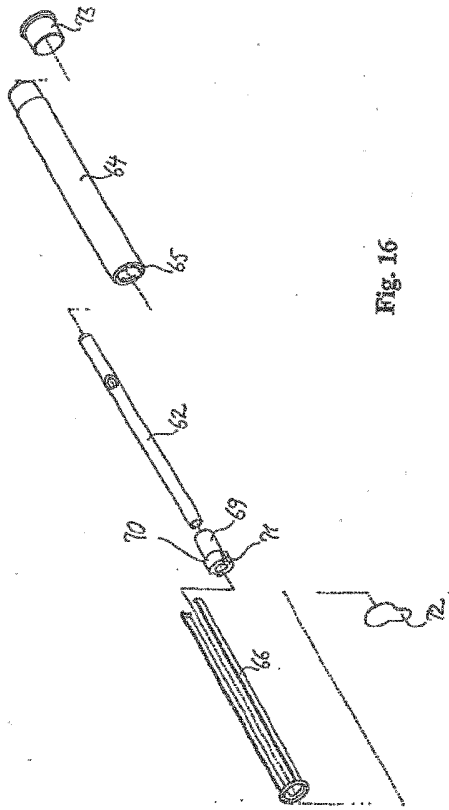


Fig. 16

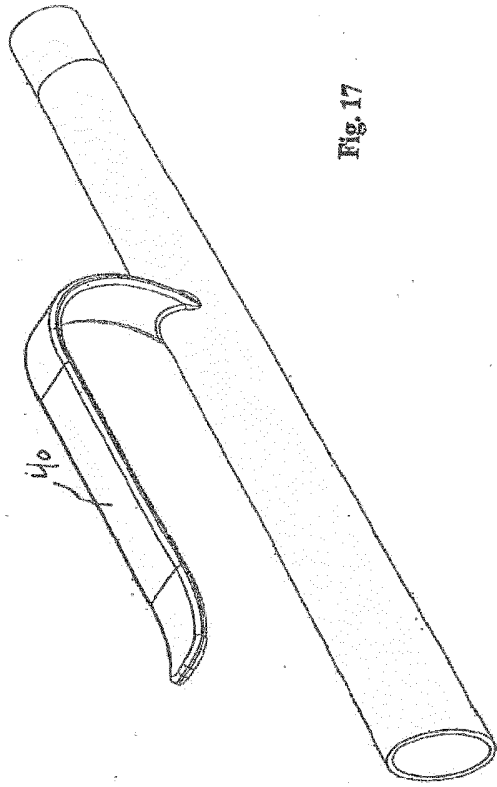


Fig. 17

Fig. 18

