



US 20080300489A1

(19) **United States**

(12) **Patent Application Publication**  
**Schutz et al.**

(10) **Pub. No.: US 2008/0300489 A1**

(43) **Pub. Date: Dec. 4, 2008**

(54) **CABLE AND CONNECTOR SYSTEM FOR AN ULTRASOUND PROBE**

**Related U.S. Application Data**

(60) Provisional application No. 60/923,323, filed on Apr. 13, 2007.

(76) Inventors: **Ronald W. Schutz**, Portland, OR (US); **Scott S. Corbett, III**, Portland, OR (US); **Kenneth N. Bates**, Beaverton, OR (US); **William McDonough**, Portland, OR (US); **Albert H. Krause**, Vancouver, WA (US)

**Publication Classification**


(51) **Int. Cl.**  
**A61B 8/14** (2006.01)  
(52) **U.S. Cl.** ..... **600/459**  
(57) **ABSTRACT**

Correspondence Address:  
**Timothy E Siegel Patent Law, PLLC**  
**601 108th Avenue, Suite 1900**  
**Bellevue, WA 98004 (US)**

A finger-mounted ultrasound probe assembly having an ultrasound probe, adapted to be mounted on a finger and a multi-conductor cable, attached to the ultrasound probe. In addition, a forearm unit is connected to the multi-conductor cable and includes a physical connector to bind the forearm unit to a user's forearm. Also, the ultrasound probe and the forearm unit are adapted to cooperatively engage so that the ultrasound probe may be engaged to and retained by the forearm unit, to stow the ultrasound probe when not in immediate use.

(21) Appl. No.: **11/895,613**

(22) Filed: **Aug. 24, 2007**

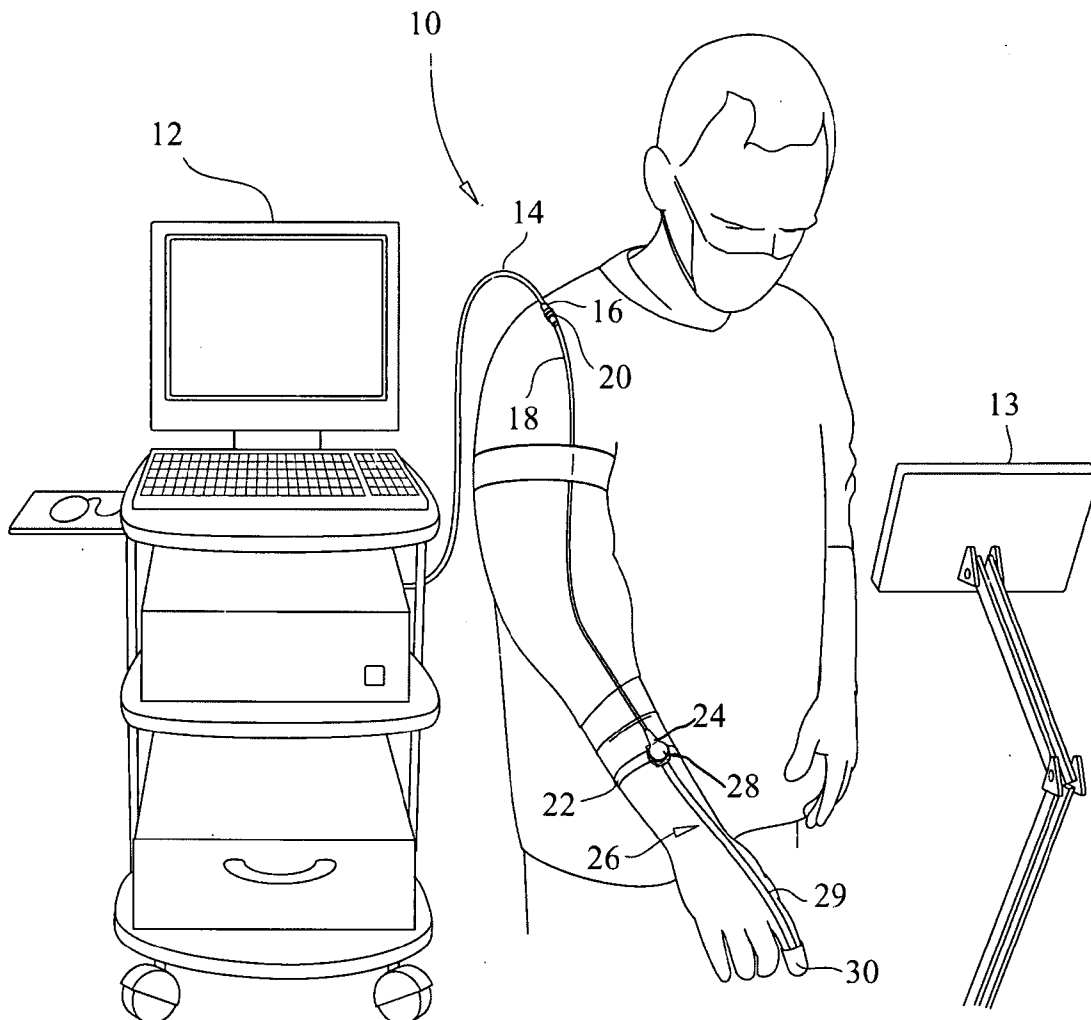



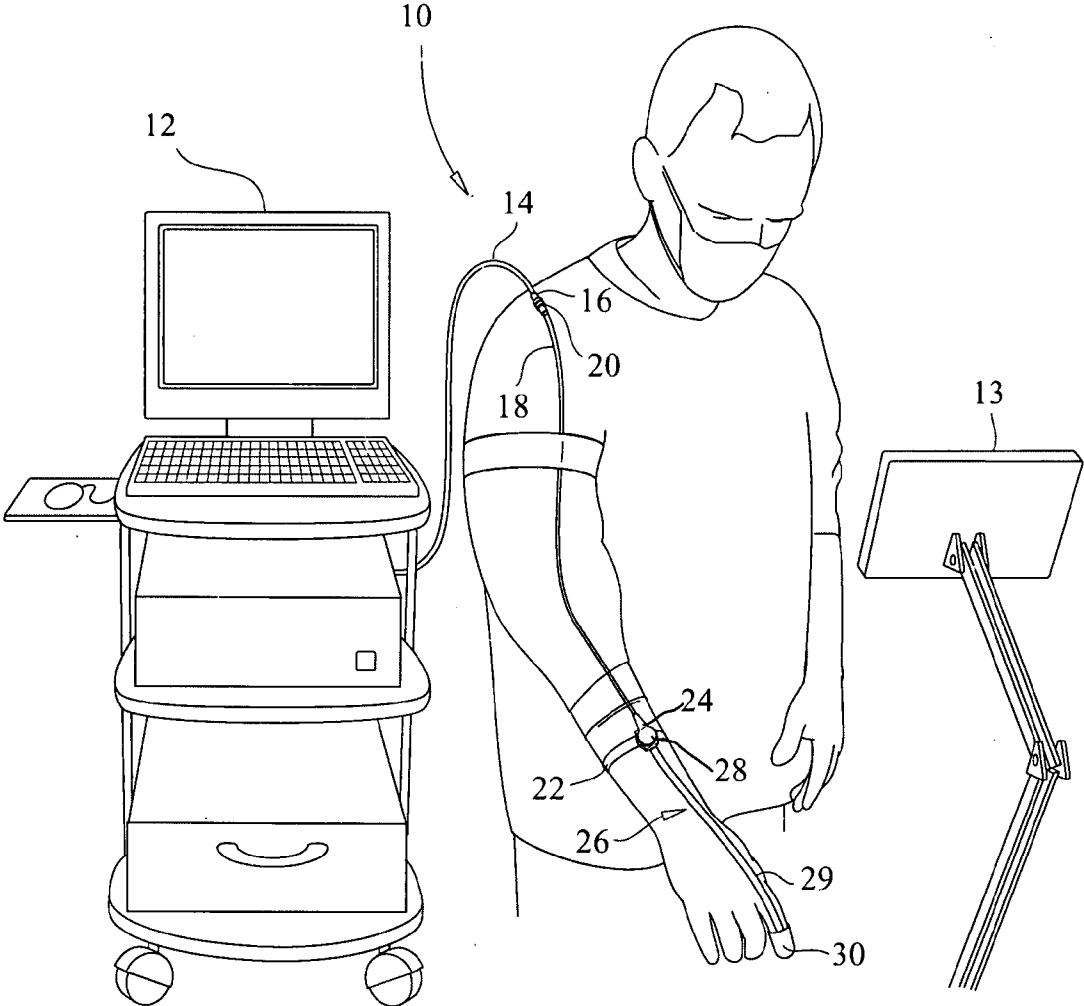



Fig. 1

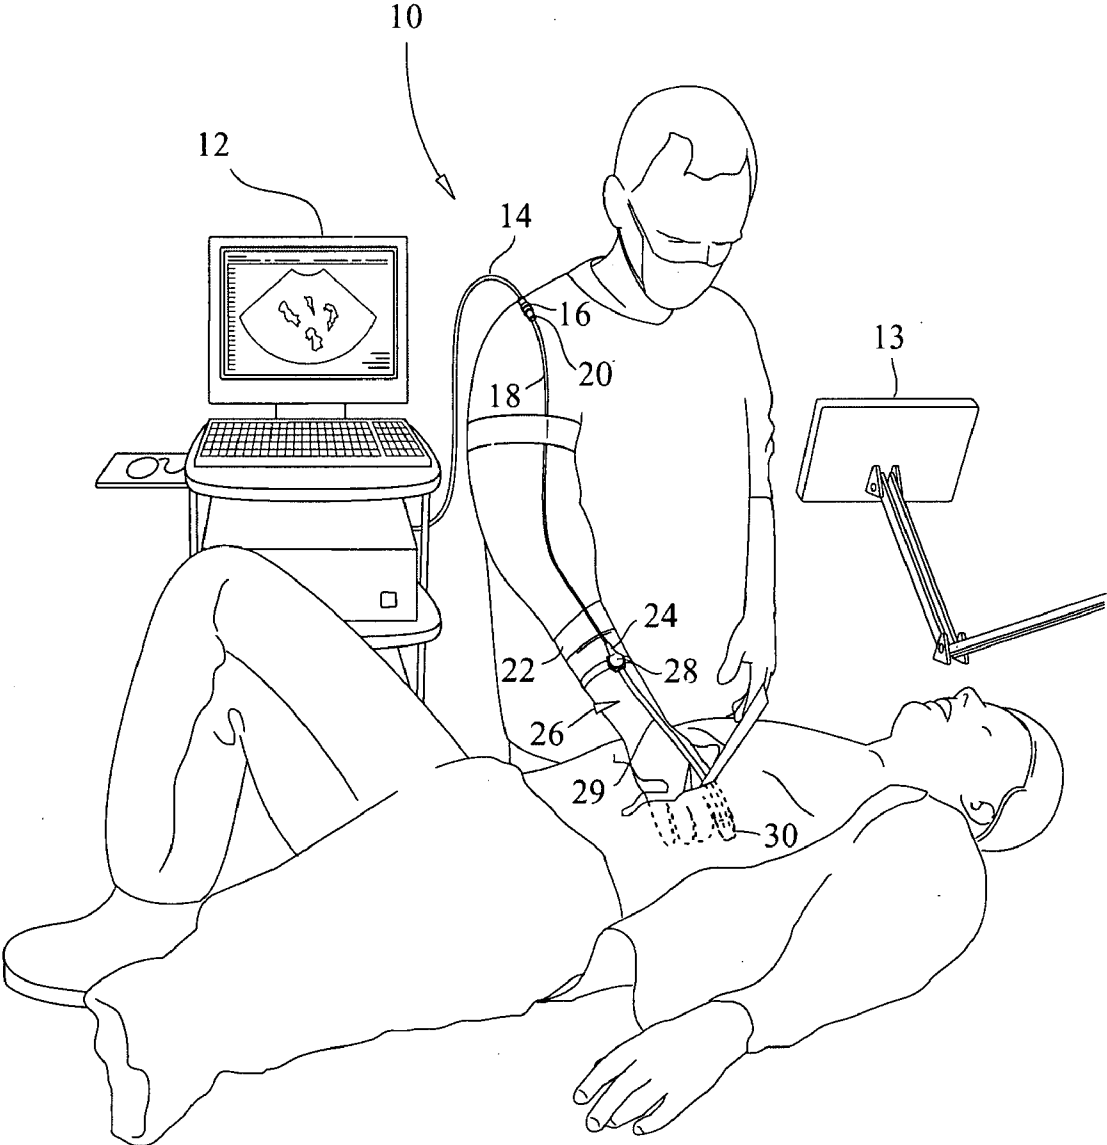

**Fig. 2**

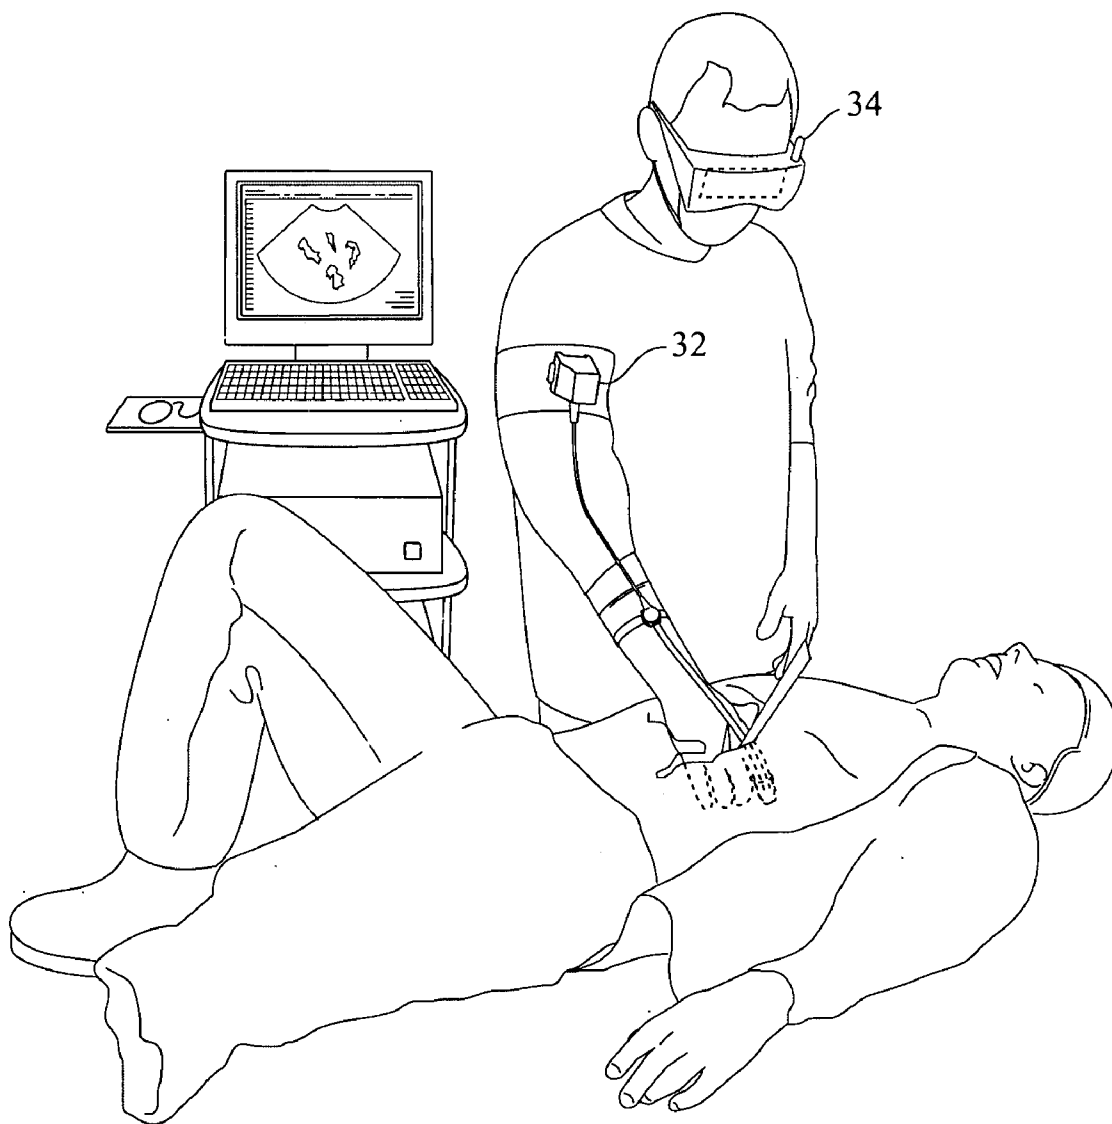

**Fig. 3**

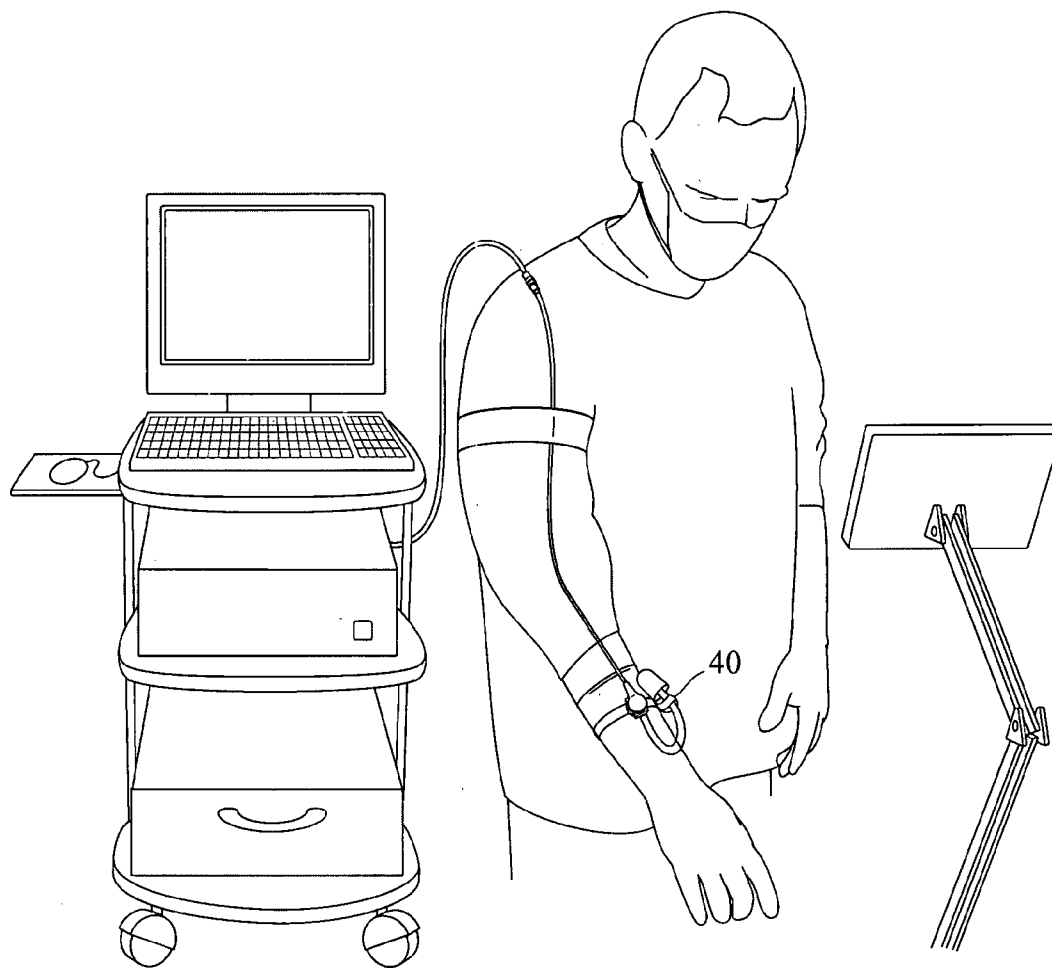

**Fig. 4**

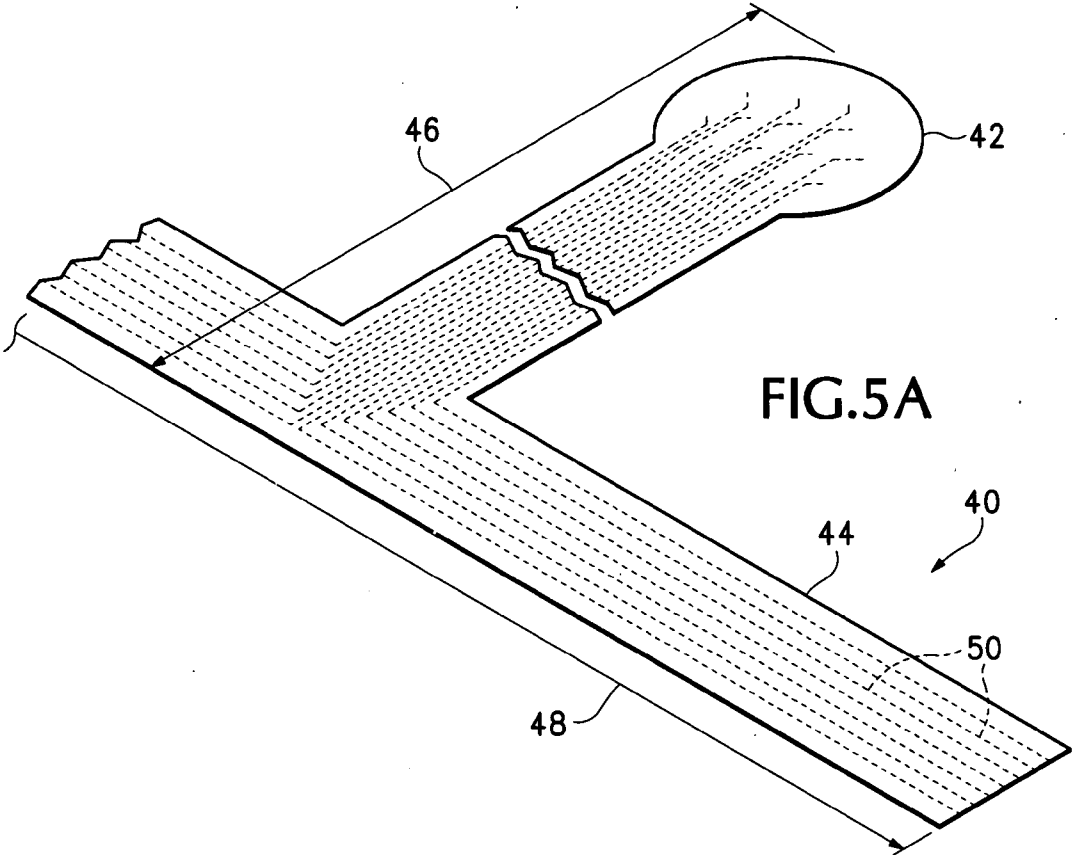


FIG. 5A

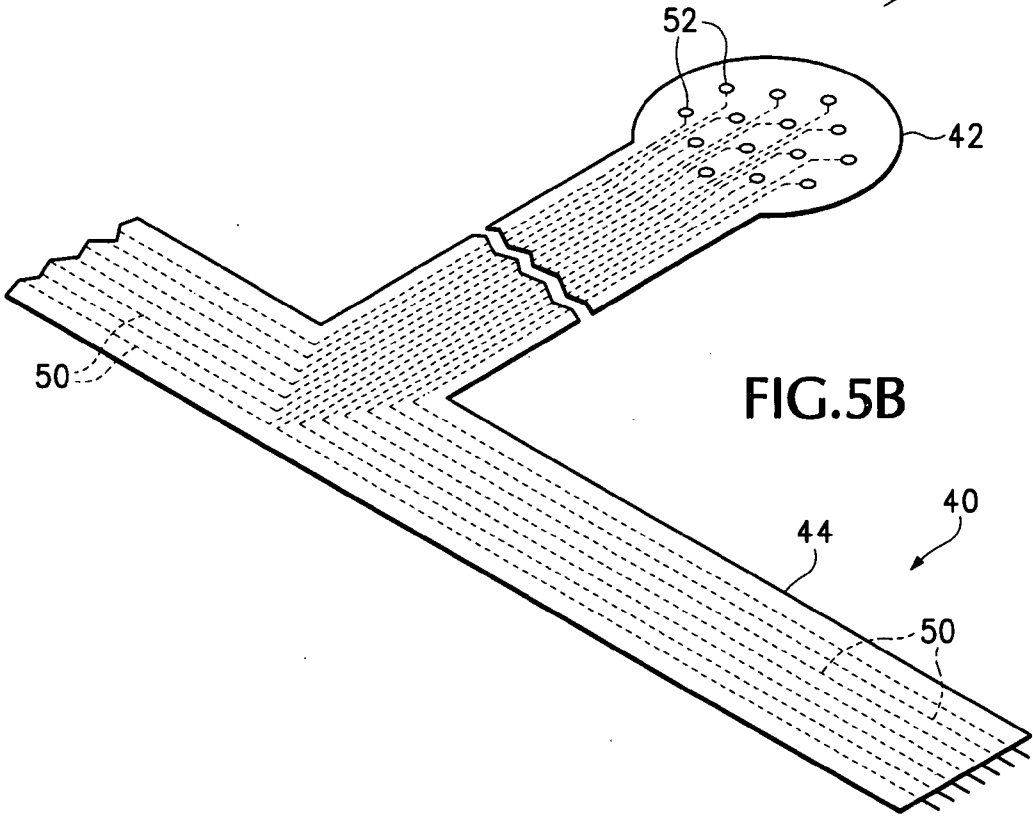
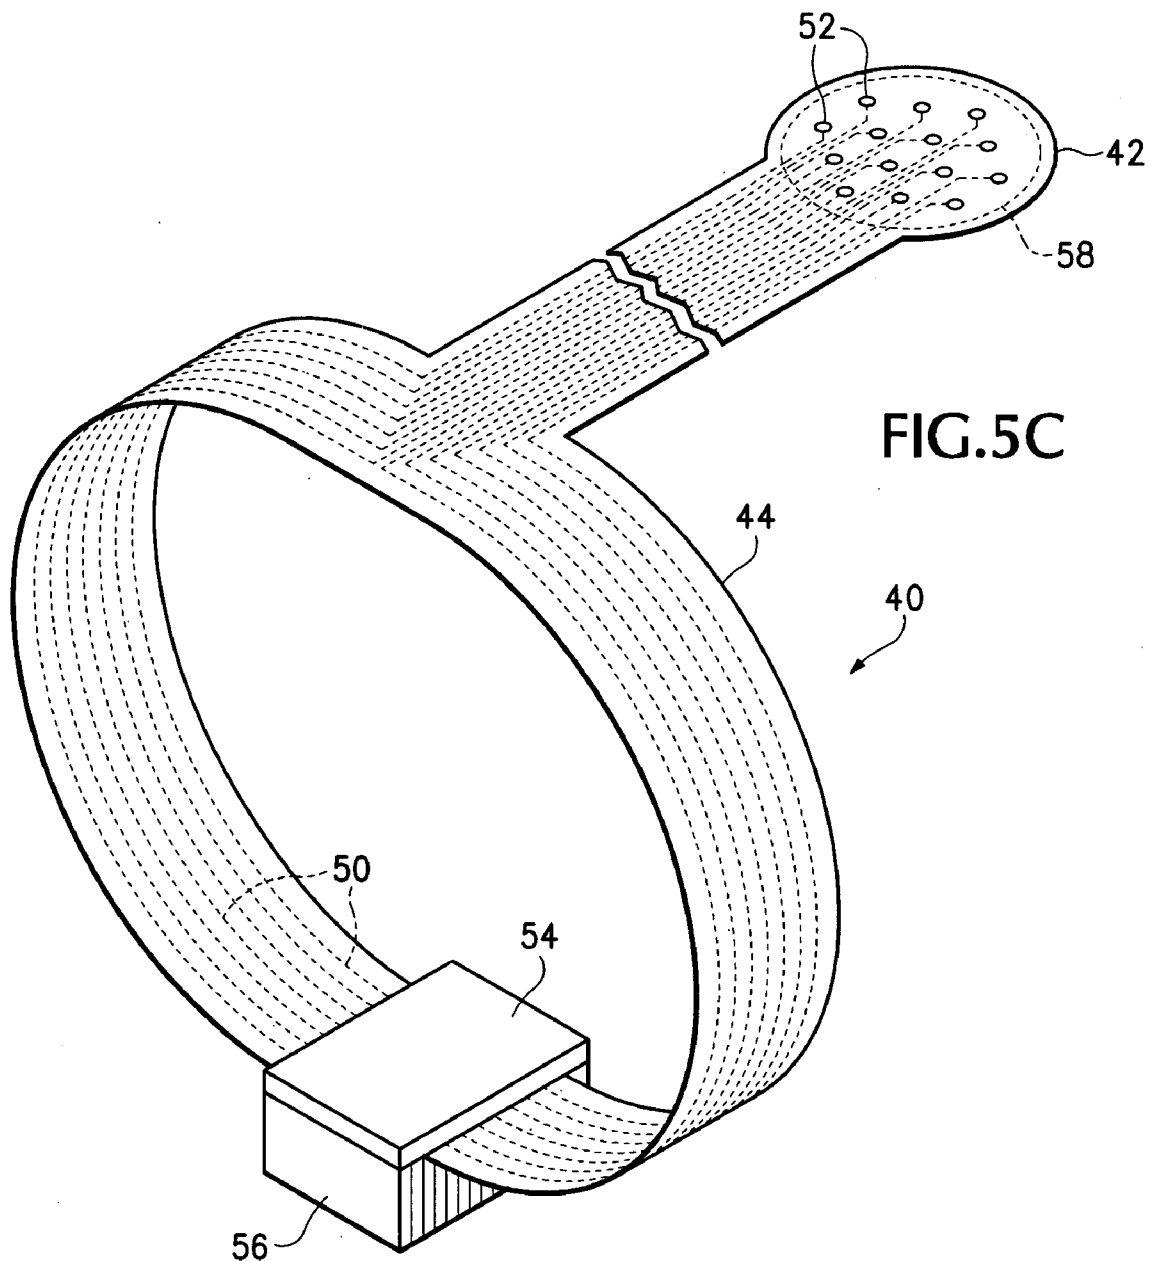


FIG. 5B



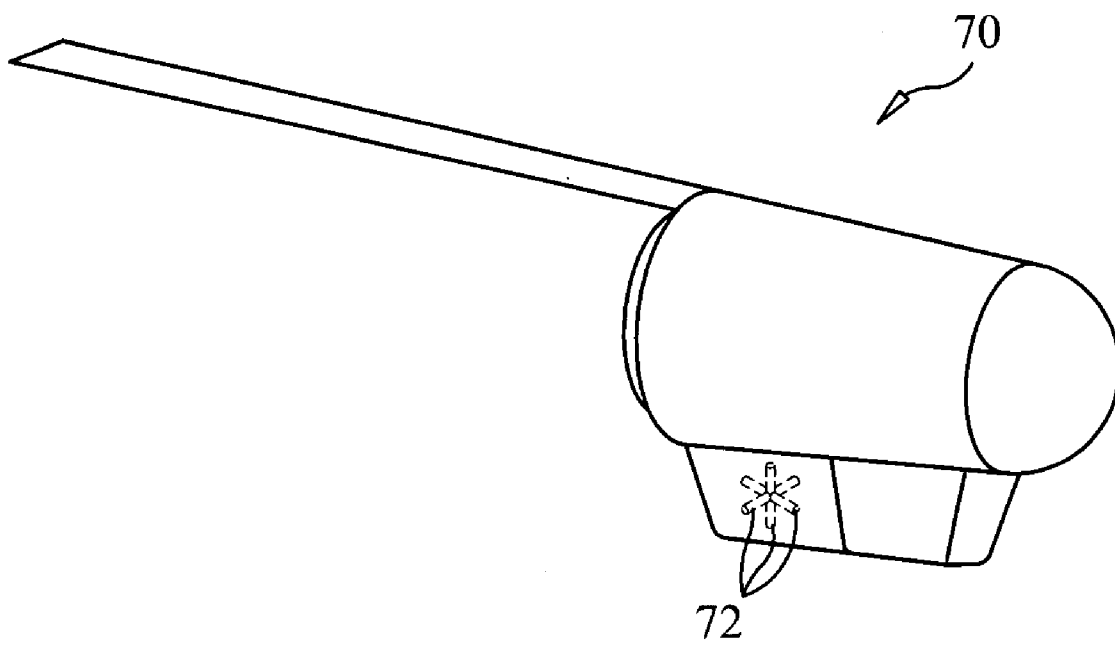
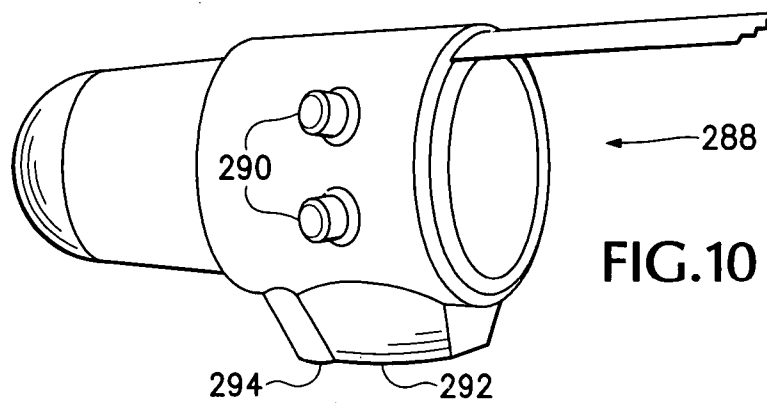
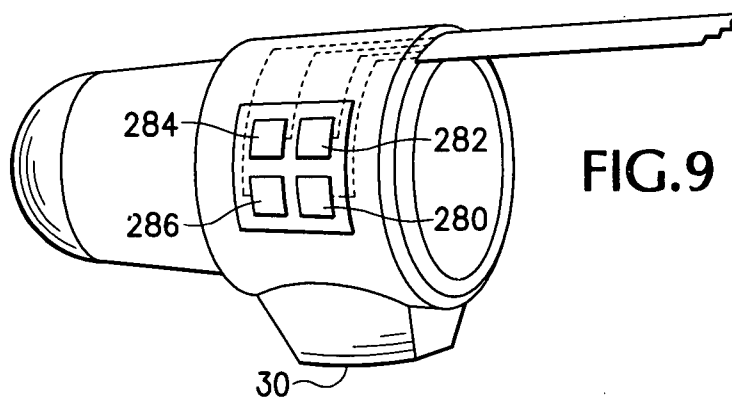
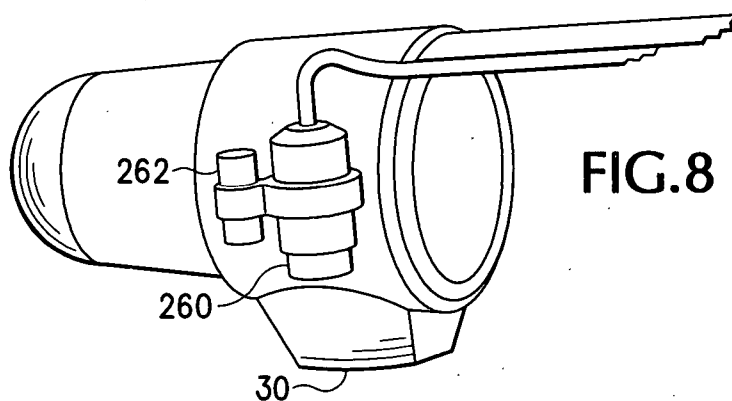
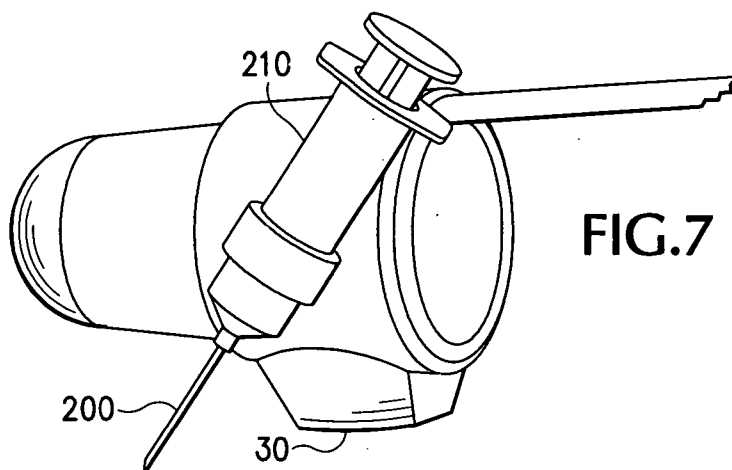


FIG. 6





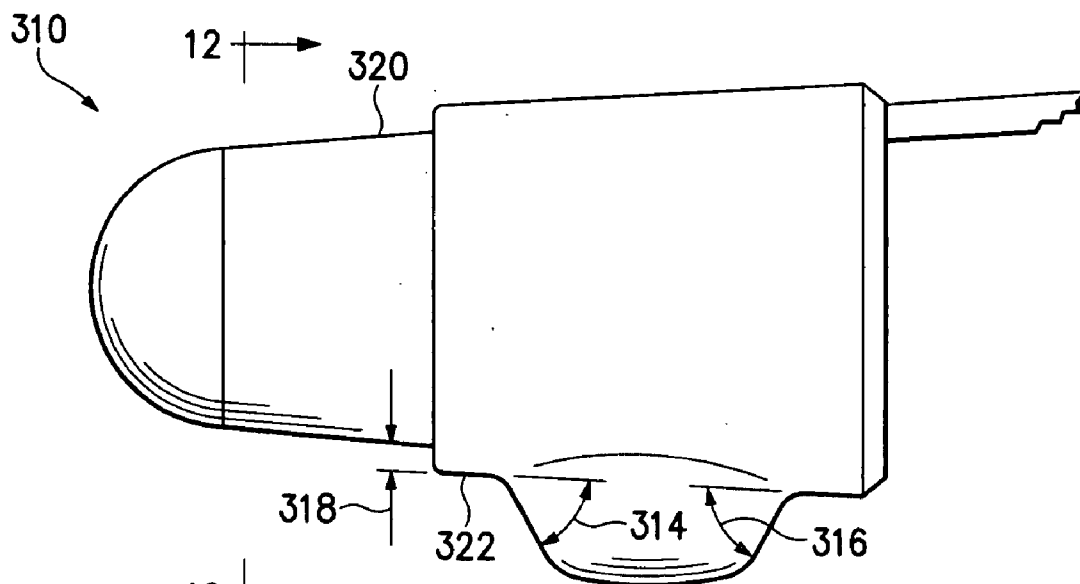


FIG. 11

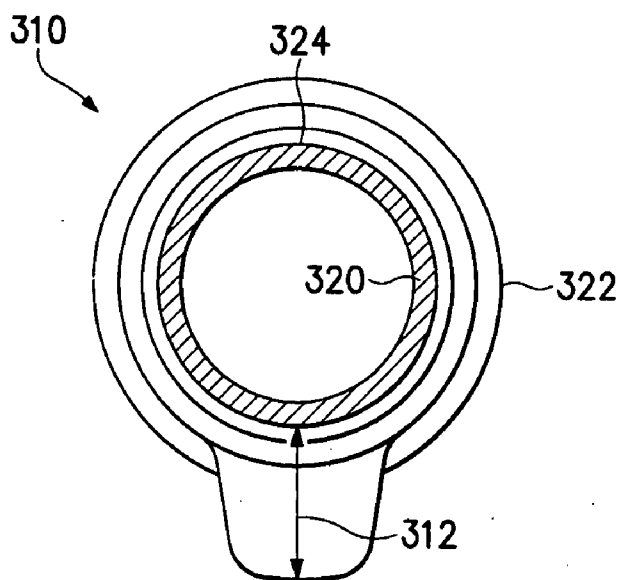


FIG. 12

**CABLE AND CONNECTOR SYSTEM FOR AN  
ULTRASOUND PROBE**

**RELATED APPLICATIONS**

[0001] This application claims priority from application Ser. No. 60/923,323 filed Apr. 13, 2007, from application Ser. No. 60/861,319 filed Nov. 27, 2006 and from application Ser. No. 10/863,644 filed Jun. 8, 2004, all of which are incorporated by reference as if fully set forth herein.

**BACKGROUND OF THE INVENTION**

[0002] During a surgical procedure the timely acquisition of ultrasound imagery can mean the difference between life and death for the patient. Many devices and techniques have been developed or suggested to facilitate the speedy acquisition of ultrasound data, including laparoscopic ultrasound probes, finger mounted probes and hand-held probes having the ability to wirelessly transmit image data. Unfortunately, a number of problems continue to hamper medical personnel in the use of these devices.

[0003] For a hand held probe, users must take an extra mental step to remember and account for the distance between the position of the sensor head and the position of the user's hand. Frequently, the user is required to perform many mental tasks simultaneously, such as reviewing imagery; manipulating the probe to effect delicate changes in the probe pressure and angle; and accessing a bank of medical knowledge in an effort to diagnose a medical problem. During the stress of a medical procedure the task of mentally calculating the probe position and orientation, based on knowledge of the probe geometry, is an extra task that taxes the already highly-taxed mental resources of the medical professional. In addition, the extra displacement of the hand from the target probe head position reduces the ability to utilize muscle memory for probe positioning.

[0004] Another problem is the disassociation, both in time and location, of the tactile input that a medical professional receives from his fingers, during a procedure, and the ultrasound imagery data. For example, for situations in which a medical procedure must be interrupted for imaging to occur, it may be quite difficult for the surgeon to match the tactile information that he notes with the imagery previously acquired. In diagnostic procedures, it may be impossible for the medical professional to gain both tactile information and image information simultaneously. The task of remembering and piecing together the two types of data presents an additional challenge to the medical professional.

[0005] Yet another problem encountered by users of currently available probes is the difficulty in fitting a probe into a small area. The human body is largely composed of delicate tissue, and the object of the medical professional is often to address a localized medical problem while disturbing surrounding or intervening tissue as little as possible. For example, one type of desired imagery that is currently very difficult to acquire is imagery from the posterior of the heart. Hand held probes and/or probes having a large cross-section present a particular difficulty when it is desirable to move the probe head through body tissue in order to obtain imagery of interest.

[0006] Still another issue presented by currently available probes is the awkwardness of use, as the probe is typically tethered by a multi-conductor coaxial cable that is one to three meters long, to an imaging station. It is typically difficult to

twist this cable, so rotating the probe about its longitudinal axis may prove difficult. In addition, the heavy weight of the cable and need to grip the probe handle have the potential to create repetitive motion injuries to sonographers and physicians who use the ultrasound probe.

[0007] Moreover, many of the tools available for imaging the internal regions of the human body may be unavailable in a particular case, due to special conditions. For example, although trans-esophageal imaging is an extremely valuable tool for cardiac surgeons, there are instances in which the esophagus is diseased, making it potentially harmful to insert a probe into the esophagus. In these situations, having some other method of imaging would be invaluable.

[0008] A problem faced specifically by cardiothoracic surgeons is that of assessing plaque deposits in a portion of the aortal arch and ascending aorta prior to accessing the portion of the aorta. If there are plaque deposits in the part of the aorta accessed, the deposit or a portion of it may break off, travel through the blood stream and lodge in a blood vessel, causing great damage to tissue that is dependent on the vessel for its blood supply. Although Doppler ultrasound probes are currently used for the assessment of plaque deposits in the aortal arch and ascending aorta, currently available intra-operative probes are about 10 cm long and rigid, for accessing interior portions of the body. Although this is potentially useful in some situations, it greatly complicates the task of successfully placing the probe for imaging a blood vessel and as in so many other intra-operative situations, permitting the user to maintain a correct sense for the orientation and position of the probe transducer.

[0009] Another issue faced by cardiothoracic surgeons is that of finding coronary arteries in a difficult-to-assess patient. Although in many patients the coronary arteries run close to or on the surface of the heart, in perhaps 10% of patients one or more coronary arteries are buried in cardiac tissue. This can create a serious problem for a cardiothoracic surgeon attempting to perform a bypass operation, in finding the correct artery. In a few unfortunate cases, an artery has been misidentified, leading to negative surgical results.

[0010] Moreover, the current configuration consisting of a permanently attached probe connected to a cable presents sterility issues. The cable typically could be autoclaved, but the sensor is too delicate. The entire sensor and cable assembly, however, is rather bulky for fitting into a bath of disinfecting liquid and the connector is typically not designed to be immersed in disinfectant. As a result, achieving satisfactory sterility of the probe and cable assembly can present a challenge to hospital personnel.

[0011] Moreover, changing the command to the sensor head, for example increasing or decreasing power, or changing the field of view of the scan or the frequency transmitted for typical current systems requires an adjustment at the imaging station, which is awkward for a medical professional in the middle of a procedure.

[0012] Although finger-mounted probes are currently known, they are typically either bulky and inflexible or they do not form precise imagery.

**SUMMARY**

[0013] The following embodiments and aspects thereof are described and illustrated in conjunction with systems, tools and methods which are meant to be exemplary and illustrative, not limiting in scope. In various embodiments, one or

more of the above-described problems have been reduced or eliminated, while other embodiments are directed to other improvements.

[0014] In a first separate aspect, the present invention is a finger-mounted ultrasound probe assembly having an ultrasound probe, adapted to be mounted on a finger and a multi-conductor cable, attached to the ultrasound probe. In addition, a forearm unit is connected to the multi-conductor cable and includes a physical connector to bind the forearm unit to a user's forearm. Also, the ultrasound probe and the forearm unit are adapted to cooperatively engage so that the ultrasound probe may be engaged to and retained by the forearm unit, to stow the ultrasound probe when not in immediate use.

[0015] In a second separate aspect, the present invention is a method of use of an image sensor assembly that includes an imaging station assembly, including an imaging station and a station multi-conductor cable assembly connected to the imaging station and terminating in a station-side probe connector-half. Also, a probe assembly has an image-sensor probe and a probe multi-conductor cable assembly, terminating on a first end in a probe-side probe connector-half adapted to mate to the station-side probe connector-half. In the method, the station multi-conductor cable assembly is connected to a forearm of the user and the probe-side probe connector-half is connected to the station-side probe connector-half. The probe is then used to examine a subject.

[0016] In a third separate aspect, the present invention is a finger mounted sensor assembly having a finger mounted sensor and an electrical connective assembly, adapted to connect the finger sensor to a display station. Also, a forearm mount unit is adapted to be mounted to a user's forearm and an electrical connective subassembly, extends from the forearm mount to the sensor. The electrical connective subassembly is thinner than 2.5 mm.

[0017] In a fourth separate aspect, the present invention is a finger mounted sensor that includes a piece of flex circuit having a first and second end and being more than 5 cm long from the first end to the second end. An ultrasound transceiver formed on the two centimeters of the piece of flex circuit nearest the first end and connective lines for the ultrasound transceiver are resident in the flex circuit and extend toward the second end.

[0018] In addition to the exemplary aspects and embodiments described above, further aspects and embodiments will become apparent by reference to the drawings and by study of the following detailed descriptions.

BRIEF DESCRIPTION OF THE DRAWINGS

[0019] FIG. 1 is a perspective view of a probe assembly according to the present invention, shown in its environment, attached to a medical professional and ready for use.

[0020] FIG. 2 is a perspective view of the probe assembly of FIG. 1, in use on a patient.

[0021] FIG. 3 is a perspective view of an alternative embodiment of the assembly of FIG. 1, having a wireless link to an imaging station, in use on a patient.

[0022] FIG. 4 is a perspective view of the assembly of FIG. 1, showing a probe retaining clasp, on the forearm unit, in use.

[0023] FIG. 5A is a perspective view of a work piece representing a first step in a manufacturing process for the finger probe that is part of the assembly of FIG. 1.

[0024] FIG. 5B is a perspective view of a work piece representing a second step in a manufacturing process for the finger probe that is part of the assembly of FIG. 1.

[0025] FIG. 5C is a perspective view of a work piece representing a final step in a manufacturing process for the finger probe that is part of the assembly of FIG. 1.

[0026] FIG. 6 is a side view of the finger probe of FIG. 1, showing navigational elements.

[0027] FIG. 7 is a perspective view of an alternative embodiment of the probe of FIG. 1, having a hypodermic needle attached.

[0028] FIG. 8 is a perspective view of an alternative embodiment of the probe of FIG. 1, having an electric camera attached.

[0029] FIG. 9 is a perspective view of an alternative embodiment of the probe of FIG. 1, having a set of sensors attached.

[0030] FIG. 10 is a perspective view of an alternative embodiment of the probe of FIG. 1, having a set of controls attached.

[0031] FIG. 11 is a side view of a finger mounted probe, defining an angle of interest.

[0032] FIG. 12 is a front view of the probe of FIG. 11, showing a distance of interest.

DETAILED DISCUSSION OF THE PREFERRED EMBODIMENT

[0033] In a first preferred embodiment, the present invention takes the form of an ultrasound imaging assembly 10. This assembly includes an imaging station 12, which can include an auxiliary display 13, for the user's convenience. Also, a first multi-conductor electrical cable 14 is electrically attached to the imaging station and terminates at a distal connector-half 16. A second multi-conductor cable 18 extends from a shoulder mounted connector half 20, which mates to the distal connector half 16 and terminates at a wrist or forearm band 22 that supports a forearm mounted connector-half 24. A finger probe sub-assembly 26 includes a finger probe sub-assembly connector-half 28 that mates with the forearm mounted connector-half 24. A cable in the form of a ribbon 29 extends from connector-half 28 to a finger-mounted probe 30.

[0034] In use, surgery may begin with the surgeon wearing the wrist band 22, which retains connector-half 24 and cable assembly 18, which includes shoulder mounted connector 20. At this stage it is possible that no finger probe sub-assembly 26 would be attached to cable 18 and that no station cable 14 would be connected to assembly 18, so that the user would be free to move about freely. This would also permit the surgeon full use of his hands while making an initial incision and further initial surgical cutting. When the area of interest in the patient's body has been accessed, the surgeon can take a sub-assembly 26, that has been kept ready for use, attach it to connector-half 24 and also have cable assembly 18 connected to imaging station 12, by way of cable 14 and connector-halves 16 and 20. This technique would destroy the sterility of the performing person's hands, so it is advisable that a person not otherwise participating in the surgery connect cable 18 to cable 14. Alternatively, a person having sterile hands could briefly don sterile gloves to effect the connection and then doff the gloves after finishing. In yet another possibility, the cable 14 is equipped with a sheath, which can be broken away and which is sterile underneath.

[0035] The surgeon can then introduce his hand, with the probe 30 attached, into the patient in order to gather imagery, as shown in FIG. 2. After the imagery is gathered, yielding an enhanced knowledge of the problem being addressed, sub-

assembly 26 can be removed and detached from connector-half 24, to free the surgeon to continue his procedure. Later on, when further imagery is required, either the same sub-assembly 26 may be reattached or another sub-assembly 26, maintained in sterility can be attached to perform the further imaging. In a preferred embodiment, various probe configurations are kept at the ready, to provide the surgeon with a variety of image gathering options. This set of probes could vary in transmit frequency also, so that a first probe permits detailed imaging of fine structures, by using a relatively high frequency (@10-20 MHz), and a second lower resolution probe permits imaging of deeper structures using a lower ultrasound frequency (@2-10 MHz). Probes of various shapes and architectures are also made available to permit varying field of views. For example a curved linear array with relatively small radius of curvature permits imaging in the near field of the probe over a wide field of view. A phased array transducer permits imaging over a wide field of view at some distance from the array, while allowing imaging through a narrow access. A linear array permits imaging over a narrower field of view but provides good imaging of structures near the surface of the array. This is frequently the type of imagery that is highly desirable in surgical situations.

**[0036]** The use of a linear array in a finger mounted probe can be particularly advantageous. The probe can be configured so that the linear array images a scan plane that is parallel to the length dimension of the finger, or in another configuration, transverse to the finger. For the parallel configuration a portion of the scan looks forward from the finger, so that if the user directs his finger to point at the body surface, the probe will image a scan plane into the body. The user can then rotate the image plane by twisting his wrist, something that is quite easy for most users to do. In the case of a curved linear array, the curved surface permits a user to rock the probe on the body or organ surface in order to view tissue over a variety of contact angles. This is particularly easy to do using a finger mounted probe, as the index finger has a good freedom of movement in several axes. The transverse mounted probe has the advantage that it permits a physician to begin his examination with his hand transverse to the length of the patient's torso, which is a more natural position than parallel to the length of the patient's torso. A straight linear array or a phased array, however, has the advantage that the probe head profile can potentially be minimized, which is very important in accessing body portions.

**[0037]** The probe assembly 10 is also very useful in non-surgical procedures, for example, examination of a patient by imaging through the body surface, at the same time the physician is gathering tactile information. For example, the physician may wish to examine a bump or discolored area on the patient's skin and could by use of assembly 10 gather imagery at the same time he touches the abnormal area to diagnose the nature of the problem. Additionally, the user can make a fuller use of his muscle memory and positional awareness to return the probe head to the same location used in a recent probe use.

**[0038]** Probe assembly 10 is also used for exploration of body cavities, such as the vagina, rectum or mouth. Again, the user could both gain tactile information about an organ, such as the prostate gland at the same time he is gaining image information.

**[0039]** A physician may use assembly 10 to view difficult-to-access areas within the body, during surgery.

**[0040]** For example during open heart surgery, the surgeon could move the probe 30 around to the posterior of the heart

to gain imagery of heart features, such as valves that are difficult to otherwise image. This would be extremely difficult with a rigid probe that is poorly shaped for moving through tissue. A probe without advantageous physical characteristics could easily damage a patient during this type of use.

**[0041]** Referring to FIG. 2, in an additional example, assembly 10 can be used in an army field hospital to assist a surgeon in the task of removing shrapnel from a wounded soldier. Although an initial evaluation of the shrapnel locations could be made by an assessment of the entry wounds and pre-surgical imaging, a great deal might still not be known about the specific locations and dimensions of the individual pieces of shrapnel. After making an initial incision near an entry wound, the surgeon attaches a sub-assembly 26 to connector-half 24 and introduces the finger mounted probe 30 into the incision, to gain a further indication of the shrapnel positions. After gaining this information, the surgeon can quickly remove sub-assembly 26, so that he can have the full use of both hands in the task of removing pieces of shrapnel identified by the imaging. Later on during the same surgery, the surgeon may wish to take further images and may reattach sub-assembly 26, or some other sub-assembly 26, either for the sake of sterility or for the sake of having different imaging characteristics.

**[0042]** In another possible application, the low profile of probe 30 lends itself to imaging a premature infant in a neonatal incubator, by reaching through the small entry orifice of the incubator. This action is difficult to do with currently available ultrasound probes.

**[0043]** The system described above, having cables 14, 18 and probe sub-assembly 26 has advantages both in providing a broad range of connectivity and in easing the task of maintaining a sterile operating theater. In a preferred embodiment, cable 18 may be sterilized in an autoclave without being damaged. Cable 14 is typically far enough removed from the sterile area so that it can be wiped down with disinfectant between instances of use. Probe sub-assembly 26 can be submerged in disinfectant fluid for sterilization. In an alternative embodiment, cable 18 is protected by a sterile sheath, which can be removed when a physician, who is wearing cable 18, needs to move to a different imaging station 12 and use a different probe assembly 26. In another alternative, probe assembly 26 is elongated, so that cable 18 does not have to extend as far toward probe 30, thereby making it more likely for cable 18 to avoid contamination from body fluids.

**[0044]** Also, cable 18 may be a universal unit, fitting to a broad range of probe makes, by having a super-set of pins, not all of which are used for any particular sub-assembly 26. An adapter is provided that would be interposed between cable 18 and imaging station 12, either where cable 18 connects to cable 14, where cable 14 connects to station 12, or as part of cable 14. A different adapter is necessary for each make of imaging station 12. It should be noted that this feature of system 10 can be used to increase the usability for ultrasound probes that are not finger probes.

**[0045]** Referring to FIG. 3, in an alternative preferred embodiment a wireless link is established between sub-assembly 26 and imaging station 12. A data processing and transmission unit 32 receives the signals from probe 30 and extracts the imagery, thereby greatly reducing the volume of data to be transmitted. The imagery is transmitted, typically by RF, to imaging station 12 and/or to heads-up display goggles 34, which superimpose the imagery on the user's

field-of-view. In an alternative preferred embodiment unit **32** is located directly on the wrist band **22**. Referring to FIG. **4**, in a preferred embodiment a catch **40** is provided on wrist band **22**, for the purpose of retaining probe **30**, so that it can be folded back, out of the way of the user's hand, when not in use. In an alternative preferred embodiment, catch **40** is implemented by a system of magnets, with mutually attractive magnets on wrist band **22** and probe **30**. Probe sub-assembly **26** is made of light weight materials and has a mass of less than 70 grams. The distal 3 cm of probe **30**, which includes the ultrasound transceiver, has a mass of about 11 grams. This low mass is very important in enabling a user to easily maneuver the probe **30**.

[0046] Applicant notes, in connection with the immediately following discussion, that flex-circuit is a term of art in the electric device industry, referencing a connective element made of a sheet of polymeric dielectric material having conductive traces formed on it by photolithographic techniques. It may be sealed with an additional sheet of polymeric material, so that the conductive traces are interposed and sealed between the two sheets. Referring to FIGS. **5A-5C**, in one preferred embodiment construction of sub-assembly **26** begins with the creation of a T-shaped piece of flex circuit **40**. In an alternative preferred embodiment, two L-shaped pieces are placed side-to-side to form a T-shape. The length **46** between a proximal end **42** and a distal end **43**, of flex circuit **40** is 25 cm. The length **48** of the T-shape top bar at distal end **43** is 2.5 cm. The distal end T-shape top bar is made of a first branch **44** and a second branch **45**. Conductive traces **50**, each turn at the T-junction and extend almost the entire extent from proximal end **42** to the end of either branch **44** or **45**.

[0047] A set of bare trace ends **53** are formed at the free ends of branches **44** and **45** by removing the end of the plastic of flex circuit **40** from about traces **50**, typically by laser ablation. An ultrasound transceiver is formed by connecting the trace ends **53**, to a piece of piezoelectric material **56**. After attachment, a high performance acoustically absorptive backing material **54** is affixed behind piezoelectric material **56**, so that trace ends **53** are encapsulated between backing material **54** and piezoelectric material **56**. Backing material **54** may be as disclosed in U.S. Pat. No. 4,779,244, issued Oct. 18, 1988, which is incorporated by reference as if fully set forth herein. In this patent a backing material having an acoustic absorbance equal to or greater than 60 db/cm/MHz is disclosed. Using such a material and given the need to attenuate a typical 5 MHz ultrasound signal emitted from the back of the array by approximately 150 dB through a two-way trip through the material (so as not to interfere with the image), the array backing would be approximately  $X_{cm} = 150 / (60 \text{ db/cm/MHz} * 2 * 5 \text{ MHz}) = 2.5 \text{ mm}$ , which provides a very low profile for a transducer to fit on the finger.

[0048] In instances where a high absorptive backing material is not available, such as for a pre-existing probe retrofit, such a probe could be modified by creating a toothed pattern, such as that found on the sides of an anechoic chamber, in the surface of the backing material that faces away from the ultrasound array. This causes the sound waves reflecting off the rear of the ultrasound array stack to scatter.

[0049] The piezoelectric material **56** is then patterned as shown, with each resultant element created by this patterning being connected to a unique trace **53**. In a preferred embodiment, even ultrasound elements are connected to branch **44**, while the interposed odd elements are connected to branch **45**, or vice versa. Skilled persons will appreciate that the

alternative method of construction noted above, in which two L-shaped pieces of flex circuit are used, rather than a single T-shaped piece, permits the step of connecting bare traces **53** to materials **54** and **56** to be performed with the two L-shaped pieces of flex circuit laying flat, thereby greatly easing this connective task. The two L-shaped pieces may then be curled up and joined at the top, thereby forming an annulus that fits about the finger.

[0050] Referring to FIG. **5C**, the branches **44** and **45** are curved downwardly to fit about a finger, so that ultrasound array **56** now faces downwardly and is oriented to sweep from forward and backward relative to the finger. A housing is added about the ring that is formed by branches **44** and **45** and materials **54** and **56**, to arrive at a final probe **30**, such as is shown in FIGS. **7-10**. A protective coating may be added to the medial portion of flex circuit **40**. Referring to FIGS. **11** and **12**, a probe **30** constructed according to the preferred methods described herein may have a distance **312** from the interior surface **324** of the finger mount to the furthest protrusion of the probe of about 1.2 cm, greatly facilitating a user in passing the probe **310** through tight passages in the body. In another embodiment distance **312** equals about 1.5 cm.

[0051] Moreover probe **30** is made in a preferred embodiment so that the ultrasound transceiver protrudes gradually outwardly (downwardly) from front to middle. Defining an angle **314**, as the angle between a probe surface that extends parallel to the user's finger and the surface of the probe as it begins to protrude outwardly, angle **314** is about 70° at its maximum. In an alternative preferred embodiment, angle **314** is about 60° at its maximum and in yet another preferred embodiment, this angle is about 50° at its maximum. In yet another preferred embodiment, angle **314** is about 40°. An additional angle **316** may be defined as the angle between a probe surface that extends parallel to the user's finger and the surface of the probe as it begins to extend outwardly, going from rear to front. It is also desirable to minimize angle **316**, so that as the probe is being removed back through tissue, it disturbs the tissue as little as possible. In a preferred embodiment this angle is about 40°. In other preferred embodiments this angle ranges from 40° to 70°.

[0052] A finger cot **320** is used to both isolate the front of the finger from tissue, provide a rounded surface at the front of the finger, which can be pushed through tissue with less chance of causing damage, and making it possible for a probe unit **310** having a fixed inner diameter **324** to accommodate a range of finger thicknesses, by providing a range of cots having different thicknesses. It is desirable to minimize the distance **318** between finger cot **320** and probe surface **322**. Although this distance is shown as being on the order of 2 mm, in another preferred embodiment distance **318** is zero, with the finger cot **320** being flush with the probe surface.

[0053] This low profile and gradual protrusion greatly facilitates a probe user in inserting the probe into small body cavities and avoiding damage to delicate tissues. Along these lines it is beneficial to have a "bullet shaped" probe that comes to a point forward of the finger and smoothly expands to the area where the transponder is located. This can be accomplished by equipping the probe with a forward section that terminates distal to the finger tip in a single point and expands transversely outwardly approximately equally and smoothly in each direction, to yield the bullet shape.

[0054] In one preferred embodiment a 128 element probe is constructed and in an alternative preferred embodiment a 256 element probe is constructed. The probe head is completed by

adding a lens and housing. Skilled persons will recognize that although a linear array is shown, a curved linear array could be constructed just as easily, using the techniques shown, simply by curving the piezoelectric material after it is diced. In an alternative preferred method of construction, a separately formed ultrasound transceiver is connected to flex circuit **40** by way of a flex circuit connective tab.

**[0055]** The use of a high absorptive backing material **54**, incorporated into the array, as well as a method of construction that obviates the need for connecting the flex circuit to a cable in the probe head permits the formation of a lower profile probe head. As noted elsewhere in this document, this low profile is critical in permitting a user to locate the probe in tight spaces internal to the human body without damaging body tissue. The benefit of this innovation may be utilized in probes that do not otherwise fit the disclosure of this application. For example, flex circuit **40**, rather than terminating in connector-half **24**, can be terminated at a multi-conductor coaxial cable, of the type that is currently standard in the ultrasound imaging industry, 5 cm or more away from the probe with or without a connector. In the typical current probe design, the multi-conductor coaxial cable terminates quite close to the probe head or in the probe head, causing the finger-mounted portion to be bulky and heavy. By extending the flex circuit portion more than 5 cm from the probe itself, and preferably more than 10 cm or even 20 cm, the finger-mounted portion is kept light and given a low profile. Accordingly, the present invention is not limited to the system connectors that although advantageous do not by themselves yield the low profile of the probe.

**[0056]** In an alternative preferred embodiment a capacitive micro-machined ultrasound transceiver (CMUT) is connected to traces **50**, using the same techniques as used for connecting piezoelectric material **56**. A CMUT transceiver tends to be thermally robust, thereby lending itself to use in a probe that may be exposed to the heat and pressure of an autoclave sterilization cycle, without being damaged.

**[0057]** Referring to FIGS. **5A-5C**, at the proximal end **42** of work piece **40**, a set of electrical contact points **52** are formed by removing the flex circuit plastic down to each trace **50**, in a particular spot. Conductive material is deposited onto contacts **52**, so that they are not recessed. Alternatively, a surface coating material covers flex traces so that only connector contacts **52** are left exposed on the surface of flex forming contacts **52**. Rigid backing material **58** is adhered underneath the flex circuit and a metal housing (not shown) is provided to finished connector-half **22**. Alternatively, the proximal end of the flex circuit can be selectively rigidized by laminating a rigid, circuit board material layer onto the flexible portion, and forming connections to the flex traces by laser or mechanical drilling and subsequent plating, to form a monolithic integrated connector assembly.

**[0058]** Referring to FIG. **6**, in a preferred embodiment a finger probe **70** includes a set of accelerometers (not shown) and/or inductors **72** that are mounted in a mutually orthogonal pattern are provided as part of finger probe **30** to permit location determination while finger probe **30** is within the body and not directly observable.

**[0059]** Referring to FIG. **7** in an additional preferred embodiment, a hypodermic needle **200** and an attached syringe **210** are releasably mounted adjacent finger probe **30**. This permits imagery gathered by finger probe **30** to assist a health care professional in finding a blood vessel of interest. Health care professionals sometime need to find a particular

blood vessel, such as the jugular vein, in order to inject fluid or drugs as soon as possible so that the substance being injected will reach a target organ as quickly as possible. In such application, known as central-line-placement, color flow ultrasound imagery, in which Doppler flow information drives the display of the blood vessels and non-Doppler information drives the display for the surrounding tissue, is particularly useful in this endeavor. In an alternative preferred embodiment, another sort of skin broaching device, such as a cannula (not shown) or a hypodermic needle connected to an intravenous drip bag is associated to the ultrasound probe. Guidance of the hypodermic needle associated with the finger probe may also be assisted by use of commercially available guidance devices, such as a pressure sensor associated with the needle, including that available from Vascular Technologies, Ness-Ziona, Israel, which provide an additional positive indication when the needle enters a vein, through sensing a pressure change.

**[0060]** An additional preferred embodiment is the same as described above except for that an optical link **260** and light source **262** is provided to permit optical viewing of body tissue. In one preferred embodiment the optical link **60** is in the form of a lens coupled to a fiber optic link on probe **30** that may terminate in a video camera. Alternatively optic link **260** is in the form of a video camera (as shown) attached to the finger probe **30** and adapted to communicate electrically with the imaging station **12**, or heads up display **34**. In either situation it is necessary to provide light for the optical link **260**. This is accomplished either by an electrically powered light source, such as a light emitting diode **262**, or a chemically powered light source (not shown), such as those available under the trade name "pin lights," from Embo-Optics of Beverly, Mass.

**[0061]** Referring to FIG. **9**, in another preferred embodiment a finger probe, such as **30**, is equipped with a sensor suite that includes a thermometer **280**, an oximeter **282**, a pressure sensor **284** and a glucometer **286**. In an alternative embodiment element **286** is an agent administration patch **286** that is electrically activated by a trace **50** to express the agent, thereby administering the agent to a precise location. In an alternative preferred embodiment, a smaller set of sensors is provided, or even a single sensor only.

**[0062]** In another preferred embodiment, a finger assembly **130** is provided that can both image tissue, using ultrasound, and that can also provide therapy, typically by cauterizing tissue, also using ultrasound. First there is an assembly **288** that includes both an imaging array **292** and a treatment array **294**. The treatment array uses up to 100 watts of power and is powered by traces that are larger in cross-sectional dimension and are therefore capable of conducting more current in order to meet the greater power demands of treatment array **294**. In an alternative embodiment a smaller number of sensors, or just one sensor, are available.

**[0063]** In another preferred embodiment of an ultrasound assembly (not shown), a single array is used for both imaging and treatment. In one variant of this embodiment, some piezoelectric elements are used for both imaging and treatment and others are used solely for imaging. Again, the array must be powered by a larger input of current and to accommodate this need, larger traces **40** (FIG. **5A**) are provided for the treatment ultrasound elements.

**[0064]** A set of thumb controls **290** are provided for probe **288**, so that the user may switch between imaging and treatment. These controls are typically in the form of a small push

button that must be pressed in a specific pattern, for example two rapid presses followed by continuous pressure during the period of time treatment is desired, in order to activate treatment mode, as any inadvertent activation could greatly harm a patient. In one preferred embodiment a warning signal is given when two rapid presses have placed the treatment probe in a “ready” state, in case some passage through tissue ever causes two rapid presses to occur. In an alternative preferred embodiment controls are placed on the wrist or forearm band 22, thereby providing easy access for a probe user.

[0065] In another preferred embodiment, buttons 290 are provided for a probe, such as probe 30, in which therapeutic ultrasound is not available. The buttons are instrumented to change the scan width and orientation; the transmit power and frequency; and imaging mode among other quantities. The buttons 290 communicate with imaging station 12 by way of traces 50 and cables 18 and 14 or by RF transmission in the embodiment of FIG. 3. The buttons 290 may also communicate or be mechanically associated with the array within the finger probe to allow a change in orientation of the array elements to effect the orientation of the scan plane.

[0066] One use of probe 30 is for the intra-operative evaluation of plaque deposits in the aortal arch and ascending aorta, prior to accessing the aorta. To perform this function a Doppler probe may be used and a measurement of the speed of the blood in the aorta formed. In the case where the aorta has been narrowed due to plaque deposits, the blood flows more rapidly. The accessing of the tissue of the aorta is greatly eased by use of a finger mounted probe, as opposed to the long, stiff intra-operative probes currently available.

[0067] While a number of exemplary aspects and embodiments have been discussed above, those of skill in the art will recognize certain modifications, permutations, additions and sub-combinations thereof. It is therefore intended that the following appended claims and claims hereafter introduced are interpreted to include all such modifications, permutations, additions and sub-combinations as are within their true spirit and scope.

1. A finger-mounted ultrasound probe assembly, comprising:

- a) an ultrasound probe, adapted to be mounted on a finger;
- b) a multi-conductor cable, attached to said ultrasound probe;
- c) a forearm unit, connected to said multi-conductor cable and including a physical connector to bind said forearm unit to a user’s forearm; and
- d) wherein said ultrasound probe and said forearm unit are adapted to cooperatively engage so that said ultrasound probe may be engaged to and retained by said forearm unit, to stow said ultrasound probe when not in immediate use.

2. The assembly of claim 1, wherein a connector releasably joins said multi-conductor cable to said forearm unit.

3. A method of use of an image sensor assembly, by a user, and comprising:

- a) providing an image sensor assembly, comprising:
  - i. an imaging station assembly, including an imaging station and a station multi-conductor cable assembly connected to said imaging station and terminating in a station-side probe connector-half;
  - ii. a probe assembly, having an image-sensor probe and a probe multi-conductor cable assembly, terminating

on a first end in a probe-side probe connector-half adapted to mate to said station-side probe connector-half; and

- b) attaching said station multi-conductor cable assembly to a forearm of said user;
- c) mating said probe-side probe connector-half to said station-side probe connector-half; and
- d) using said probe to examine a subject.

4. The method of claim 3, wherein said step of using said probe to examine a subject, more specifically includes using said probe to examine plaque in the aorta of said subject.

5. The method of claim 3, wherein said step of using said probe to examine a subject, more specifically includes using said probe to locate a cardiac blood vessel that is hidden in tissue.

6. The method of claim 3, further including the step of said user disconnecting said probe-side probe connector-half from said station-side probe connector-half, after using said probe.

7. The method of claim 4, further including the step of reconnecting said station-side probe connector-half to said probe-side probe connector-half after disconnecting from said probe-side probe connector-half.

8. The method of claim 4, further including the steps of providing an additional probe assembly having a probe-side probe connector-half and mating said probe-side probe connector-half of said additional probe assembly to said station-side probe connector-half.

9. The method of claim 3, wherein said station assembly multi-conductor cable assembly is divided into a proximal multi-conductor cable sub-assembly that connects to said station and includes a proximal connector-half; and

a medial multi-conductor cable sub-assembly that includes a medial connector-half, which mates with said proximal connector-half.

10. The method of claim 7, further comprising disconnecting said medial connector-half from said proximal connector-half, thereby leaving said user disconnected from said imaging station.

11. The method of claim 7, further including the step of disconnecting said probe sub-assembly, after using said probe.

12. The method of claim 9, wherein said probe sub-assembly is placed in a sterilizing medium, after it is disconnected.

13. The method of claim 9, further including the step of disconnecting said medial connector-half from said proximal connector-half, after use of said probe.

14. The method of claim 11, further including placing said medial multi-conductor cable sub-assembly into an autoclave and operating said autoclave to sterilize said medial multi-conductor cable sub-assembly.

15. The method of claim 11, further including placing said medial multi-conductor cable sub-assembly into a bath of antiseptic fluid in order to sterilize said medial multi-conductor cable sub-assembly.

16. The method of claim 11, further including the step of connecting said medial multi-conductor cable to a second imaging station and second probe, after disconnecting from said imaging station and probe.

17. The method of claim 14, wherein said medial multi-conductor cable is originally protected by a sterile sheath, which is removed before attaching it to said second imaging station.

18. The method of claim 3, wherein said image sensor is adapted to be mounted on a finger of said user.



19. The method of claim 3, wherein said probe multi-conductor cable assembly is flexible enough to offer no significant resistance to wrist movement by said user.

20. The method of claim 3, wherein said probe multi-conductor cable assembly includes a flex-circuit.

21. The method of claim 3, wherein when said probe-side probe connector-half and said station-side probe connector-half are mated together, they together extend no more than 2 cm outwardly from said arm of said user, to which said second station-side probe connector-half is mounted.

22. The method of claim 3, wherein said imaging station is also a signal processing station that processes raw data from said image sensor assembly to create images.

23. The method of claim 3, wherein said display station is mounted at a location more than 0.7 meters from said second connector-half.

- 24. A finger mounted sensor assembly, comprising:
  - a) a finger mounted sensor;
  - b) an electrical connective assembly, adapted to connect said finger sensor to a display station, and including:
    - i. a forearm mount unit, adapted to be mounted to a user's forearm;
    - ii. an electrical connective subassembly, extending from said forearm mount to said sensor; and
  - c) wherein said electrical connective subassembly is thinner than 2.5 mm.

25. The assembly of claim 22, wherein said electrical conductive assembly has a width of between 2 cm and 10 cm.

26. The assembly of claim 22, wherein said forearm mount unit includes a first connector-half and a second connector-

half mated to said first connector-half and further being affirmatively connected to said electrical connective subassembly, so that said second connector-half can be detached from said first connector-half to disconnect said finger mounted sensor from said display station.

27. The assembly of claim 22, wherein said finger mounted sensor incorporates a piece of flex-circuit and wherein said piece of flex circuit extends more than 5 cm from said finger sensor toward said forearm mount unit.

28. The assembly of claim 22, wherein said forearm mount is electrically and physically connected to said display station by way of an electrical cable.

29. The assembly of claim 26, wherein said display station is mounted on a surface separate from said user's forearm.

30. The assembly of claim 26, wherein said electrical cable is more than 1 meter long.

- 31. A finger mounted sensor, comprising:
  - a) a piece of flex circuit having a first and second end and being more than 5 cm long from said first end to said second end;
  - b) an ultrasound transceiver formed on the two centimeters of said piece of flex circuit nearest said first end; and
  - c) connective lines for said ultrasound transceiver being resident in said flex circuit and extending toward said second end.

32. The finger mounted sensor of claim 29, wherein said piece of flex circuit is 10 cm long.

\* \* \* \* \*