



US 20050022823A1

(19) **United States**

(12) **Patent Application Publication**

Davison et al.

(10) **Pub. No.: US 2005/0022823 A1**

(43) **Pub. Date: Feb. 3, 2005**

(54) **APPARATUS, SYSTEM AND METHOD FOR TREATING DRY EYE CONDITIONS AND PROMOTING HEALTHY EYES**

(52) **U.S. Cl. 128/858**

(76) **Inventors: Suzanne Davison, Pleasanton, CA (US); Roy Paulson, Temecula, CA (US); Fernando Moto, Moreno Valley, CA (US)**

(57) **ABSTRACT**

Correspondence Address:
Steven B. Pokotilow, Esq.
Stroock & Stroock & Lavan LLP
180 Maiden Lane
New York, NY 10038 (US)


An apparatus and system, and methods for using such apparatus and system, is provided for preserving the eye's natural and artificial tears. The apparatus comprises two soft, pliable eyecups, which each include a curved lens and a contoured frame, connected by a soft, pliable bridge. The lenses are maintained within a pliable, and contoured frame that is designed and constructed to encircle the orbital bone of the eye sockets, creating a custom fit and effective seal over each eye. Attached to each frame is a gasket that further seals the apparatus over the eyes and provides additional comfort to the wearer. A contoured strap, which is attached to each frame, maintains the position of the apparatus on the wearer.

(21) **Appl. No.: 10/632,188**

(22) **Filed: Jul. 30, 2003**

Publication Classification

(51) **Int. Cl.⁷ A61F 9/00**

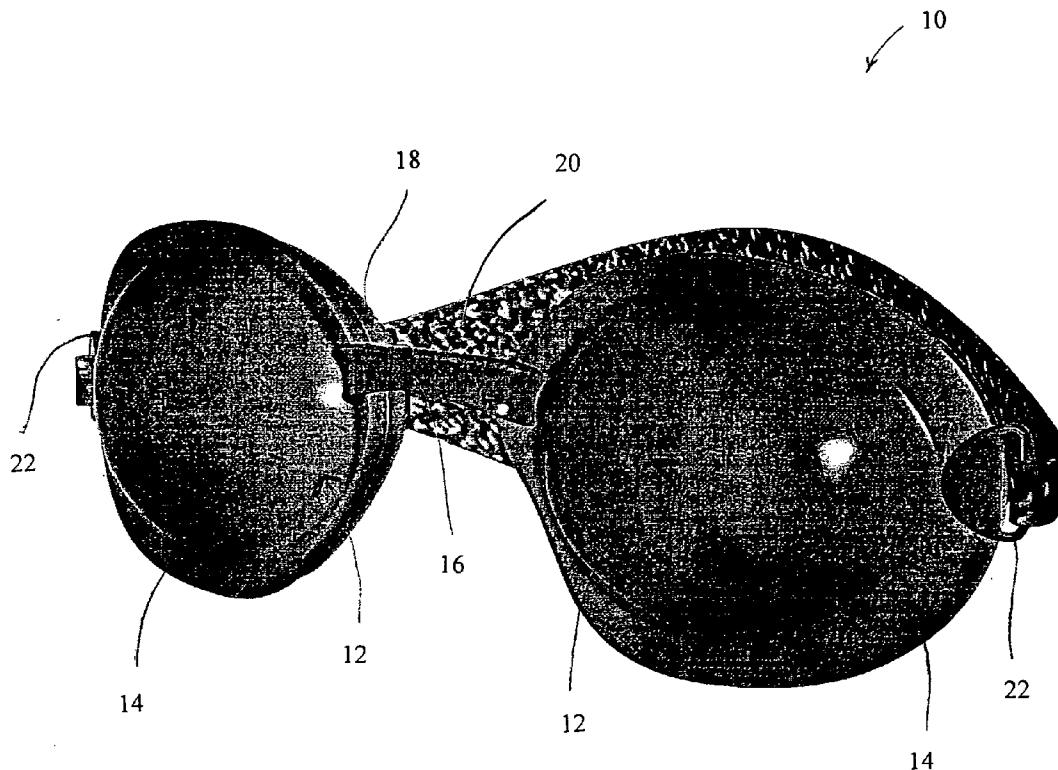

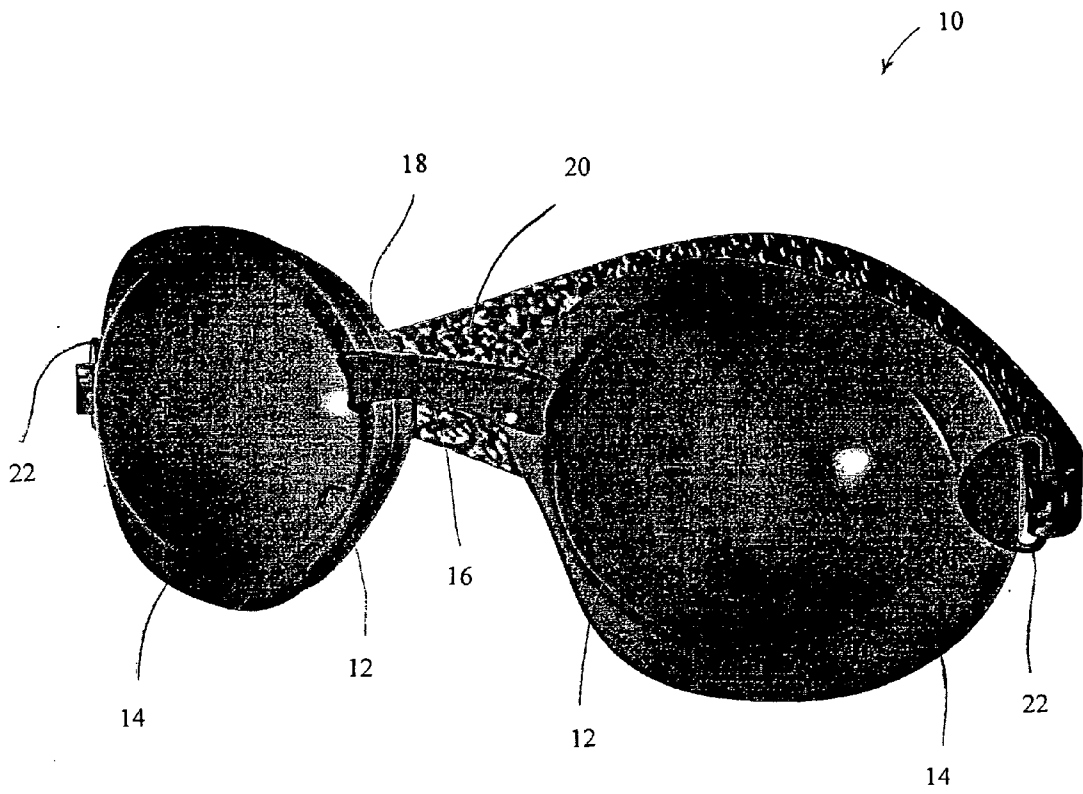


FIG. 1

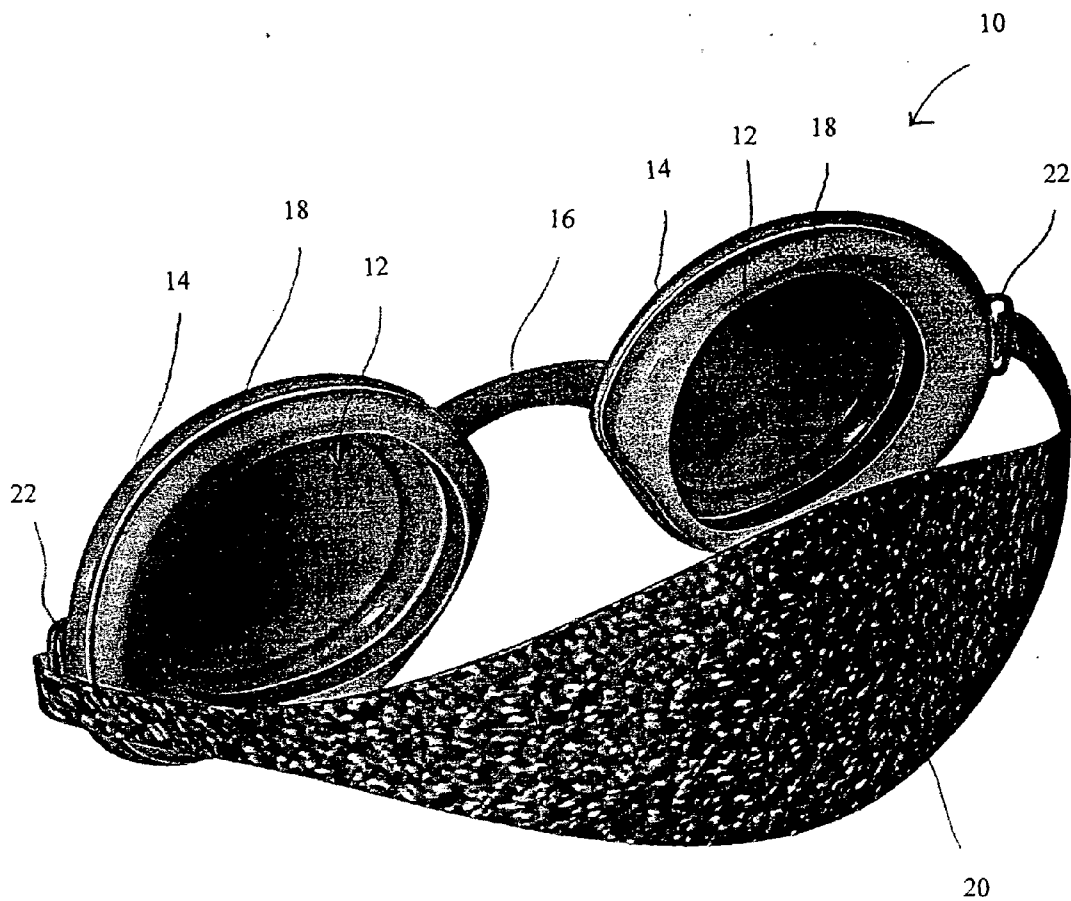


FIG. 2

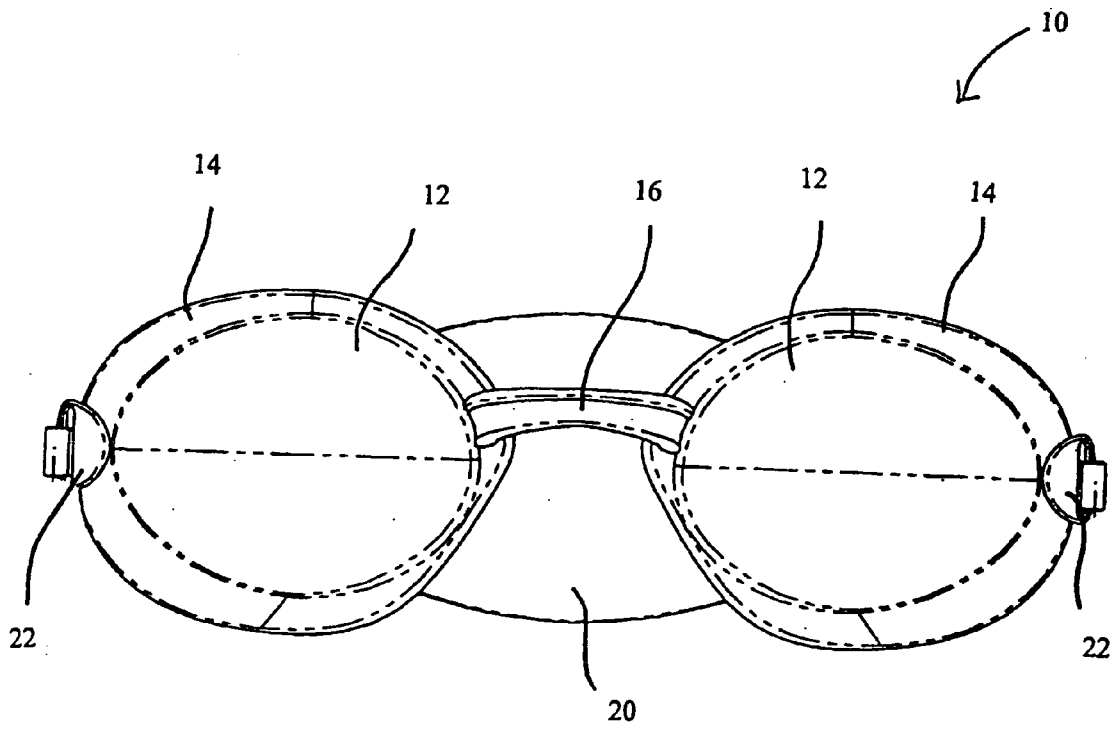


FIG. 3

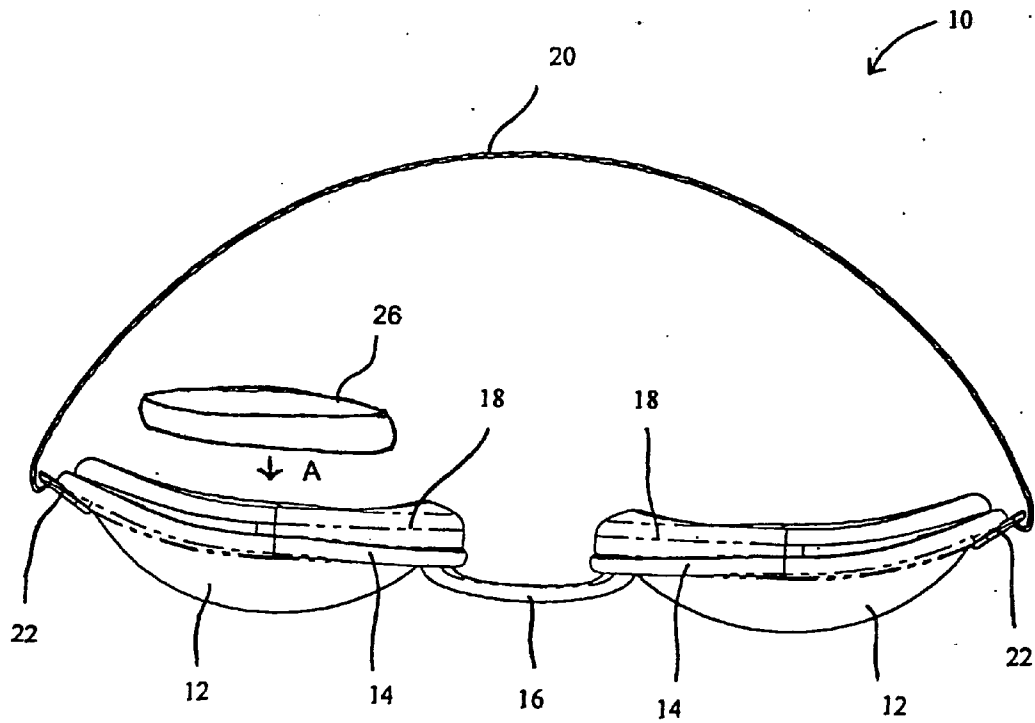


FIG. 4

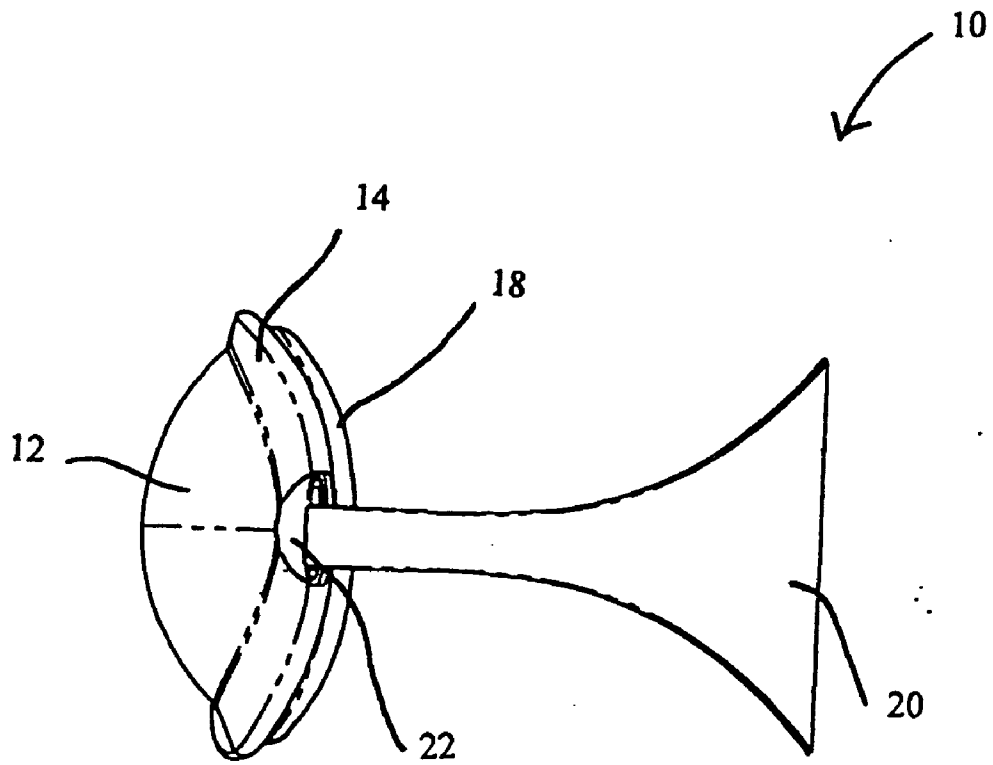


FIG. 5

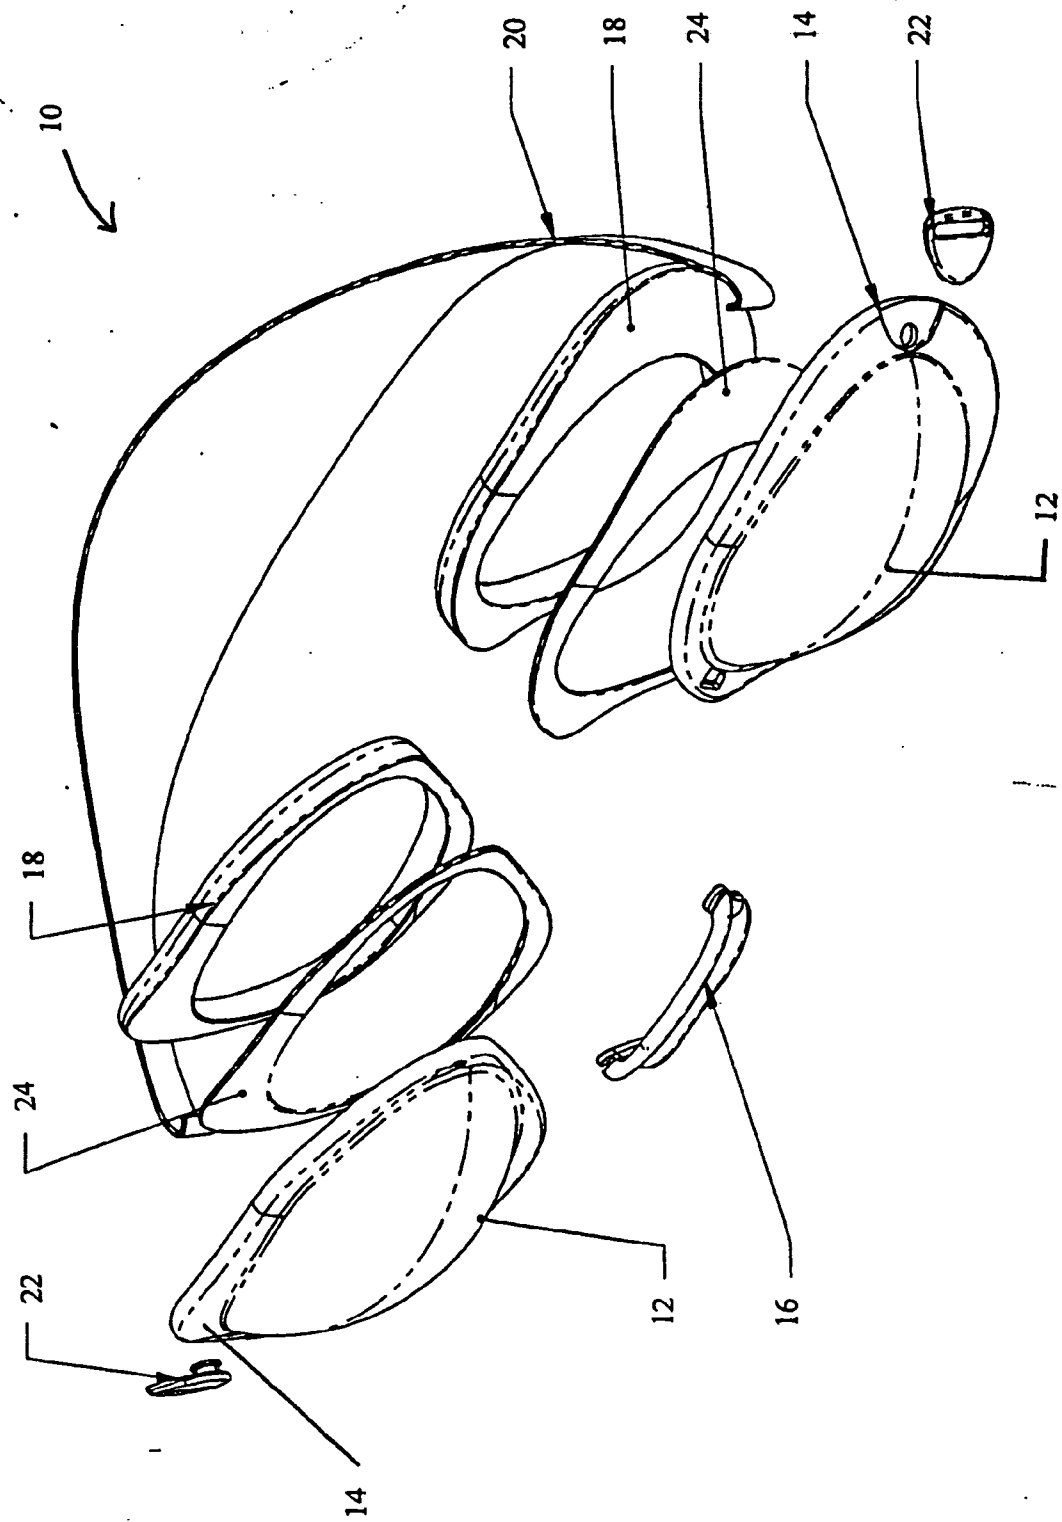


FIG. 6

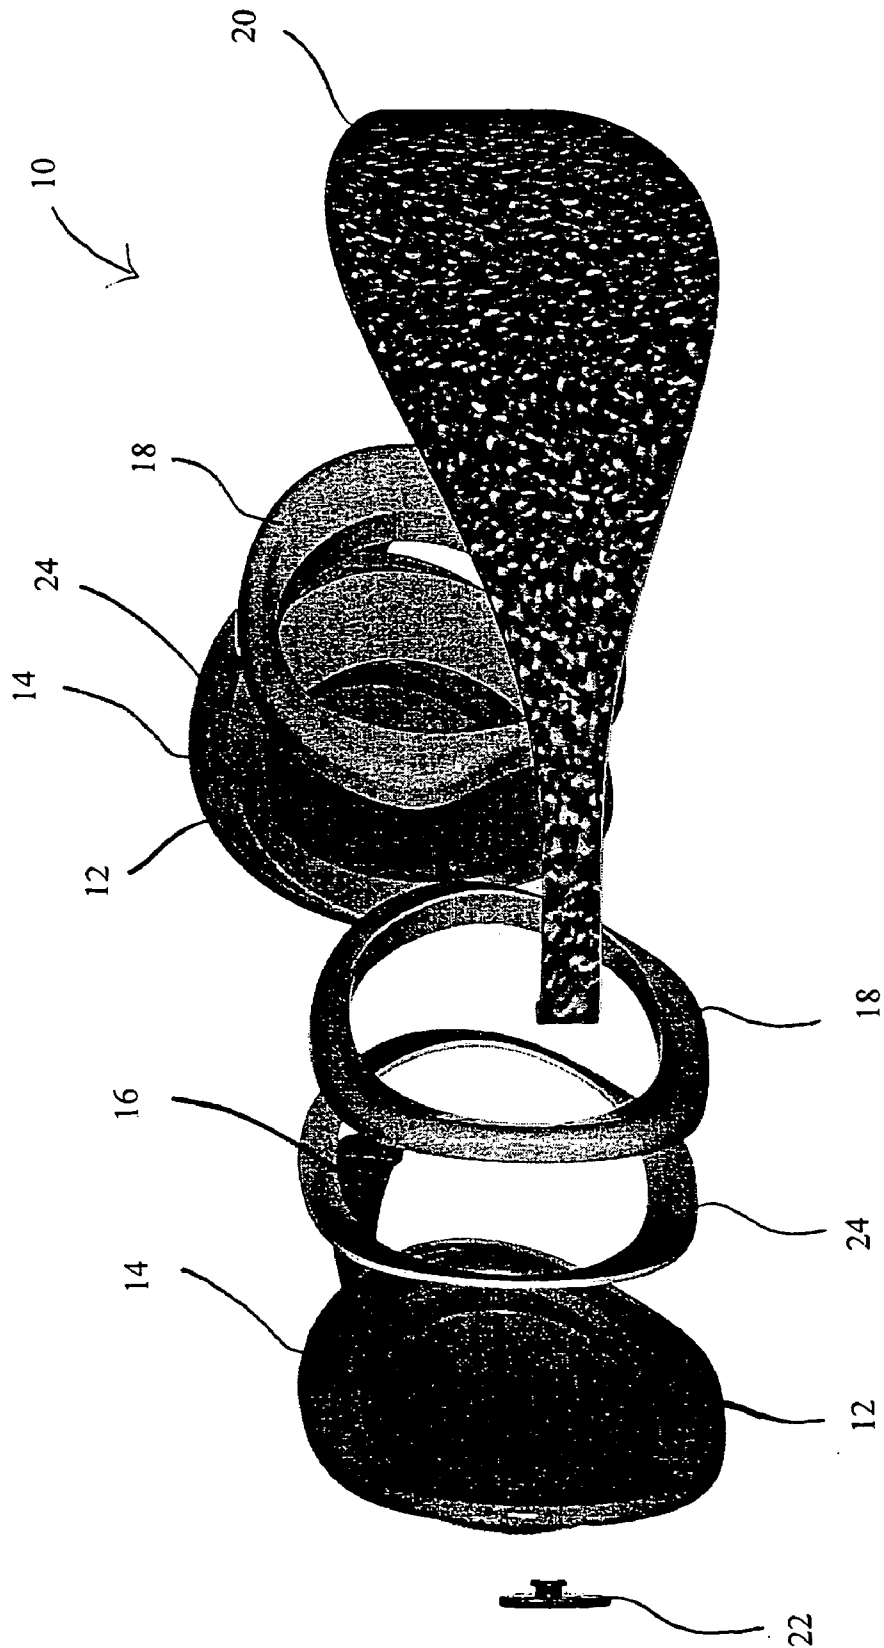


FIG. 7

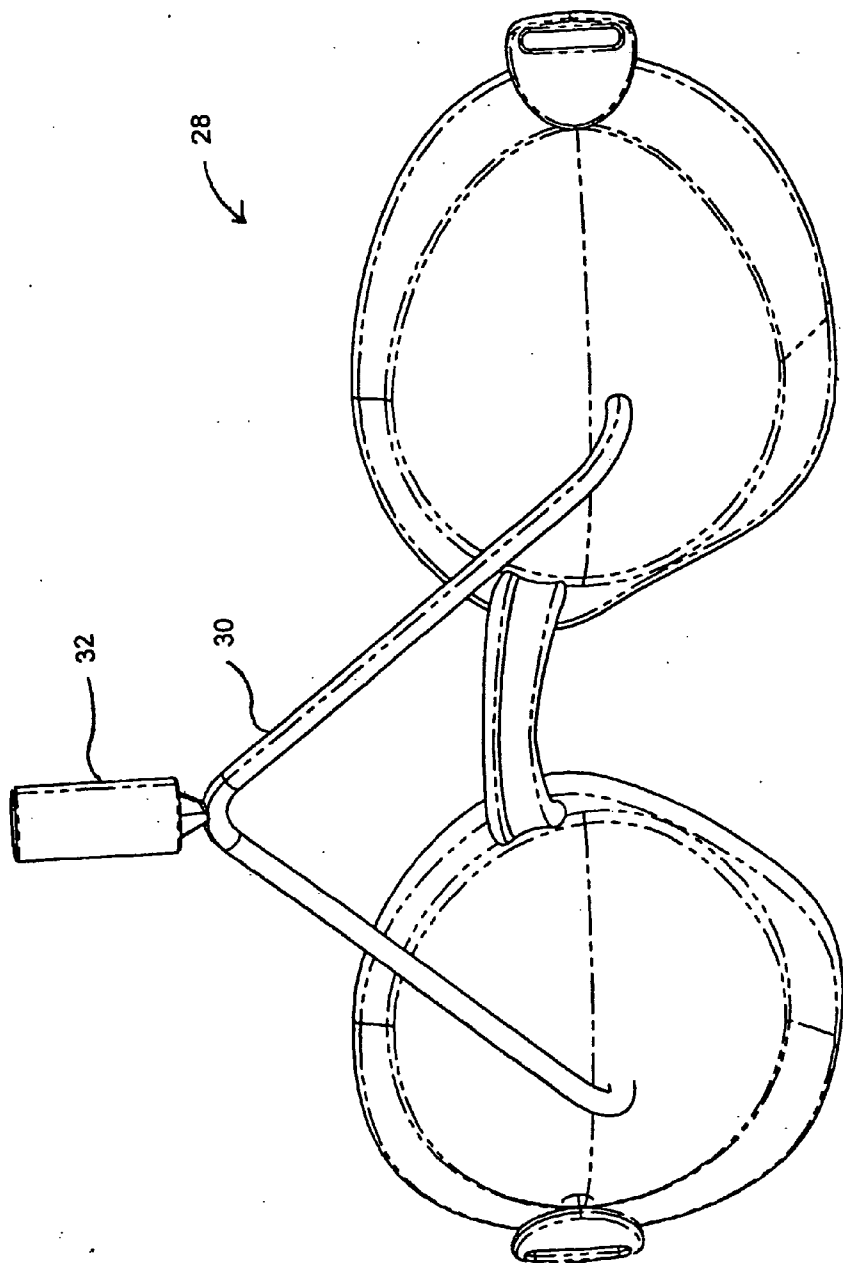


FIG. 8

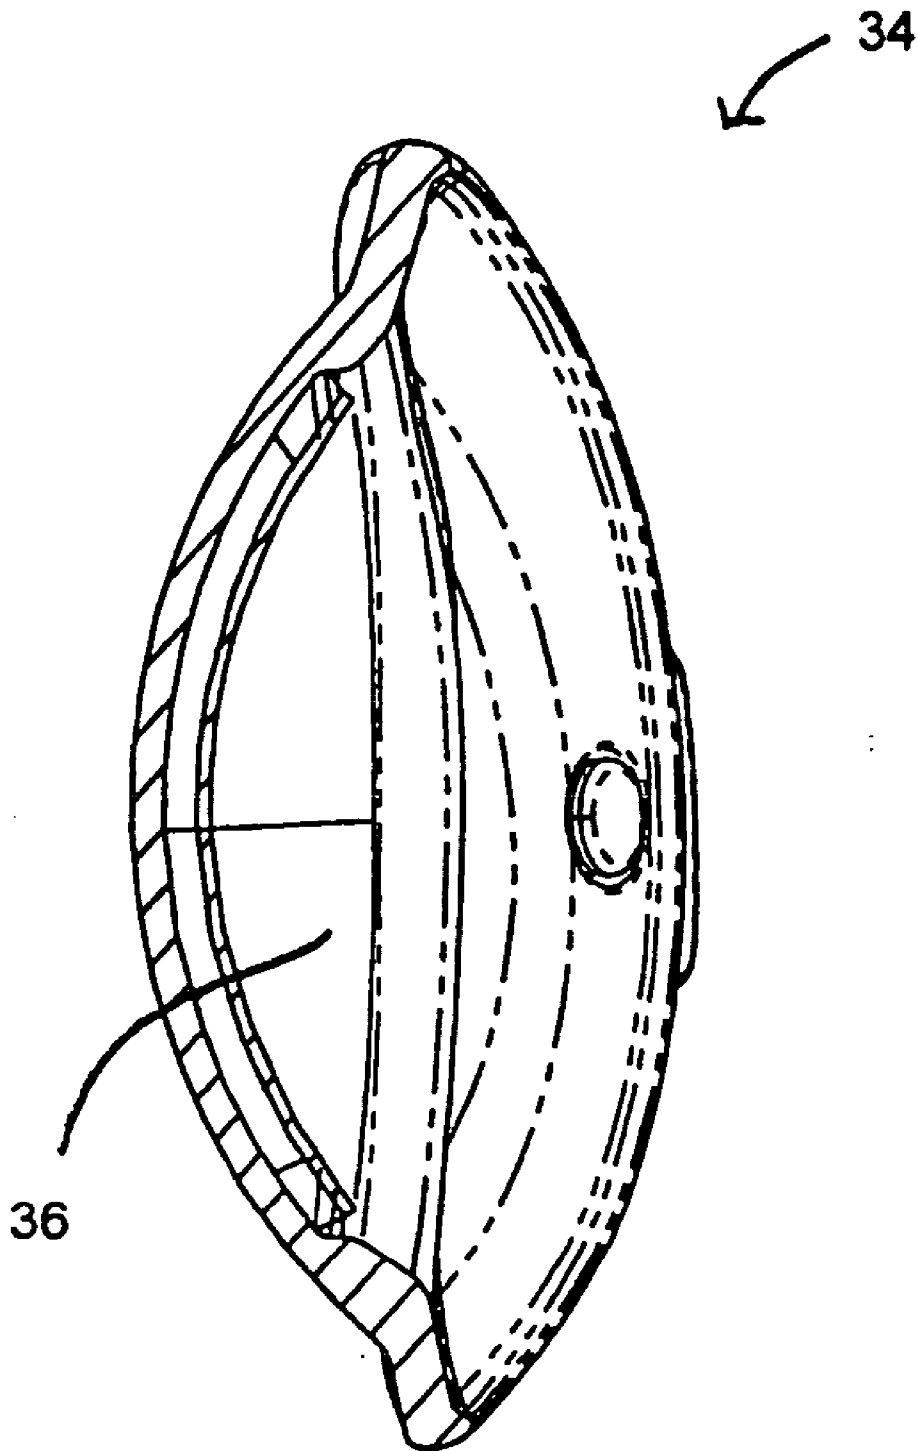


FIG. 9

38
↙

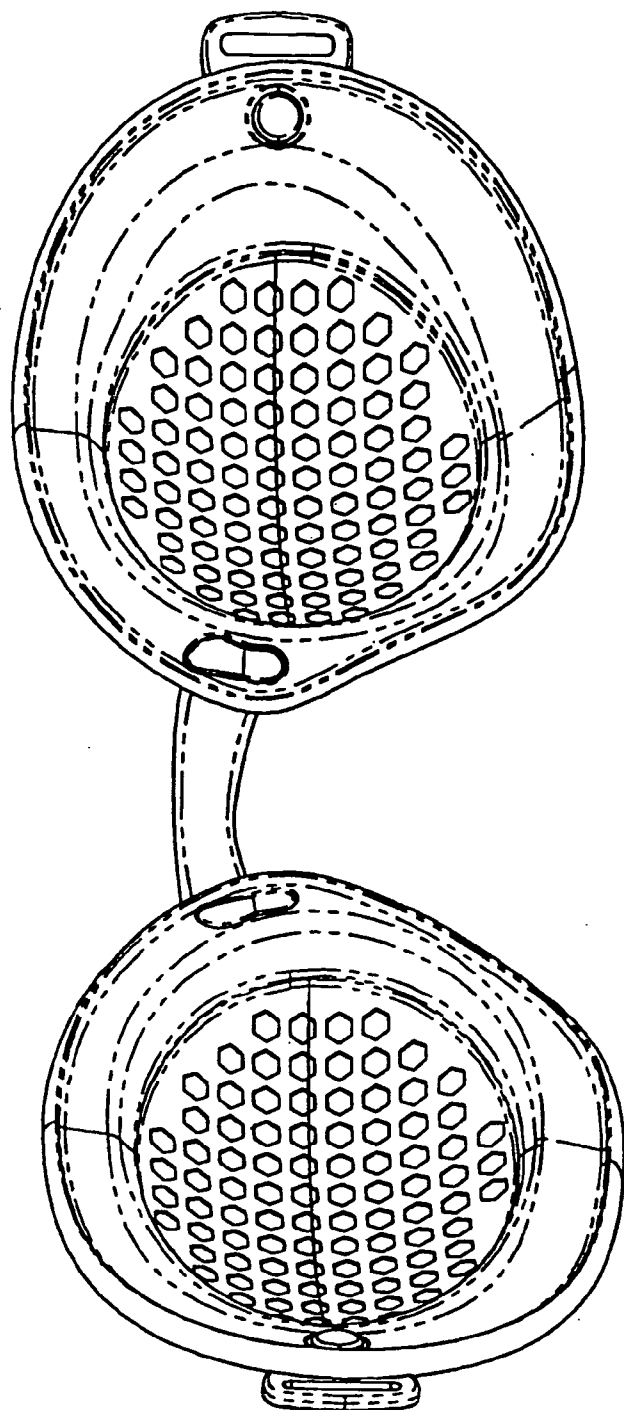


FIG. 10

**APPARATUS, SYSTEM AND METHOD FOR
TREATING DRY EYE CONDITIONS AND
PROMOTING HEALTHY EYES**

FIELD OF THE INVENTION

[0001] This invention relates generally to an apparatus, system and method for treating dry and irritated eye conditions. Particularly, this invention relates to an apparatus constructed and adapted to help control, maintain, and/or increase the temperature and humidity around the eye to aid in limiting evaporation of natural and/or artificial tears, which aids in thickening of the lipid layer, thereby improving the overall health of the eye. This invention also relates to an apparatus, system and method that provides for controlled application of medicine to the eyes.

BACKGROUND OF THE INVENTION

[0002] Approximately 60 million Americans suffer from dry eye conditions alone. Of these, approximately 10 million Americans have been diagnosed with severe dry eye conditions, e.g., Dry Eye Syndrome or Chronic Dry Eye Disease (CDED), both clinically known as keratoconjunctivitis sicca. CDED is a condition that results from inflammation of the eye, as well as inflammation of the tear-producing glands. This inflammation decreases the eyes' ability to produce natural tears, which help protect the eyes from irritation and keep them moisturized and lubricated. People who suffer from CDED often experience constant pain from eye irritation, including a sandy or gritty sensation that, if untreated, can lead to scarring or ulceration of the cornea, which can lead to a partial or total loss of vision.

[0003] Most cases of CDED result from normal aging of the eye; however, CDED or dry, irritated, tired eyes can occur at any age. It is estimated that nearly 75% of people over the age of 65 will experience CDED conditions. CDED occurs in both men and women; however, it is most common in women who are post-menopausal or pregnant. Approximately 4 million Americans, of which approximately 90% are women, have CDED as a consequence of Sjögren's syndrome, which is a chronic, slowly progressive autoimmune disease characterized by dryness of the eyes and mouth and recurrent salivary enlargement. Other diseases, such as rheumatoid arthritis, lupus, scleroderma, and thyroid disease, can also cause CDED. In addition, health, environmental, and lifestyle conditions can also cause CDED. For example, people suffering from allergies (approximately 50 million people) and people who wear contact lenses (approximately 38 million Americans), have a greater risk of developing CDED. Other circumstances that significantly dry, irritate, and fatigue the eye include: computer use; low humidity environments, such as flying in an airplane, in which the relative humidity is typically between 5% to 15%; certain medications; eye surgery; and certain medical conditions, such as blepharitis (inflammation of the eyelids).

[0004] Some early signs of CDED include: 1) an occasional burning sensation in the eyes when a person is in an area of low humidity or high pollution; 2) a persistent and painful gritty sensation in the eyes; 3) an inability to cry under emotional stress; 4) decreased tolerance of contact lenses; and 5) in extreme cases, unusual sensitivity to light, severe eye pain, or diminished vision. In the early stages of the disorder, these symptoms may come and go, but become

more persistent as the condition worsens. For most CDED cases, patients experience a greater discomfort as the day progresses.

[0005] Over 25,000 people a day turn 50 years old in the U.S. alone. It is estimated that by 2010, over 140,000,000 Americans will be over the age of 50. As mentioned above, if dry eye conditions are left untreated a person may develop CDED and, eventually, a loss of vision. Thus, with a significant portion of the population aging, the incidence of dry eyes will increase significantly, as will the risk of developing CDED.

[0006] The hydration process of eyes and, in particular, the corneal epithelium, includes tear production, evaporation, and outflow loss. Indeed, studies suggest that dry eye conditions are associated with an increased evaporation of tears from the ocular surface. Further, increased humidity around the eye significantly reduces, if not stops, the evaporation of tears and can restore and thicken the lipid layer. See William D. Mathers, M. D., et al., *Tear Flow and Evaporation in Patients with and without Dry Eye*, *Ophthalmology*, Vol. 103, no. 4 (April 1996), pp. 664-669; William D. Mathers, M. D., *Ocular Evaporation in Meibomian Gland Dysfunction and Dry Eye*, *Ophthalmology*, Vol. 100, no. 3 (March 1993), pp. 347-351; Donald R. Korb, O. D., et al., *Effect of Periocular Humidity on the Tear Film Lipid Layer*, *Cornea*, Vol. 15, no. 2 (1996), pp. 129-134.

[0007] Presently there is no cure for CDED; however, there exist various treatments that are designed to alleviate the often debilitating pain and discomfort caused by dry eye conditions. Such treatments include: artificial tear solutions, moisture chamber glasses, and punctal occlusion.

[0008] The most common treatment for people with dry, irritated, or tired eyes is artificial tear solutions, both prescription and over-the-counter eye drops. Artificial tear solutions may or may not contain preservatives. The preservatives used in artificial tear solutions have little or no toxicity; however, artificial tear solutions with preservatives can cause irritation if used frequently. In fact, artificial tear solutions with preservatives are not recommended for frequent use. CDED patients typically need to frequently apply artificial tears, which prohibits the use of artificial tears with preservatives. Preservative-free solutions are available; however, they are expensive and prone to bacterial contamination. While artificial tears primarily increase the comfort of people suffering from dry, irritated eyes, when used frequently they may rinse away the natural tears necessary to reestablish a normal tear film. Frequent use of artificial tears is also expensive; individuals suffering from CDED can spend approximately \$300 a year on artificial tears.

[0009] Another treatment for dry, irritated eyes is ointments. Typically used for nighttime relief, ointments often blur vision, are messy, awkward to apply, and often do not provide an effective treatment.

[0010] Another treatment includes the use of moisture chamber glasses. Moisture chamber glasses are custom-made products designed to alleviate the pain and discomfort caused by dry eye conditions. There are no commercially available moisture chamber glasses, they must be custom fit by an optician, and can be prohibitively expensive for the average consumer. Studies have suggested that conventional swim goggles may also be helpful in preserving moisture in

dry eyes, as well as protecting eyes from exposure to air currents, such as air conditioning and wind gusts. See, e.g., Donald R. Korb, O. D., et al., *Effect of Periocular Humidity on the Tear Film Lipid Layer, Cornea*, Vol. 15, no. 2 (1996), pp. 129-134. However, conventional swim goggles are not designed for prolonged use and can be uncomfortable to the wearer. Although conventional swim goggles are well designed for the intended use of swimming, the application of conventional swim goggles as a moisture chamber has numerous drawbacks, including: 1) the optics and field of view are designed for swimming; 2) conventional swim goggles typically have a narrow orbital seal that is designed to keep water out and which is located inside the orbital bone and supported by the sensitive inner ocular area; 3) the straps are designed for short-term wear, under tension, and are not designed for sleeping; 4) the lens and body design is manufactured of a polycarbonate rigid plastic, which is inherently uncomfortable because of its rigid nature and because the exterior contour creates pressure on the eye socket when the wearer is laying down; 5) conventional swim goggles encompass a smaller surface area around the eye, thereby reducing the potential to trap moisture and heat from the skin surrounding the eye; 6) conventional swim goggle designs tend to cut off capillary blood vessels of the skin in the area surrounding the eyes; 7) conventional swim goggle lenses are typically treated with an anti-fog coating, which is either hydrophobic, hydrophilic, or a blend of the two, and which can cause irritation to the eyes.

[0011] Punctal occlusion, the closure of the tear ducts, is another type of treatment for dry eyes that can provide an increased volume of tears remaining in the eye area by decreasing drainage. Under this method of treatment, the lower puncta, which carry away the majority of tears, are sealed using a collagen or silicone plug, or by surgery, via electrocautery or an argon laser. Plugging is typically done for evaluation purposes or when the sufferer's dry eye conditions vary in severity. A collagen plug lasts only a short time, may not occlude completely, and is eventually absorbed. The silicone plug is not absorbed, but can easily be removed. Surgical occlusion is a permanent treatment option for dry eye sufferers; however, surgery may have to be repeated because the puncta tend to reopen. Punctal occlusion can be an expensive treatment for dry eye conditions, ranging in price from \$500 to \$650.

[0012] Thus, a need exists for an apparatus, system and method for treating dry eye and/or irritated eye conditions that is natural, easy to use, comfortable and safe to the wearer, inexpensive, and which provides therapeutic benefits for the eyes without the discomfort, invasiveness, and limited use of the currently available treatments. A need also exists for an apparatus, system and method that can be used to promote healthy eyes and can reduce the possibility of developing CDED by improving the health of the lipid layer.

SUMMARY OF THE INVENTION

[0013] Generally speaking, the present invention is directed towards an apparatus, system and method for treating dry eye and/or irritated eye conditions and which helps control, maintain and/or increase the temperature and humidity around the eyes to aid in limiting evaporation of natural and/or artificial tears. The present invention is also directed towards an apparatus, system and method for promoting healthy eyes by aiding in thickening the lipid layer.

The present invention is also directed towards an apparatus, system and method that provides for controlled application of medicine to the eyes.

[0014] The apparatus of the present invention comprises two soft, pliable eyecups, that each include a curved lens and contoured frame. The eyecups are connected by a soft, pliable bridge. The soft lenses of the present invention are maintained within the soft contoured frame, which is designed and constructed to encircle the orbital bones of the eye sockets, creating a custom, comfortable fit and effective seal over each eye. In a preferred embodiment, attached to each frame is a gasket that further aids in sealing the apparatus over the eyes and which provides additional comfort to the wearer. A contoured strap, which is attached to the eyecups, maintains the proper positioning of the apparatus on the wearer.

[0015] The present invention is also directed to a system comprising the apparatus described above used in conjunction with a moisture pad. The moisture pad can be inserted between the apparatus and the eyes of the wearer to provide further aid in treating dry eye and/or irritated eye conditions. The moisture pad can be moistened, moistened and heated, or moistened and cooled to further aid in alleviating dry eye and/or irritated eye conditions.

[0016] Accordingly, it is an object of the invention to provide an apparatus and system, and methods for using such an apparatus and system, to provide an improved treatment for sufferers of dry eyes, dry eye syndrome, CDED, and irritated eyes that is simple and comfortable.

[0017] Another object of this invention is to provide an apparatus and system, and methods for using such an apparatus and system, to provide improved treatment for sufferers of dry eyes, dry eye syndrome, CDED, and irritated eyes that can be used for immediate and long-lasting relief.

[0018] A further object of this invention is to provide an apparatus and system, and methods for using such an apparatus and system, that improves quality of rest or sleep and reduces the need for other dry eye treatments, such as artificial solutions and ointments.

[0019] Still another object of this invention is to provide an apparatus and system, and methods for using such an apparatus and system, that improves comfort during air travel.

[0020] Still another object of this invention is to provide an apparatus and system, and methods for using such an apparatus and system, that creates a moisture retaining chamber around each eye, which promotes the health of the eyes while at the same time preventing and/or inhibiting the development of severe dry eyes.

[0021] Still another object of this invention is to provide an apparatus and system, and methods for using such an apparatus and system, that can alleviate, reduce, and/or prevent dry eye syndrome and/or CDED.

[0022] Still another object of this invention is to provide an apparatus and system, and methods for using such an apparatus and system, that increases hydration of the eyes.

[0023] Still another object of this invention is to provide an apparatus and system, and methods for using such an apparatus and system, that can promote healthy eyes.

[0024] Still another object of this invention is to provide an apparatus and system, and methods for using such an apparatus and system, that aids in the application of particular medicines.

[0025] The invention accordingly comprises the features of construction, combination of elements, and arrangement of parts which will be exemplified by the constructions hereinafter set forth, and the scope of the invention will be indicated in the claims.

BRIEF DESCRIPTION OF THE DRAWING FIGURES

[0026] In the drawing figures, which are not to scale, and which are merely illustrative and wherein like reference characters denote similar elements throughout the several views:

[0027] **FIG. 1** is a front perspective view of an apparatus for treating dry eye conditions constructed in accordance with one aspect of the present invention.

[0028] **FIG. 2** is a back perspective view of an apparatus for treating dry eye conditions constructed in accordance with one aspect of the present invention.

[0029] **FIG. 3** is a front plan view of an apparatus for treating dry eye conditions constructed in accordance with one aspect of the present invention.

[0030] **FIG. 4** is a top plan view of an apparatus for treating dry eye conditions constructed in accordance with one aspect of the present invention.

[0031] **FIG. 5** is a side plan view of an apparatus for treating dry eye conditions constructed in accordance with one aspect of the present invention.

[0032] **FIG. 6** is a detailed exploded front view of an apparatus for treating dry eye conditions constructed in accordance with one aspect of the present invention.

[0033] **FIG. 7** is a detailed exploded back view of an apparatus for treating dry eye conditions constructed in accordance with one aspect of the present invention.

[0034] **FIG. 8** is a front view of an alternate embodiment of an apparatus for treating dry eye conditions.

[0035] **FIG. 9** is a side plan view of an alternate embodiment of an apparatus for treating dry eye conditions.

[0036] **FIG. 10** is a back view of an alternate embodiment of an apparatus for treating dry eye conditions.

DETAILED DESCRIPTION OF THE EXEMPLARY EMBODIMENTS

[0037] Generally speaking, the present invention is directed towards an apparatus, system and method for treating dry eye and/or irritated eye conditions and which helps control, maintain and/or increase the temperature and humidity around the eyes to aid in limiting evaporation of natural and/or artificial tears. The present invention is also directed towards an apparatus, system and method for promoting healthy eyes by aiding in thickening the lipid layer. The present invention is also directed towards an apparatus, system and method that provides for controlled application of medicine.

[0038] In developing the apparatus, system and method of the present invention, the following information and design characteristics were taken into consideration:

[0039] **Description of the Orbits from Gray's Anatomy**—The orbits are two quadrilateral, pyramidal cavities, situated at the upper and anterior part of the face, their bases directed forward and outward, and their apices backward and inward so the axes of the two, if continued backward, would meet over the body of the sphenoid bone. Each orbit is formed of seven bones, i.e., frontal, sphenoid, ethmoid, superior maxillary, malar, lachrymal, and palate, three of which are shared by both orbits, i.e., the frontal, ethmoid, and sphenoid.

[0040] **Anatomical Considerations in the Design of the Invention**—The design of the present invention takes into account the shape and contour of the bones of the face and the orbit region and uses this structure as support for the apparatus. Specifically, the frontal (supra-orbital ridge), superior maxillary, malar, and nasal bones were considered when determining the shape and contour of the apparatus. Due to ethnic variation, size, and gender, an optimized profile was determined that minimizes the pressure points on critical areas of this sensitive area. The present invention also is designed to minimize tissue pressure and occlusion of various vessels and nerves in the area of contact. Specifically, the present invention utilizes the bone structure for support and relies upon the muscle structure of the orbit area as additional protection of the arteries, veins, lymph vessels, and nerves.

[0041] **Muscle Structure Considerations in the Design of the Invention**—The apparatus of the present invention mimics the contour and general shape of the orbicularis palpebrarum, also referred to as the orbicularis oculi muscle, muscle structure. The frontalis portion of the occipitofrontalis muscle, the continuation of the pyramidalis nasi, and the corrugator supercilii, further protect the upper and nasal portions of the contact area.

[0042] **Nerve Considerations in the Design of the Invention**—The facial nerve divides in front of the ear into six branches that serve the scalp, forehead, eyelids, muscles of facial expression, cheeks, and jaw. The design of the present invention avoids the main trunk and minimizes pressure points on these nerves when the invention is worn, or if the patient were to lie on a pillow placing extra pressure on this area during sleep.

[0043] **Blood Vessel Considerations in the Design of the Invention**—The angular artery, orbital artery, and branches of the anterior temporal artery anastomose with the infra-orbital, and after supplying the lachrymal sac and orbicularis palpebrarum muscle, terminate by anastomosing with the nasal branch of the ophthalmic artery. Closing off the blood supply, or reducing the anastomosing, reduces blood flow in the area. Blood flow is further reduced if the capillaries are compressed by producing a design that compromises these delicate structures.

[0044] Primarily, the frontal vein and the communicating branch with the ophthalmic vein were considered in the shaping of the present invention in the nasal area. The nasal arch vein is avoided by the clearance provided by a flexible nose bridge. As the frontal vein moves down the face alongside the inner nasal, the present invention also avoids pressuring the angular vein.

[0045] The important anastomosis of the angular vein and the sinus is associated with proper circulation and is within the contact area of the invention. Thus, the present invention design in the described areas was modified to optimize fit and minimize the occlusion of these important veins. The health and well-being of the vein structures around the eye are associated with visual beauty in modern society; therefore, it is important in the design of the present invention to maximize health and beauty aspects of the invention, thus, occlusion of the veins should be avoided.

[0046] Lymphatic Vessels in the Orbital Area—Superficial lymphatic vessels of the face are numerous and generally accompany the frontal vessels in the area of the orbits. Compression of the superficial lymphatic vessels is minimized by the minimal localized pressure exerted by the apparatus of the present invention.

[0047] Fitting the greatest range of face sizes, ages, bone structures, and accommodating sensitive skin, determined the combination of materials of the present invention. Raw anthropomorphic data was utilized from ANSI Z87.1 1989, Alderson Head Form data and percentiles, and from *The Measure of Man & Woman: Human Factors in Design*, Revised Edition, by Alvin R. Tilley and Stephen B. Wilcox, December 2001.

[0048] Application and intended use were other factors taken into consideration for the design of the present invention, namely, when and how to use a dry eye treatment to derive the greatest therapeutic benefits. The present invention is designed for use when resting or sleeping. The design of the apparatus and system of the present invention prevents a sufferer of dry eye conditions from inadvertently touching or rubbing the eyes during the night, which can be a significant problem after many types of eye surgery. Also, incomplete closure of the eyelids while sleeping causes excessive drying of the eye that may cause significant damage to the cornea. These problems can be avoided if the present invention is utilized at night. As such, the present invention can improve the quality of sleep, support post-eye surgery healing, and aid in the acceleration of healing due to the improved conditions when the present invention is worn.

[0049] Taking into account all of the above design considerations, the apparatus of the present invention comprises two soft eyecups, that each include a soft lens and a soft frame, and which are connected by a soft, pliable bridge. The lenses, which are curved, and the frames are each made of a soft, pliable material. The lenses are maintained within a soft, pliable, and contoured frame that is designed and constructed to encircle the orbital bone of the eye sockets, creating a custom, comfortable fit and effective seal over each eye. In a preferred embodiment, attached to each frame is a gasket that further aids in sealing the apparatus over the eyes and which provides additional comfort to the wearer. A contoured strap, which is attached to each frame, helps maintain the proper positioning of the apparatus on the wearer.

[0050] Referring now to FIGS. 1 through 5, the apparatus for treating dry eyes and irritated eyes, generally indicated as 10, has curved lenses, generally indicated as 12, which may be either translucent, opaque, transparent, and/or of optical quality in order to provide maximum comfort to the wearer. Lenses 12 are coupled to frames, generally indicated as 14, which together make up the eyecup and which are

connected to a second eyecup by a bridge, generally indicated as 16. A gasket, generally indicated as 18, is coupled to each frame 14. A strap, generally indicated as 20, is affixed to frames 14 via fasteners 22 to maintain apparatus 10 on the wearer. The apparatus of the present invention, when constructed of the appropriate materials and used as described herein, helps maintain and/or increase the humidity within the apparatus thus aiding in alleviating, treating, preventing and/or reducing the effects of dry eye syndrome and CDED.

[0051] The lenses and the frames are designed and constructed to balance the planned material, primary physical properties of Flex Modulus, 6000 psi and ASTM D790, Durometer Hardness, a scale “90” ASTM D2240, and Compression Set, 20% ASTM D395 73° F., 22 hr., with the mechanical shape and how it is influenced by these factors. Anthropomorphic data was applied in the design and ranges of fit were established for the area around the less sensitive occipital bones. This area varies within the established ranges, and to make the apparatus as comfortable as possible, the apparatus self-conforms and seals this area for moisture retention. Comfort is a primary concern and established comfort criteria include reduction of pressure points in the contact area. The design of the apparatus of the present invention also takes into consideration that the patient may create additional pressure loading on the mechanism by lying on the pillow face down or turning during the night.

[0052] The eyecup is functionally unique in that the hemispherical lens provides a resilient support mechanism for the flowing anthropomorphic frame area. On any point of the frame area the anthropomorphic shape is designed to flex, follow, and move as needed by the individual’s unique facial contour. Additionally, if the pressure on the gasket, which will be described in greater detail below, exceeds the limit of comfortable compression, the frame will then accommodate the pressure maintaining the seal and comfort. The actual flexibility of the invention is primarily achieved by the combination of the flexural modulus of the material and engineered shaping of the hemispherical area and frame. The variable part thickness also influences the final performance and characteristics to create the unique attributes described for this invention. Commonly, products for the eye protection industry are manufactured with a hemispherical rigid lens and a frame based on simple geometric shapes. These rigid materials and non-specific designs are ineffective at sealing the complex area of the occipital bone structure or providing the comfort required for people who need to use this type of product.

[0053] The eyecup, including a lens and frame, and the bridge of the present invention can be manufactured using a thermoplastic, including, but not limited to: ABS (Acrylonitrile Butadiene Styrene), Acetal (POM)-(Acetal (polyacetal)), Acrylic (Acrylic), Acrylic (PMMA)-(Polymethyl Methacrylate), Acrylic (SMMA)-(Styrene Methyl Methacrylate Copolymer), Cellulose Acetate, Cellulose Acetate Butyrate, Ethylene Vinyl Acetate, HDPE (polyethylene, high density), HIPS (polystyrene, high impact), Ionomer, LPDE (polyethylene, low density), MDPE (polyethylene, medium density), Nylon (Polyamide-nylon), PBT (Polybutylene Terephthalate), PC (polycarbonate), PCT (Polycyclohexylene Terephthalate), PCTG (Polycyclohexylene Dimethylene Terephthalate), Polyethylene, PET (Polyethylene Terephthalate), PETG (Polyethylene Terephthalate Glycol

Comonomer), PP (Polypropylene), PPO (Polyphenylene Oxide), PS (Polystyrene), PUR (Polyurethane), PVC (Polyvinyl Chloride), PVC+PUR (Polyvinyl Chloride+Polyurethane Alloy), Polyester TP (Polyester, thermoplastic), Polyester TS (Polyester Thermoset), SAN (Styrene Acrylonitrile), SB (Styrene Butadiene Block Copolymer), SBS (Styrene Butadiene Styrene Block), SEBS (Styrene Ethylene Butylene Styrene Block Copolymer), SIS (Styrene Isoprene Styrene Block Copolymer), TPE (Thermoplastic Elastomer), TPO—(Thermoplastic Olefin Elastomer), TPU (Polyurethane, Thermoplastic Elastomer—TPE).

[0054] The following thermoset materials, which have similar properties, are also appropriate for application to the present invention: silicone, Rubber, neoprene, Buna-N (nitrile) Rubber, Butyl Rubber, EPDM (ethylene-propylenediene methylene), SBR rubber (styrene butadiene), Epichlorohydrin Sponge Rubber, Gum Rubber, Hypalon Rubber, Latex (Natural Rubber), Neoprene Rubber, Polyurethane Rubber, and any other thermoset not listed but with properties appropriate for application to this invention.

[0055] Additionally, the eyecup and the bridge could be manufactured from a flexible cellular material, including, but not limited to: Polyurethane ether based foam, Polyurethane ester based foam, Polyethylene foam, Polyethylene cross-linked foam, Ethylene Vinyl Acetate foam, Silicone foam, PVC (Polyvinyl Chloride) foam, Polyimide foam, Ionomer foam, and any other flexible cellular material.

[0056] Alternatively, in addition to the thermoplastic and thermoset materials, the eyecup and the bridge can be manufactured using a gel, fluid, or particle-filled structure.

[0057] There are any number of ways of manufacturing the eyecup and the bridge of the present invention, including, but not limited to: injection molding, compression molding, vacuum forming, pressure forming, mechanical forming, casting, hot sealing, sonic welding, or other methods used in the fabrications of the above listed materials.

[0058] Lenses 12, depicted in FIGS. 1 through 7, are curved to create a humidity chamber above the wearer's eyes. In a preferred embodiment, lenses 12 have an eight-base curvature to allow for blinking. Lenses 12 are made of a soft, pliable material, such as silicone or flexible polyurethane, or any one of the materials listed above, and can be translucent, opaque, transparent, and/or of optical quality to provide maximum comfort to the wearer. In a preferred embodiment, lenses 12 are formed of flexible polyurethane. Lenses 12 can also be colored to promote additional therapeutic benefits such as light and/or color therapy.

[0059] Lenses 12 can be either permanently affixed to frames 14, or may be removably mounted or maintained within frames 14 in a manner known in the art. For example, lenses 12 can be constructed to snap into a groove (not shown) located in the inner perimeter of frames 14. In an alternate embodiment, the frames and lenses can be formed of a single unitary piece.

[0060] Frames 14 also are made of a soft, pliable material, such as silicone or flexible polyurethane, or any one of the materials listed above, and are preferably contoured to conform to the orbital bone around the eye socket to provide a snug, comfortable, and effective fit for the wearer. Bridge 16 connects frames 14 and can be adjustable to provide a custom, comfortable fit for the wearer. Bridge 16 is also

constructed of a soft, pliable material such as flexible polyurethane. In an alternate embodiment, the frames, lenses, and bridge can be formed of a single unitary piece.

[0061] Gasket 18, as depicted in FIGS. 1 through 2 and 4 through 7, can be coupled to frames 14 to provide additional comfort to the wearer and to also provide a more effective seal around the eye sockets. In one embodiment, gasket 18 is permanently affixed to frames 14. In an alternate embodiment, gasket 18 can be removable from frames 14. For example, as shown in FIGS. 6 and 7, apparatus 10 can further comprise an attaching mechanism, generally indicated as 24, which is coupled to frames 14, to which gasket 18 can removably attach. The attaching mechanism 24 can also be formed integrally with frames 14 as a matter of application specific design choice. Although attaching mechanism 24 can take any number of forms and materials as known in the art to achieve its intended function, in a preferred embodiment, attaching mechanism 24 comprises a Velcro® strip to facilitate easy and quick interchanging of gasket 18. To attach gasket 18 to attaching mechanism 24, gasket 18 can have a compatible attaching mechanism, such as a Velcro®-compatible material affixed to one side. In such an embodiment the wearer can replace gasket 18 upon extended use or the like.

[0062] Gasket 18 can be formed of any type of material that will provide a comfortable fit for the wearer while at the same time meeting the functional requirements of the gasket, for example, foam or a thin silicone member. In a preferred embodiment, gasket 18 is made of a visco-elastic, thermal-forming foam, such as the commercially-available foam supplied by PAC Foam Products Corporation in Costa Mesa, Calif. Such a foam gasket will conform to the wearer's orbital bone structure, especially when warmed by body heat, to thereby create a comfortable and effective seal around the eyes.

[0063] In the preferred embodiment, balancing Indention Force Deflection (IFD) @25%, IFD @65%, and specific pound density of the present invention, relieves pressure points along the orbital area. This balancing works in combination with the tension of strap 20 and the anthropomorphic design of the eyecup.

[0064] In an alternate embodiment, gasket 18 is integral with the eyecup. For example, gasket 18 may be an extension of the hemispherical section of the lens, a portion of the frame, or a structure that is emanating from any or all of these sections and, as such, gasket 18 can be formed of any one of the materials listed above for the eyecup. In this alternate embodiment, the desired balance between the IFD @25%, the IFD @65%, and the pound density can be achieved by, for example, the frame itself without the addition of a separate gasket 18.

[0065] In an alternate embodiment, gasket 18 is an inflated structure comprised of a bladder that surrounds the orbital area.

[0066] In an alternate embodiment, gasket 18 is a gel-, fluid-, or particle-filled structure that self-conforms to the orbital structure. Gasket 18, when a filled structure, can be heated or cooled to promote the therapeutic benefits of the present invention.

[0067] Strap 20 is preferably made of a soft, and flexible or elastic material and is coupled to frames 14, preferably at

opposite outer sides of frames **14**. In the embodiment depicted in **FIGS. 1 through 7**, strap **20** is coupled to fasteners **22**, which can be made of a flexible polyurethane or any one of the materials listed above for use in the eyecup, and which are coupled to opposite outer sides of frames **14**. The design of fasteners **22** permits the wearer to sleep with the apparatus and contact the pillow or bedding without unnecessary pressure points on the wearer. See para. 42, *Nerve Considerations in the Design of the Invention*. In an alternate embodiment, frames **14** include two parallel slits on opposite outer sides for affixing strap **20** to frames **14**. Other means of attaching strap **20** to frames **14** are known in the art. Strap **20** can be both removable and adjustable.

[0068] In a preferred embodiment, strap **20** is formed of an elastic material, such as a two-way stretch polyester blend, four-way stretch polyester blend, or cotton, polyester, and lycra blend materials, or any combination thereof, which aids in preventing snagging and pulling, thereby providing additional comfort to the wearer. In a preferred embodiment, strap **20** is shaped as shown in **FIGS. 2 and 7**, that is, strap **20** has a greater width at its mid-point, which further aids in holding the apparatus on the wearer and provides greater comfort to the wearer.

[0069] In the preferred embodiment, strap **20** is designed for low tension and maintains position of the apparatus with minimal interference to the capillary blood vessels of the skin and blood supply to glands and structure in the area surrounding the eyes. Additionally, the design of strap **20** minimizes the potential interference of the lachrymal glands and ducts. See paras. 39 and 40, *Description of the Orbits from Gray's Anatomy and Anatomical Considerations in the Design of the Invention*, respectively. This is achieved with a combination of the low-required strap tension and the rebound characteristics of the visco-elastic foam.

[0070] In the preferred embodiment, the "dynamic tension" which strap **20** and gasket **18** work together to achieve is the key to the long-term wearing comfort of the apparatus of the present invention. In the preferred embodiment, gasket **18** is made of a foam material that has an IFD @ 25% in a ratio to the strap tension and in combination with the pound density, although surface area of contact has a bearing on the comfort factors. The second measure of IFD is at 65%, which determines that the foam will not bottom out under normal strap tension, which brings into play the flexibility and design of the eyecup and its particular structural design.

[0071] The attachment mechanism of strap **20** can also include, but is not limited to: elastic head strap; synthetic and/or non-synthetic head strap; fabric head strap; stretch fabric head strap; designs that utilize the ear as the locator and support of any of the materials listed; designs that are open and woven in the fashion of a hair net; designs of a fabric, synthetic, non-synthetic, foam or plastic that encircle the head at or about the coronal line as defined by ANSI Z87.1-1989; designs that are adjustable or non-adjustable for straps, bands, or ear located attachments; designs that utilize snaps, Velcro®, buttons, other standard fasteners or custom fasteners to attach strap **20** or that are used to adjust the tension or the combination of both; designs that utilize gravity, such as weighted fixtures that position and create the dynamic tension necessary to seal the unit to the orbital area, these would be used when a patient was being provided a spa

facial and the head in a position to be conducive to dry eye therapy; designs that utilize an adhesive to attach the unit to the face, such as an adhesive that directly attaches to the eyecup and is located on the surface of the eyecup that comes into direct contact with the skin; methods such as placing the eyecup into position and taping the apparatus from the exterior, this type of application has particular value for juvenile patient applications or patients who may accidentally remove the apparatus or when critical cleanliness is required; or any combination of the attachment methods listed above can be used.

[0072] In another aspect of the present invention, in a system for treating dry eye and/or irritated eye conditions, shown in **FIG. 4**, apparatus **10** further comprises a moisture pad, generally indicated as **26**. As shown in **FIG. 4**, moisture pad **26** can be inserted between apparatus **10** and the eyes of the wearer in direction **A**. In a preferred embodiment, the moisture pads are made of viscous-elastic foam, which, when moistened, further help maintain, increase, and/or regulate the temperature and humidity within the chamber around the eye socket. The moisture pads can be moistened using water, artificial tears, or any other solution known in the art. In addition to being moistened, the moisture pads can be moistened and heated, or moistened and cooled, prior to being inserted into the cavity of lenses **12**. The wearer can apply the apparatus including the moisture pads for a set amount of time, after which the wearer can remove the moisture pads and continue to wear the apparatus. The moisture pads, when used in combination with the apparatus of the present invention, can further increase and maintain the relative humidity within the chamber surrounding the eye socket for aiding in treating the effects of dry eyes, irritated eyes, and for promoting healthy eyes.

[0073] Moisture pad **26** and/or gasket **18** can be manufactured from materials including, but not limited to: visco-elastic polyurethane foam, hydrophilic polyurethane foam (e.g., Aquazone product by Foamex), polyurethane ether based foam, polyethylene foam, polyethylene cross-linked foam, ethylene vinyl acetate foam, silicone foam, PVC (Polyvinyl Chloride), Polyimide foam, Ionomer foam, Polyester based foam, latex foam, anti-microbial materials (e.g., anti-microbial foam or fabric), sponge (natural or synthetic), gauze, pulp, fiber, fabric (natural or synthetic), paper products, or any synthetic or natural material, which has the capacity to absorb and release moisture or other liquids.

[0074] Moisture pad **26** and/or gasket **18** can be made of a material listed above, and then covered, in whole or in part, in a fabric to further increase comfort to the wearer or add specific characteristics to the product.

[0075] In an alternate embodiment, the moisture pad can be used to administer medicine, for example, medicine can be infused into the moisture pad material and then delivered in a controlled manner. Specifically, medicines could evaporate, sublimate, or combine with the natural moisture present in the apparatus and be delivered to the eye. Moisture pad **26** can be used to administer medicinal eye drops by absorbing the medicinal eye drops. This type of administration would contain the medicinal eye drops in a superior manner by containing the medicine within the orbital area. Moisture pad **26** and/or gasket **18** also can be infused with an herbal treatment or a counter-irritant.

[0076] In another aspect of the present invention, gasket **18** can be used for medicinal administration via skin contact.

For example, hormone therapy, which is typically administered via a skin patch and which can be used to alleviate dry eye conditions, could be administered via gasket 18, which is in contact with the skin of the wearer when wearing the apparatus of the present invention.

[0077] In another aspect of the present invention, the current realization of the moisture pad places the surface away from the eye, actually allowing room for uninterrupted blinking action; however, the moisture pad can be designed and administered to apply controlled pressure onto the closed eye. The pressure would be controlled by factors previously described in measuring the thickness, IFD @25%, IFD @65%, and the density.

[0078] In another aspect of the present invention, moisture pad 26 and/or gasket 18 can be constructed of a material that has endothermic or exothermic properties. That is, moisture pad 26 and/or gasket 18 can be constructed of a material that automatically heats or cools the apparatus of the present invention and thereby improve eye comfort and health. For example, moisture pads 26 can be comprised of the same materials as used in hot packs, which are used for muscle comfort or warmth, such as for winter outdoor activities.

[0079] In another aspect of the present invention, the apparatus and system, including moisture pad 26, can be heated or cooled to provide further comfort to the wearer. For example, the apparatus, along with moisture pad 26, could be placed in a microwave for a short period of time.

[0080] In alternate embodiments, shown in FIGS. 8 and 9, the apparatus of the present invention can be used to aid moisture delivery by adding moisture to lens within the eyecup. FIG. 8 depicts an alternate embodiment, generally indicated as 28, in which the delivery system that feeds the moisture into the eyecup can be through a tube, generally indicated as 30, from a separate remote reservoir, generally indicated as 32. Alternately, FIG. 9 depicts an alternate embodiment in which the delivery system can feed moisture into the eyecup by an internal reservoir system built into the eyecup, generally indicated as 34. For example, as shown in FIG. 9, the internal reservoir can be a pocket or a double lens design, generally indicated as 36, that is filled with moisture and is designed to slowly transfer into the chamber surrounding the eyes. This transfer of moisture into the orbital area can be by direct openings in the reservoir or membrane technology, such as a Gortex membrane, or wicking mechanism which utilizes a material to wick the moisture from the reservoir into the orbital area.

[0081] In another method for adding moisture to the eyecup, generally indicated as 38 in FIG. 10, the interior surface design of the eyecup is molded with a textured pattern, for example, a shallow honeycomb design. This honeycomb texture can be sized to accept moisture into the pockets, yet the diameter would be small enough so that the meniscus of the liquid would retain the moisture rather than allowing the liquid to run out of the honeycomb pockets by gravity. This design can hold the pre-charge of moisture and create a large surface area for evaporation, thereby raising the relative humidity in the eyecup without the addition of a moisture pad.

[0082] In another method for adding moisture to the eyecup, the interior surface of the eyecup can be sprayed with water, artificial tear solution, spray eye mist, for

example Biomist, or any other solution known in the art, before the wearer dons the apparatus of the present invention.

[0083] Data from tests of the apparatus and system of the present invention confirms the utility and efficacy of the invention. Specifically, testing confirms that use of the invention increases the temperature and relative humidity of the area surrounding the eyes, thereby reducing, and possibly preventing evaporation of natural and/or artificial tears, and/or preventing problems associated with increased evaporation, i.e., the dry eye conditions discussed above.

[0084] The results of testing the apparatus and system of the present invention on subjects without dry eye conditions are depicted in Table 1 below. For each test, temperature and humidity were measured over time, using a traceable hygrometer/thermometer, model no. 35519-020, calibrated to comply with ISO 17025. In Test 1 the subject wore the apparatus of the present invention for approximately 30 minutes during which the subject's eyes were closed 50% of the time and open 50% of the time. As Table 1 depicts, the temperature around the eyes increased 7.29% and the relative humidity increased by 52.29%. Use of the invention together with the moisture pads caused an even greater increase in temperature and relative humidity of the area surrounding the eyes. Notably, in Test 3 in which the subject wore the invention for ten minutes with the moisture pads and continued wearing the product for an additional forty-seven minutes, the temperature increased by 8.11% and the relative humidity increased by 83.90%. The other tests, which included varying the length of time the subject wore the invention with the moisture pads, and base line relative humidity in the room, also demonstrate increases in the temperature and relative humidity of the area surrounding the eyes.

TABLE 1

Testing of Apparatus on Subjects with Normal Eyes					
Time	Temperature	% Change from Base Temperature	Relative Humidity (RH)	% Change from Base RH	Comments
Test 1: Pleasanton, CA, Apr. 20, 2003					
7:44 PM	73.5		41.47		No moisture added.
7:46 PM	75	2.04%	47	13.33%	
7:50 PM	76.32	3.84%	52.2	25.87%	Eyes 50% open/50% closed.
7:55 PM	77.5	5.44%	55.89	34.77%	
8:00 PM	77.9	5.99%	58.23	40.41%	
8:05 PM	78.35	6.60%	60.3	45.41%	
8:16 PM	78.86	7.29%	63.36	52.79%	
Test 2: Pleasanton, CA, Apr. 20, 2003					
8:33 PM	75		44.4		Warm cloth on face for 5 minutes. Eyes closed.
8:40 PM	81	8.00%	67.21	51.37%	
8:43 PM	81	8.00%	70.49	58.76%	
Test 3: Pleasanton, CA, Apr. 21, 2003					
3:50 PM	74.45		43.78		No moisture added, eyes closed.
3:58 PM	77	3.43%	45.3	3.47%	
4:20 PM	83.75	12.49%	69.48	58.70%	Warm, moist moisture pads inserted for 10 minutes.
4:40 PM	77.89	4.62%	79	80.45%	
4:55 PM	80.49	8.11%	80.51	83.90%	

TABLE 1-continued

Testing of Apparatus on Subjects with Normal Eyes					
Time	Temperature	% Change from Base Temperature	Relative Humidity (RH)	% Change from Base RH	Comments
Test 4: Pleasanton, CA, Apr. 22, 2003					
7:30 PM	70		48		Warm, moist moisture pads inserted. Eyes closed.
7:35 PM	71	1.43%	65	35.42%	
7:40 PM	71	1.43%	70	45.83%	
7:50 PM	70	0.00%	74.7	55.63%	
8:00 PM	70	0.00%	76	62.50%	
Test 5: New York, NY, Apr. 24, 2003					
10:21	63.74		26.63		Warm, moist moisture pads inserted for 5 minutes. Eyes closed.
10:40	71	11.39%	66	147.84%	
10:50	71	11.39%	72	170.37%	
Test 6: New York, NY, Apr. 25, 2003					
8:15 PM	70		35		Generous spray of Nature's Tears eye mist added.
8:30 PM	73	4.29%	67	91.43%	
8:40 PM	73	4.29%	73	108.57%	
8:45 PM	74	5.71%	75	114.29%	
8:51 PM	74	5.71%	78	122.86%	
9:00 PM	74	5.71%	79	125.71%	

[0085] The results of the testing the apparatus and system of the present invention on subjects with dry eye conditions are depicted in Table 2 below. As Table 2 depicts, the temperature and relative humidity increased over time during each test. Notably, the longer the subject wore the apparatus of the present invention, the greater the temperature and humidity increased. Additionally, patients who participated in the tests experienced significant relief from their dry eye conditions for up to six hours following the use of the present invention.

TABLE 2

Testing of Apparatus on Subjects with Dry Eye Conditions					
Time	Temperature	% Change from Base Temperature	Relative Humidity (RH)	% Change from Base RH	Comments
Test 7: Campbell, CA, May 29, 2003					
6:20 PM	74		44		Added Moisture Pad Removed Moisture Pad
6:26 PM	76	2.70%	62	40.91%	
6:30 PM	75	1.35%	70.2	59.55%	
6:35 PM	76	2.70%	72	63.64%	
6:40 PM	76	2.70%	74	68.18%	
6:45 PM	77	4.05%	77.54	76.23%	
Test 8: Campbell, CA, May 29, 2003					
7:02 PM	74		46		Added Moisture Pads Removed Moisture Pads
7:07 PM	75.5	2.03%	63.6	38.26%	
7:14 PM	78	5.41%	67	45.65%	
7:22 PM	77	4.05%	73	58.70%	
7:28 PM	77.4	4.59%	76	65.22%	
Test 9: Campbell, CA, May 29, 2003					
7:56 PM	73		45		Added Moisture Pads Removed
8:05 PM	76	4.11%	78	73.33%	
8:08 PM	76	4.11%	81.1	80.22%	
8:14 PM	78.44	7.45%	85.82	90.71%	

TABLE 2-continued

Testing of Apparatus on Subjects with Dry Eye Conditions					
Time	Temperature	% Change from Base Temperature	Relative Humidity (RH)	% Change from Base RH	Comments
8:19 PM	79	8.22%	85.03	88.96%	Moisture Pads
8:25 PM	80	9.59%	86.6	92.44%	

[0086] The results of testing the apparatus and system of the present invention on subjects in a low-humidity environment, i.e., on an airplane, are depicted in Table 3 below. As Table 3 depicts, the temperature and relative humidity increased over time for each test. Notably, the relative humidity increased by over 100% for each test. Additionally, the relative humidity of the area surrounding the eyes continued to increase, even while the relative humidity within the plane continued to decline, even upon descent of the airplane.

TABLE 3

Testing of Apparatus on Subjects with Dry Eye Conditions					
Time	Temperature	% Change from Base Temperature	Relative Humidity (RH)	% Change from Base RH	Comments
Test 10: Airplane, Jun. 18, 2003					
10:01 AM	74		21		Added little moisture to lens cavity (1 drop, spread around lens cavity) 10 minutes at 10,000 ft.
10:11 AM	76	2.70%	52	147.62%	
Test 11: Airplane, Jun. 18, 2003					
10:23 AM	74		17.1		Sprayed eyes lightly with Biomist 13 minutes at 10,000 ft.
10:40 AM	77	4.05%	61	256.73%	

[0087] As evident from the data of Tables 1, 2, and 3 the present invention fulfills a long-felt need in the industry to treat and/or alleviate dry eye symptoms while at the same time promoting healthy eyes. The present invention overcomes various shortcomings of the currently available treatments, including providing a natural, inexpensive, easy to use and comfortable device that can be used in the treatment of dry eye conditions and to promote overall eye health.

[0088] It will thus be seen that the objects set forth above, among those made apparent from the preceding description, are efficiently attained and, since certain changes may be made in the above construction without departing from the spirit and the scope of the invention, it is intended that all matter contained in the above description and shown in the accompanying drawings shall be interpreted as illustrative and not in a limiting sense.

[0089] It is also to be understood that the following claims are intended to cover all the generic and specific features of

the invention herein described and all statements of the scope of the invention which, as a matter of language, might be said to fall therebetween.

What is claimed is:

1. An apparatus for treating dry eye conditions comprising:

a pair of soft, pliable, curved lenses, each of said lenses maintained within a soft, pliable frame;

a soft, pliable gasket on a back portion of each of said frames, said gasket designed to substantially encircle and contact the orbital bone of an eye socket of the wearer;

a bridge coupling said frames; and

a flexible, contoured strap having two end portions and a center portion, wherein said two end portions are coupled to said frames and said center portion is designed so as to maintain said apparatus on a wearer;

said apparatus adapted and constructed to increase or maintain the humidity around the eyes of the wearer by reducing the evaporation of natural or artificial tears, or added moisture, and by increasing or maintaining the temperature around the eyes of the wearer.

2. The apparatus of claim 1, further comprising a moisture pad adapted to be maintained between said apparatus and the eyes of the wearer, said moisture pad designed and constructed to aid in increasing or maintaining the humidity around the eyes of the wearer.

3. The apparatus of claim 2, wherein said moisture pad is formed of an endothermic or exothermic material.

4. The apparatus of claim 2, wherein said moisture pad is formed of a visco-elastic foam.

5. The apparatus of claim 1, wherein each of said lenses and said frames are formed as unitary structures.

6. The apparatus of claim 1, wherein said lenses, said frames, and said bridge are formed as a unitary structure.

7. The apparatus of claim 1, wherein said lenses and said frames are each formed of flexible polyurethane.

8. The apparatus of claim 1, wherein said lenses are removable from said frames.

9. The apparatus of claim 1, wherein said lenses are opaque.

10. The apparatus of claim 1, wherein said lenses are translucent.

11. The apparatus of claim 1, wherein said lenses are colored.

12. The apparatus of claim 1, wherein said lenses comprise a textured surface.

13. The apparatus of claim 1, wherein said gaskets are formed of visco-elastic foam.

14. The apparatus of claim 1, wherein said gaskets are removable from said frames.

15. The apparatus of claim 1, wherein said gaskets are formed of an endothermic or exothermic material.

16. The apparatus of claim 1, wherein said gaskets are at least partially covered with a fabric.

17. The apparatus of claim 1, wherein said center portion of said strap is wider than said two end portions of said strap.

18. The apparatus of claim 17, wherein said strap is formed of a four-way stretch polyester blend.

19. An apparatus for treating dry eye conditions comprising:

a pair of soft, pliable, curved eyecups, each of said eyecups designed and constructed to substantially encircle and contact the orbital bones of the eye sockets of the wearer, while minimizing tissue pressure and occlusion of the blood and lymphatic vessels in the orbital area, so as to comfortably increase or maintain the humidity around the eyes of the wearer by reducing the evaporation of natural or artificial tears, or added moisture, and by increasing or maintaining the temperature around the eyes of the wearer.

20. The apparatus of claim 19, further comprising a visco-elastic gasket positioned on each of said eyecups.

21. The apparatus of claim 19, further comprising a moisture pad adapted to be maintained between said eyecups and the eyes of the wearer, said moisture pad designed and constructed to aid in increasing or maintaining the humidity around the eyes of the wearer.

22. An apparatus for treating dry eye conditions comprising:

a pair of soft, pliable, curved eyecups, each of said eyecups designed and constructed to substantially encircle and contact the orbital bones of an eye socket of the wearer;

a thin, soft elastic strap having two end portions attached to said eyecups and designed so as to maintain the apparatus on the wearer; and

wherein said eyecups and strap each are formed of specific flexible materials such that said apparatus can be adjusted in the as worn position so that the dynamic tension between the eyecups and the strap provide a comfort level associated with a maximum 50% IFD of said eyecups while the humidity proximate the eye sockets of the wearer.

23. The apparatus of claim 22, further comprising a pair of visco-elastic gaskets positioned on said eyecups, wherein said gaskets provide an effective seal around the eye sockets of the wearer.

24. An apparatus for treating dry eye conditions comprising:

a pair of soft, pliable, curved lenses, each of said lenses maintained within a soft, pliable frame;

a soft, pliable gasket on a back portion of each of said frames, said gasket designed to substantially encircle and contact the orbital bones of an eye socket of the wearer;

a bridge coupling said frames;

said apparatus adapted and constructed to increase or maintain the humidity around the eyes of the wearer by reducing the evaporation of natural or artificial tears, or added moisture and by increasing or maintaining the temperature around the eyes of the wearer.

25. A method for treating dry eye conditions comprising:

providing an apparatus of soft, pliable materials and designed and constructed to substantially encircle and contact the orbital bones of an eye socket of the wearer, and

placing said apparatus on a sufferer of dry eye conditions for an effective amount of time.

26. The method according to claim 25, further comprising adding a moisture solution to said apparatus.

27. The method according to claim 25, further comprising providing a moisture pad adapted and constructed to be insertable between said apparatus and the eye sockets of the wearer.

28. The method according to claim 27, further comprising moistening, heating or cooling said moisture pad.

29. The method according to claim 27, further comprising adding a medicinal solution to said moisture pad.

30. A method for administering medicine via dermal absorption comprising:

providing medicine with skin absorption properties to an apparatus adapted to be worn by a wearer proximate the eyes of the wearer;

placing said apparatus with said medicine proximate the eyes of the wearer such that said medicine can be administered proximate the eyes of the wearer.

31. The method of claim 30, wherein said apparatus comprises a gasket and wherein said medicine is administered via said gasket.

* * * * *