



US007815648B2

(12) **United States Patent**  
**Triplett et al.**

(10) **Patent No.:** **US 7,815,648 B2**  
(45) **Date of Patent:** **Oct. 19, 2010**

(54) **SURGICAL MEASUREMENT SYSTEMS AND METHODS**

3,247,000 A 4/1966 Talyor

(75) Inventors: **Daniel J. Triplett**, Providence, UT (US);  
**T. Wade Fallin**, Hyde Park, UT (US)

(Continued)

FOREIGN PATENT DOCUMENTS

(73) Assignee: **Facet Solutions, Inc.**, Hopkinton, MA (US)

CN 2386790 Y 7/2000

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(Continued)

OTHER PUBLICATIONS

(21) Appl. No.: **12/240,457**

Goh JC, et al., "Influence of PLIF cage size on lumbar spine stability", Spine, Jan. 2000 25:1, PubMed abstract.

(22) Filed: **Sep. 29, 2008**

(Continued)

(65) **Prior Publication Data**

US 2009/0024135 A1 Jan. 22, 2009

**Related U.S. Application Data**

(60) Division of application No. 10/989,971, filed on Nov. 15, 2004, now Pat. No. 7,588,578, which is a continuation-in-part of application No. 10/860,778, filed on Jun. 2, 2004, now Pat. No. 7,588,590, which is a continuation-in-part of application No. 10/860,543, filed on Jun. 2, 2004, which is a continuation-in-part of application No. 10/860,495, filed on Jun. 2, 2004, which is a continuation-in-part of application No. 10/860,487, filed on Jun. 2, 2004.

*Primary Examiner*—Eduardo C Robert

*Assistant Examiner*—Elana B Fisher

(74) *Attorney, Agent, or Firm*—Peter K Johnson; James Larson; G. Jo Hays

(57) **ABSTRACT**

A measurement tool is designed to measure the relative displacements between two bony landmarks of a spine, such as pedicles and facet surfaces. The measurement tool may have a registration interface designed to be registered to a first bony landmark, and a contact feature shaped to contact a second bony landmark. The registration interface may be registered to a frame rigidly coupled relative to the first bony landmark. The measurement tool also has a displacement structure that permits motion of the contact feature relative to the registration interface along multiple dimensions. The displacement structure may have two or three sliding joints that enable relative translation along orthogonal axes. Each sliding joint may have a rod with a plurality of markings that can easily be read to acquire measurement from the displacement structure.

(51) **Int. Cl.**  
**A61B 17/58** (2006.01)

(52) **U.S. Cl.** ..... **606/102**

(58) **Field of Classification Search** ..... **606/247,**  
**606/102**


See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,677,369 A 5/1954 Knowies

**18 Claims, 48 Drawing Sheets**

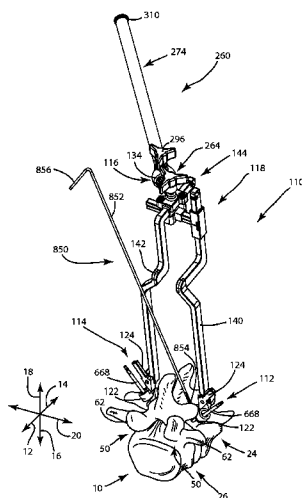

U.S. PATENT DOCUMENTS					
3,298,372 A	1/1967	Feinberg	5,366,455 A	11/1994	Dove et al.
3,426,364 A	2/1969	Lumb	5,370,697 A	12/1994	Baumgartner
3,486,505 A	12/1969	Gordon	5,375,823 A	12/1994	Navas
3,508,954 A	4/1970	Rudolph et al.	5,387,213 A	2/1995	Breard et al.
3,648,691 A	3/1972	Lumb et al.	5,391,168 A	2/1995	Sanders et al.
3,857,642 A	12/1974	Miller	5,401,269 A	3/1995	Buttner-Janz et al.
3,857,643 A	12/1974	Bardocz	5,415,661 A	5/1995	Holmes
3,867,728 A	2/1975	Stubstad et al.	5,437,669 A	8/1995	Yuan et al.
3,875,595 A	4/1975	Froning	5,437,672 A	8/1995	Alleyne
4,003,376 A	1/1977	McKay	5,439,464 A	8/1995	Shapiro
4,092,078 A	5/1978	Klotz et al.	5,443,516 A	8/1995	Albrektsson et al.
4,175,555 A	11/1979	Herbert	5,456,722 A	10/1995	McLeod et al.
4,271,836 A *	6/1981	Bacal et al. .... 606/86 A	5,458,641 A	10/1995	Ramirez Jimenez
4,289,123 A	9/1981	Dunn	5,458,642 A	10/1995	Beer et al.
4,349,921 A	9/1982	Kuntz	5,458,643 A	10/1995	Oka et al.
4,369,769 A	1/1983	Edwards	5,464,439 A	11/1995	Gendler
4,479,491 A	10/1984	Martin	5,470,333 A	11/1995	Ray
4,483,334 A	11/1984	Murray	5,474,551 A	12/1995	Finn
4,501,269 A	2/1985	Bagby	5,476,463 A	12/1995	Boachie-Adjei et al.
4,554,914 A	11/1985	Kapp et al.	5,480,401 A	1/1996	Navas
4,599,086 A	7/1986	Doty	5,486,174 A	1/1996	Fournet-Fayard
4,604,995 A	8/1986	Stephens et al.	5,489,308 A	2/1996	Kuslich et al.
4,611,581 A	9/1986	Steffee	5,496,318 A	3/1996	Howland et al.
4,641,636 A	2/1987	Cotrel	5,501,684 A	3/1996	Schlapfer
4,653,481 A	3/1987	Howland et al.	5,507,745 A	4/1996	Logroscino et al.
4,657,550 A	4/1987	Daher	5,507,813 A	4/1996	Dowd et al.
4,696,290 A	9/1987	Steffee	5,514,180 A	5/1996	Heggeness et al.
4,743,260 A	5/1988	Burton	5,522,899 A	6/1996	Michelson
4,759,769 A	7/1988	Hedman et al.	5,527,312 A	6/1996	Ray
4,772,287 A	9/1988	Ray et al.	5,531,745 A	7/1996	Ray
4,790,303 A	12/1988	Steffee	5,531,747 A	7/1996	Ray
4,800,874 A	1/1989	David et al.	5,534,028 A	7/1996	Bao et al.
4,805,602 A	2/1989	Puno et al.	5,534,030 A	7/1996	Navarro et al.
4,827,918 A	5/1989	Olerud	5,534,031 A	7/1996	Matsuzaki et al.
4,863,476 A	9/1989	Shepperd	5,540,688 A	7/1996	Navas
4,863,477 A	9/1989	Monson	5,545,166 A	8/1996	Howland
4,892,545 A	1/1990	Day et al.	5,545,229 A	8/1996	Parsons et al.
4,904,260 A	2/1990	Ray et al.	5,549,607 A	8/1996	Olson et al.
4,911,718 A	3/1990	Lee et al.	5,556,431 A	9/1996	Buttner-Janz
4,946,458 A	8/1990	Harms et al.	5,556,687 A	9/1996	McMillin
4,955,908 A	9/1990	Frey et al.	5,562,735 A	10/1996	Margulies
5,011,484 A	4/1991	Breard	5,562,736 A	10/1996	Ray et al.
5,015,255 A	5/1991	Kuslich	5,562,737 A	10/1996	Graf
5,047,055 A	9/1991	Bao et al.	5,569,248 A	10/1996	Mathews
5,053,034 A	10/1991	Olerud	5,571,189 A	11/1996	Kuslich
5,071,437 A	12/1991	Steffee	5,571,191 A	11/1996	Fitz
5,092,866 A	3/1992	Breard et al.	5,572,191 A	11/1996	Lundberg
5,092,867 A	3/1992	Harms et al.	5,582,612 A	12/1996	Lin
5,092,893 A	3/1992	Smith	5,584,832 A	12/1996	Schlapfer
5,127,912 A	7/1992	Ray et al.	5,603,713 A	2/1997	Aust et al.
5,129,900 A	7/1992	Asher et al.	5,609,634 A	3/1997	Voydeville
5,147,361 A	9/1992	Ojima et al.	5,645,597 A	7/1997	Krapiva
5,147,404 A	9/1992	Downey	5,645,599 A	7/1997	Samani
5,171,279 A	12/1992	Mathews	5,649,926 A	7/1997	Howland
5,171,280 A	12/1992	Baumgartner	5,653,762 A	8/1997	Pisharodi
5,180,393 A	1/1993	Commarmond	5,666,243 A	9/1997	Brent
5,192,326 A	3/1993	Bao et al.	5,672,175 A	9/1997	Martin
5,236,460 A	8/1993	Barber	5,674,295 A	10/1997	Ray et al.
5,246,458 A	9/1993	Graham	5,674,296 A	10/1997	Bryan
5,258,031 A	11/1993	Salib et al.	5,676,701 A	10/1997	Yuan et al.
5,261,910 A	11/1993	Warden et al.	5,681,310 A	10/1997	Yuan et al.
5,263,953 A	11/1993	Bagby	5,683,464 A	11/1997	Wagner et al.
5,282,863 A	2/1994	Burton	5,683,465 A	11/1997	Shinn et al.
5,304,178 A	4/1994	Stahurski	5,688,272 A	11/1997	Montague et al.
5,306,275 A	4/1994	Bryan	5,690,629 A	11/1997	Asher et al.
5,306,308 A	4/1994	Gross et al.	5,702,392 A	12/1997	Wu et al.
5,306,309 A	4/1994	Wagner et al.	5,702,450 A	12/1997	Bisserie
5,313,962 A	5/1994	Obenchain	5,702,453 A	12/1997	Rabbe et al.
5,318,567 A	6/1994	Vichard	5,704,936 A	1/1998	Mazel
5,329,933 A	7/1994	Graf	5,713,900 A	2/1998	Benzel et al.
5,360,430 A	11/1994	Lin	5,716,415 A	2/1998	Steffee
			5,725,582 A	3/1998	Bevan et al.
			5,728,097 A	3/1998	Mathews

5,735,899 A	4/1998	Schwartz et al.	6,413,259 B1	7/2002	Lyons et al.
5,749,873 A	5/1998	Fairley	6,419,676 B1	7/2002	Zucherman et al.
5,755,796 A	5/1998	Ibo et al.	6,419,677 B2	7/2002	Zucherman et al.
5,772,661 A	6/1998	Michelson	6,419,703 B1	7/2002	Fallin et al.
5,797,909 A	8/1998	Michelson	6,419,704 B1	7/2002	Ferree
5,814,046 A	9/1998	Hopf	6,428,544 B1	8/2002	Ralph
5,824,093 A	10/1998	Ray et al.	6,436,102 B1	8/2002	Ralph
5,824,094 A	10/1998	Serhan et al.	6,440,169 B1	8/2002	Elberg et al.
5,836,948 A	11/1998	Zucherman et al.	6,447,546 B1	9/2002	Bramlet et al.
5,860,977 A	1/1999	Zucherman et al.	6,447,548 B1	9/2002	Ralph
5,865,846 A	2/1999	Bryan et al.	6,451,019 B1	9/2002	Zucherman et al.
5,868,745 A	2/1999	Alleyne	6,451,020 B1	9/2002	Zucherman et al.
5,876,404 A	3/1999	Zucherman et al.	6,451,021 B1	9/2002	Ralph
5,888,223 A	3/1999	Bray, Jr.	6,458,131 B1	10/2002	Ray
5,893,889 A	4/1999	Harrington	6,461,359 B1	10/2002	Tribus et al.
RE36,221 E	6/1999	Breard et al.	6,468,310 B1	10/2002	Ralph
5,916,267 A	6/1999	Tienboon	6,471,704 B2	10/2002	Gertzbein et al.
5,951,555 A	9/1999	Rehak et al.	6,471,725 B1	10/2002	Ralph
5,961,516 A	10/1999	Graf	6,475,219 B1	11/2002	Shelokov
5,986,169 A	11/1999	Gjunter	6,478,796 B2	11/2002	Zucherman et al.
5,989,291 A	11/1999	Ralph	6,478,801 B1	11/2002	Ralph
6,001,130 A	12/1999	Bryan et al.	6,481,440 B2	11/2002	Gielen et al.
6,004,322 A	12/1999	Bernstein	6,485,518 B1	11/2002	Cornwall et al.
6,014,588 A	1/2000	Fitz	6,500,178 B2	12/2002	Zucherman et al.
6,019,759 A	2/2000	Rogozinski	6,514,239 B2	2/2003	Shimmura
6,019,792 A	2/2000	Cauthen	6,514,256 B2	2/2003	Zucherman et al.
6,039,761 A	3/2000	Li et al.	6,527,806 B2	3/2003	Ralph et al.
6,039,763 A	3/2000	Shelokov	6,540,747 B1	4/2003	Marino
6,048,342 A	4/2000	Zucherman et al.	6,540,785 B1	4/2003	Gill et al.
6,063,088 A	5/2000	Winslow	6,554,864 B2	4/2003	Ralph
6,063,090 A	5/2000	Schlapfer	6,562,047 B2	5/2003	Ralph
6,063,121 A	5/2000	Xavier et al.	6,565,605 B2	5/2003	Goble et al.
6,066,325 A	5/2000	Wallace et al.	6,579,319 B2	6/2003	Goble et al.
6,068,630 A	5/2000	Zucherman et al.	6,582,433 B2	6/2003	Yun
RE36,758 E	6/2000	Fitz	6,585,769 B1	7/2003	Muhanna et al.
6,074,390 A	6/2000	Zucherman et al.	6,607,559 B2	8/2003	Ralph
6,080,157 A	6/2000	Cathro et al.	6,610,091 B1	8/2003	Reiley
6,090,110 A	7/2000	Metz-Stavenhagen	6,610,092 B2	8/2003	Ralph
6,090,112 A	7/2000	Zucherman et al.	6,616,669 B2	9/2003	Ogilvie et al.
6,093,205 A	7/2000	McLeod et al.	6,623,525 B2	9/2003	Ralph
6,113,637 A	9/2000	Gill et al.	6,626,909 B2	9/2003	Chin
6,113,639 A	9/2000	Ray et al.	6,626,944 B1	9/2003	Taylor
6,132,464 A	10/2000	Martin	6,645,249 B2	11/2003	Ralph
6,132,465 A	10/2000	Ray et al.	6,652,527 B2	11/2003	Zucherman et al.
6,146,421 A	11/2000	Gordon et al.	6,652,534 B2	11/2003	Zucherman et al.
6,149,652 A	11/2000	Zucherman et al.	6,652,585 B2	11/2003	Lange
6,151,934 A	11/2000	Chong et al.	6,669,729 B2	12/2003	Chin
6,152,926 A	11/2000	Zucherman et al.	6,669,730 B2	12/2003	Ralph
6,156,038 A	12/2000	Zucherman et al.	6,669,731 B2	12/2003	Ralph
6,156,067 A	12/2000	Bryan et al.	6,673,113 B2	1/2004	Ralph
6,176,861 B1	1/2001	Bernstein et al.	6,695,842 B2	2/2004	Zucherman et al.
6,179,838 B1	1/2001	Fiz	6,699,246 B2	3/2004	Zucherman et al.
6,183,471 B1	2/2001	Zucherman et al.	6,699,247 B2	3/2004	Zucherman et al.
6,187,005 B1	2/2001	Brace	6,706,068 B2	3/2004	Ferree
6,190,387 B1	2/2001	Zucherman et al.	6,723,127 B2	4/2004	Ralph
6,190,414 B1	2/2001	Young et al.	6,733,534 B2	5/2004	Sherman
6,206,882 B1	3/2001	Cohen	6,740,117 B2	5/2004	Ralph
6,206,922 B1	3/2001	Zdeblick et al.	6,740,119 B2	5/2004	Ralph
6,228,118 B1	5/2001	Gordon	6,758,861 B2	7/2004	Ralph
6,235,030 B1	5/2001	Zucherman et al.	6,761,719 B2	7/2004	Justis et al.
6,238,397 B1	5/2001	Zucherman et al.	6,761,720 B1	7/2004	Senegas
6,241,730 B1	6/2001	Alby	6,764,515 B2	7/2004	Ralph
6,264,655 B1	7/2001	Pisharodi	6,783,527 B2	8/2004	Drewry et al.
6,267,764 B1	7/2001	Elberg	6,796,983 B1	9/2004	Zucherman et al.
6,280,444 B1	8/2001	Zucherman et al.	6,805,716 B2	10/2004	Ralph
6,290,700 B1	9/2001	Schmotzer	6,811,567 B2	11/2004	Reiley
6,293,949 B1	9/2001	Justis et al.	6,827,719 B2	12/2004	Ralph
6,312,469 B1	11/2001	Gielen et al.	6,835,205 B2	12/2004	Atkinson et al.
6,314,325 B1	11/2001	Fitz	6,835,207 B2	12/2004	Zacouto et al.
6,332,882 B1	12/2001	Zucherman et al.	6,837,904 B2	1/2005	Ralph
6,332,883 B1	12/2001	Zucherman et al.	6,840,940 B2	1/2005	Ralph
6,379,355 B1	4/2002	Zucherman et al.	6,855,151 B2	2/2005	Ralph
6,402,750 B1	6/2002	Atkinson et al.	6,863,688 B2	3/2005	Ralph

6,863,689 B2	3/2005	Ralph	2001/0012938 A1	8/2001	Zucherman et al.
6,887,273 B2	5/2005	Ralph	2001/0016743 A1	8/2001	Zucherman et al.
6,887,274 B2	5/2005	Ralph	2001/0021850 A1	9/2001	Zucherman et al.
6,896,676 B2	5/2005	Zubok	2001/0031965 A1	10/2001	Zucherman et al.
6,902,580 B2	6/2005	Fallin	2001/0039452 A1	11/2001	Zucherman et al.
6,908,484 B2	6/2005	Zubok	2002/0029039 A1	3/2002	Zucherman et al.
6,918,934 B2	7/2005	Ralph	2002/0065557 A1	5/2002	Goble et al.
6,949,123 B2	9/2005	Reiley	2002/0072800 A1	6/2002	Goble et al.
6,966,930 B2	11/2005	Arnin	2002/0091446 A1	7/2002	Zucherman et al.
6,974,478 B2	12/2005	Reiley	2002/0099384 A1	7/2002	Scribner et al.
6,976,988 B2	12/2005	Ralph	2002/0111682 A1	8/2002	Ralph
6,989,032 B2	1/2006	Errico	2002/0111687 A1	8/2002	Ralph
7,011,685 B2	3/2006	Arnin	2002/0116000 A1	8/2002	Zucherman et al.
7,022,139 B2	4/2006	Errico	2002/0123806 A1	9/2002	Reiley
7,041,136 B2	5/2006	Goble	2002/0143331 A1	10/2002	Zucherman et al.
7,044,969 B2	5/2006	Errico	2002/0151895 A1	10/2002	Soboleski et al.
7,044,970 B2	5/2006	Errico	2002/0151896 A1	10/2002	Ferree
7,051,451 B2 *	5/2006	Augustino et al. .... 33/512	2002/0183746 A1	12/2002	Zucherman et al.
7,060,098 B2	6/2006	Errico	2003/0004572 A1	1/2003	Goble et al.
7,066,959 B2	6/2006	Errico	2003/0009226 A1	1/2003	Graf
D524,443 S	7/2006	Blain	2003/0014115 A1	1/2003	Ralph
7,074,237 B2	7/2006	Goble	2003/0028250 A1	2/2003	Reiley et al.
7,074,238 B2	7/2006	Stinson	2003/0040797 A1	2/2003	Fallin et al.
7,087,084 B2	8/2006	Reiley	2003/0055427 A1	3/2003	Graf
7,090,698 B2	8/2006	Goble	2003/0065330 A1	4/2003	Zucherman et al.
7,094,242 B2	8/2006	Ralph	2003/0073998 A1	4/2003	Pagliuca et al.
7,101,398 B2	9/2006	Dooris	2003/0109880 A1	6/2003	Shirado et al.
7,101,399 B2	9/2006	Errico	2003/0153912 A1	8/2003	Graf
7,115,132 B2	10/2006	Errico	2003/0171750 A1	9/2003	Chin
7,118,599 B2	10/2006	Errico	2003/0191469 A1	10/2003	Ralph
7,122,055 B2	10/2006	Ralph	2003/0191470 A1	10/2003	Ritland
7,141,069 B2	11/2006	Errico	2003/0191532 A1	10/2003	Goble
D533,277 S	12/2006	Blain	2003/0204259 A1	10/2003	Goble
7,147,664 B2	12/2006	Louis	2003/0216810 A1	11/2003	Ralph
7,153,325 B2	12/2006	Kim	2003/0220642 A1	11/2003	Freudiger
7,160,327 B2	1/2007	Errico	2003/0220643 A1	11/2003	Ferree
7,163,559 B2	1/2007	Errico	2004/0006341 A1	1/2004	Shaolian et al.
7,166,107 B2	1/2007	Anderson	2004/0006391 A1	1/2004	Reiley
7,169,182 B2	1/2007	Errico	2004/0024458 A1	2/2004	Senegas et al.
7,186,268 B2	3/2007	Errico	2004/0030402 A1	2/2004	Arnin
D539,934 S	4/2007	Blain	2004/0034420 A1	2/2004	Errico
7,198,643 B2	4/2007	Zubok	2004/0034421 A1	2/2004	Errico
7,204,853 B2	4/2007	Gordon	2004/0034422 A1	2/2004	Errico
D541,940 S	5/2007	Blain	2004/0049189 A1	3/2004	Le Couedic et al.
7,214,244 B2	5/2007	Zubok	2004/0049190 A1	3/2004	Biedermann et al.
7,223,269 B2	5/2007	Chappuis	2004/0049272 A1	3/2004	Reiley
7,223,290 B2	5/2007	Errico	2004/0049273 A1	3/2004	Reiley
7,223,291 B2	5/2007	Errico	2004/0049274 A1	3/2004	Reiley
7,235,081 B2	6/2007	Errico	2004/0049275 A1	3/2004	Reiley
7,258,699 B2	8/2007	Errico	2004/0049276 A1	3/2004	Reiley
7,261,738 B2	8/2007	Casey	2004/0049277 A1	3/2004	Reiley
7,267,688 B2	9/2007	Ferree	2004/0049278 A1	3/2004	Reiley
7,282,064 B2	10/2007	Chin	2004/0049281 A1	3/2004	Reiley
7,282,065 B2	10/2007	Kirschman	2004/0059429 A1	3/2004	Amin
7,290,347 B2	11/2007	Augustino	2004/0073215 A1	4/2004	Carli
7,291,150 B2	11/2007	Graf	2004/0073311 A1	4/2004	Ferree
7,291,171 B2	11/2007	Ferree	2004/0078082 A1	4/2004	Lange
7,316,714 B2	1/2008	Gordon	2004/0082954 A1	4/2004	Teitelbaum et al.
7,338,491 B2	3/2008	Baker	2004/0087950 A1	5/2004	Teitelbaum
7,338,527 B2	3/2008	Blatt	2004/0106995 A1	6/2004	Le Couedic et al.
7,351,261 B2	4/2008	Casey	2004/0111154 A1	6/2004	Reiley
7,354,168 B2	4/2008	Holderer	2004/0116835 A1	6/2004	Holmes
7,361,192 B2	4/2008	Doty	2004/0116927 A1	6/2004	Graf
7,361,196 B2	4/2008	Fallin	2004/0117017 A1	6/2004	Pasquet et al.
7,371,238 B2	5/2008	Soboleski	2004/0122427 A1	6/2004	Holmes
7,377,942 B2	5/2008	Berry	2004/0127989 A1	7/2004	Dooris et al.
7,387,643 B2	6/2008	Michelson	2004/0143264 A1	7/2004	Mcafee
7,393,361 B2	7/2008	Zubok	2004/0143331 A1	7/2004	Errico
7,396,360 B2	7/2008	Lieberman	2004/0147928 A1	7/2004	Landry et al.
D574,495 S	8/2008	Petersen	2004/0148027 A1	7/2004	Errico
D574,957 S	8/2008	Petersen	2004/0153071 A1	8/2004	Zucherman et al.
7,406,775 B2	8/2008	Funk	2004/0153158 A1	8/2004	Errico
2001/0007073 A1	7/2001	Zucherman et al.	2004/0158245 A1	8/2004	Chin

2004/0167520	A1	8/2004	Zucherman et al.	2005/0228498	A1	10/2005	Andres
2004/0172025	A1	9/2004	Drewry et al.	2005/0228500	A1	10/2005	Kim
2004/0181282	A1	9/2004	Zucherman et al.	2005/0234551	A1	10/2005	Fallin
2004/0181285	A1	9/2004	Simonson	2005/0234552	A1	10/2005	Reiley
2004/0186475	A1	9/2004	Falahee	2005/0235508	A1	10/2005	Augustino
2004/0193272	A1	9/2004	Zubok	2005/0240264	A1	10/2005	Tokish, Jr.
2004/0204718	A1	10/2004	Hoffman	2005/0240265	A1	10/2005	Kuiper
2004/0220568	A1	11/2004	Zucherman et al.	2005/0240266	A1	10/2005	Kuiper
2004/0225289	A1	11/2004	Biedermann et al.	2005/0246022	A1	11/2005	Zubok
2004/0230192	A1	11/2004	Graf	2005/0251256	A1	11/2005	Reiley
2004/0230201	A1	11/2004	Yuan et al.	2005/0256578	A1	11/2005	Blatt
2004/0230304	A1	11/2004	Yuan et al.	2005/0261770	A1	11/2005	Kuiper
2004/0236327	A1	11/2004	Paul et al.	2005/0267579	A1	12/2005	Reiley
2004/0236328	A1	11/2004	Paul et al.	2005/0273167	A1	12/2005	Triplett
2004/0236329	A1	11/2004	Panjabi	2005/0273171	A1	12/2005	Gordon
2004/0243239	A1	12/2004	Taylor	2005/0273173	A1	12/2005	Gordon
2004/0254574	A1	12/2004	Morrison	2005/0273174	A1	12/2005	Gordon
2005/0010291	A1	1/2005	Stinson et al.	2005/0273175	A1	12/2005	Gordon
2005/0010293	A1	1/2005	Zucherman et al.	2005/0277930	A1	12/2005	Parsons
2005/0010298	A1	1/2005	Zucherman et al.	2005/0277938	A1	12/2005	Parsons
2005/0015146	A1	1/2005	Louis	2005/0278026	A1	12/2005	Gordon
2005/0027361	A1	2/2005	Reiley	2005/0283238	A1	12/2005	Reiley
2005/0033431	A1	2/2005	Gordon	2005/0283244	A1	12/2005	Gordon
2005/0033432	A1	2/2005	Gordon	2005/0283245	A1	12/2005	Gordon
2005/0033434	A1	2/2005	Berry	2005/0283247	A1	12/2005	Gordon
2005/0033439	A1	2/2005	Gordon	2006/0004448	A1	1/2006	Casey
2005/0043797	A1	2/2005	Lee	2006/0004449	A1	1/2006	Goble
2005/0043799	A1	2/2005	Reiley	2006/0004451	A1	1/2006	Goble
2005/0049705	A1	3/2005	Hale	2006/0009847	A1	1/2006	Reiley
2005/0055096	A1	3/2005	Hassam et al.	2006/0009848	A1	1/2006	Reiley
2005/0060035	A1	3/2005	Errico	2006/0009849	A1	1/2006	Reiley
2005/0070899	A1	3/2005	Doubler	2006/0036243	A1	2/2006	Sasso
2005/0071011	A1	3/2005	Ralph	2006/0036323	A1	2/2006	Carl
2005/0071013	A1	3/2005	Zubok	2006/0036324	A1	2/2006	Sachs
2005/0080486	A1	4/2005	Fallin	2006/0041311	A1	2/2006	McLeer
2005/0113927	A1	5/2005	Malek	2006/0052785	A1	3/2006	Augustino et al.
2005/0119657	A1	6/2005	Goldsmith	2006/0058787	A1	3/2006	David
2005/0119748	A1	6/2005	Reiley et al.	2006/0058790	A1	3/2006	Carl
2005/0131405	A1	6/2005	Molz, IV	2006/0058791	A1	3/2006	Broman
2005/0131406	A1*	6/2005	Reiley et al. .... 606/61	2006/0079895	A1	4/2006	McLeer
2005/0131409	A1	6/2005	Chervitz	2006/0084976	A1	4/2006	Borgstrom
2005/0131537	A1	6/2005	Hoy	2006/0084982	A1	4/2006	Kim
2005/0131538	A1	6/2005	Chervitz	2006/0084984	A1	4/2006	Kim
2005/0131545	A1	6/2005	Chervitz	2006/0084987	A1	4/2006	Kim
2005/0137705	A1	6/2005	Reiley	2006/0084991	A1	4/2006	Borgstrom
2005/0137706	A1	6/2005	Reiley	2006/0085072	A1	4/2006	Funk
2005/0143818	A1	6/2005	Yuan	2006/0085075	A1	4/2006	McLeer
2005/0149023	A1	7/2005	Ritland	2006/0085076	A1	4/2006	Krishna
2005/0149190	A1	7/2005	Reiley	2006/0089717	A1	4/2006	Krishna
2005/0154461	A1	7/2005	Humphreys	2006/0100707	A1	5/2006	Stinson
2005/0154464	A1	7/2005	Humphreys	2006/0100709	A1	5/2006	Reiley
2005/0154465	A1	7/2005	Hodges	2006/0111780	A1	5/2006	Petersen
2005/0154466	A1	7/2005	Humphreys	2006/0111781	A1	5/2006	Petersen
2005/0154467	A1	7/2005	Peterman	2006/0111782	A1	5/2006	Petersen
2005/0159746	A1	7/2005	Grob	2006/0129239	A1	6/2006	Kwak
2005/0165407	A1	7/2005	Diaz	2006/0142759	A1	6/2006	Arnin
2005/0171538	A1	8/2005	Sgier	2006/0149229	A1	7/2006	Kwak
2005/0171608	A1	8/2005	Peterman	2006/0149230	A1	7/2006	Kwak
2005/0171609	A1	8/2005	Humphreys	2006/0149239	A1	7/2006	Winslow
2005/0171610	A1	8/2005	Humphreys	2006/0149254	A1	7/2006	Laurysen
2005/0177166	A1	8/2005	Timm	2006/0149272	A1	7/2006	Winslow
2005/0177240	A1	8/2005	Blain	2006/0149289	A1	7/2006	Winslow
2005/0187537	A1	8/2005	Loeb	2006/0149373	A1	7/2006	Winslow
2005/0192572	A1	9/2005	Abdelgany	2006/0149374	A1	7/2006	Winslow
2005/0192574	A1	9/2005	Blain	2006/0149375	A1	7/2006	Yuan
2005/0197700	A1	9/2005	Boehm, Jr.	2006/0149383	A1	7/2006	Arnin
2005/0197705	A1	9/2005	Arnin	2006/0184180	A1	8/2006	Augustino
2005/0203532	A1	9/2005	Ferguson	2006/0190083	A1	8/2006	Arnin
2005/0203533	A1	9/2005	Ferguson	2006/0195192	A1	8/2006	Gordon
2005/0209694	A1	9/2005	Loeb	2006/0200137	A1	9/2006	Soboleski
2005/0209698	A1	9/2005	Gordon	2006/0200149	A1	9/2006	Hoy
2005/0222681	A1	10/2005	Richley	2006/0200239	A1	9/2006	Rothman
2005/0228497	A1	10/2005	Ferree	2006/0200240	A1	9/2006	Rothman

2006/0200241	A1	9/2006	Rothman	2007/0149976	A1	6/2007	Hale
2006/0200242	A1	9/2006	Rothman	2007/0149983	A1	6/2007	Link
2006/0200243	A1	9/2006	Rothman	2007/0156237	A1	7/2007	Kwak
2006/0212033	A1	9/2006	Rothman	2007/0162002	A1	7/2007	Tornier
2006/0212034	A1	9/2006	Triplett	2007/0167946	A1	7/2007	Triplett
2006/0217718	A1	9/2006	Chervitz	2007/0167947	A1	7/2007	Gittings
2006/0217719	A1	9/2006	Albert	2007/0168029	A1	7/2007	Yuan
2006/0217728	A1	9/2006	Chervitz	2007/0168035	A1	7/2007	Koske
2006/0217809	A1	9/2006	Albert	2007/0179616	A1	8/2007	Braddock, Jr.
2006/0229612	A1	10/2006	Rothman	2007/0179617	A1	8/2007	Brown
2006/0229616	A1	10/2006	Albert	2007/0179619	A1	8/2007	Grob
2006/0229620	A1	10/2006	Rothman	2007/0185492	A1	8/2007	Chervitz
2006/0229729	A1	10/2006	Gordon	2007/0185576	A1	8/2007	Goble
2006/0235389	A1	10/2006	Albert	2007/0191847	A1	8/2007	Arnin
2006/0235403	A1	10/2006	Blain	2007/0191945	A1	8/2007	Yu
2006/0235409	A1	10/2006	Blain	2007/0191949	A1	8/2007	Arnin
2006/0235411	A1	10/2006	Blain	2007/0198091	A1	8/2007	Boyer
2006/0235412	A1	10/2006	Blain	2007/0203494	A1	8/2007	Arnin
2006/0235518	A1	10/2006	Blain	2007/0213717	A1	9/2007	Trieu
2006/0235533	A1	10/2006	Blain	2007/0213719	A1	9/2007	Hudgins
2006/0241597	A1	10/2006	Mitchell	2007/0213720	A1	9/2007	Gordon
2006/0241642	A1	10/2006	Arnin	2007/0213724	A1	9/2007	Arnin
2006/0241758	A1	10/2006	Peterman	2007/0213822	A1	9/2007	Trieu
2006/0241769	A1	10/2006	Gordon	2007/0225813	A1	9/2007	Haines
2006/0241771	A1	10/2006	Gordon	2007/0227547	A1	10/2007	Trieu
2006/0247632	A1	11/2006	Winslow	2007/0233092	A1	10/2007	Falahee
2006/0247633	A1	11/2006	Winslow	2007/0233256	A1	10/2007	Ohrt
2006/0247635	A1	11/2006	Gordon	2007/0233262	A1	10/2007	Arnin
2006/0247650	A1	11/2006	Yerby	2007/0244483	A9	10/2007	Winslow
2006/0247769	A1	11/2006	Molz	2007/0250166	A1	10/2007	McKay
2006/0247779	A1	11/2006	Gordon	2007/0250169	A1	10/2007	Lang
2006/0259142	A1	11/2006	Dooris	2007/0255411	A1	11/2007	Reiley
2006/0259147	A1	11/2006	Krishna	2007/0265706	A1	11/2007	Reiley
2006/0264933	A1	11/2006	Baker	2007/0270865	A1	11/2007	Arnin
2006/0265069	A1	11/2006	Goble	2007/0270952	A1	11/2007	Wistrom
2006/0265070	A1	11/2006	Stinson	2007/0270959	A1	11/2007	Dubousset
2006/0265074	A1	11/2006	Krishna	2007/0270962	A1	11/2007	Arnin
2006/0271046	A1	11/2006	Kwak	2007/0270967	A1	11/2007	Fallin
2006/0271195	A1	11/2006	Thramann	2007/0270972	A1	11/2007	Gordon
2006/0276787	A1	12/2006	Zubok	2007/0282445	A1	12/2007	Reiley
2006/0276790	A1	12/2006	Dawson	2007/0282449	A1	12/2007	de Villiers
2006/0282080	A1	12/2006	Albert	2007/0288005	A1	12/2007	Arnin
2007/0016195	A1	1/2007	Winslow	2007/0288006	A1	12/2007	Arnin
2007/0016196	A1	1/2007	Winslow	2007/0288009	A1	12/2007	Brown
2007/0016218	A1	1/2007	Winslow	2007/0288094	A1	12/2007	Krishna
2007/0016296	A1	1/2007	Triplett	2007/0299446	A1	12/2007	Chin
2007/0016297	A1	1/2007	Johnson	2008/0004706	A1	1/2008	Arnin
2007/0035795	A1	2/2007	Hubbard	2008/0009881	A1	1/2008	Blatt
2007/0050032	A1	3/2007	Gittings	2008/0009947	A1	1/2008	Arnin
2007/0050033	A1	3/2007	Reo	2008/0015583	A1	1/2008	Reiley
2007/0055236	A1	3/2007	Hudgins	2008/0015585	A1	1/2008	Berg
2007/0055245	A1	3/2007	Sasso	2008/0021457	A1	1/2008	Anderson
2007/0055373	A1	3/2007	Hudgins	2008/0027543	A1	1/2008	Eisermann
2007/0073290	A1	3/2007	Boehm, Jr.	2008/0027548	A9	1/2008	Ferree
2007/0073396	A1	3/2007	Arnin	2008/0027549	A1	1/2008	Kirschman
2007/0073406	A1	3/2007	Gordon	2008/0033562	A1	2/2008	Krishna
2007/0079517	A1	4/2007	Augustino	2008/0058954	A1	3/2008	Trieu
2007/0083200	A1	4/2007	Gittings	2008/0065078	A1	3/2008	Graf
2007/0083264	A1	4/2007	Arnin	2008/0065211	A1	3/2008	Albert
2007/0083265	A1	4/2007	Malone	2008/0077137	A1	3/2008	Balderston
2007/0083266	A1	4/2007	Lang	2008/0077242	A1	3/2008	Reo
2007/0088358	A1	4/2007	Yuan	2008/0077244	A1	3/2008	Robinson
2007/0093816	A1	4/2007	Arnin	2008/0077245	A1	3/2008	Lee
2007/0093833	A1	4/2007	Kuiper	2008/0082171	A1	4/2008	Kuiper
2007/0093897	A1	4/2007	Gerbec	2008/0086213	A1	4/2008	Reiley
2007/0112351	A1	5/2007	Assell	2008/0091200	A1	4/2008	Kuiper
2007/0112428	A1	5/2007	Lancial	2008/0091201	A1	4/2008	Reiley
2007/0118118	A1	5/2007	Kwak	2008/0091202	A1	4/2008	Reiley
2007/0118218	A1	5/2007	Hooper	2008/0091204	A1	4/2008	Kuiper
2007/0123863	A1	5/2007	Winslow	2008/0091205	A1	4/2008	Kuiper
2007/0123868	A1	5/2007	Culbert	2008/0091210	A1	4/2008	Reiley
2007/0123985	A1	5/2007	Errico	2008/0091268	A1	4/2008	Reiley
2007/0135814	A1	6/2007	Farris	2008/0097437	A1	4/2008	Reiley

2008/0097438	A1	4/2008	Reiley
2008/0097439	A1	4/2008	Reiley
2008/0097440	A1	4/2008	Reiley
2008/0097446	A1	4/2008	Reiley
2008/0097609	A1	4/2008	Reiley
2008/0097612	A1	4/2008	Reiley
2008/0097613	A1	4/2008	Reiley
2008/0103501	A1	5/2008	Ralph
2008/0103512	A1	5/2008	Gately
2008/0103600	A1	5/2008	Casey
2008/0119845	A1	5/2008	Stone
2008/0125814	A1	5/2008	Yuan
2008/0125864	A1	5/2008	de Villiers
2008/0132951	A1	6/2008	Reiley
2008/0140121	A1	6/2008	McLEER
2008/0140125	A1	6/2008	Mitchell
2008/0140134	A1	6/2008	Markworth
2008/0147195	A1	6/2008	Kwak
2008/0161810	A1	7/2008	Melkent
2008/0161833	A1	7/2008	Ray
2008/0161929	A1	7/2008	McCormack
2008/0167688	A1	7/2008	Fauth
2008/0177308	A1	7/2008	McLeer
2008/0177309	A1	7/2008	McLeer
2008/0177310	A1	7/2008	Reiley
2008/0177311	A1	7/2008	Winslow
2008/0177332	A1	7/2008	Reiley
2008/0177333	A1	7/2008	Ferguson
2008/0183209	A1	7/2008	Robinson
2008/0195154	A1	8/2008	Brown
2008/0195206	A1	8/2008	Chee
2008/0195212	A1	8/2008	Nguyen
2008/0195213	A1	8/2008	Halverson
2008/0200953	A1	8/2008	Reiley
2008/0208249	A1	8/2008	Blain
2008/0208341	A1	8/2008	McCormack

FOREIGN PATENT DOCUMENTS

EP	408489	A1	1/1991
EP	322334	B1	2/1992
EP	667127	A1	8/1995
EP	767637	B1	11/1998
EP	768843	B1	2/1999
EP	669109	B1	5/1999
EP	1239785	B1	9/2004
EP	1343424	B1	9/2004
EP	1399078	B1	12/2004
FR	2721501	B1	8/1996
JP	10179622	A2	7/1998
JP	10277070	A2	10/1998
SU	1468543	A1	3/1989
SU	1517953	A1	10/1989
WO	WO8707827	A1	12/1987
WO	WO9421185	A1	9/1994
WO	WO9505783	A1	3/1995
WO	WO9505784	A1	3/1995
WO	WO9505785	A1	3/1995
WO	WO9505786	A1	3/1995
WO	WO9600049	A1	1/1996
WO	WO9822033	A1	5/1998
WO	WO9848707	A1	11/1998
WO	WO9848717	A1	11/1998
WO	WO9856301	A1	12/1998
WO	WO9905995	A1	2/1999
WO	WO9921500	A1	5/1999
WO	WO9921501	A1	5/1999
WO	WO9923963	A1	5/1999
WO	WO9965412	A1	12/1999
WO	WO9960957	A1	5/2000
WO	WO0038582		7/2000

WO	WO0062684	A1	10/2000
WO	WO0130248	A1	5/2001
WO	WO0145576	A1	6/2001
WO	WO0149192	A1	7/2001
WO	WO0156489	A1	8/2001
WO	WO0164142	A1	9/2001
WO	WO0164144	A2	9/2001
WO	WO0191657	A1	12/2001
WO	WO0191658	A1	12/2001
WO	WO0197721	A2	12/2001
WO	WO0200124	A1	1/2002
WO	WO0203882	A2	1/2002
WO	WO0207621	A1	1/2002
WO	WO0207622	A1	1/2002
WO	WO0207623	A1	1/2002
WO	WO0213732	A3	2/2002
WO	WO0230336	A2	4/2002
WO	WO0234120	A2	5/2002
WO	WO0243603	A1	6/2002
WO	WO02067792	A2	9/2002
WO	WO02067793	A2	9/2002
WO	WO02089712	A1	11/2002
WO	WO02102259	A2	12/2002
WO	WO03009737	A1	2/2003
WO	WO03011147	A1	2/2003
WO	WO03015646	A2	2/2003
WO	WO03045262	A2	6/2003
WO	WO03077806	A1	9/2003
WO	WO2004017817	A2	3/2004
WO	WO2004019762	A2	3/2004
WO	WO2004024010	A1	3/2004
WO	WO2004032794	A2	4/2004
WO	WO2004039239	A2	5/2004
WO	WO2004039243	A2	5/2004
WO	WO2004041066	A2	5/2004
WO	WO2004073533	A1	9/2004
WO	WO2004098423	A1	11/2004
WO	WO2004098452	A2	11/2004
WO	WO2004105577	A2	12/2004
WO	WO2004105580	A2	12/2004
WO	WO2005013864		2/2005
WO	WO2005037149		4/2005
WO	WO2005044152	A1	5/2005

OTHER PUBLICATIONS

Head WC, Wagner surface replacement arthroplasty of the hip. Analysis of fourteen failures in forty-one hips.; J Bone Joint Surg. [Am], Mar. 1981 63:3, PubMed Abstract.

Kotani Y, et al., "The effects of spinal fixation and destabilization on the biomechanical and histologic properties of spinal fixation and destabilization on the biomechanical and histologic properties of spinal ligaments. An in vivo study.", Spine, Mar. 15, 1998 23:6, PubMed abstract.

Lemaire JP, et al., "Intervertebral Disc Prosthesis: Results and Prospects for the Year 2000", Clinical Orthopaedics and related Research, PubMed abstract.

Nagata H, et al., "The effects of immobilization of long segments of the spine on the adjacent and distal facet force and lumbrosacral motion", Dec. 1993 18:16. PubMed abstract.

Nibu K, et al., Multidirectional stabilizing potential of BAK interbody spinal fusion system for anterior surgery, J Spinal Discord, Aug. 1997 10:4, PubMed abstract.

Tsantrizos A, et al., "Segmental stability and compressive strength of posterior lumbar interbody fusion implants", Spine, Aug. 1, 2000 25:15, PubMed abstract.

Todd Anres; *Facet Joint Arthroplasty: A Glimpse of the Future of Spine Technology*, Othopaedic Product News, Sep./Oct. 2005 p. 38, 40.

\* cited by examiner





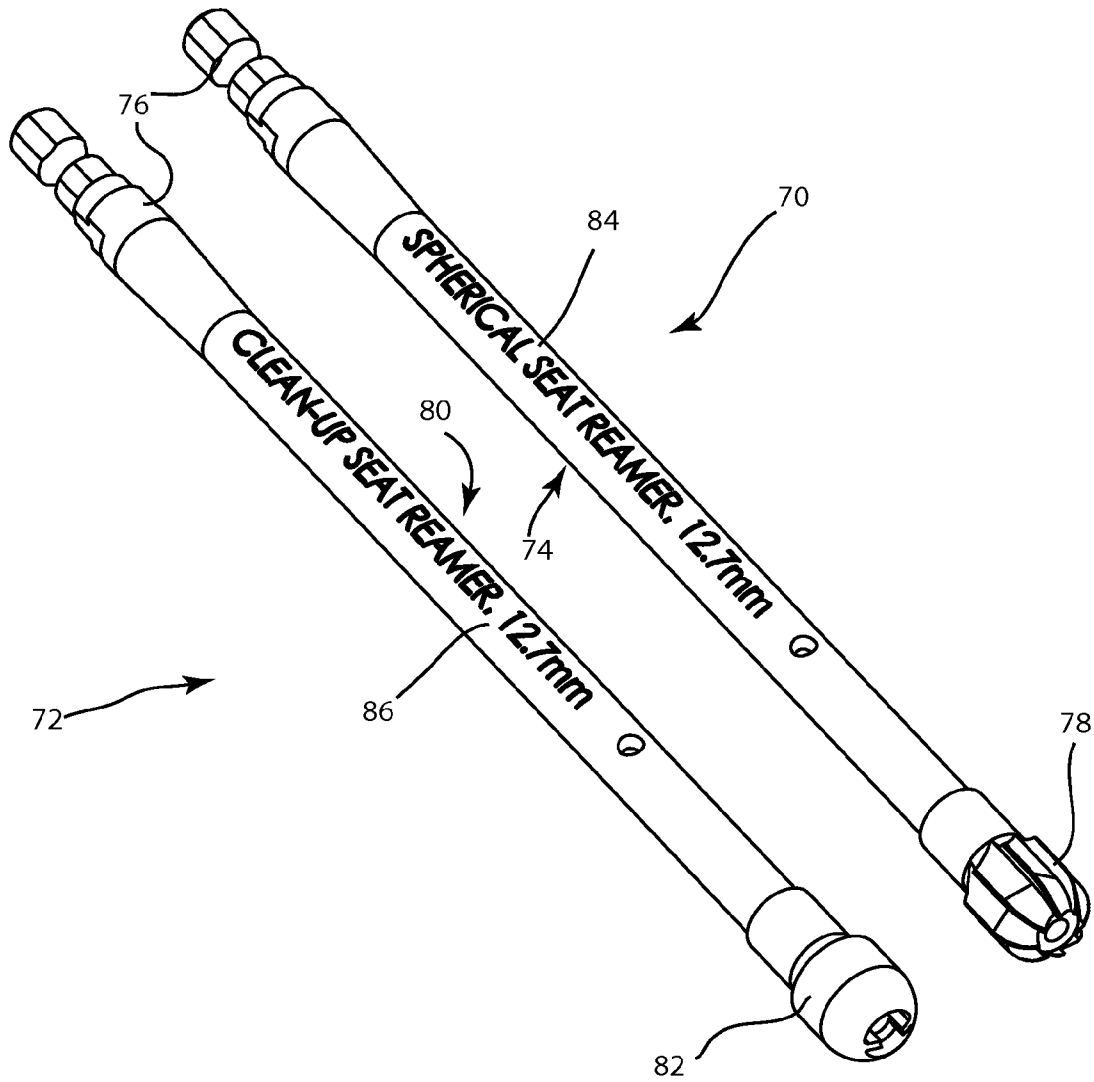


Fig. 2

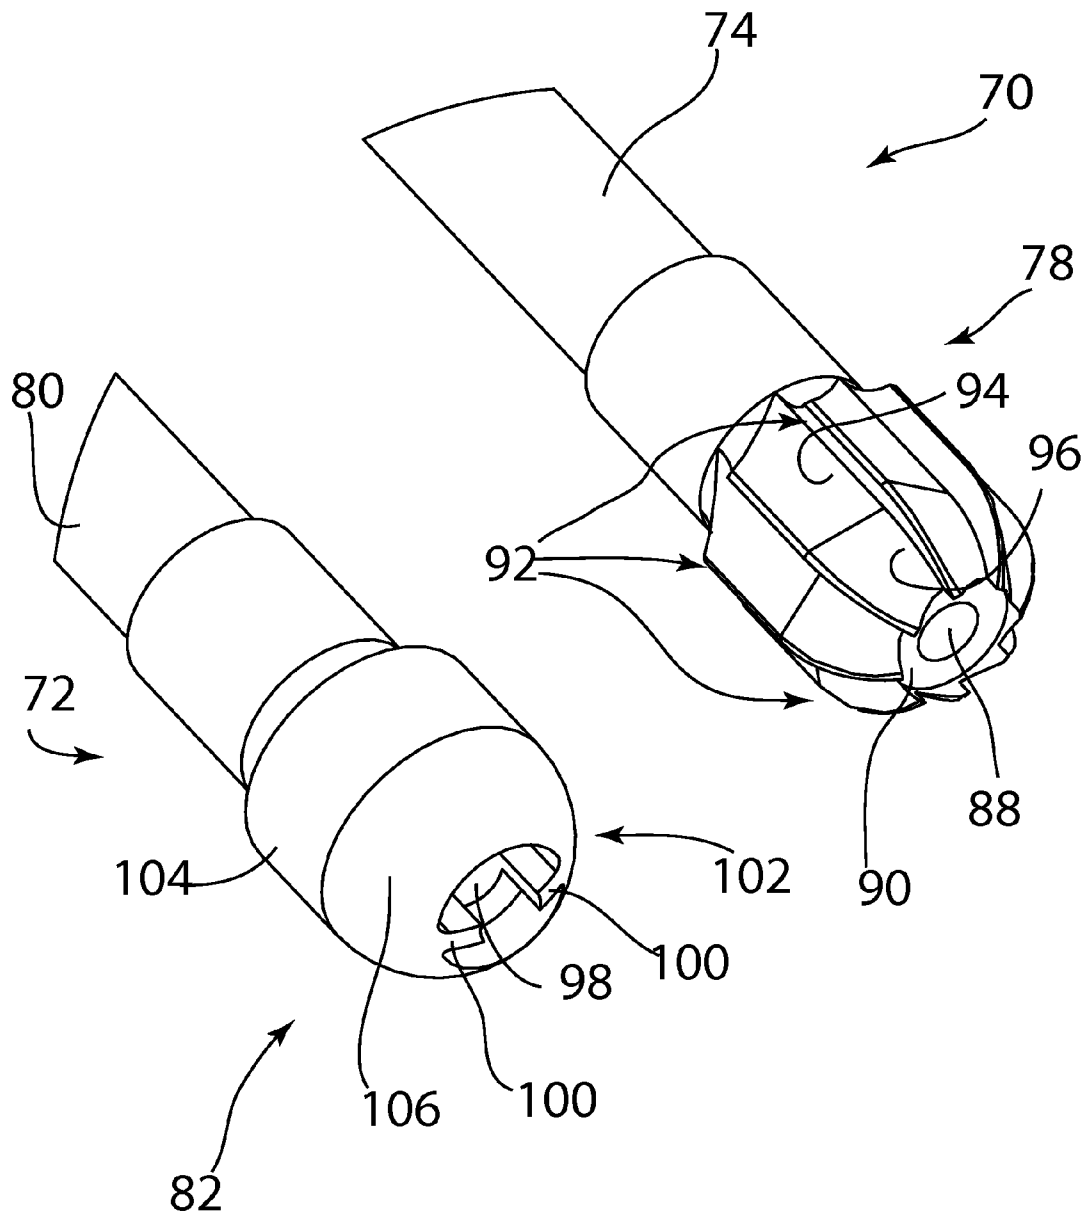


Fig. 3



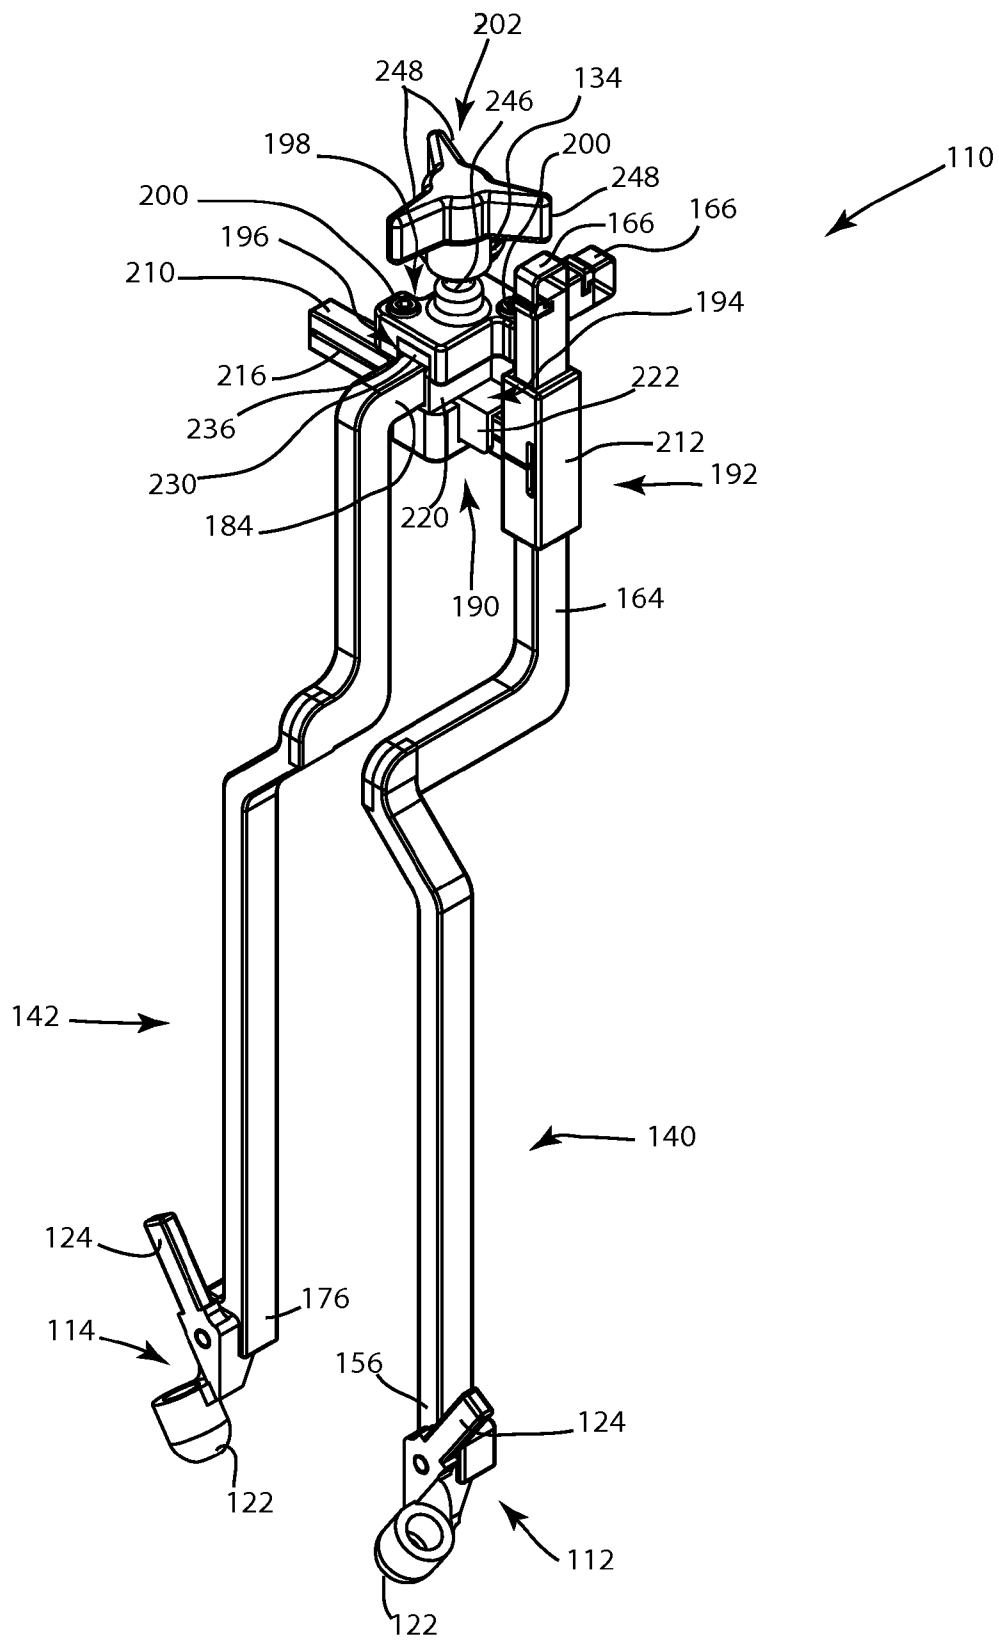


Fig. 5

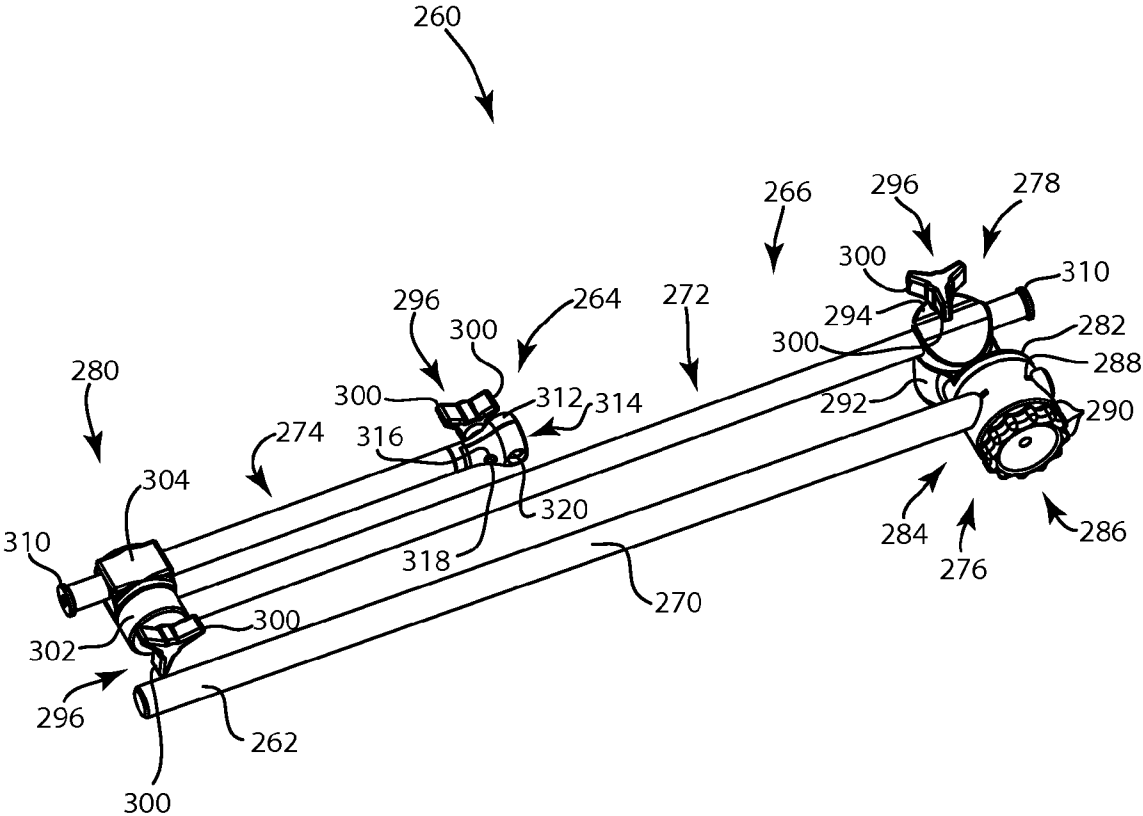


Fig. 6

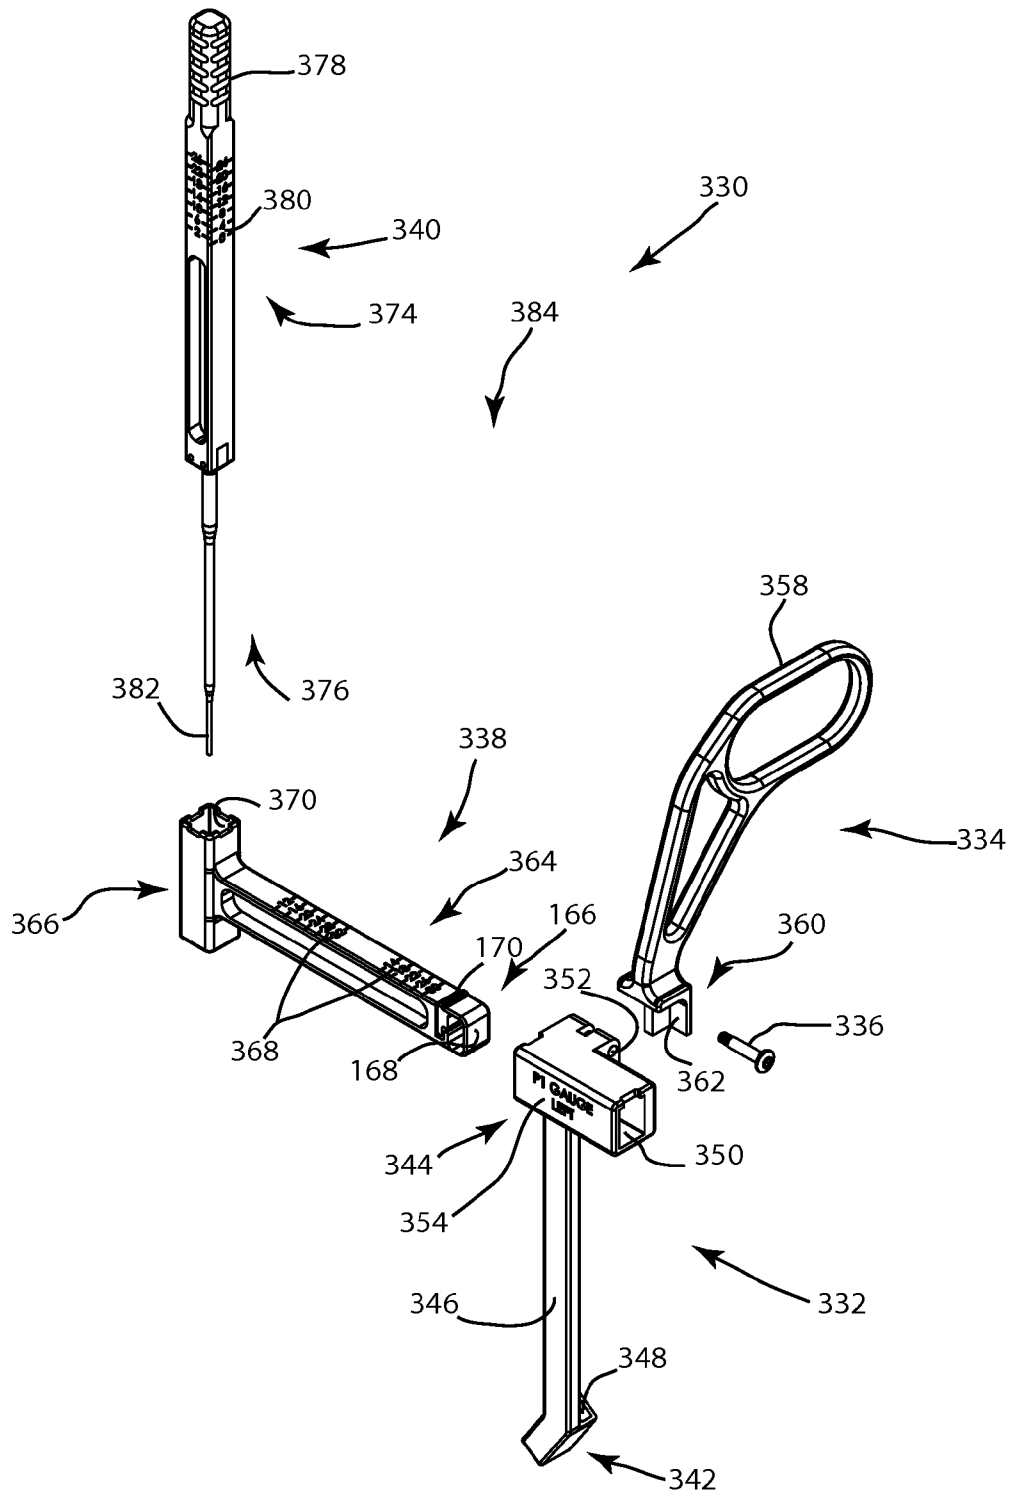


Fig. 7

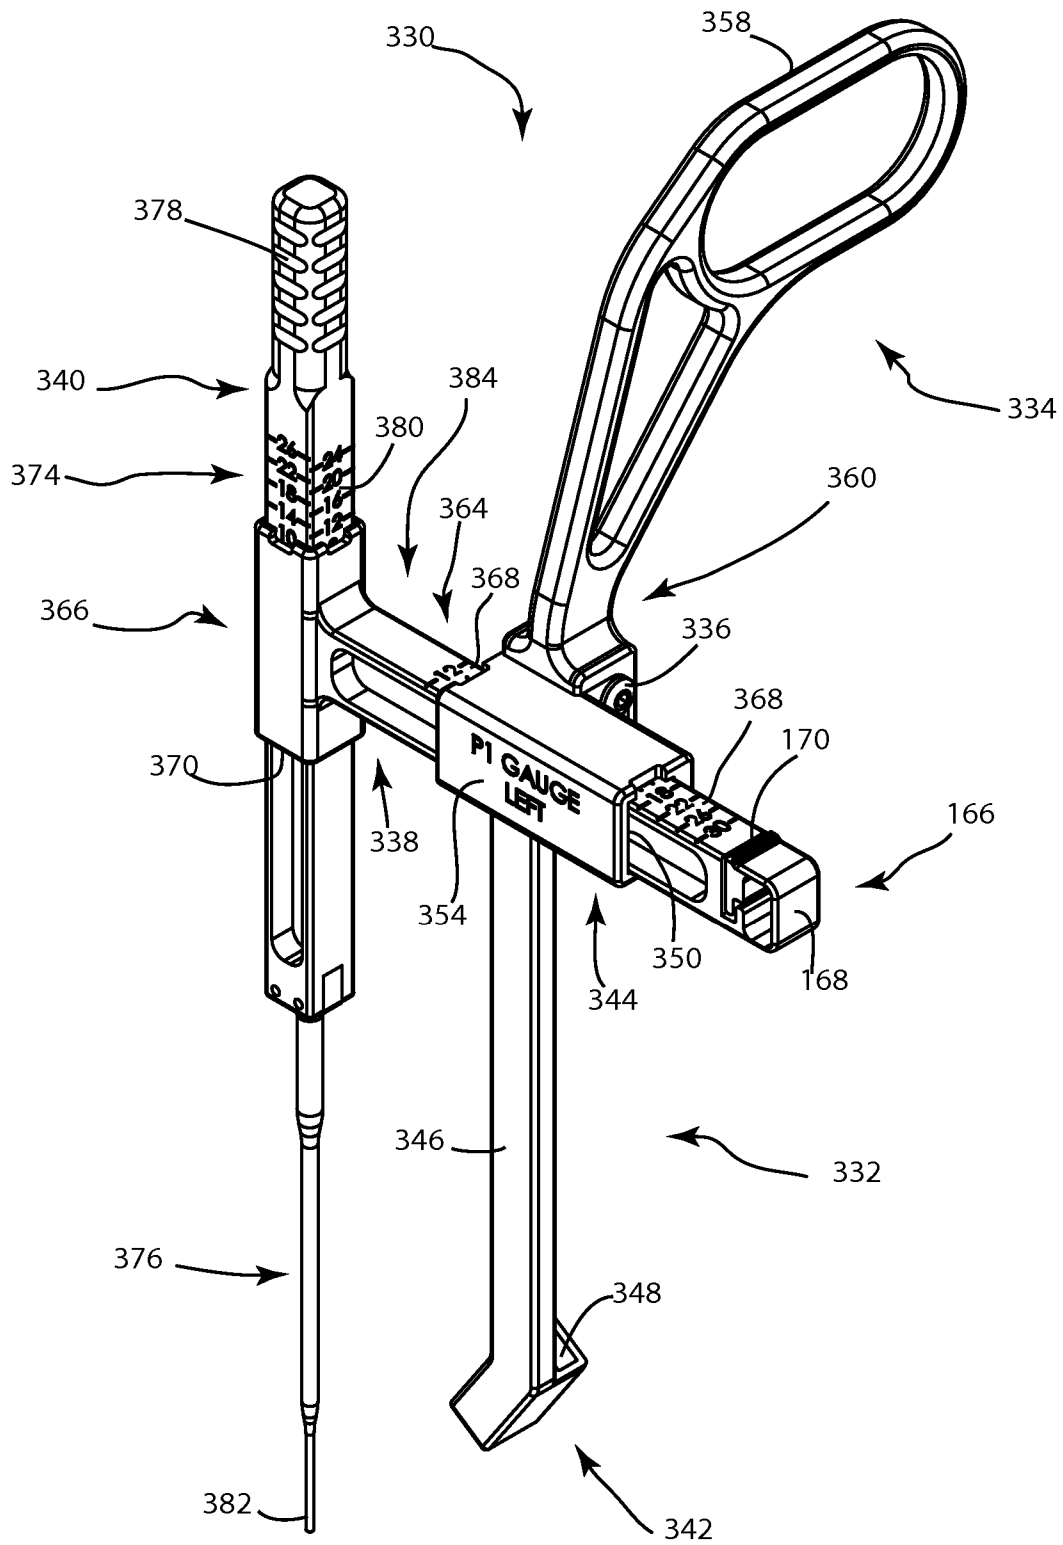


Fig. 8

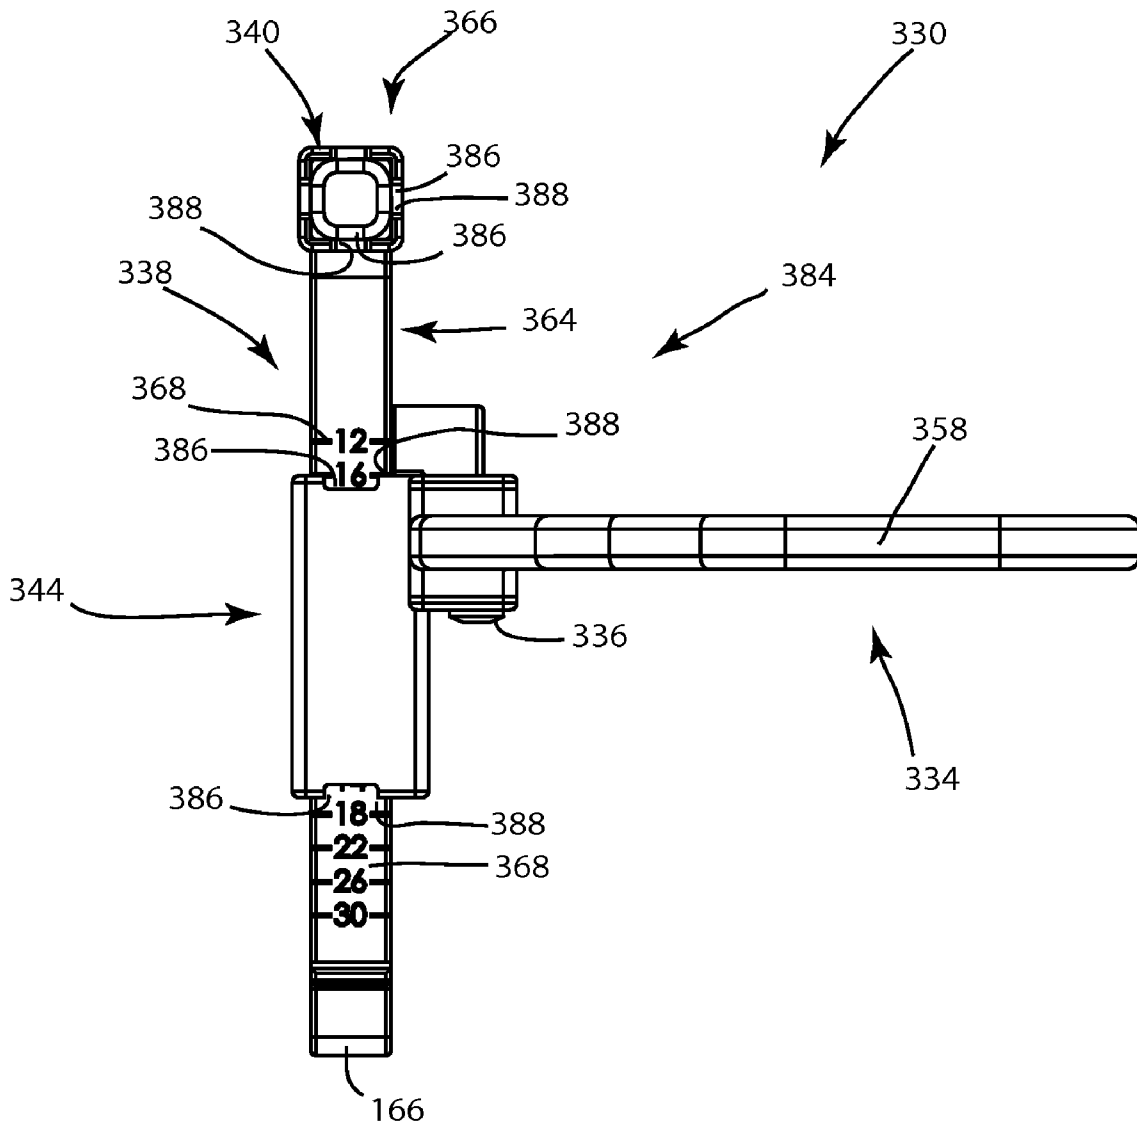


Fig. 9



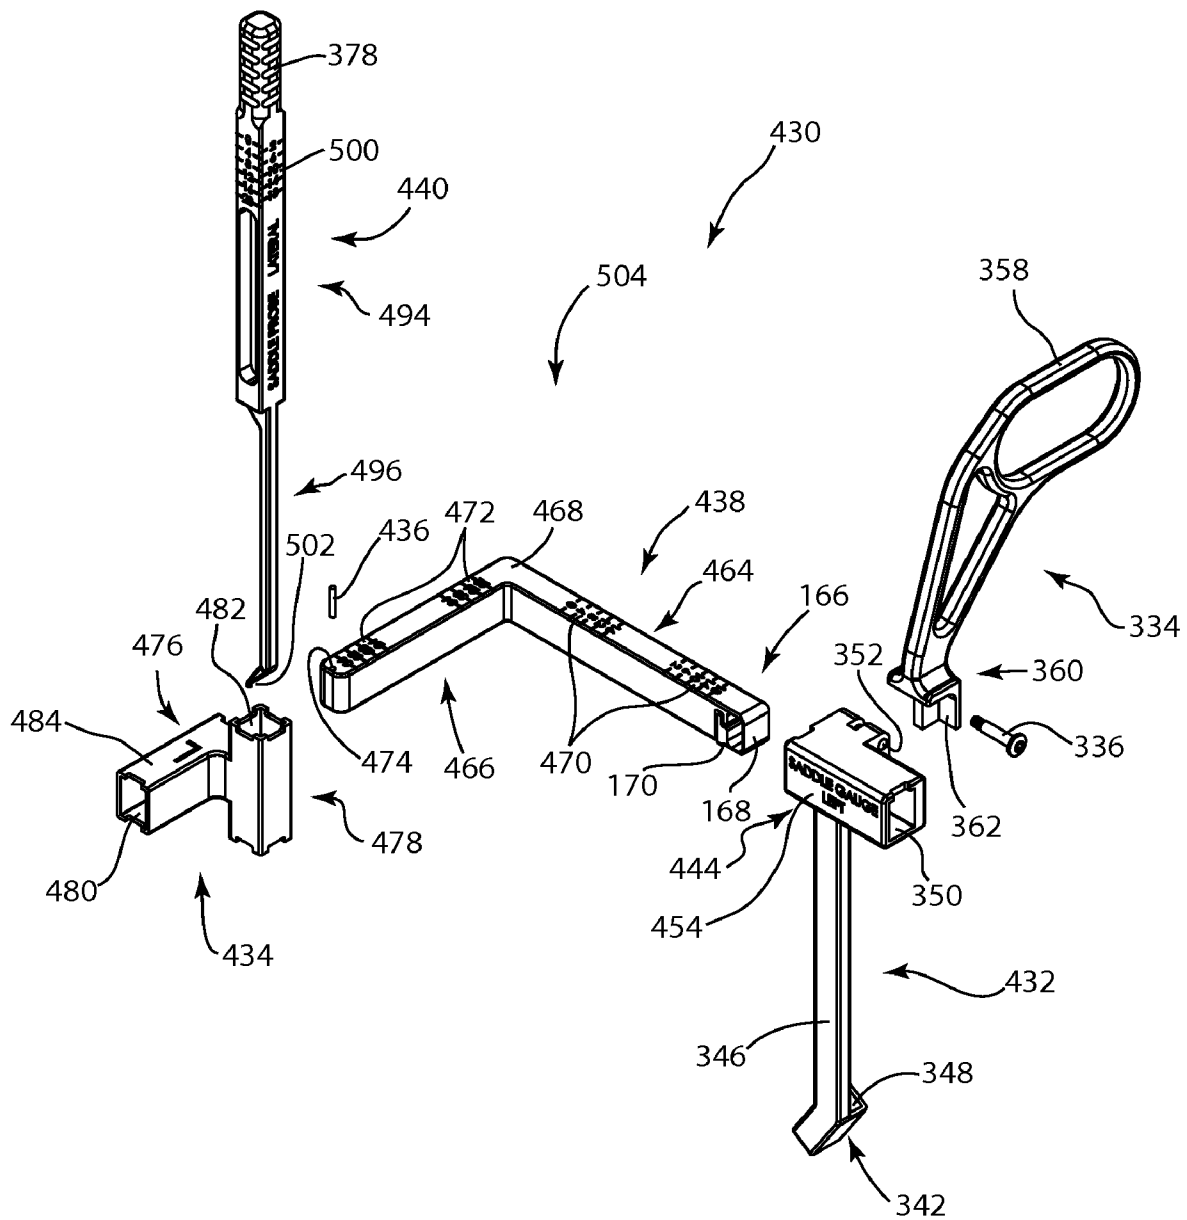


Fig. 10

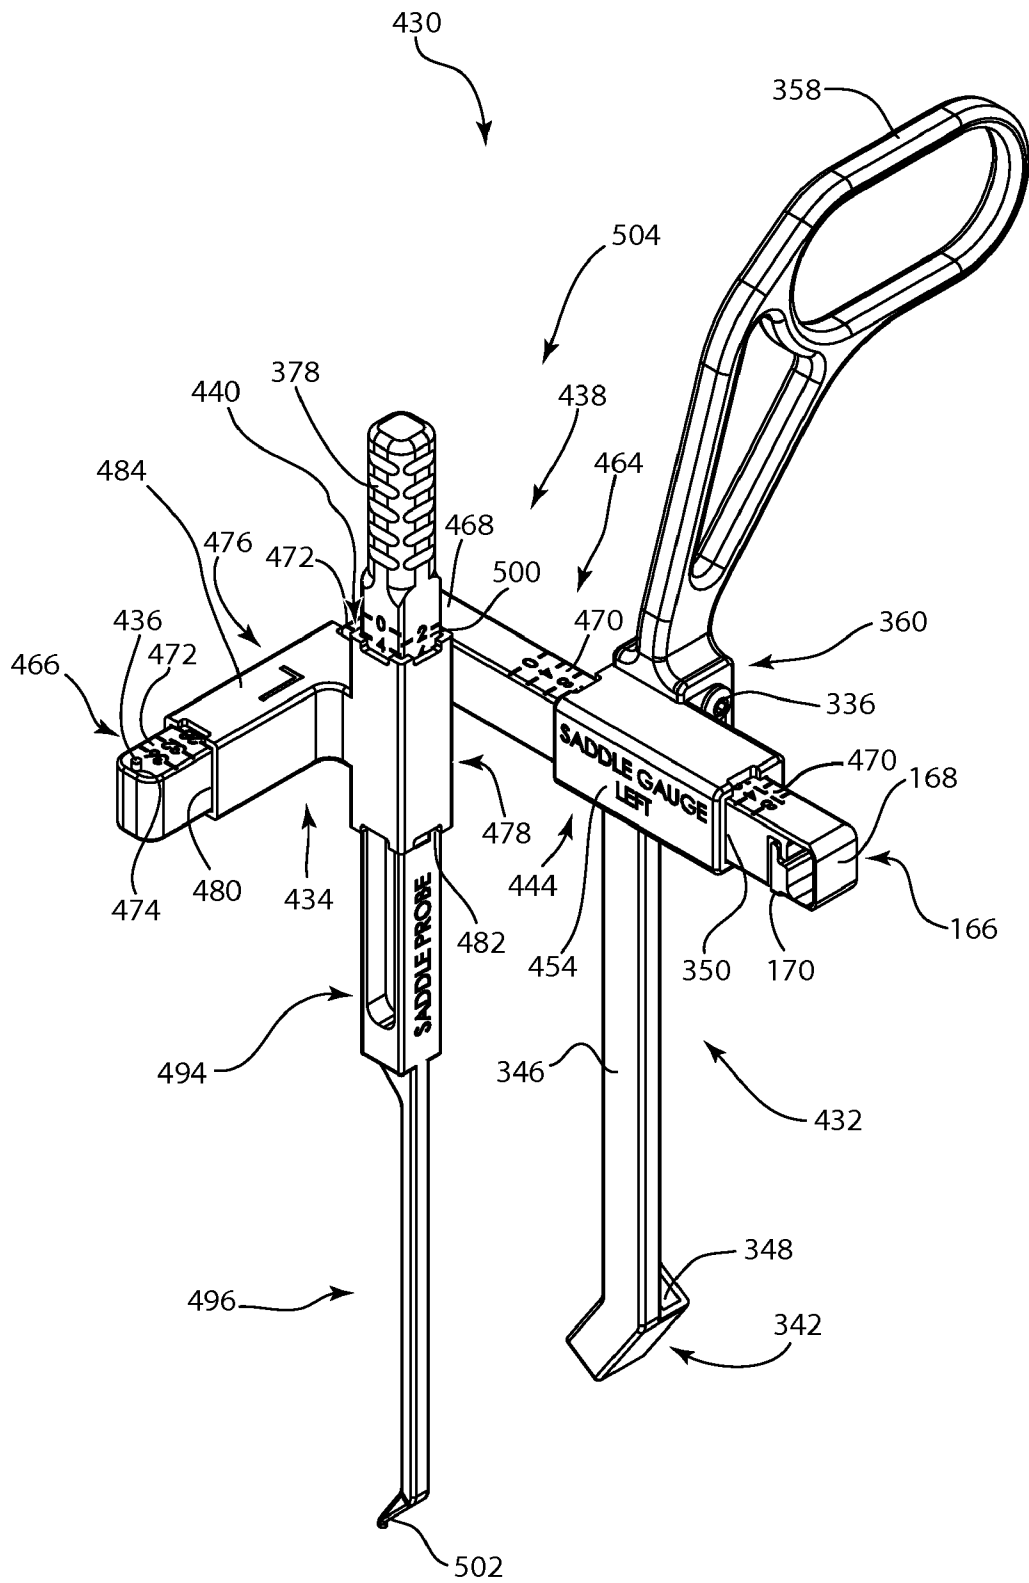


Fig. 11

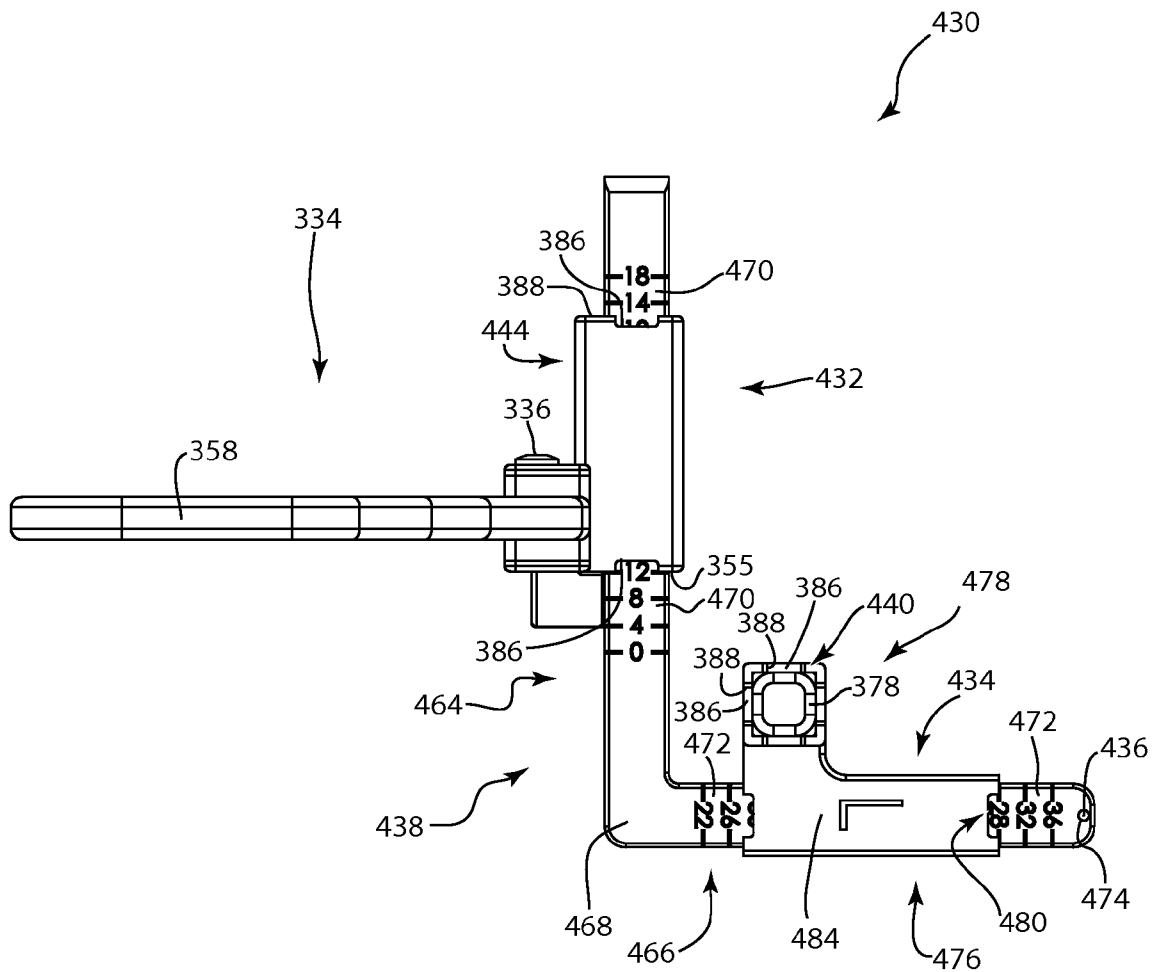


Fig. 12

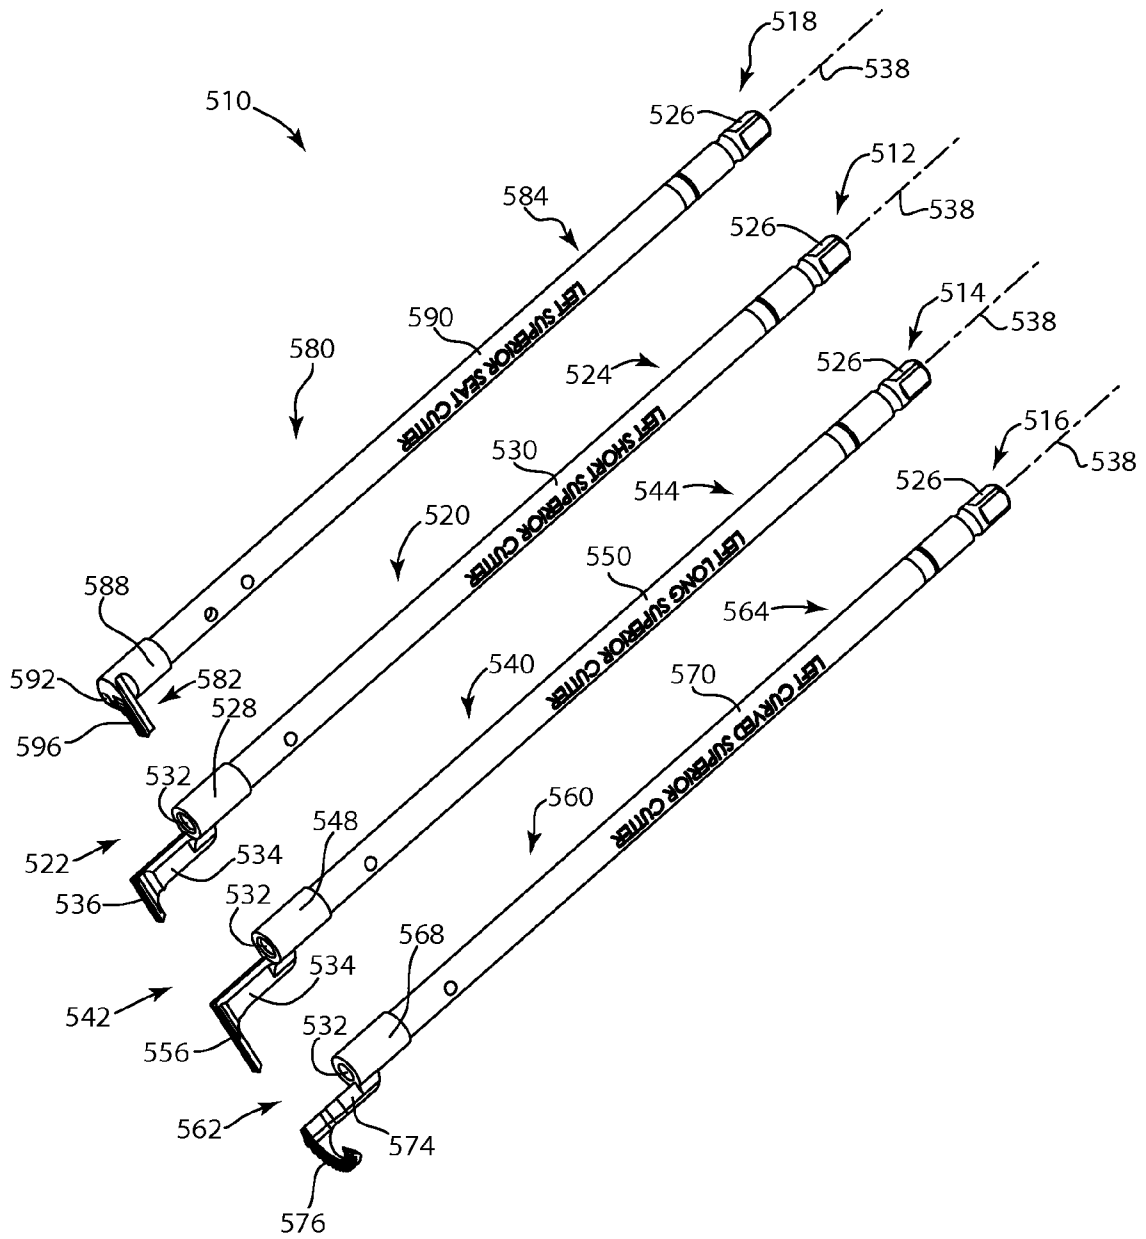


Fig. 13

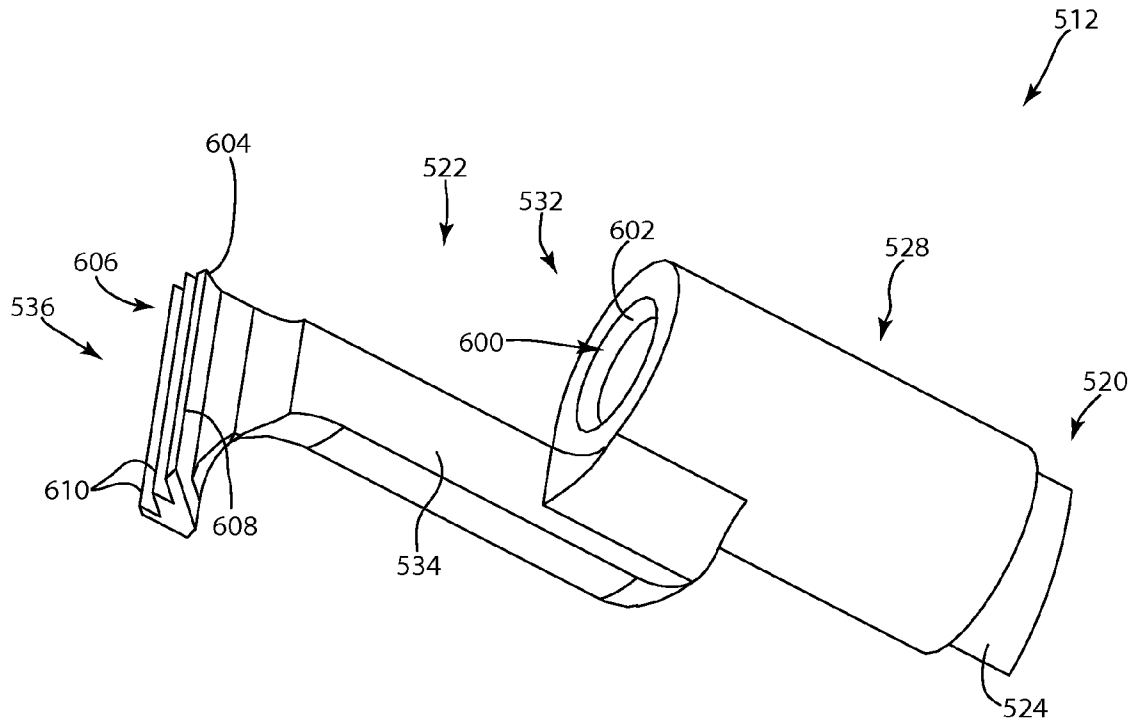


Fig. 14

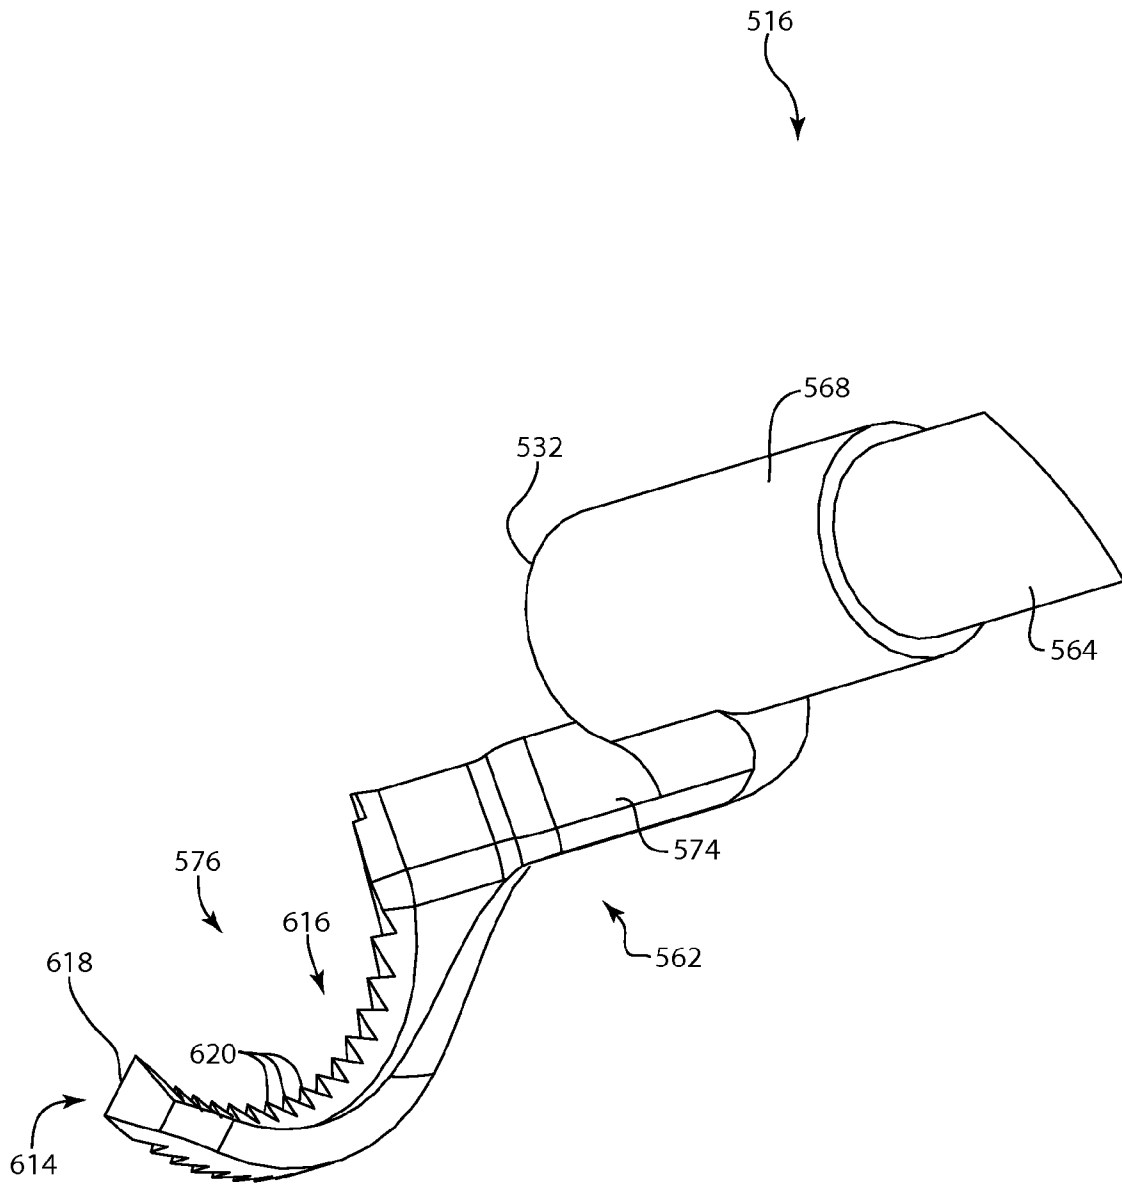


Fig. 15

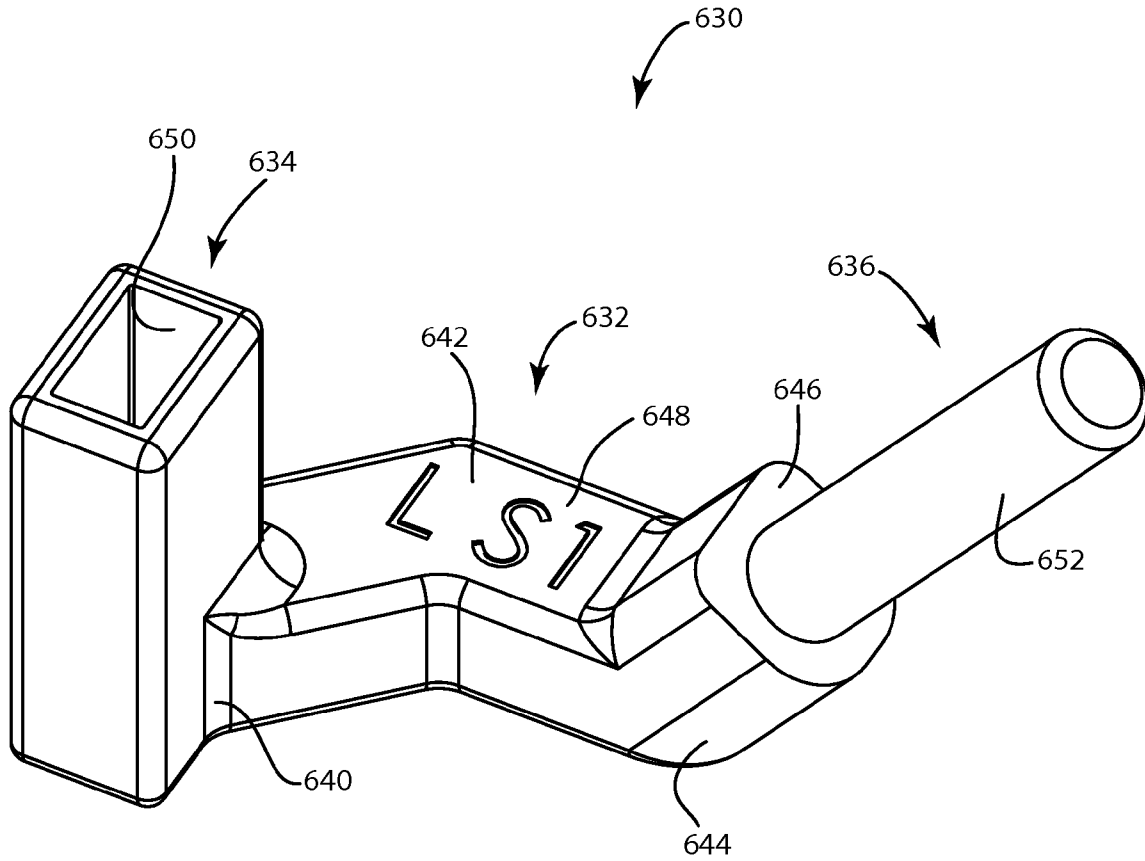


Fig. 16

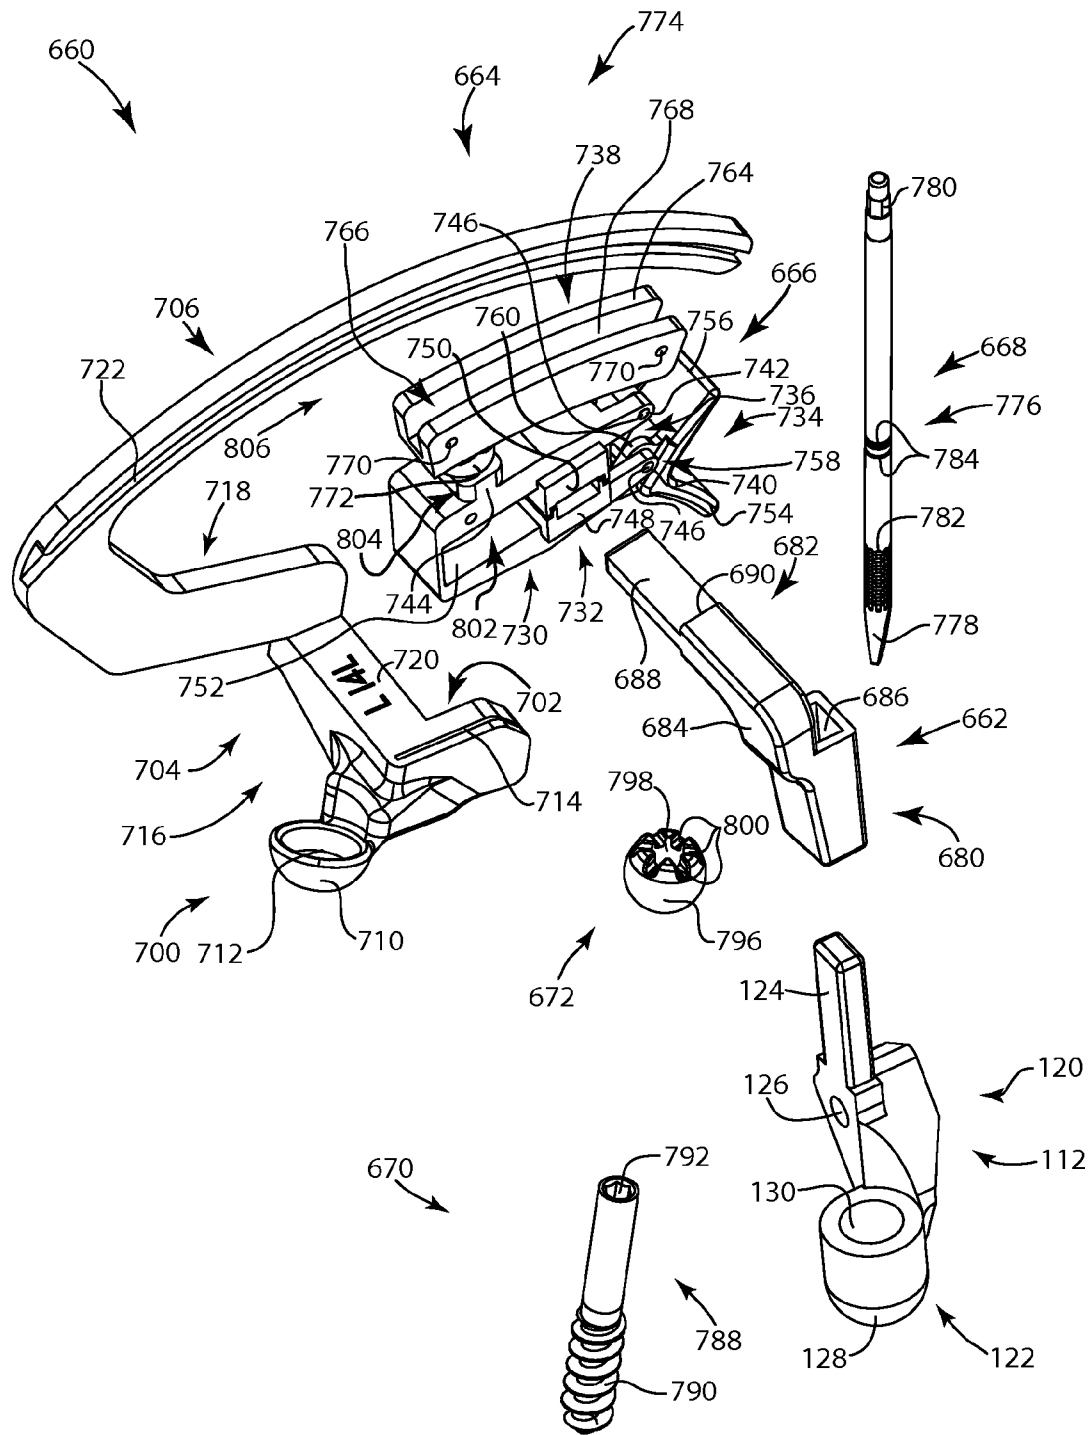


Fig. 17



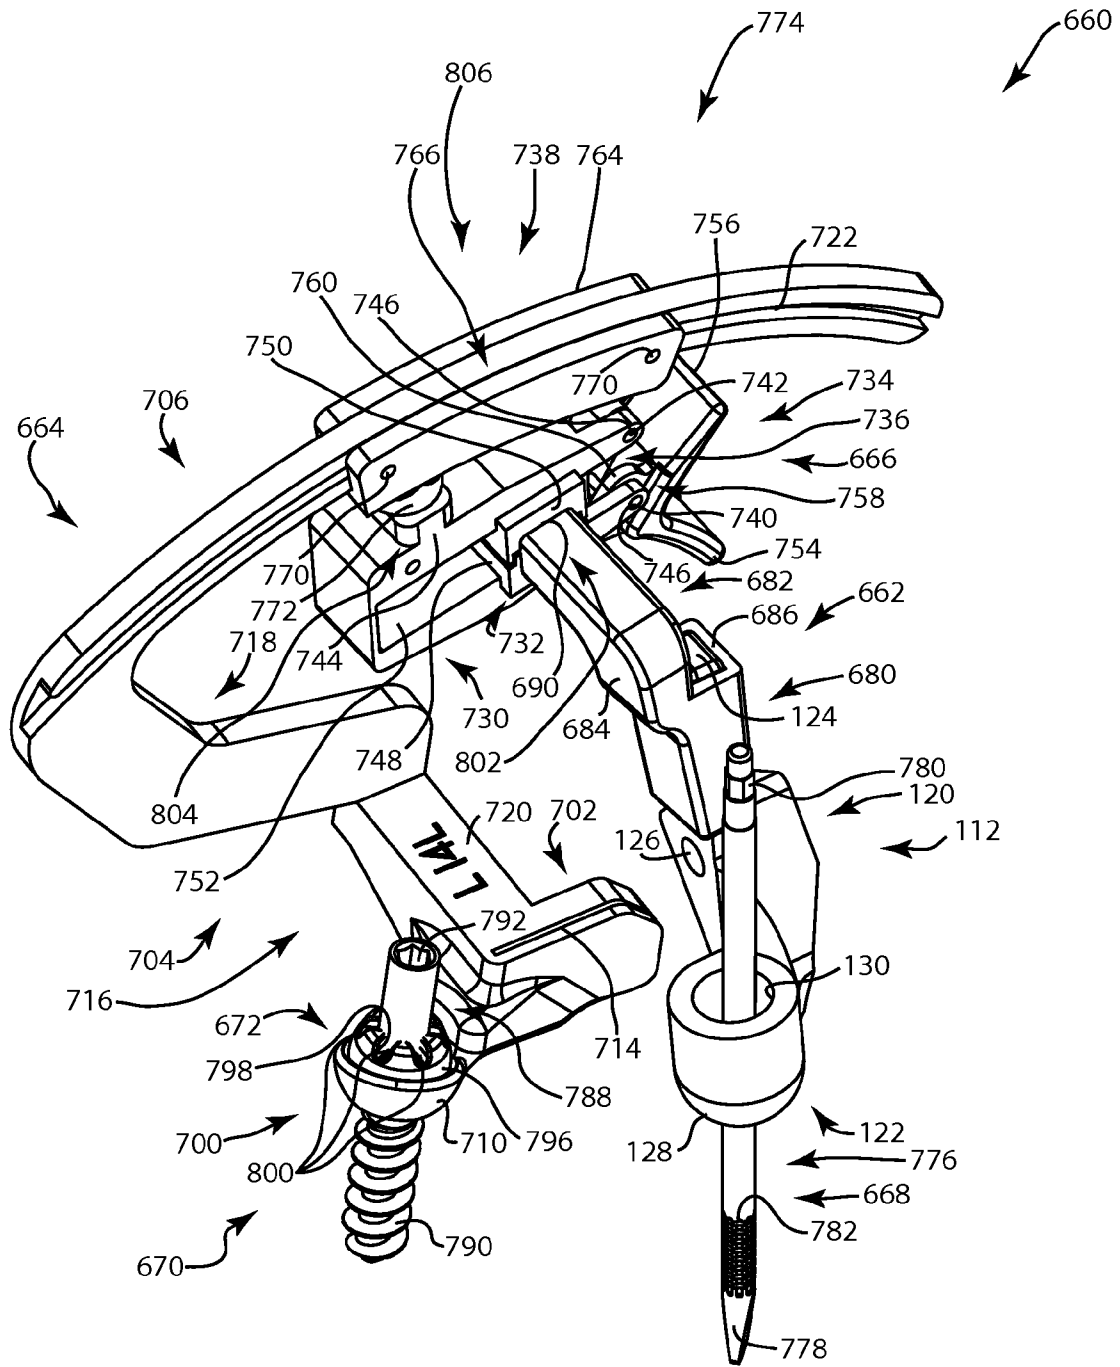


Fig. 18

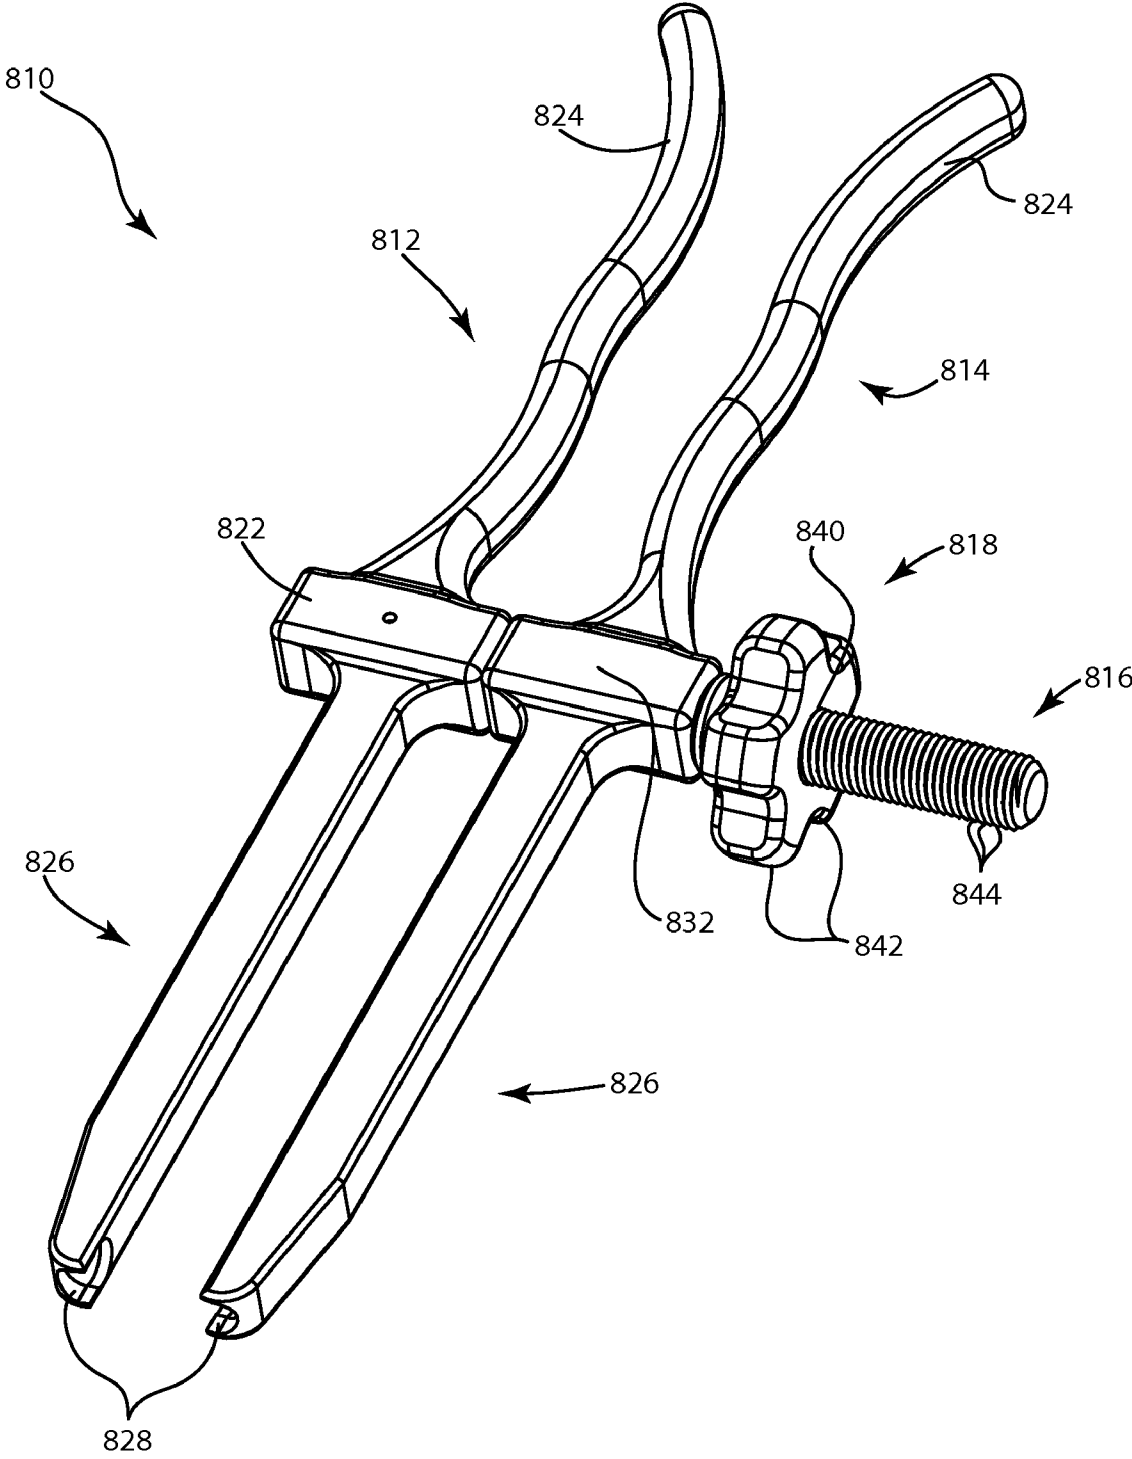


Fig. 19

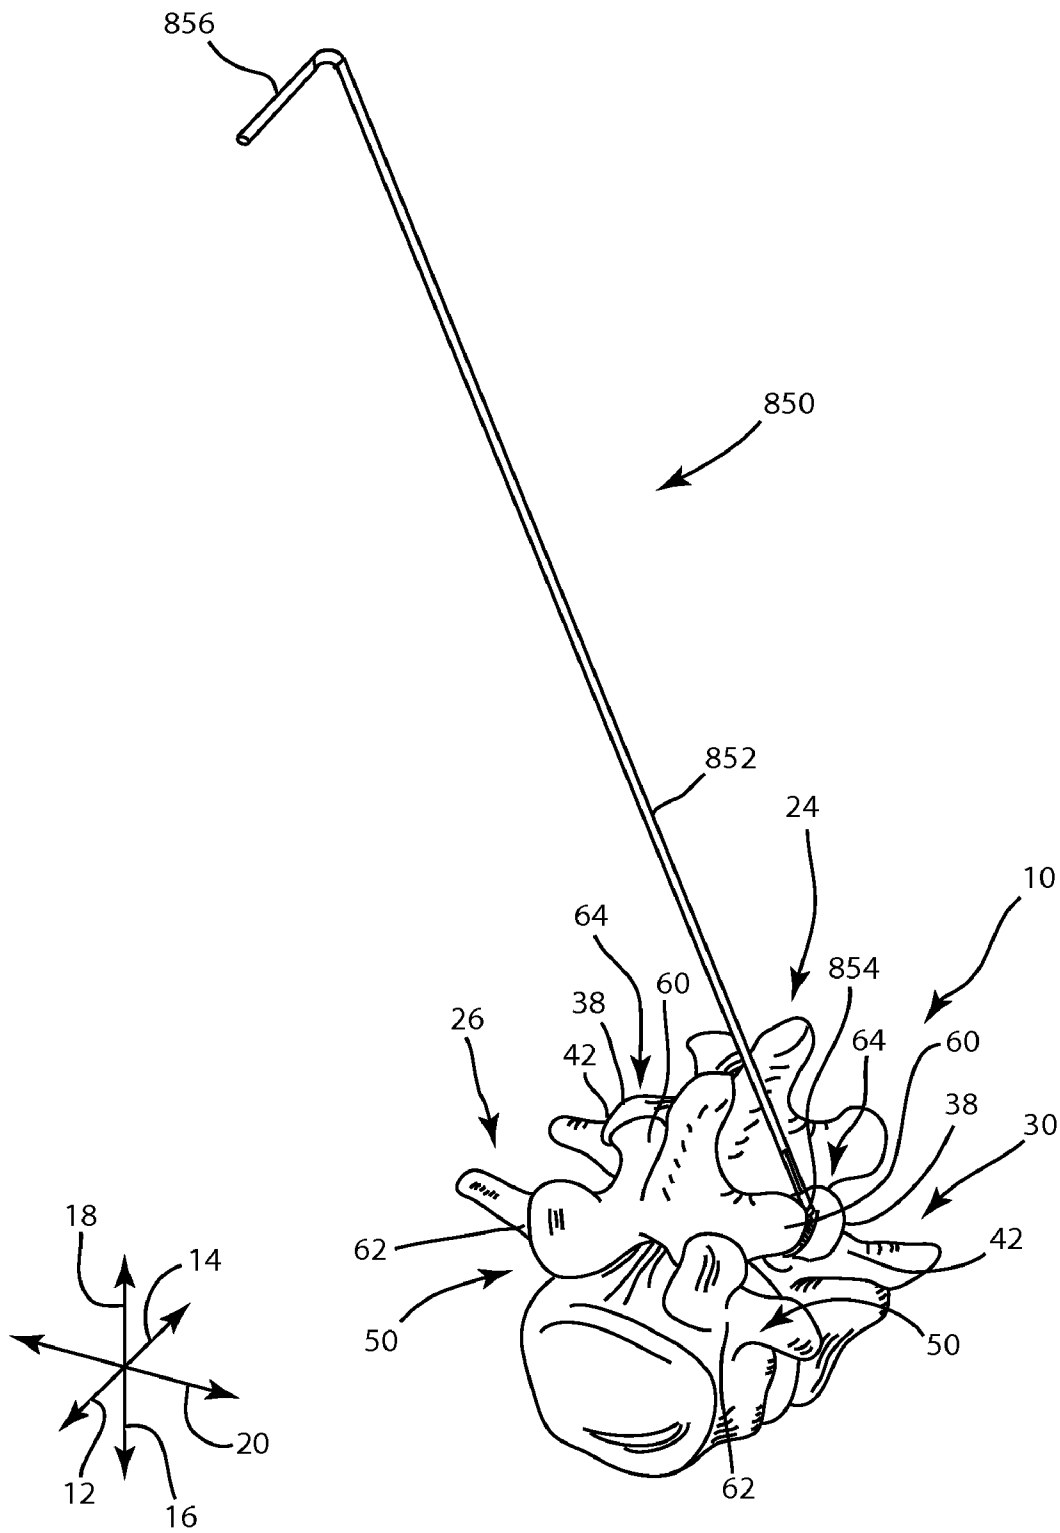


Fig. 20

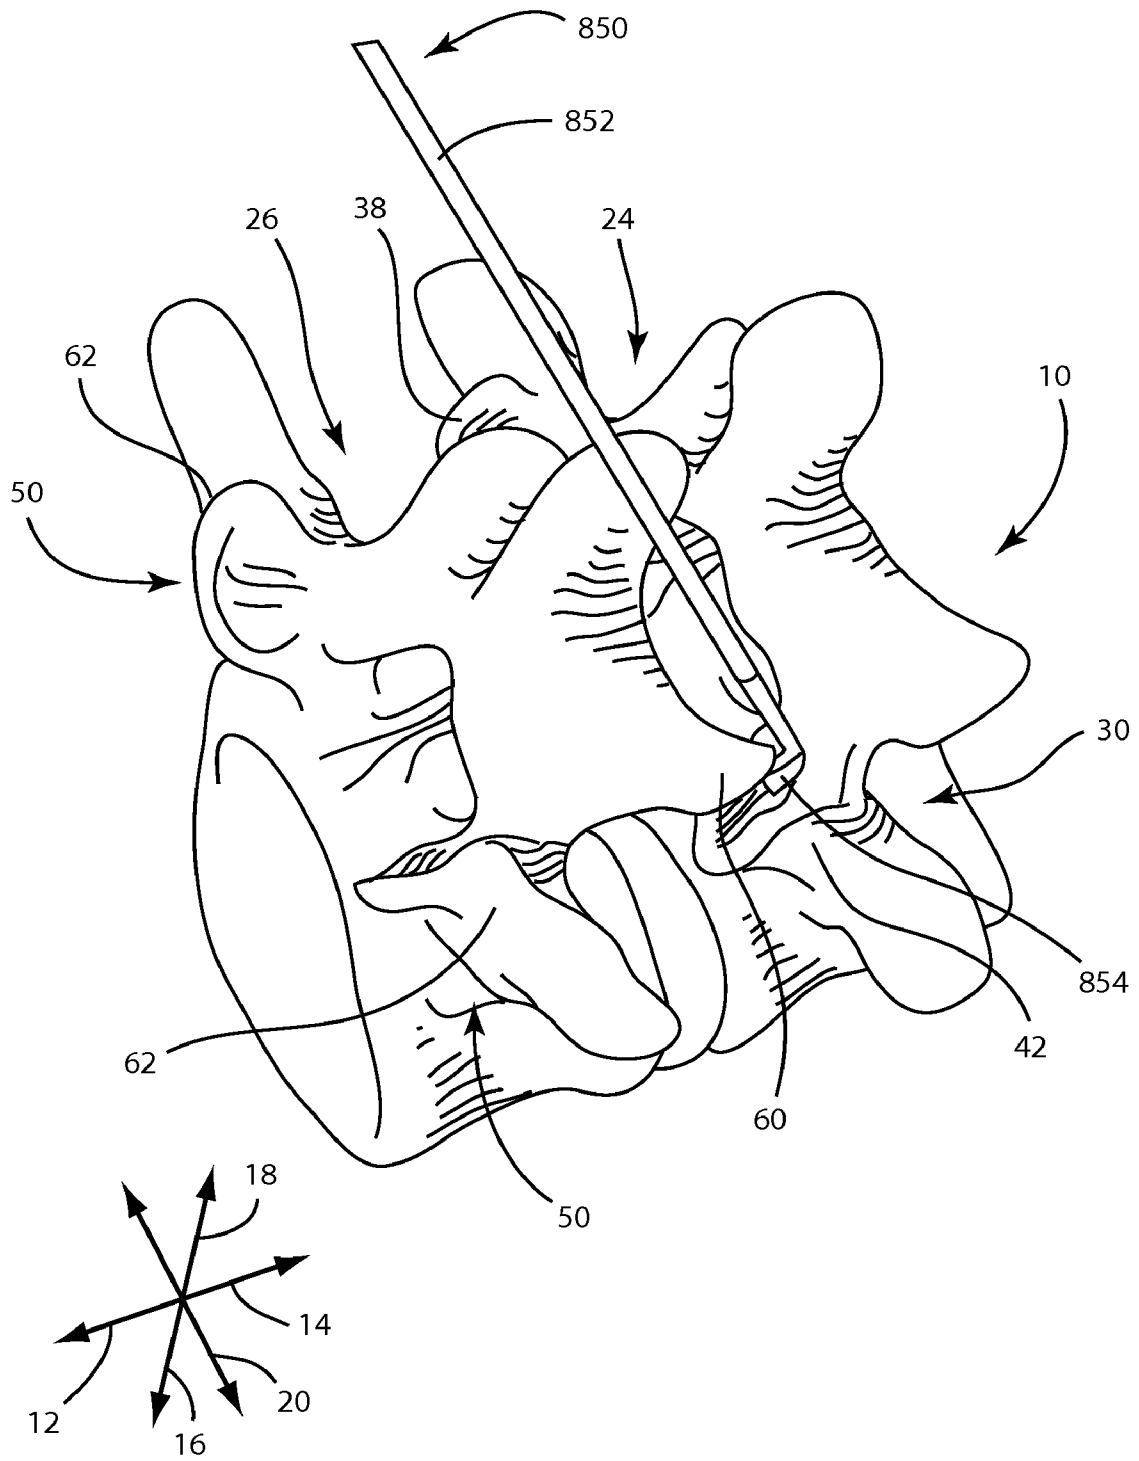


Fig. 21

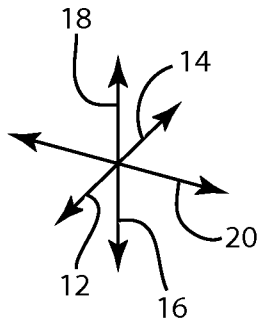
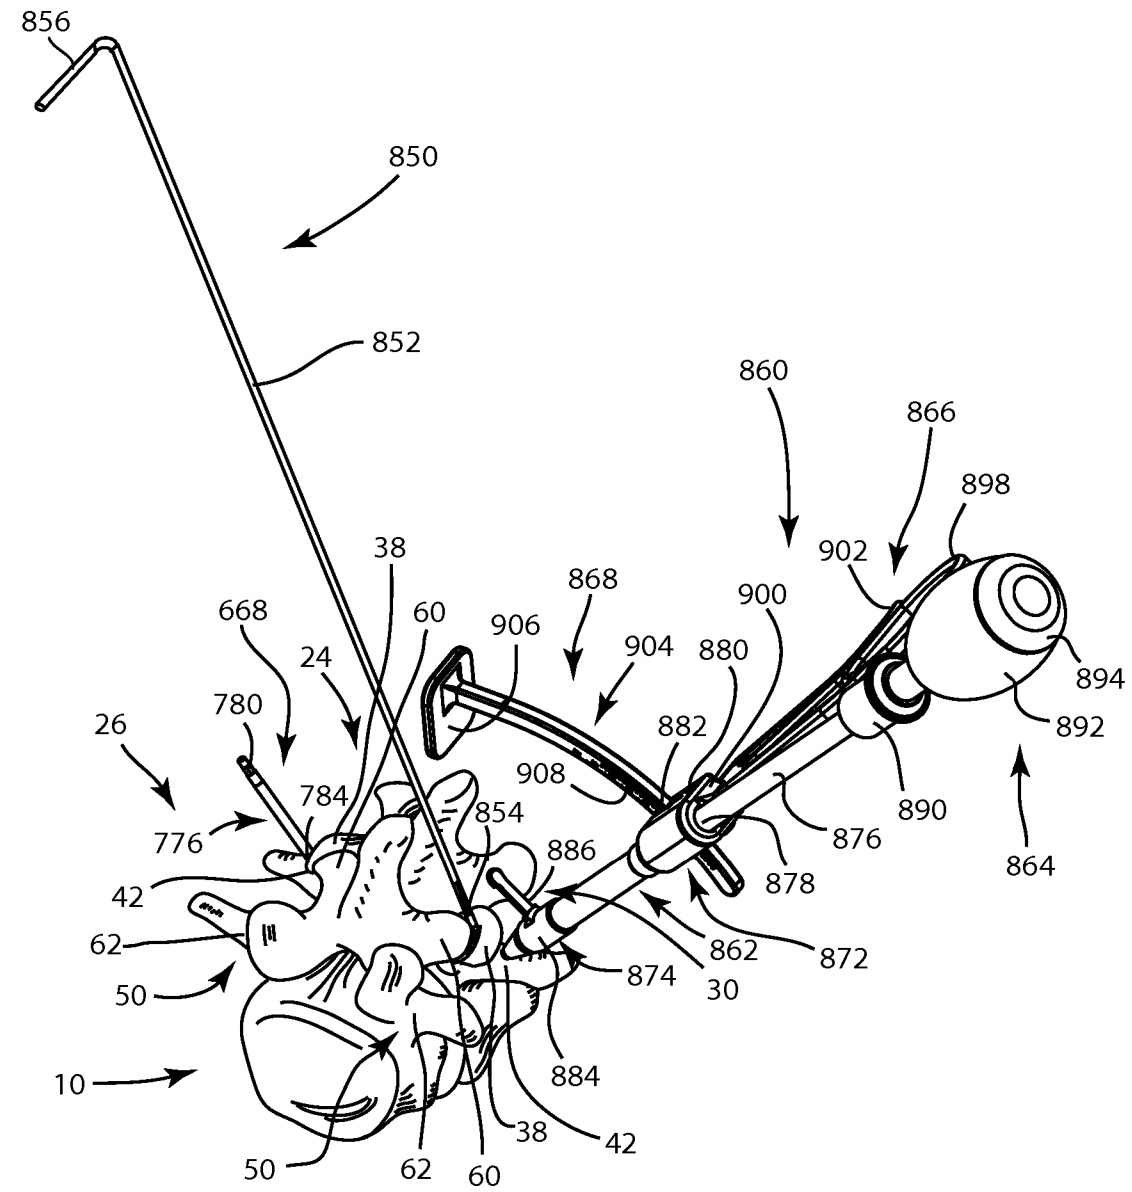


Fig. 22

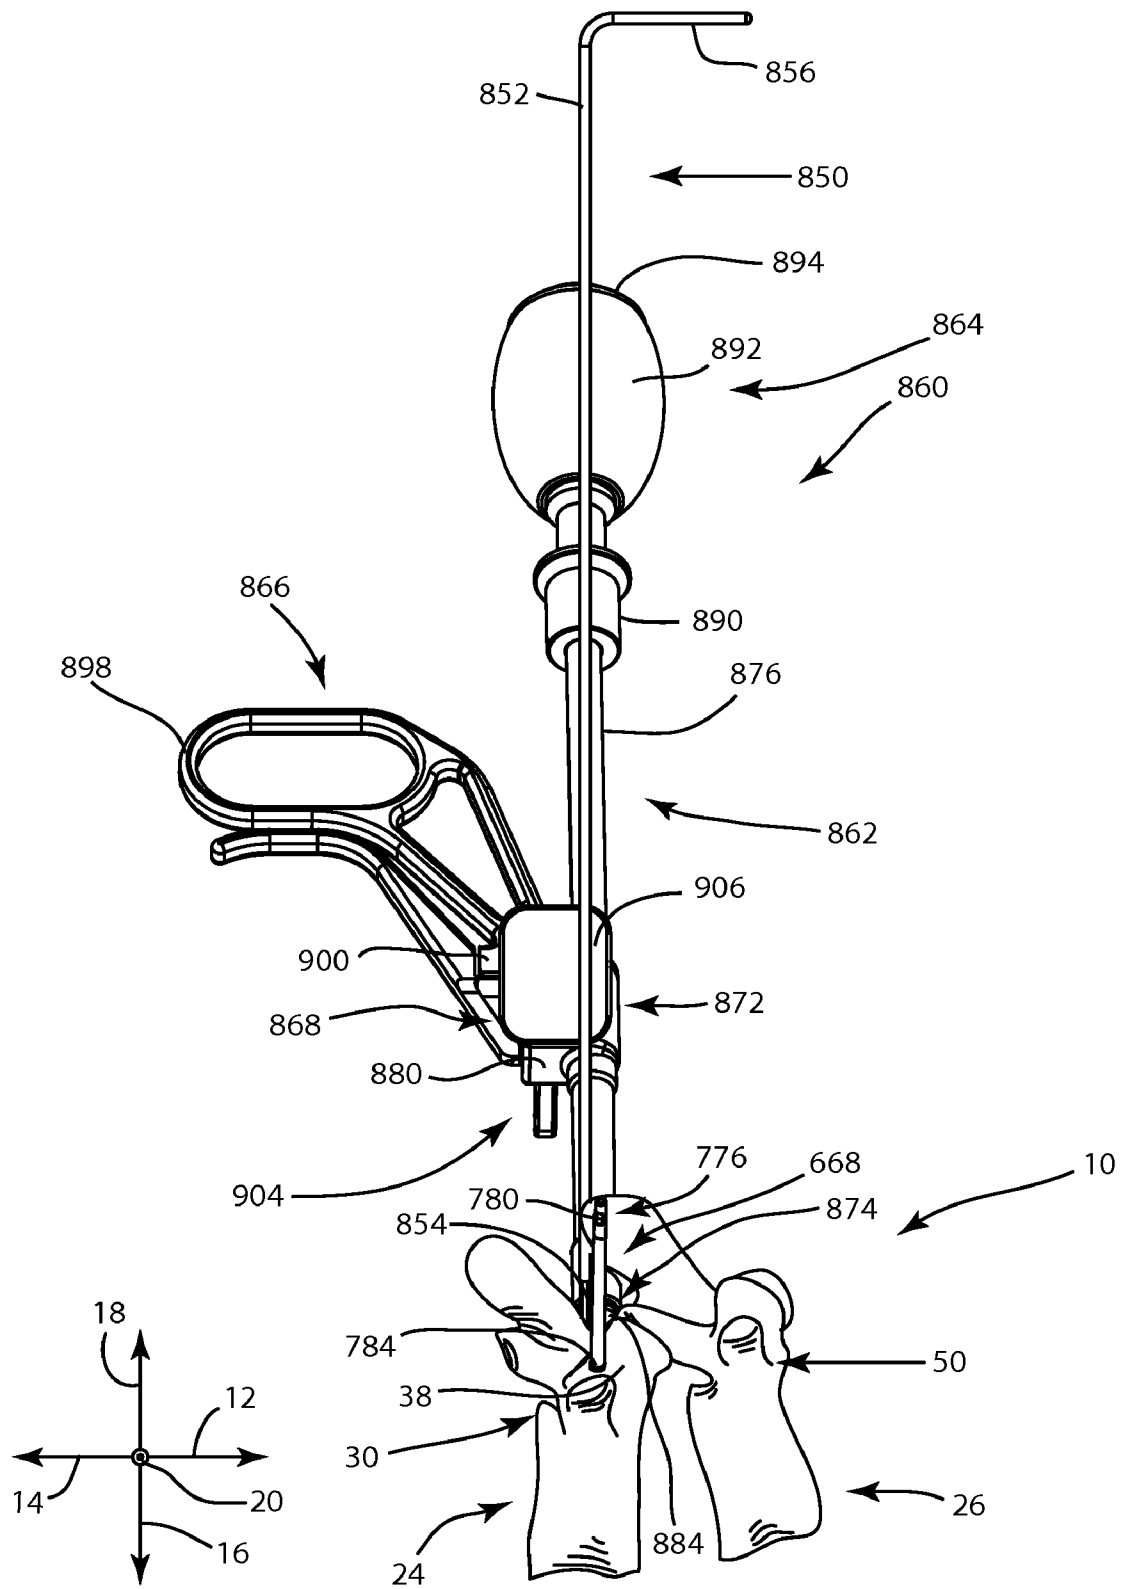


Fig. 23

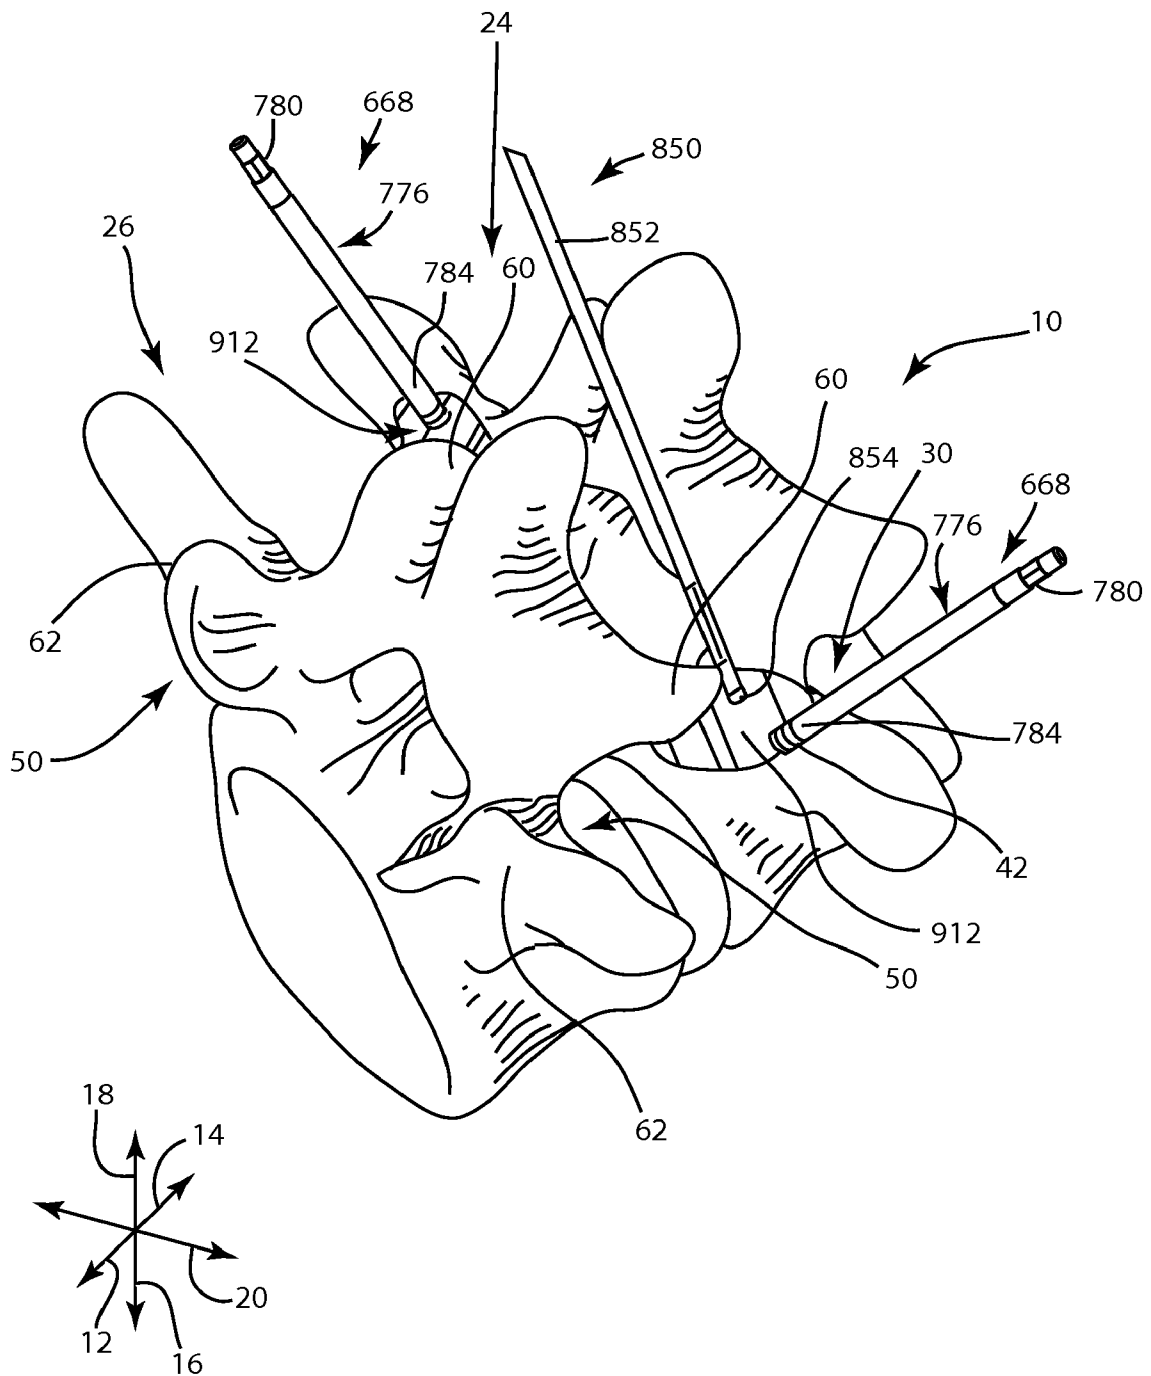


Fig. 24


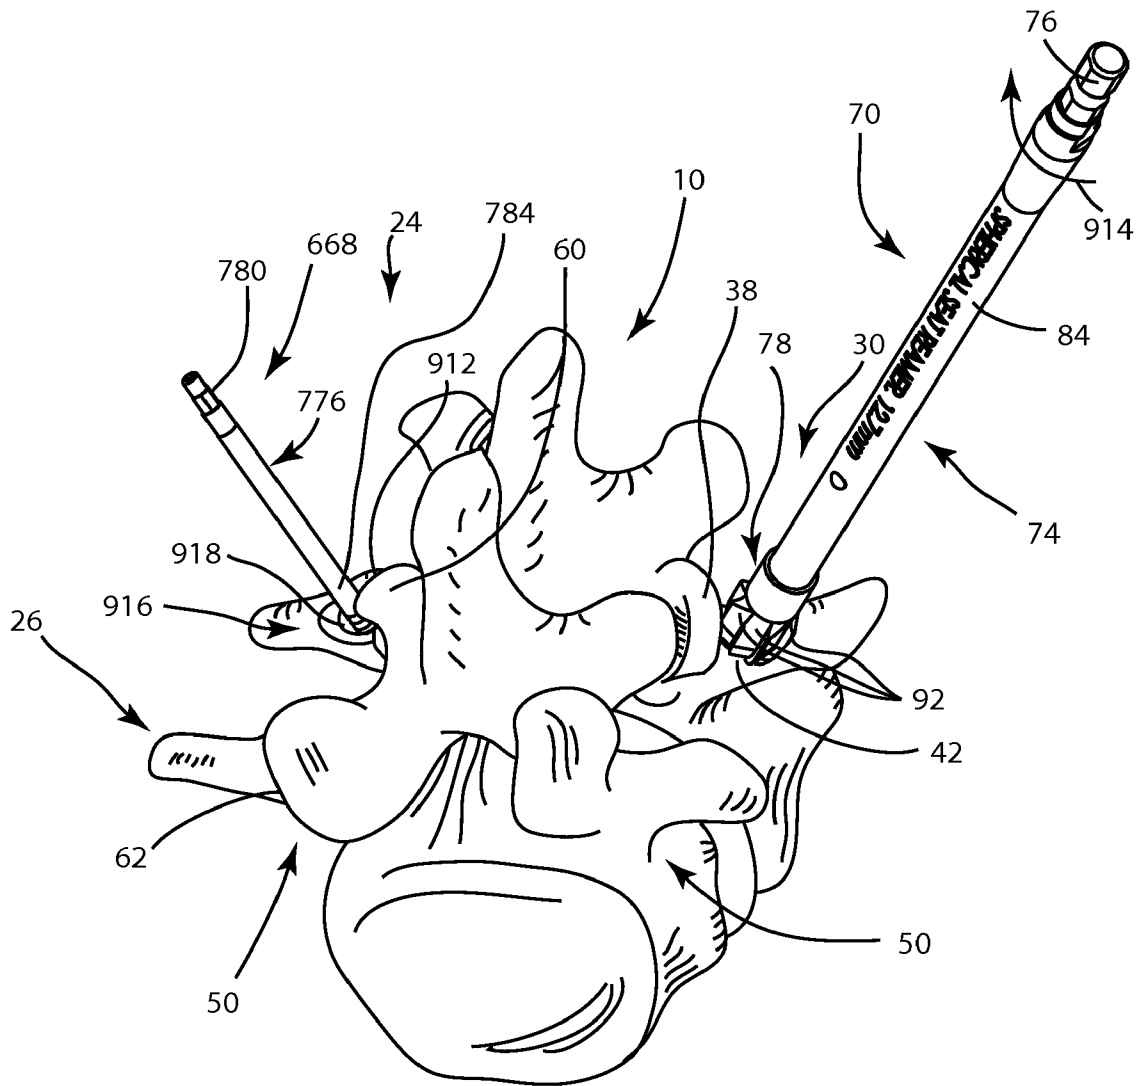


Fig. 25



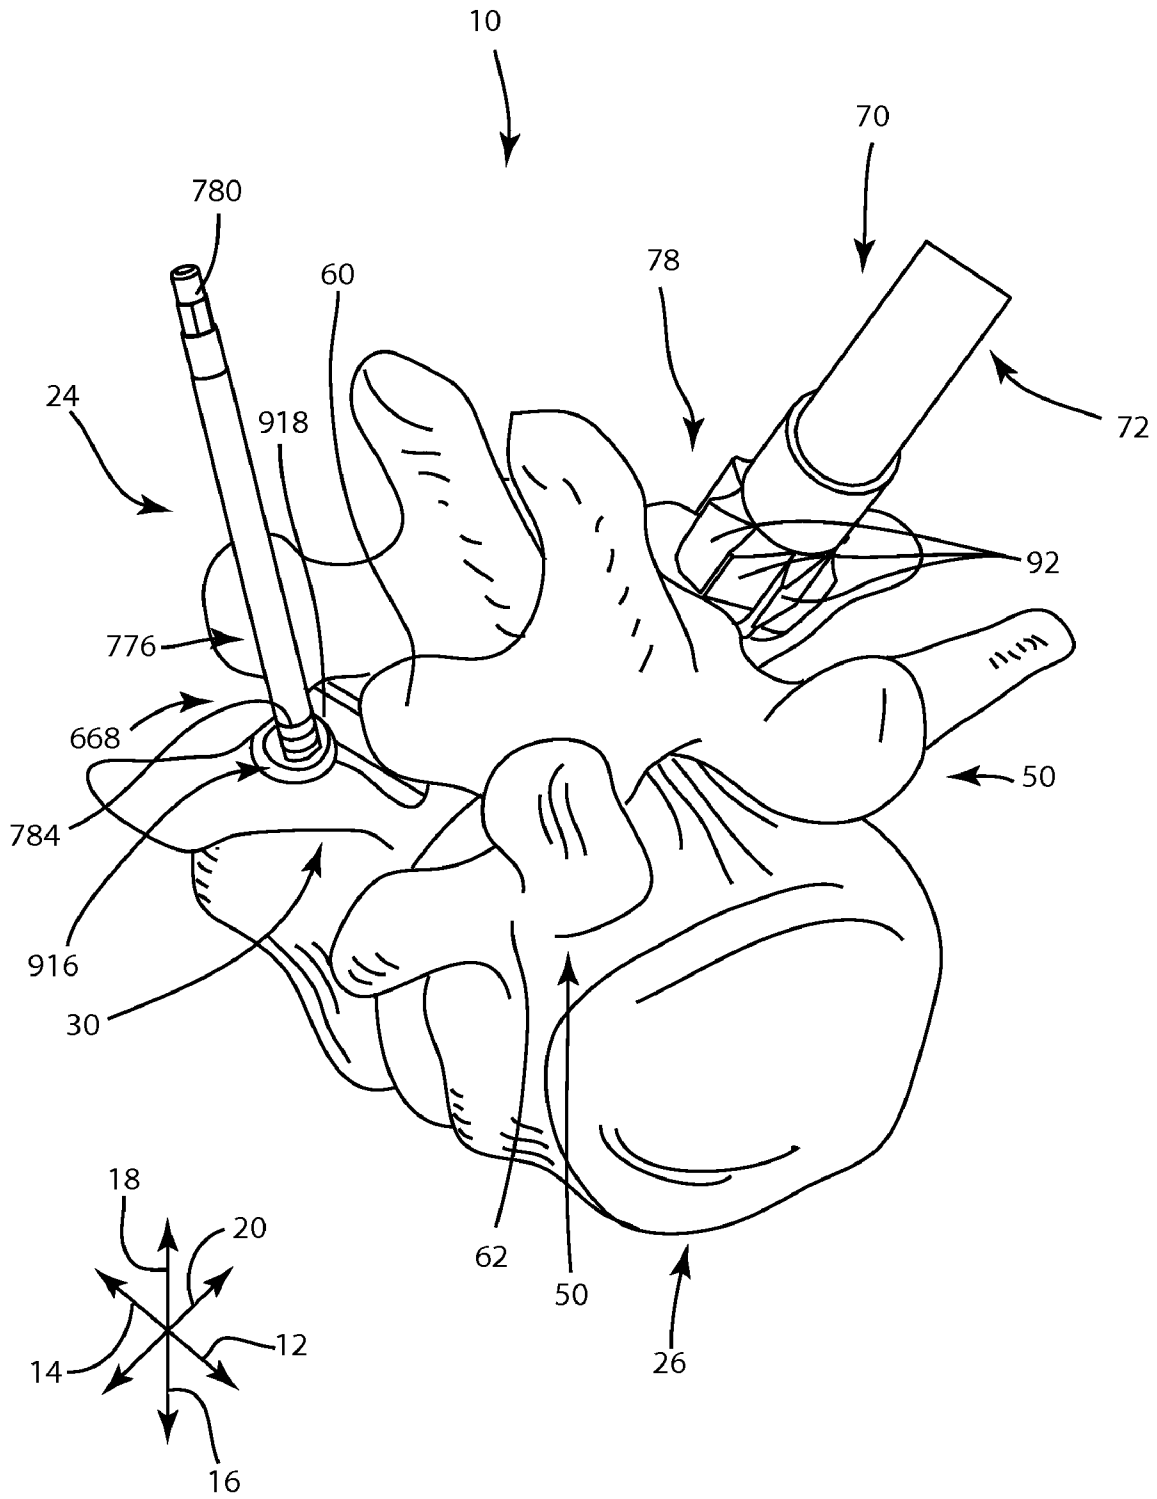


Fig. 26





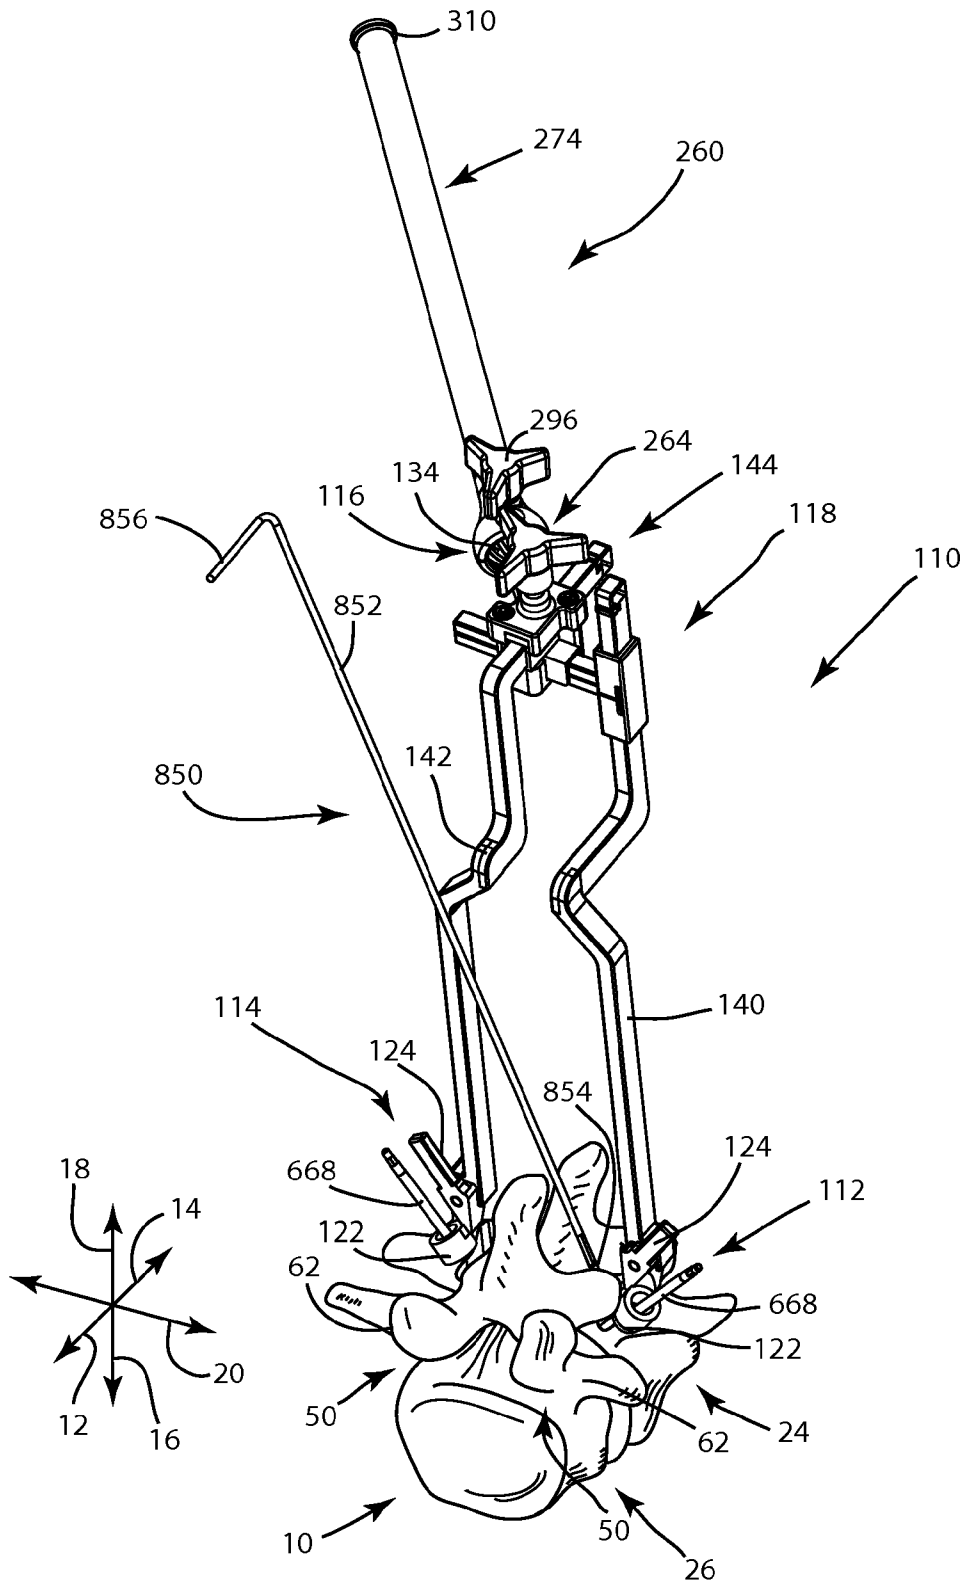


Fig. 29

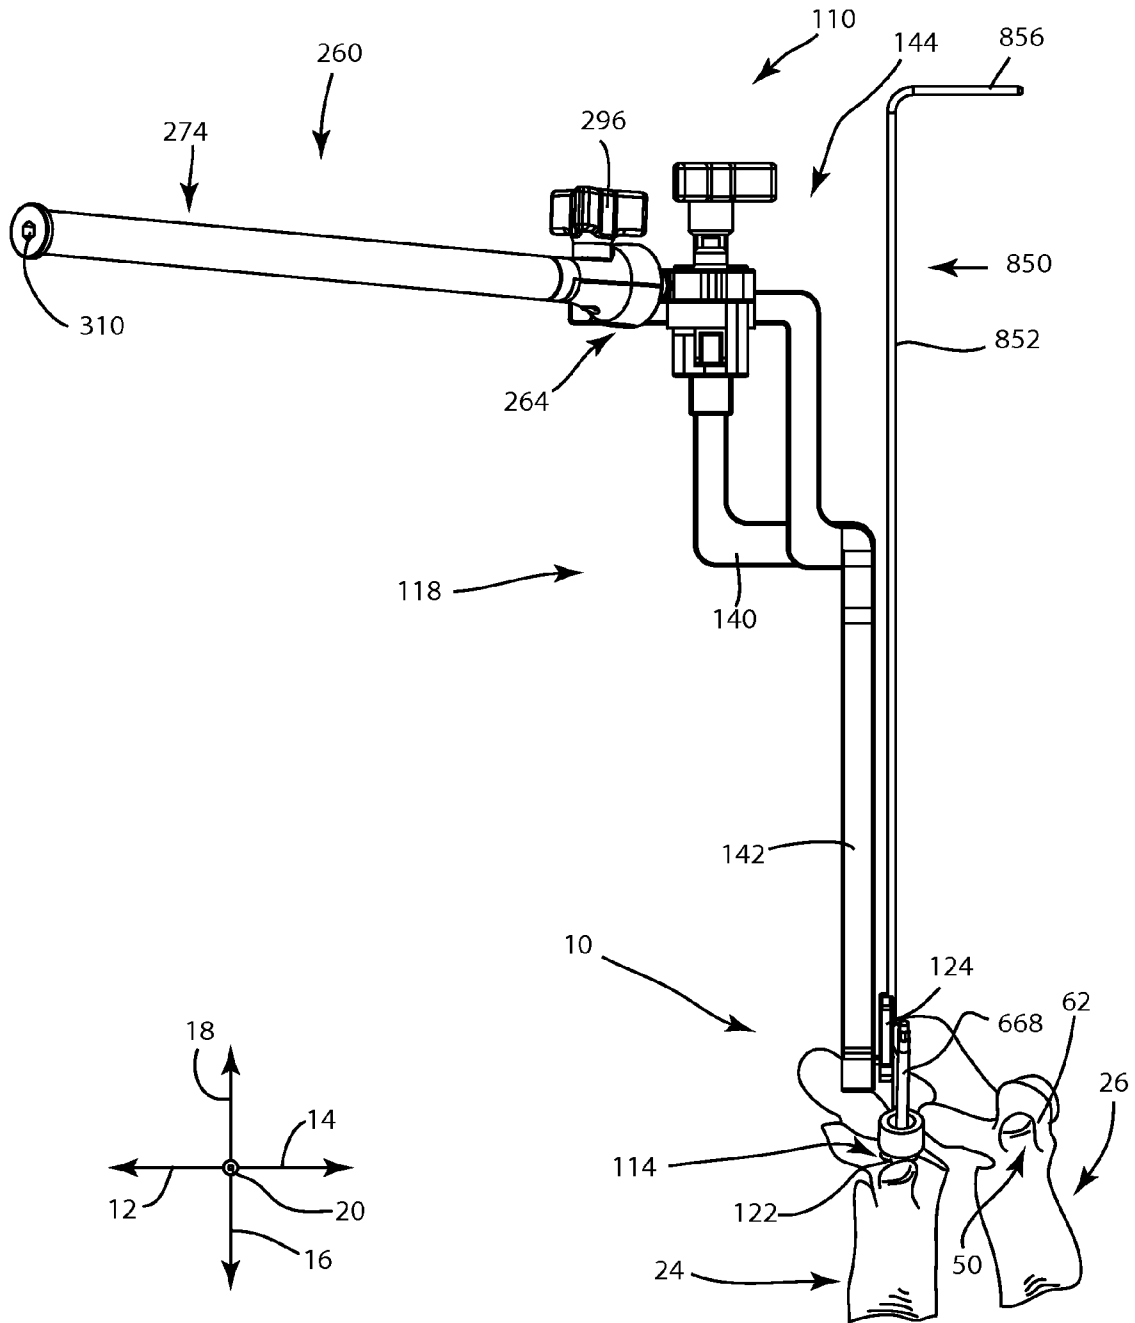


Fig. 30

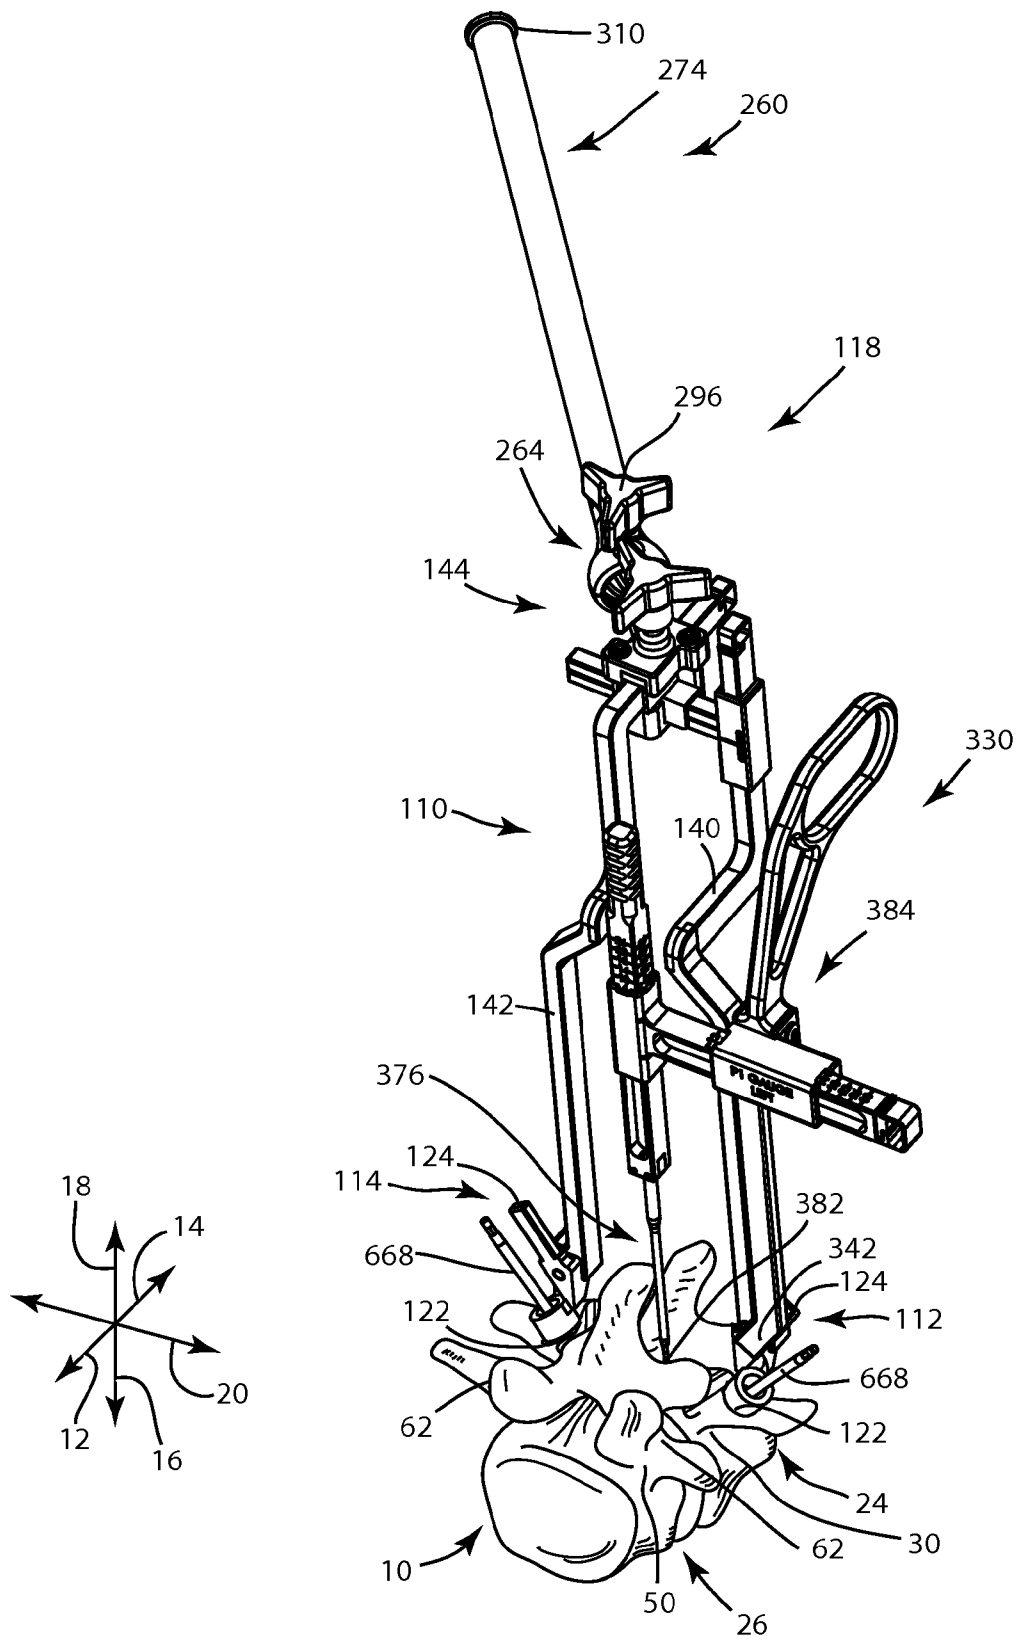


Fig. 31

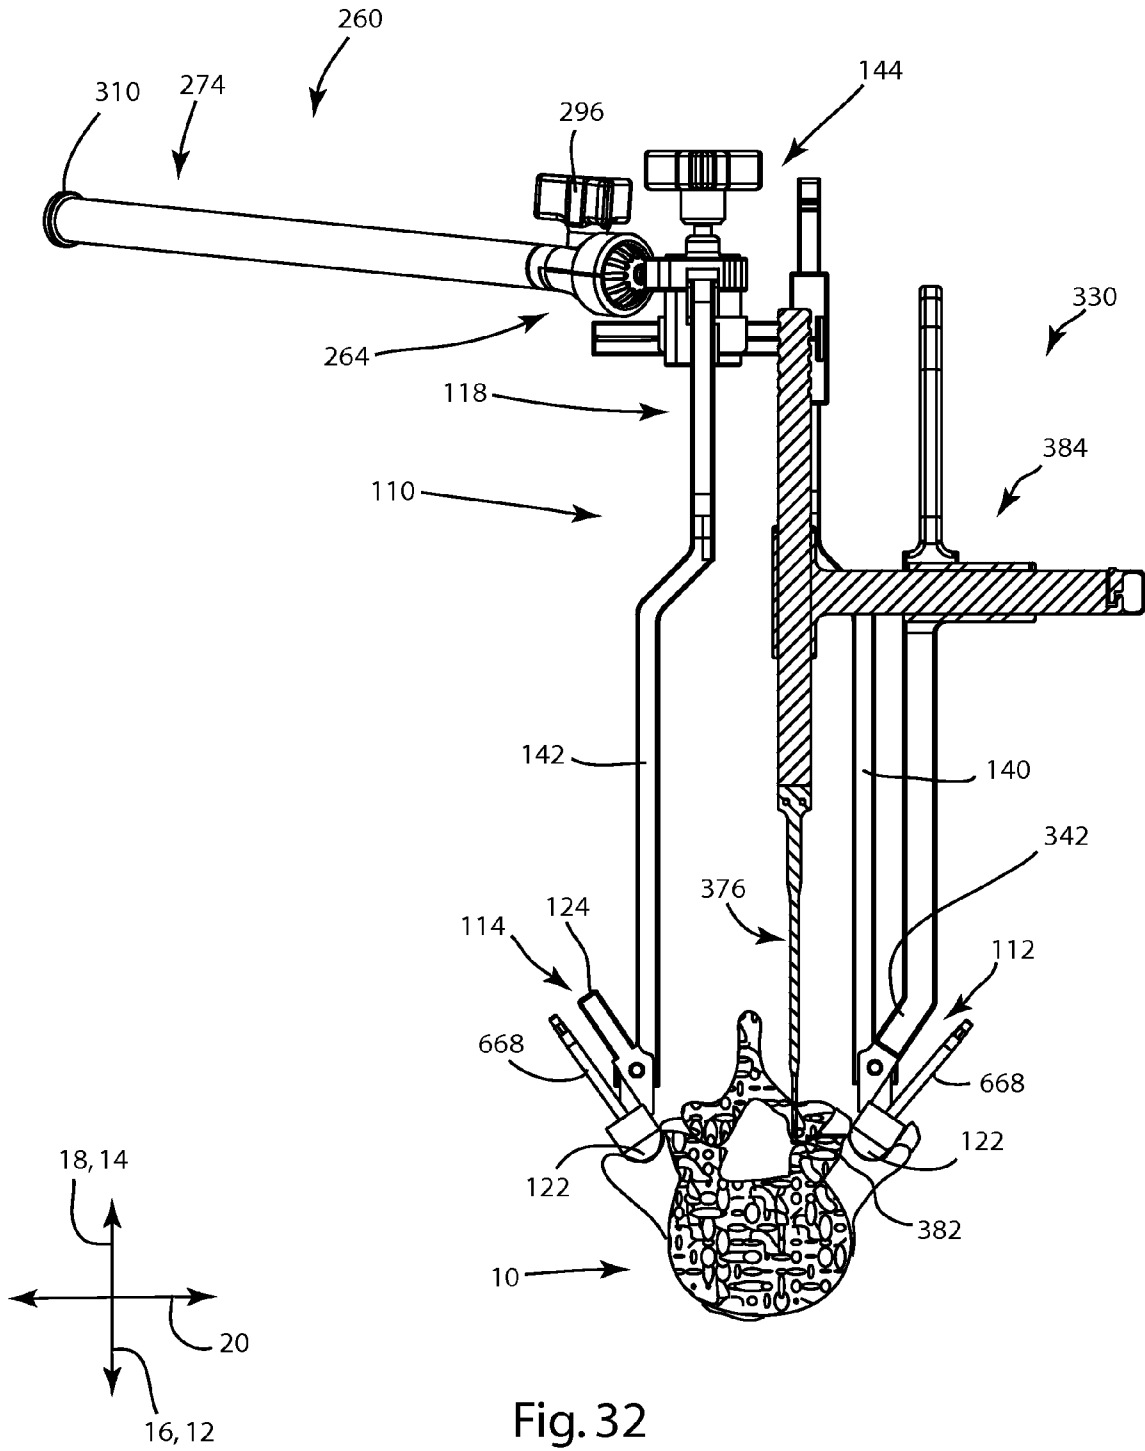


Fig. 32





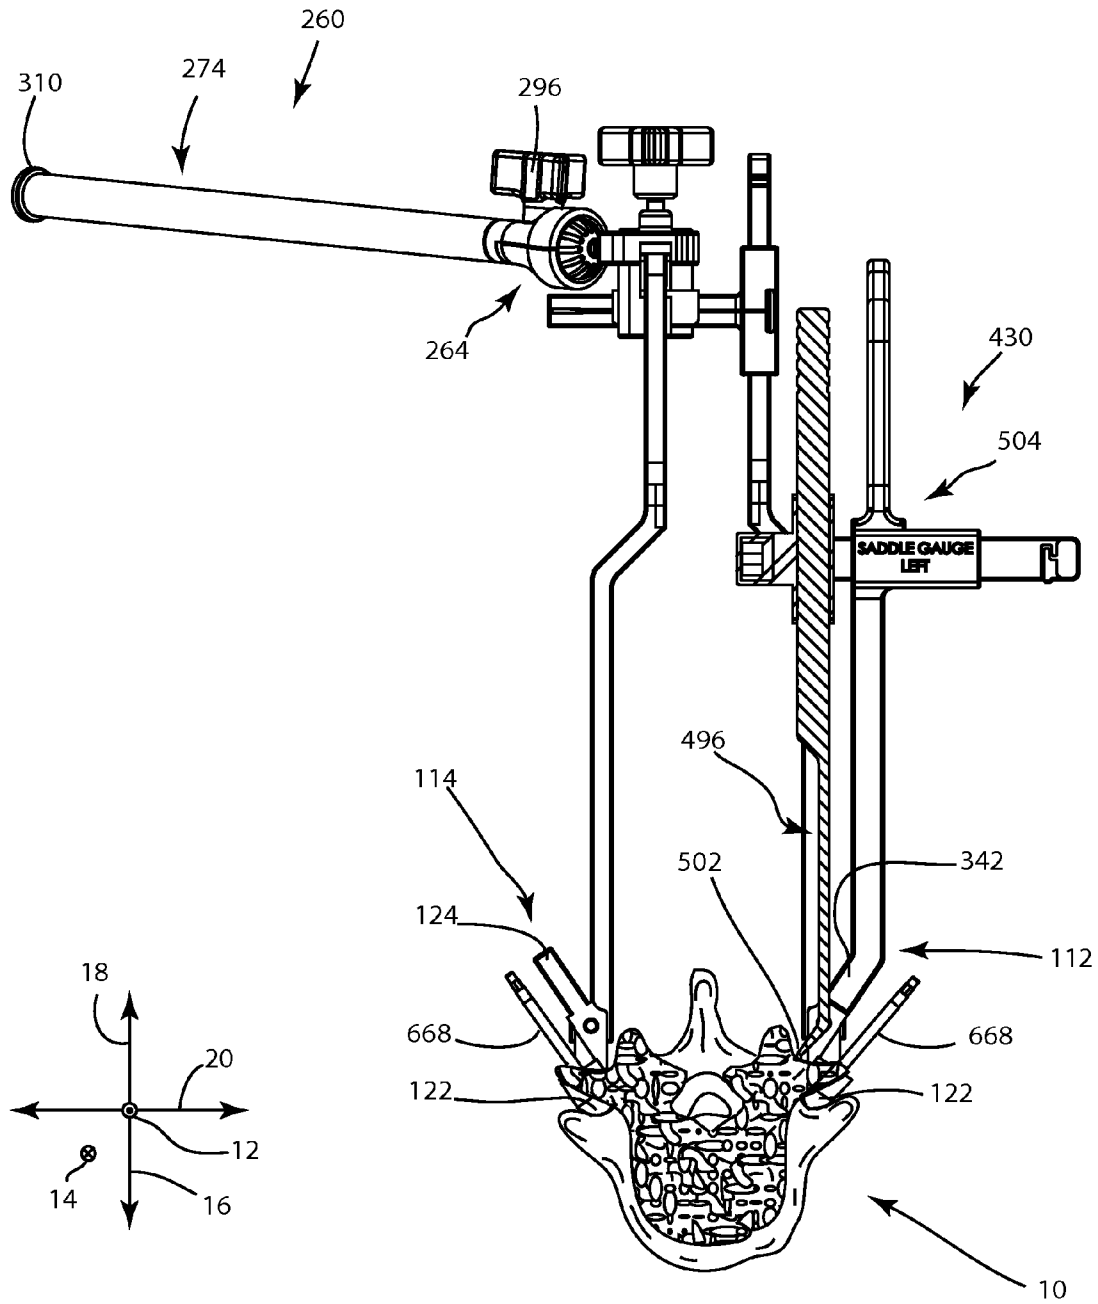


Fig. 34



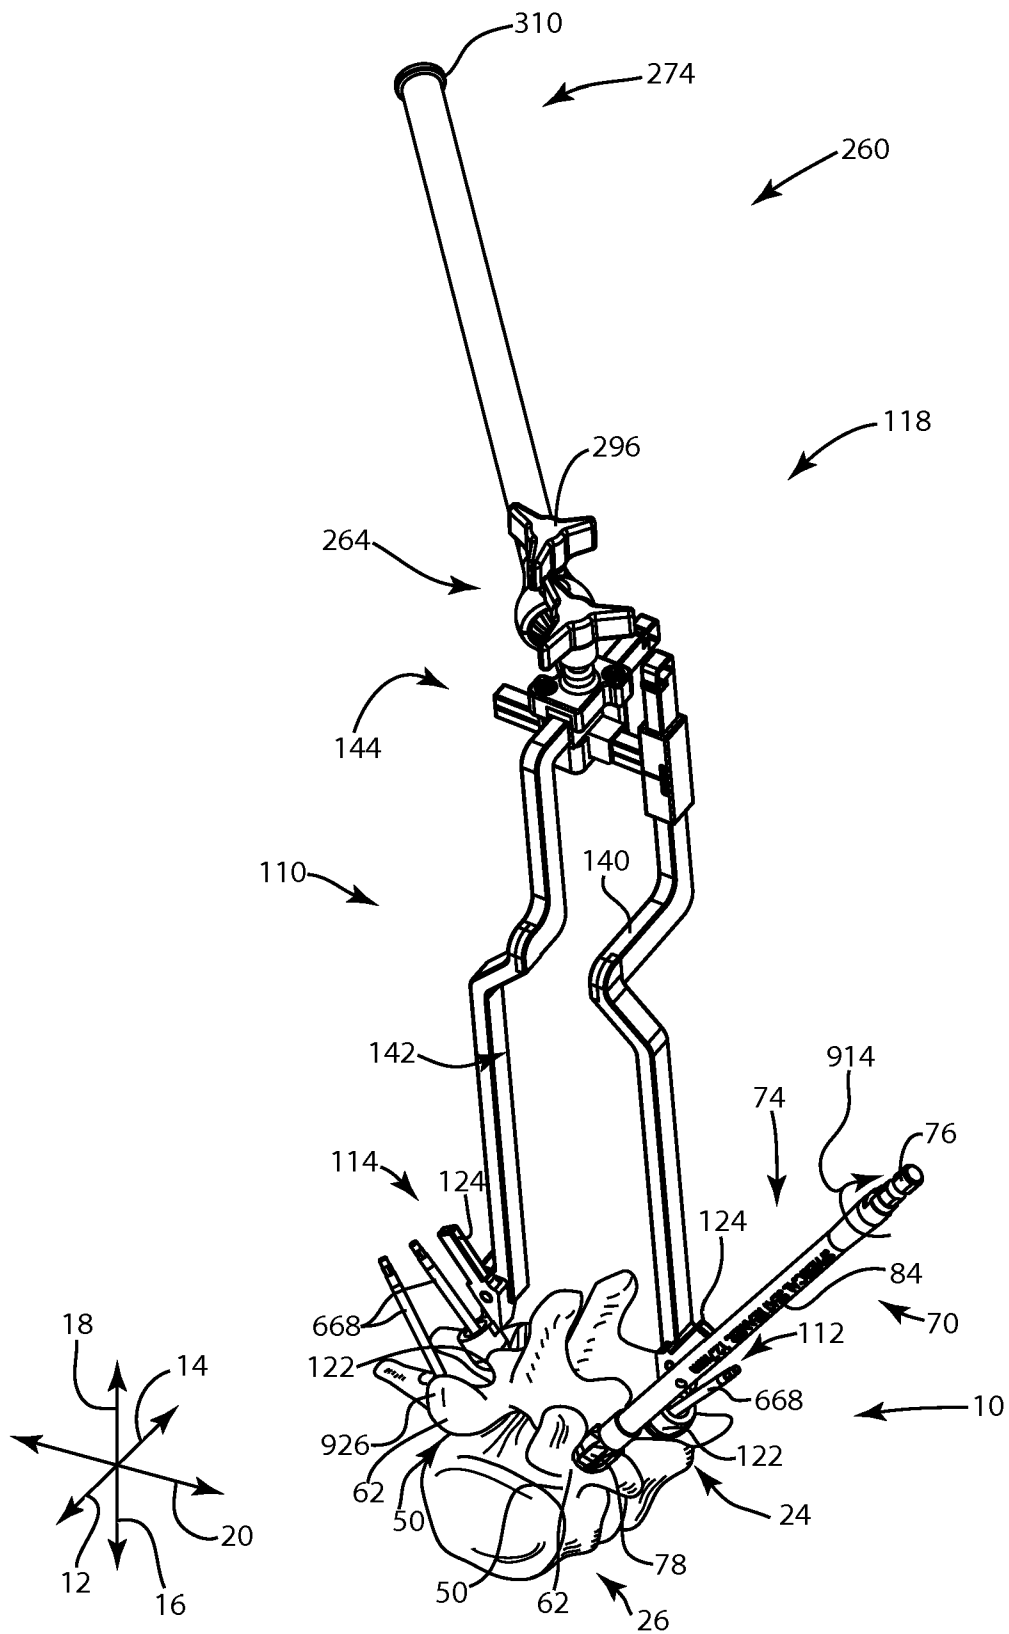


Fig. 36



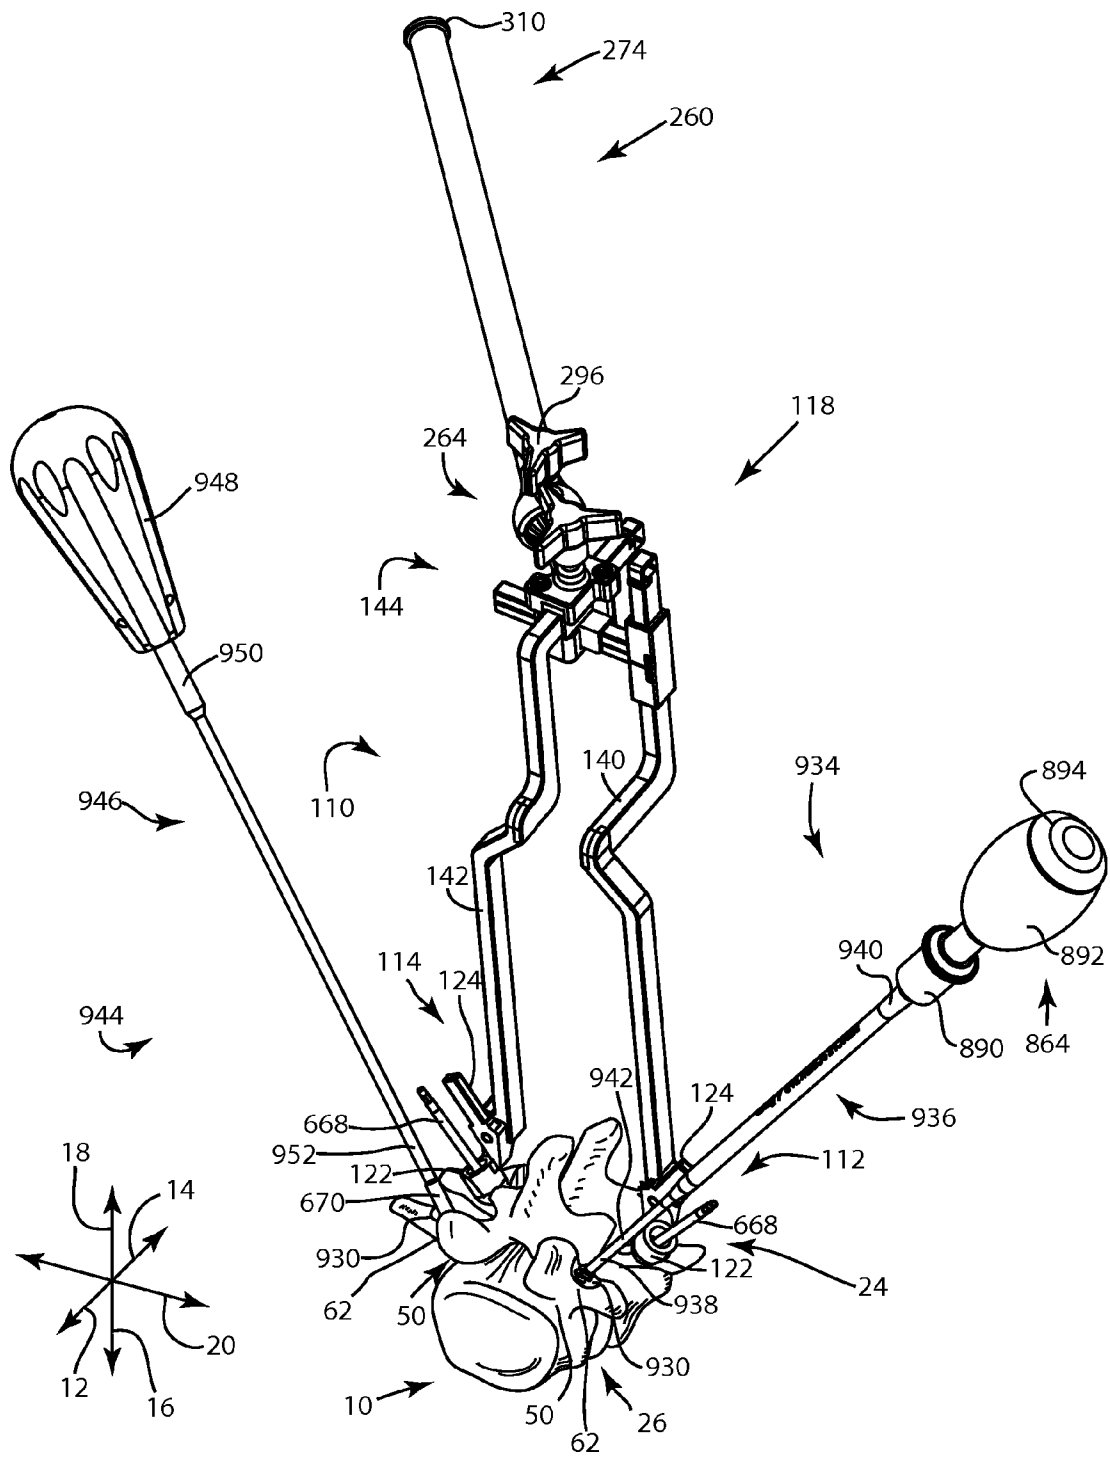


Fig. 38

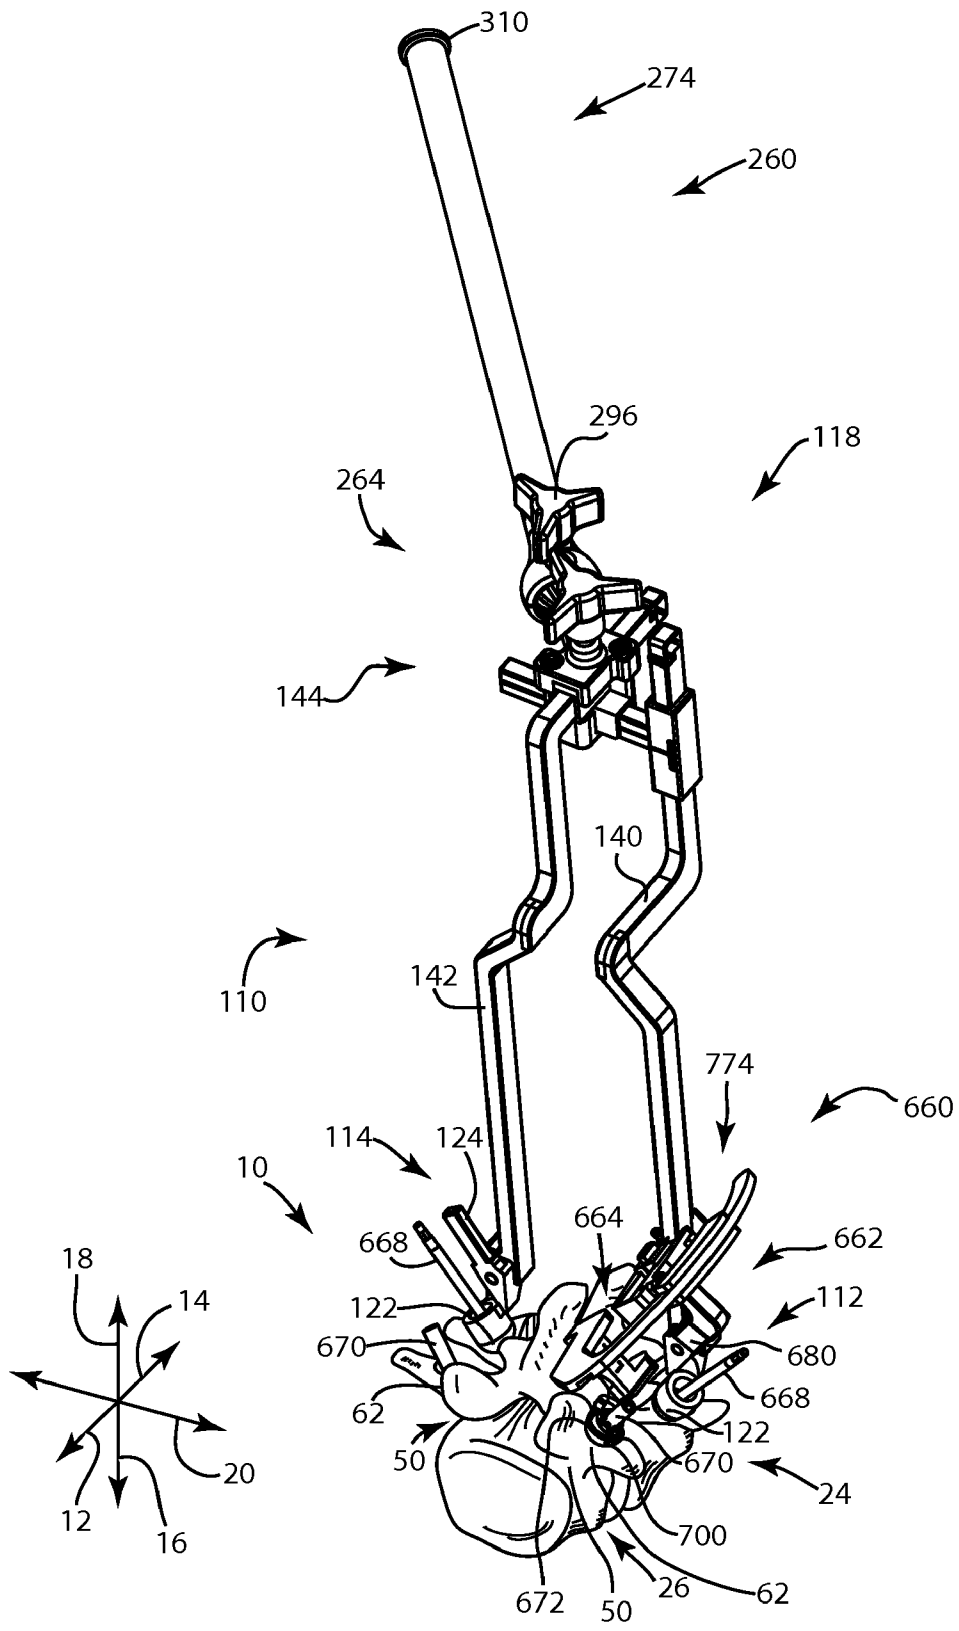


Fig. 39

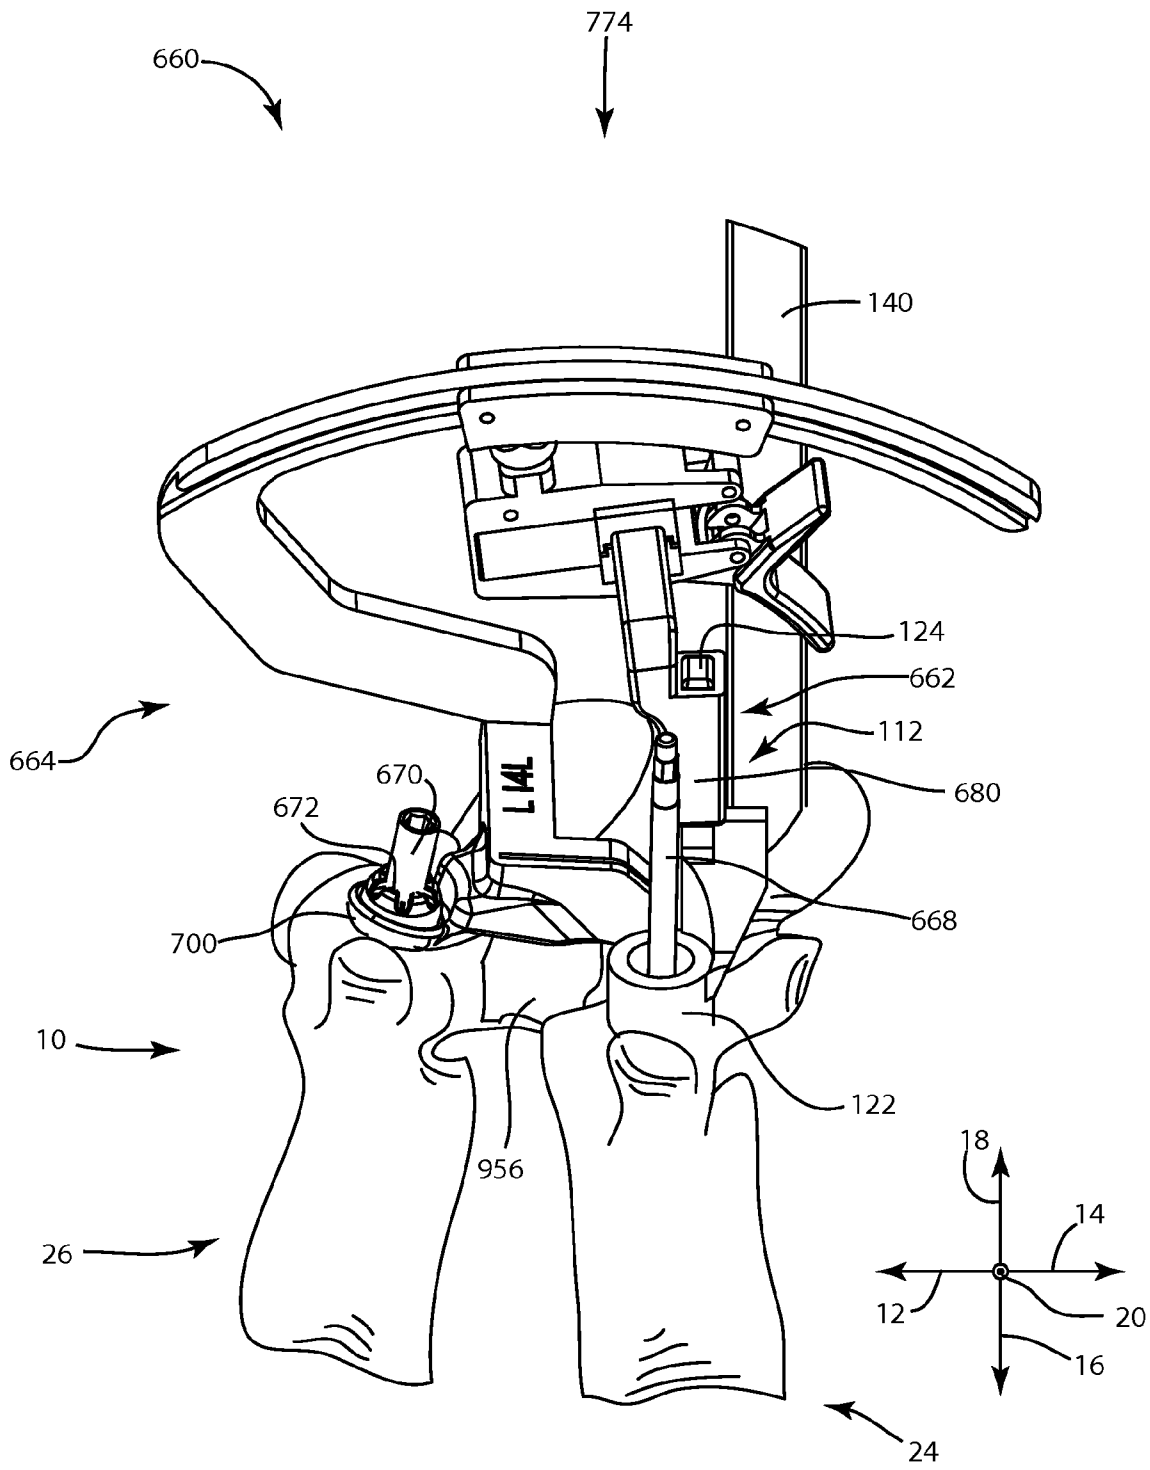


Fig. 40

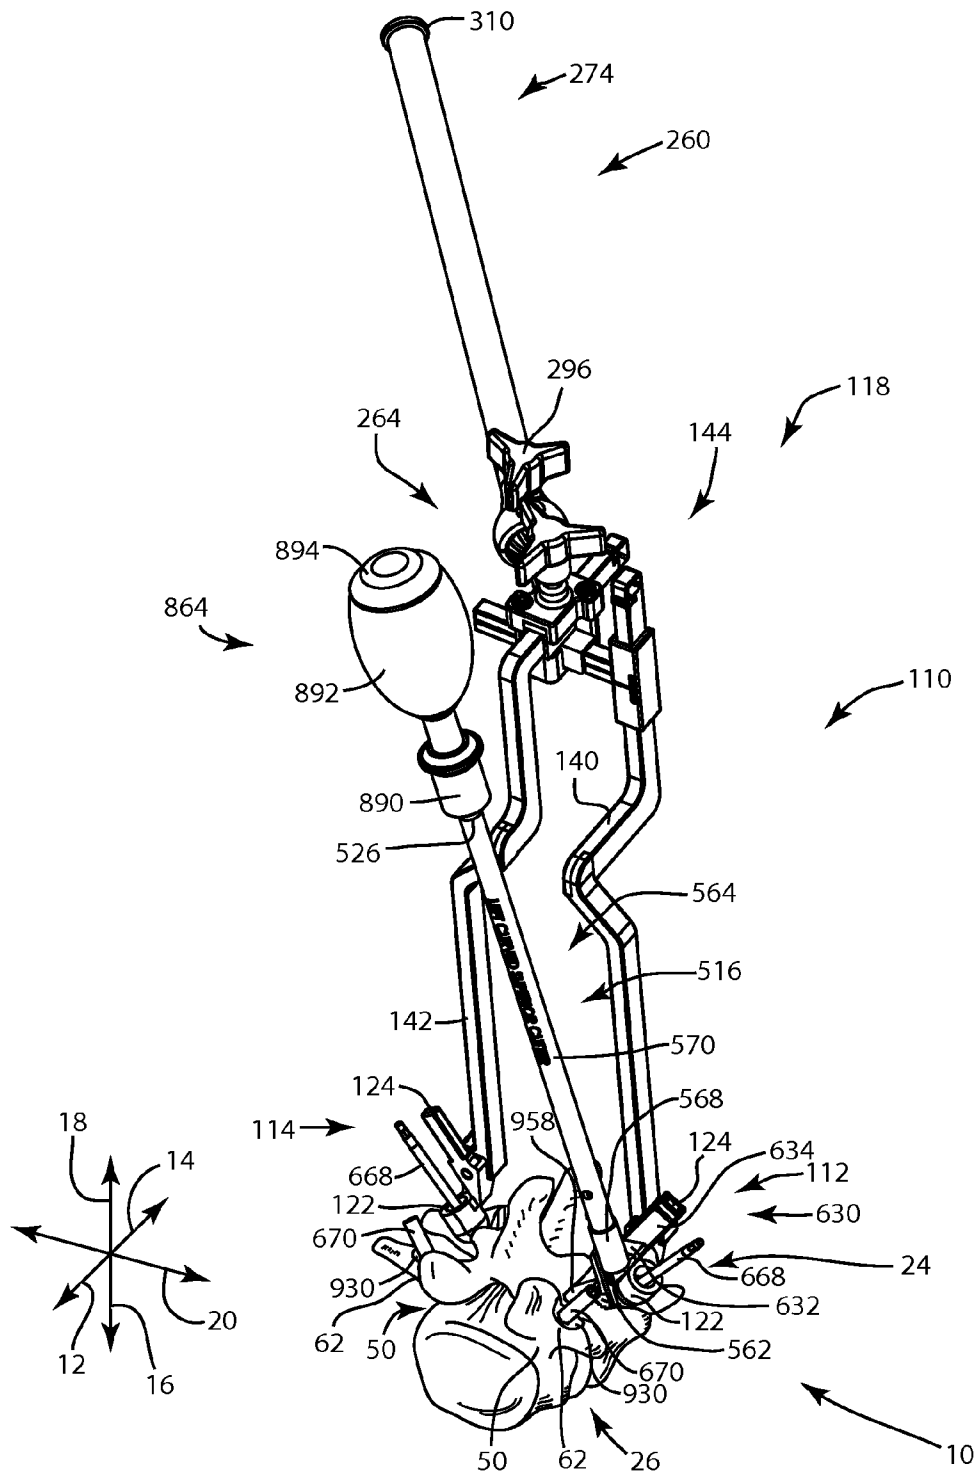
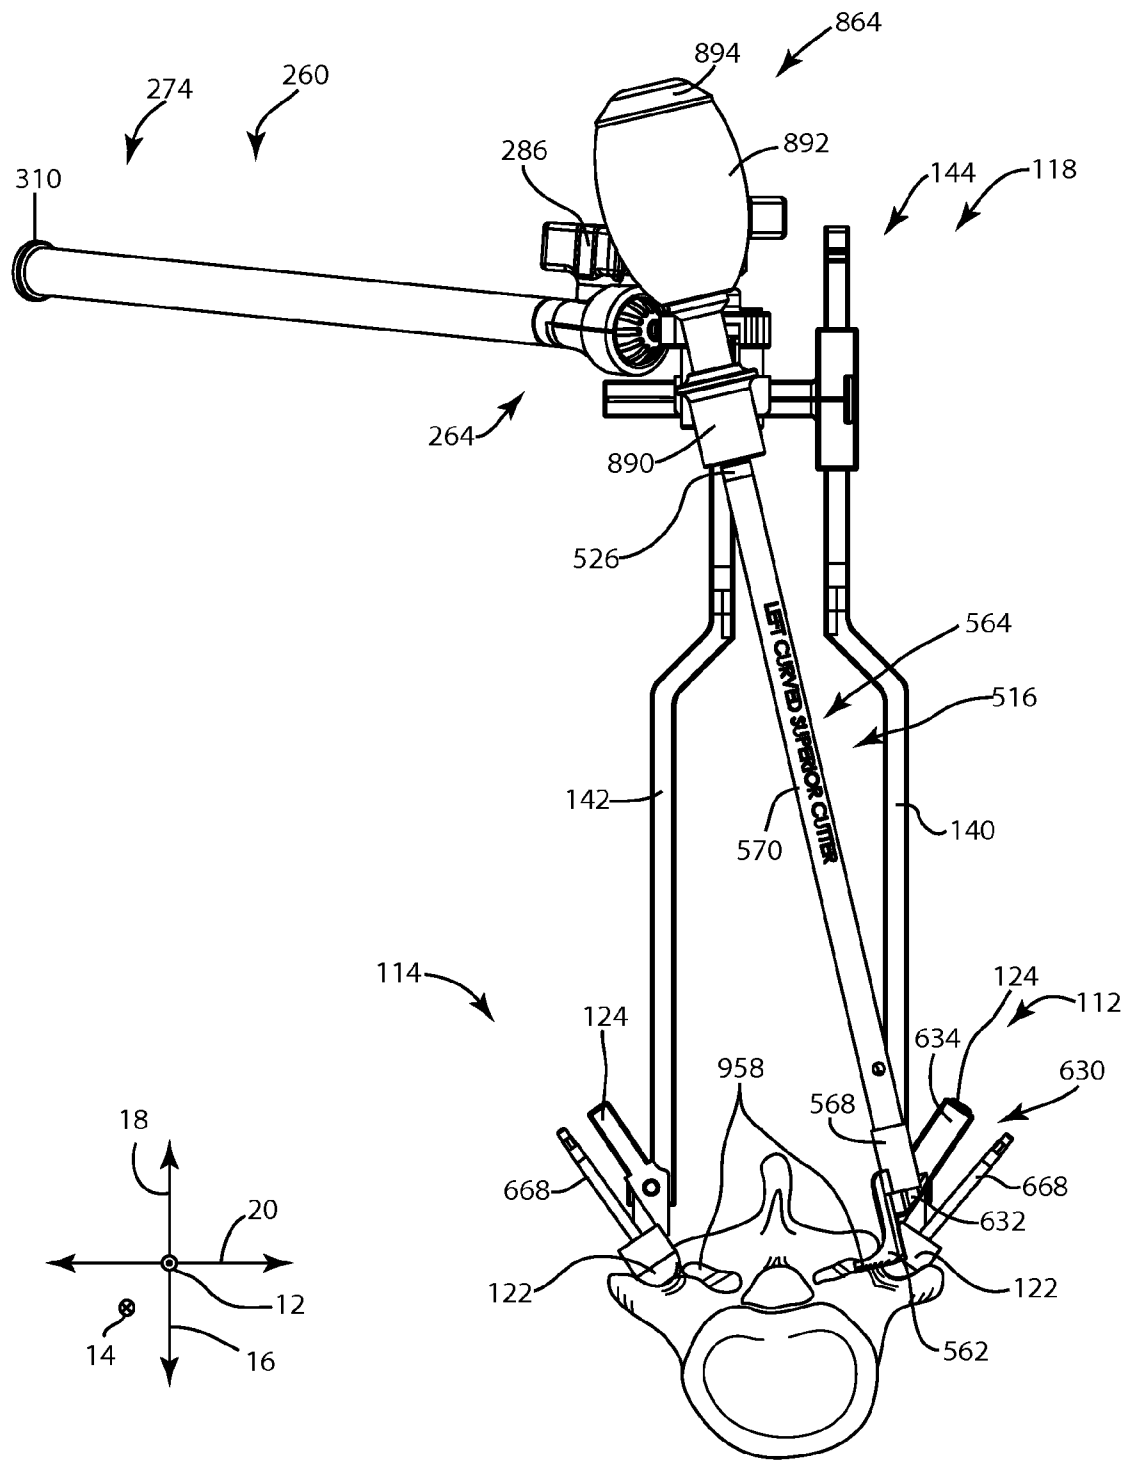


Fig. 41





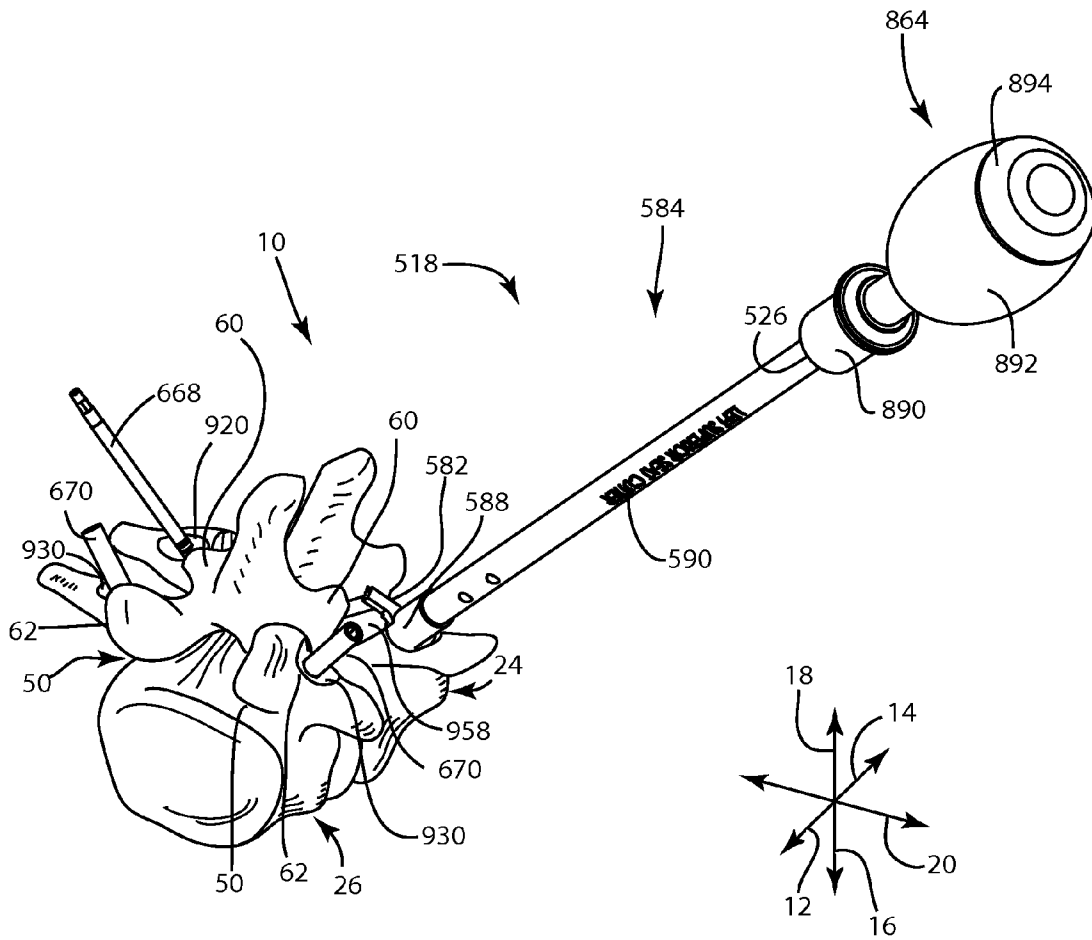


Fig. 43

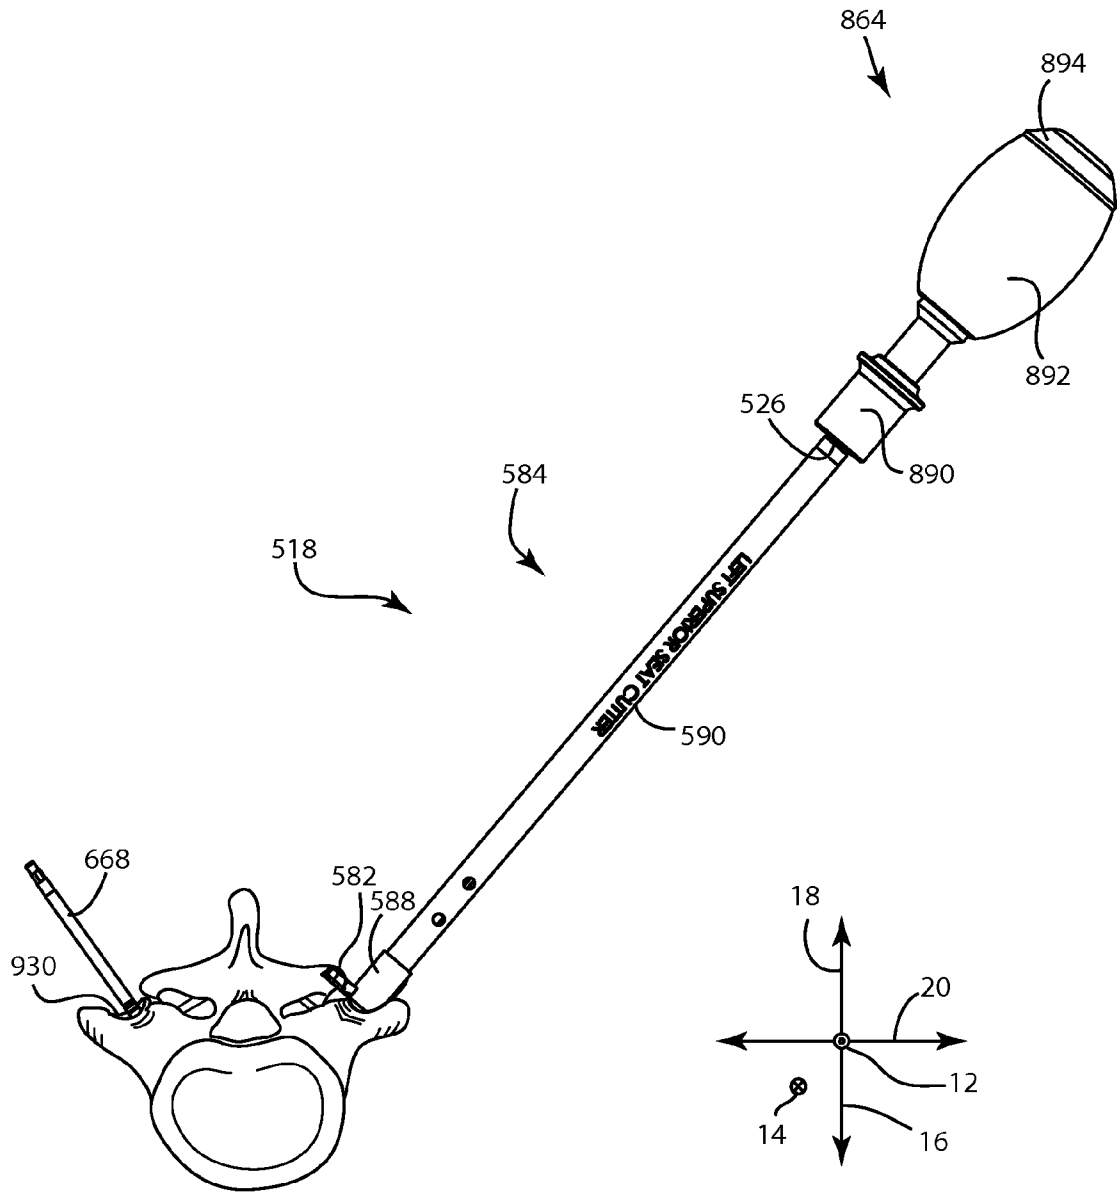


Fig. 44

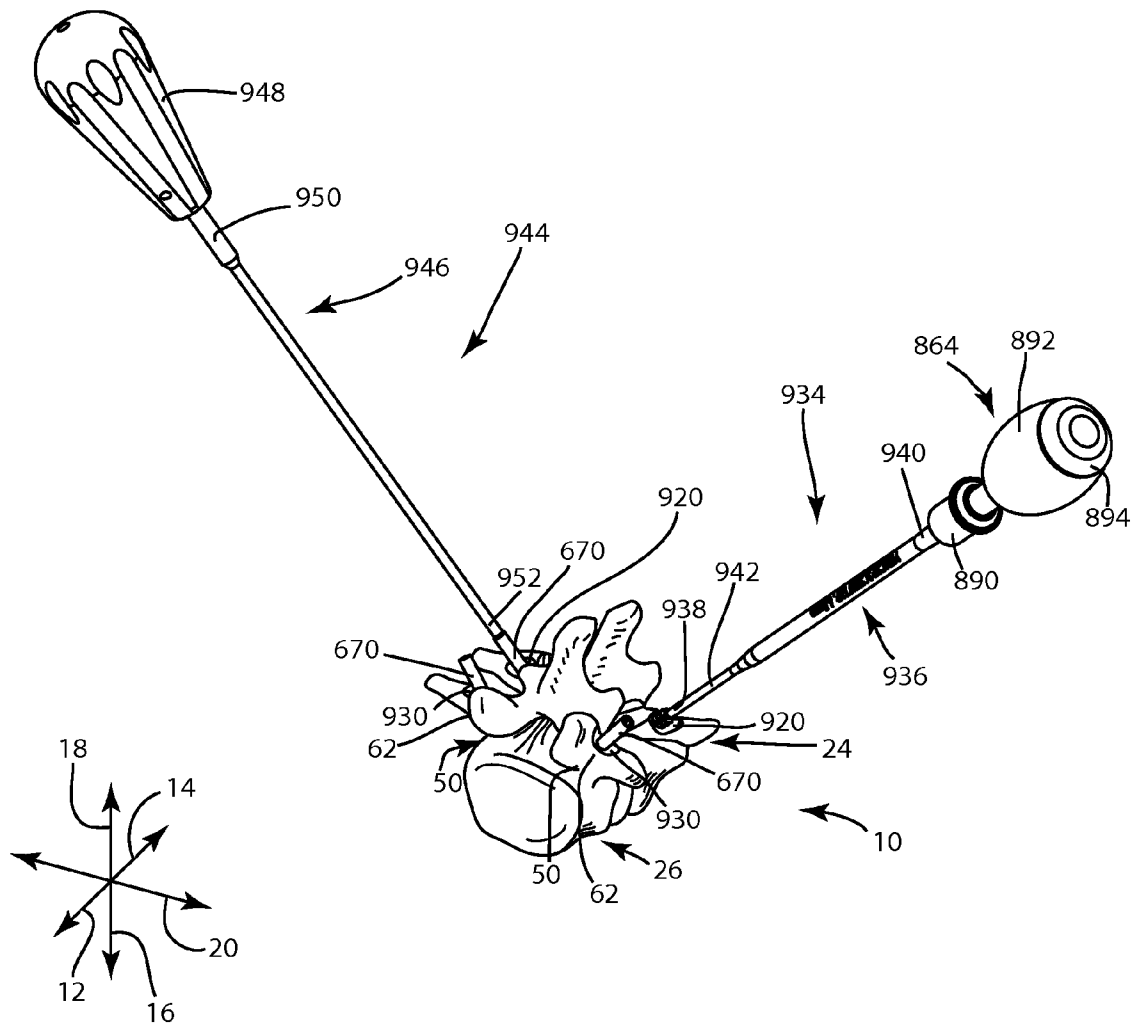


Fig. 45

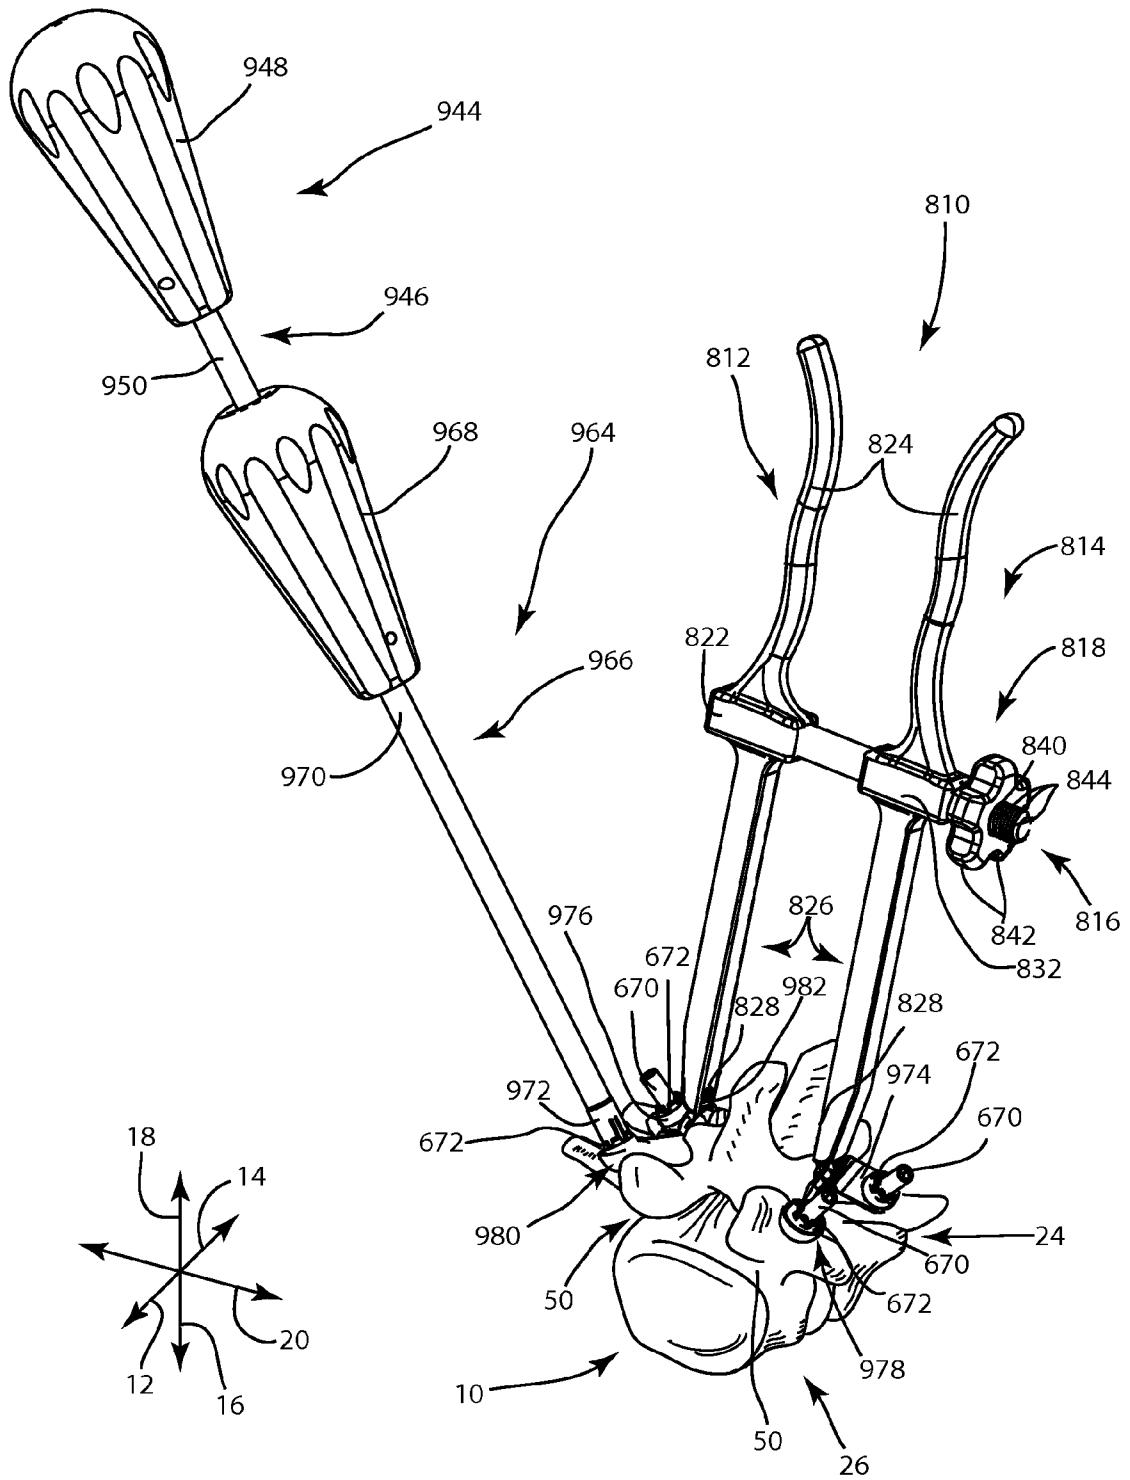


Fig. 46



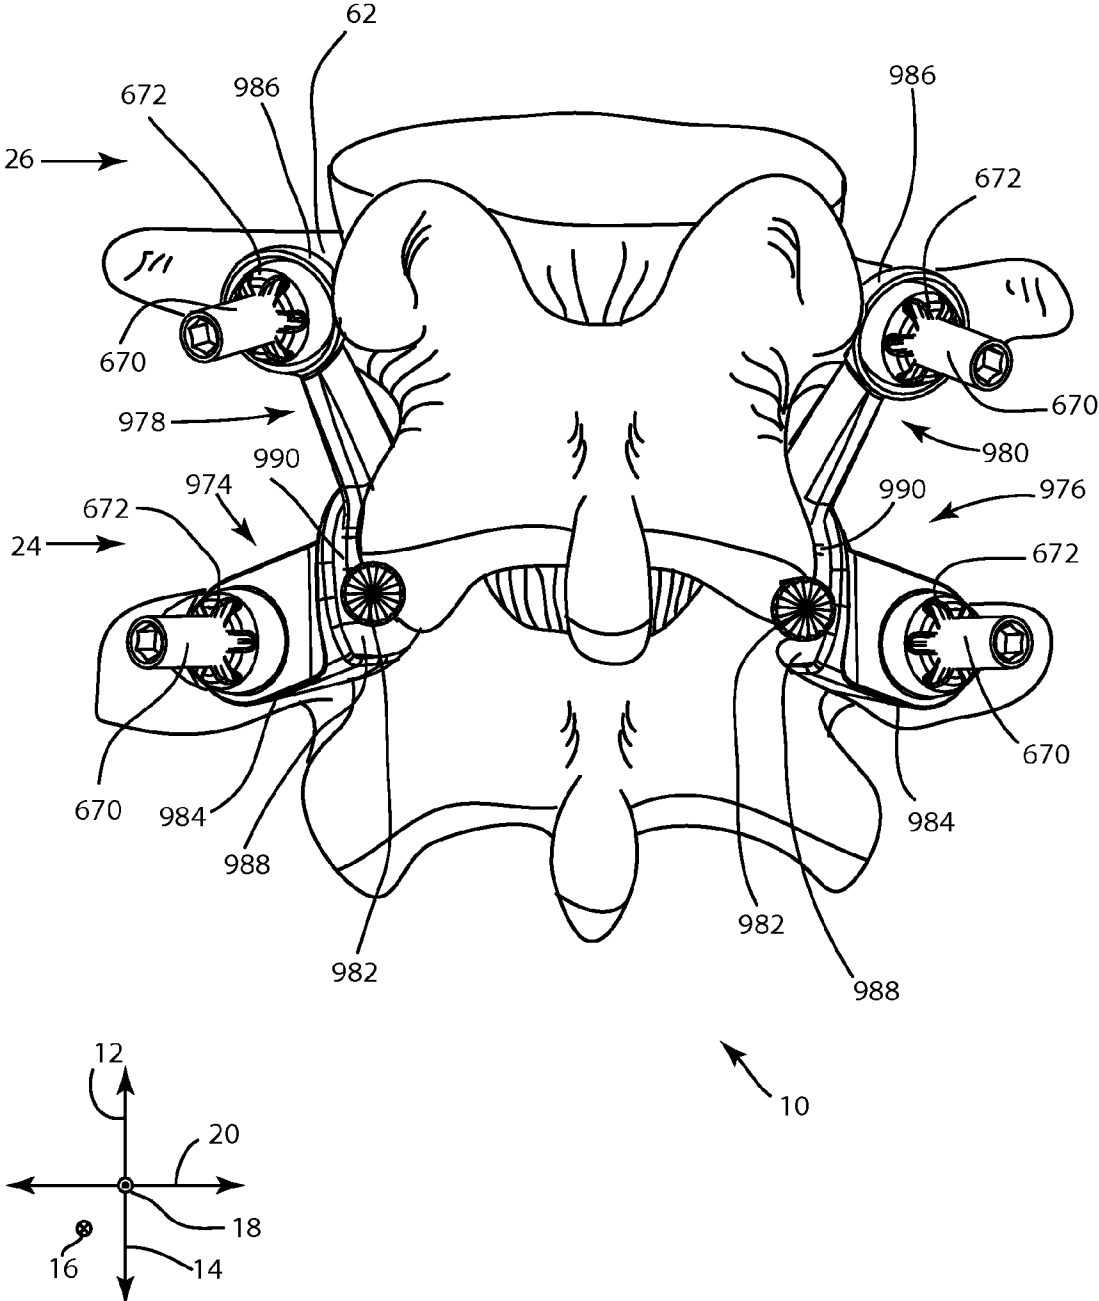


Fig. 48

## SURGICAL MEASUREMENT SYSTEMS AND METHODS

### CROSS-REFERENCE TO RELATED APPLICATIONS

This application is a divisional of the following:

pending U.S. patent application Ser. No. 10/989,971, Applicants' filed on Nov. 11, 2004 and entitled SURGICAL MEASUREMENT SYSTEMS AND METHODS, which is a continuation-in-part of U.S. patent application Ser. No. 10/860,778, Applicants' filed on Jun. 2, 2004 and entitled SPINAL FACET IMPLANT WITH SPHERICAL IMPLANT APPPOSITION SURFACE AND BONE BED AND METHODS OF USE, a continuation-in-part of U.S. patent application Ser. No. 10/860,543, Applicants' filed on Jun. 2, 2004 and entitled SPINAL FACET IMPLANTS WITH MATING ARTICULATING BEARING SURFACE AND METHODS OF USE, a continuation-in-part of U.S. patent application Ser. No. 10/860,495, Applicants' filed on Jun. 2, 2004 and entitled LINKED BILATERAL SPINAL FACET IMPLANTS AND METHODS OF USE, and a continuation-in-part of U.S. patent application Ser. No. 10/860,487, Applicants' filed on Jun. 2, 2004 and entitled SPINAL FACET JOINT IMPLANT, the disclosures of which are incorporated herein by reference.

### BACKGROUND OF THE INVENTION

#### 1. The Field of the Invention

The present invention relates generally to systems and methods for measuring and/or resecting bone, and more particularly, to systems and methods for measuring and resecting spinal facets for replacement with facet prostheses.

#### 2. The Relevant Technology

Many people experience back pain. Back pain is not only uncomfortable, but can be particularly debilitating. Many people who wish to participate in sports, manual labor, or even sedentary employment are unable to do so because of pains that arise from motion of or pressure on the spinal column. Such pains are often caused by traumatic, inflammatory, metabolic, synovial, neoplastic and degenerative disorders of the spine.

One of the most common surgical interventions today is arthrodesis, or spine fusion, of one or more motion segments, with approximately 300,000 procedures performed annually in the United States. Clinical success varies considerably, depending upon technique and indications, and consideration must be given to the concomitant risks and complications. For example, spine fusion may decrease function by limiting the range of motion for patients in flexion, extension, rotation, and lateral bending. Furthermore, spine fusion may create increased stresses and, therefore, accelerated degeneration of adjacent non-fused motion segments. Additionally, pseudoarthrosis, as a result of an incomplete or ineffective fusion, may reduce or even eliminate pain relief for the patient. Finally, the fusion device, whether artificial or biological, may migrate out of the fusion site.

Recently, several attempts have been made to recreate the natural biomechanics of the spine by use of an artificial disc. Artificial discs provide for articulation between vertebral bodies to recreate the full range of motion allowed by the elastic properties of the natural intervertebral disc which directly connects two opposed vertebral bodies. However, artificial discs do not fully address the mechanics of motion of the spinal column.

In addition to the intervertebral disc, posterior elements called the facet joints help to support axial, torsional and shear loads that act on the spinal column. The facet joints are diarthroidal joints that provide both sliding articulation and load transmission features. The facet joints also help to maintain the appropriate level of stiffness in the spinal column in all planes of motion, including flexion and extension, lateral bending, and rotation.

Recently, some procedures for replacing facet joints have been proposed. Unfortunately, spinal anatomy is very complex and highly variable from one person to another. Accordingly, making accurate spinal measurements and resections can be very difficult. Spinal resection is made even more difficult by the need to avoid nerve roots positioned in close proximity to the bony features that are to be resected. Facet joint replacement adds additional difficulties because the facet joints articulate to provide three distinct planes of motion. Accordingly, replacement of the facet joints requires that each plane of motion be reproduced in order to accurately preserve the natural biomechanics of the spine. Hence, a need exists for systems and methods that facilitate accurate measurement and resection of spinal bone tissue.

### BRIEF DESCRIPTION OF THE DRAWINGS

Various embodiments of the present invention will now be discussed with reference to the appended drawings. It is appreciated that these drawings depict only typical embodiments of the invention and are therefore not to be considered limiting of its scope.

FIG. 1 is a perspective view of the L4 and L5 vertebrae of a spinal column.

FIG. 2 is a perspective view of a primary reamer and a secondary reamer usable to provide semispherical resections in the spinal column of FIG. 1.

FIG. 3 is an enlarged, perspective view of the heads of the primary and secondary reamers of FIG. 2.

FIG. 4 is an exploded, perspective view of a frame attachable to the L5 vertebra of FIG. 1 to guide measurement and resection of bony landmarks of the spinal column.

FIG. 5 is a perspective view of the frame of FIG. 4, in a fully assembled state.

FIG. 6 is a perspective view of a stationary external support attachable to the frame of FIG. 4 to stabilize the frame.

FIG. 7 is an exploded, perspective view of a facet measurement tool capable of registering on the frame of FIG. 4 to measure the position of a most medial and anterior surface of a superior facet of the spinal column.

FIG. 8 is a perspective view of the facet measurement tool of FIG. 7, in a fully assembled state.

FIG. 9 is a plan view of the facet measurement tool of FIG. 7, in a fully assembled state.

FIG. 10 is an exploded, perspective view of a pedicle measurement tool capable of registering on the frame of FIG. 4 to measure the position of a saddle point of a pedicle of the spinal column.

FIG. 11 is a perspective view of the pedicle measurement tool of FIG. 10, in a fully assembled state.

FIG. 12 is a plan view of the pedicle measurement tool of FIG. 10, in a fully assembled state.

FIG. 13 is a perspective view of a short cutting tool, a long cutting tool, a curved cutting tool, and a seat cutting tool, all of which are designed to resect a superior facet of the spinal column.

FIG. 14 is an enlarged, perspective view of one end of the resection feature of the short cutting tool of FIG. 13.



FIG. 15 is a perspective view of one end of the resection feature of the curved cutting tool of FIG. 13.

FIG. 16 is a perspective view of a cutting guide usable to couple the cutting tools of FIG. 13 to the frame of FIG. 4.

FIG. 17 is an exploded, perspective view of an inferior resection tool designed to guide resection of an inferior facet of the spinal column, as well as a guide wire, pedicle screw, and castle nut.

FIG. 18 is a perspective view of the inferior resection tool of FIG. 17, in a fully assembled state.

FIG. 19 is a perspective view of a clamping tool that facilitates attachment of inferior facet prostheses to the spinal column.

FIG. 20 is a perspective view of the L4 and L5 vertebrae of the spinal column of FIG. 1 with an insertion plate of a joint flag inserted between the facets of the facet joint.

FIG. 21 is an enlarged, perspective view of the vertebrae of the spinal column of FIG. 1 with the joint flag in place.

FIG. 22 is a perspective view of the L4 and L5 vertebrae with the joint flag in place, a guide wire inserted along the axis of one pedicle of the L5 vertebra, and a guide wire inserter aligned with the joint flag to facilitate insertion of a guide wire into the other pedicle of the L5 vertebra.

FIG. 23 is a lateral view of the L4 and L5 vertebrae with the joint flag and guide wire in place and the guide wire inserter aligned with the joint flag.

FIG. 24 is a perspective view of the L4 and L5 vertebrae with the joint flag in place, guide wires inserted along the axis of each pedicle of the L5 vertebra, and the superior facets of the L5 vertebrae preliminarily resected.

FIG. 25 is a perspective view of the L4 and L5 vertebrae with the guide wires in place, with one pedicle of the L5 vertebra partially reamed to provide a roughened semispherical surface, and the primary reamer positioned to ream the other pedicle of the L5 vertebra.

FIG. 26 is an enlarged, perspective view of the L4 and L5 vertebrae with the guide wires and the primary reamer in place.

FIG. 27 is a perspective view of the L4 and L5 vertebrae with the guide wires and the joint flag in place, with one pedicle of the L5 vertebra fully reamed to provide a semi-spherical surface, and with the secondary reamer positioned to ream the other pedicle of the vertebra in alignment with the joint flag.

FIG. 28 is an enlarged, perspective view of the L4 and L5 vertebrae with the guide wires, joint flag, and secondary reamer in place.

FIG. 29 is a perspective view of the L4 and L5 vertebrae with the guide wires and the joint flag in place and the frame attached to the stationary external support and to the reamed surfaces of the pedicles of the L5 vertebra, in alignment with the joint flag.

FIG. 30 is a lateral view of the L4 and L5 vertebrae with the guide wires, joint flag, frame, and stationary external support in place.

FIG. 31 is a perspective view of the L4 and L5 vertebrae with the guide wires, frame, and stationary external support in place, with the facet measurement tool registered to the frame to measure the position of the most medial and anterior surface of a superior facet of the L5 vertebra.

FIG. 32 is a cephalad section view of the L4 and L5 vertebrae with the guide wires, frame, stationary external support, and facet measurement tool in place.

FIG. 33 is a perspective view of the L4 and L5 vertebrae with the guide wires, frame, and stationary external support in

place, with the pedicle measurement tool registered to the frame to measure the position of the pedicle of the L4 vertebra.

FIG. 34 is a cephalad section view of the L4 and L5 vertebrae with the guide wires, frame, stationary external support, and pedicle measurement tool in place.

FIG. 35 is a perspective view of the L4 and L5 vertebrae with the L5 guide wires, frame, and stationary external support in place, with an additional guide wire inserted along the axis of one pedicle of the L4 vertebra, and the guide wire inserter positioned to facilitate insertion of another guide wire into the other pedicle of the L4 vertebra.

FIG. 36 is a perspective view of the L4 and L5 vertebrae with the L4 and L5 guide wires, frame, and stationary external support in place, with one pedicle of the L4 vertebra partially reamed to provide a roughened semispherical surface, and the primary reamer positioned to ream the other pedicle of the L4 vertebra.

FIG. 37 is a perspective view of the L4 and L5 vertebrae with the L4 and L5 guide wires, frame, and stationary external support in place, with one pedicle of the L4 vertebra fully reamed to provide a semispherical surface, and the secondary reamer positioned to ream the other pedicle of the L4 vertebra.

FIG. 38 is a perspective view of the L4 and L5 vertebrae with the L5 guide wires, frame, and stationary external support in place, with a pedicle tapping tool positioned to tap one pedicle of the L4 vertebra, and a screw insertion tool positioned to insert a pedicle screw in the other pedicle of the L4 vertebra.

FIG. 39 is a perspective view of the L4 and L5 vertebrae with the L5 guide wires, L4 pedicle screws, frame, and stationary external support in place, with one of the inferior facets of the L4 vertebra resected, and with the inferior resection tool registered to the frame and coupled to the L4 vertebra via the castle nut to facilitate resection of the other inferior facet of the L4 vertebra.

FIG. 40 is a lateral view of the L4 and L5 vertebrae with the L5 guide wires, L4 pedicle screws, castle nut, frame, stationary external support, and inferior resection tool in place.

FIG. 41 is a perspective view of the L4 and L5 vertebrae with the L5 guide wires, L4 pedicle screws, frame, and stationary external support in place, with one superior facet of the L5 vertebra partially resected, and with the curved cutting tool registered to the frame to facilitate resection of the other superior facet of the L5 vertebra.

FIG. 42 is a cephalad view of the L5 vertebra with the L5 guide wires, frame, stationary external support, and curved cutting tool in place.

FIG. 43 is a perspective view of the L4 and L5 vertebrae with the L5 guide wires and L4 pedicle screws in place, with one superior facet of the L5 vertebra fully resected, and with the seat cutting tool registered to one of the guide wires to facilitate further resection of the other superior facet of the L5 vertebra.

FIG. 44 is a cephalad view of the L5 vertebra with the L5 guide wires and the seat cutting tool in place.

FIG. 45 is a perspective view of the L4 and L5 vertebrae with the L4 pedicle screws in place, with a pedicle tapping tool positioned to tap one pedicle of the L5 vertebra, and the screw insertion tool positioned to insert a pedicle screw in the other pedicle of the L5 vertebra.

FIG. 46 is a perspective view of the L4 and L5 vertebrae with the L4 and L5 pedicle screws in place, with superior facet prostheses attached to replace the superior facets of the L5 vertebra via castle nuts, with inferior facet prostheses positioned to replace the inferior facets of the L4 vertebra,

with a nut tightening tool positioned in cooperation with the screw insertion tool to secure one of the inferior facet prostheses to the L4 vertebra via a castle nut, and with the clamping tool positioned to retain the inferior facet prostheses.

FIG. 47 is a perspective view of the L4 and L5 vertebra with the L4 and L5 pedicle screws, castle nuts, superior facet prostheses, and inferior facet prostheses in place.

FIG. 48 is a posterior view of the L4 and L5 vertebra with the L4 and L5 pedicle screws, castle nuts, superior facet prostheses, and inferior facet prostheses in place.

#### DETAILED DESCRIPTION

The present invention advances the state of the art by providing systems and methods that can be used to more accurately measure and resect structural tissue, and more particularly, spinal bone tissue. The present invention can be used to facilitate facet joint replacement, thereby alleviating back pain resulting from traumatic, inflammatory, metabolic, synovial, neoplastic and degenerative spinal disorders. The configuration and operation of at least one embodiment of the invention will be shown and described in greater detail with reference to FIGS. 1 through 48, as follows.

In this application, “registration” refers to a process by which one object is coupled to another in such a manner that translation and/or rotation of the second object is limited relative to the first object, so that the first object serves as a reference frame for motion or operation of the second object. “Coupling” refers to direct contact between two objects or indirect contact (i.e., contact via a third object) by which relative motion between the first two objects is limited. Two objects that are integrally formed with each other may also be said to be “coupled” together (i.e., via integral formation).

A “registration feature” is any part of a first object that can be used as a coupling point for registration of a second object with respect to the first object. A “registration interface” is any part of a second object that can be used to register the second object to a first object. “Attachment” refers to a form of coupling in which a first object is restricted from translating or rotating away from a second object. “Connecting” does not require restriction of relative motion between two objects; any form of direct or indirect contact is sufficient.

“Semispherical” does not require a half sphere; rather, any shape with a surface that replicates any portion of the surface of a sphere may be termed “semispherical.” A “bony landmark” is a pre-established portion of a bone having a recognizable shape. A “pivot feature” is any pivotable joint or rounded surface that provides generally rotary motion with respect to an object such as a bone. “Rotation” does not require full-circle motion; indeed, oscillatory pivotal motion is one form of rotation. A “displacement” refers to a linear or angular separation between two objects, or mathematical entities. An “axis” of an object is generally an axis of symmetry, or where the object is not symmetrical, may be a direction along which the length of the object is oriented.

A “cutting tool” is a tool designed to remove a portion of an object, such as a bone. A “resection tool” need not actually have an implement for cutting, but may simply be a guide for a cutting tool. A “guide feature” is any feature capable of guiding an object such as a cutting blade; accordingly, a guide feature may be a slot, hole, surface having a shape that provides a pre-established guide pattern, or the like.

Referring to FIG. 1, a perspective view illustrates a portion of a spine 10. The spine 10 has a cephalad direction 12, a caudal direction 14, an anterior direction 16, a posterior direction 18, and a medial/lateral axis 20, all of which are oriented as shown by the arrows bearing the same reference numerals.

The spine 10 has a sagittal plane 22, which defines the plane of symmetry of the spine 10, and is thus positioned between the left and right sides of the spine 10. The sagittal plane 22 is perpendicular to the medial/lateral axis 20. In this context, “symmetry” is used loosely because natural anatomical differences will be present between the left and right sides of the spine 10. “Left” and “right” are used with reference to a posterior view, i.e., a view from behind the spine 10. “Medial” refers to a position or orientation toward the sagittal plane 22, and “lateral” refers to a position or orientation relatively further from the sagittal plane 22.

As shown, the portion of the spine 10 illustrated in FIG. 1 includes a first vertebra 24, which may be the L5 (Fifth Lumbar) vertebra of a patient, and a second vertebra 26, which may be the L4 (Fourth Lumbar) vertebra of the patient. The systems and methods may be applicable to any vertebra or vertebrae of the spine 10 and/or the sacrum (not shown); however, the embodiment shown the Figures may be particularly applicable to the L4 and L5 vertebrae. In this application, the term “vertebra” may be broadly interpreted to include the sacrum.

As shown, the first vertebra 24 has two pedicles 30 and a posterior arch, or lamina 32, that extends between the posterior ends of the pedicles 30 to couple the pedicles 30 together. The first vertebra 24 also has a pair of transverse processes 34 that extend laterally from the pedicles 30 generally along the medial/lateral axis 20, and a spinous process 36 that extends from the lamina 32 along the posterior direction 18.

The first vertebra 24 also has a pair of superior facets 38, which are positioned toward the top of the first vertebra 24 and face generally medially. Additionally, the first vertebra 24 has inferior facets 40, which are positioned toward the bottom of the first vertebra 24 and face generally laterally. Each of the pedicles 30 of the first vertebra 24 has a saddle point 42, which is positioned generally at the center of the juncture of each superior facet 38 with the adjacent transverse process 34.

Similarly, the second vertebra 26 has two pedicles 50 and a posterior arch, or lamina 52, that extends between the posterior ends of the pedicles 50 to couple the pedicles 50 together. The second vertebra 26 also has a pair of transverse processes 54 that extend from the pedicles 50 generally along the medial/lateral axis 20, and a spinous process 56 that extends from the lamina 52 along the posterior direction 18.

The second vertebra 26 also has a pair of superior facets 58, which are positioned toward the top of the second vertebra 26 and face generally inward. Additionally, the second vertebra 26 has inferior facets 60, which are positioned toward the bottom of the second vertebra 26 and face generally outward. Each of the pedicles 60 of the second vertebra 26 has a saddle point 62, which is positioned generally at the center of the juncture of each superior facet 58 with the adjacent transverse process 54.

The superior facets 38 of the first vertebra 24 articulate (i.e., slide and/or press) against the inferior facets 60 of the second vertebra 26 to limit relative motion between the first and second vertebrae 24, 26. Thus, the combination of each superior facet 38 with the adjacent inferior facet 60 provides a facet joint 64. The first and second vertebrae 24, 26 thus define two facet joints 64 that span the distance between the first and second vertebrae 24, 26. The inferior facets 40 of the first vertebra 40 and the superior facets 58 of the second vertebra 26 are part of other facet joints that control motion between the first and second vertebrae 24, 26 and adjacent vertebrae (not shown) and/or the sacrum (also not shown).

Each of the facet joints 64 may be covered by a capsule (not shown) containing a fluid (not shown) that reduces wear of the

facets **38, 60** and facilitates articulation. Additionally, layers of cartilage (not shown) may cover the facets **38, 60** to further reduce wear and facilitate articulation. These anatomical structures, as well as the various muscles, ligaments, and nerves of the spine, will not be depicted in the Figures to enhance the clarity of the disclosure.

Referring to FIG. 2, a perspective view illustrates a primary reamer **70** and a secondary reamer **72** that may be used to form semispherical interfaces, or semispherical surfaces, on the saddle points **42, 62** of the vertebrae **24, 26**, as will be illustrated subsequently. The primary reamer **70** has a shaft **74**, a torque interface **76**, which may include a hexagonal cross-section designed to facilitate receipt of torque from a source such as a handle or a motor, and a head **78** designed to cut away bone tissue. Similarly, the secondary reamer **72** has a shaft **80**, a torque interface **76**, and a head **82**.

Each of the reamers **70, 72** may have an indicator that clearly specifies its identity and/or intended use. For example, the shaft of the primary reamer **70** has an indicator **84** that indicates that it is for primary reaming of a spherical seat, and the secondary reamer **72** has an indicator **86** that indicates that it may be used to clean or finish a previously reamed semispherical seat.

Referring to FIG. 3, an enlarged, perspective view illustrates the heads **78, 82** of the reamers **70, 72** of FIG. 2. As shown, the primary reamer **70** has a bore **88** that may pass through the head **78** and into the shaft **74**. The bore **88** is sized to receive a guide wire or a similar structure to control the position of the head **78**. Furthermore, the head **78** has a flat surface **90** oriented generally perpendicular to an axis (not shown) of the shaft **74**. The head **78** also has a plurality of cutting flanges **92** distributed about the circumference of the head **78**. Each of the cutting flanges **92** has a straight portion **94** and an arcuate portion **96** adjacent to the flat surface **90**.

In operation, the primary reamer **70** is registered on a guide wire or the like, and advanced toward the bone surface to be resected. The arcuate portions **96** then contact the bone and resect away bone tissue to provide a generally semispherical indentation in the bone. The primary reamer **70** continues to advance into the bone until the flat surface **90** abuts the bone. The primary reamer **70** is then substantially unable to advance further. Thus, the flat surface **90** controls the depth of reaming.

The secondary reamer **72** also has a bore **98** that passes through the head **82** of the secondary reamer **72** and into the corresponding shaft **80**. The bore **98** may also receive a guide wire or the like to help control positioning of the head **82**. The head **82** has a pair of central teeth **100** that protrude inward on either side of an (not shown) of the shaft **80**. The head **82** also has a dome **102** with a straight portion **104** having a generally cylindrical shape, and an arcuate portion **106** with a semispherical profile that caps the cylindrical shape of the straight portion **104**.

In operation, the secondary reamer **72** may be used to remove bone tissue left by the primary reamer **70**. More precisely, the primary reamer **70** leaves the portion of bone abutting the flat surface **90** intact, and thus forms a surface that is not entirely semispherical. The secondary reamer **72** removes the excess bone left by the primary reamer **70**. The secondary reamer **72** may be registered in the same manner as the primary reamer **70**, and advanced into the indentation formed by the primary reamer **70**. The central teeth **82** remove the central bone portion that abutted the flat surface **90** to leave an indentation that is more precisely semispherical. The dome **102** is unable to remove any additional bone tissue, so the secondary reamer **72** is unable to significantly deepen the indentation.

Referring to FIG. 4, an exploded, perspective view illustrates a "sagittal bridge," or frame **110**, that can be attached to the spine **10** to serve as a base for measurement and resection. The frame **110** includes a first anchor **112** and a second anchor **114** that may be generally symmetrically positioned on either side of the sagittal plane **22** and attached, for example, to the saddle points **42** of the pedicles **30** of the first vertebra **24**. The frame **110** also has an external anchor **116** that facilitates attachment of the frame **110** to an external structure such as an operating table or the like. A bridging structure **118** couples the first anchor **112**, second anchor **114**, and external anchor **116** together in a manner that permits adjustment of the relative positions of the first and second anchors **112, 114** to account for anatomical differentiation in spinal anatomy.

As shown, each of the first and second anchors **112, 114** has a main body **120**, an anchoring feature **122**, and a registration feature in the form of a guide post **124**. Each main body **120** has a generally rectangular, tapered shape and is integrally formed with the corresponding anchoring feature **122** and guide post **124**. Each of the anchoring features **122** has a semispherical surface **128** that may be substantially half-spherical in shape. Each of the anchoring features **122** also has a bore **130** that extends through the corresponding semispherical surface **128**.

Each of the guide posts **124** may have a generally rectangular cross section. The generally rectangular cross section may have two long sides and two short sides, so that a corresponding generally rectangular bore of a surgical instrument may only slide into engagement with the guide post **124** in two different orientations. Of the two orientations, the wrong orientation may be made obvious via interference of the frame **110** with the surgical instrument, handle positioning, marking of the surgical instrument, or any other method known in the art. In alternative embodiments, a registration post may have a shape that is engageable with a corresponding bore in only one orientation. For example, a circular shaft with a single flat side, a trapezoidal shape, or the like may be used to ensure that engagement is able to occur along only one relative orientation.

The external anchor **116** has an attachment post that permits attachment of the external anchor **116** to the bridging structure **118**. Additionally, the external anchor **116** has an external anchoring feature **134** that can easily be gripped by a stationary external support. The external anchoring feature **134** has a generally spherical surface **136** with a plurality of grooves **138** distributed about its surface. The generally spherical surface may easily be gripped by a grip (not shown in FIG. 4) having a corresponding concave semispherical surface.

As shown in FIG. 4, the bridging structure **118** has a first arm **140** and a second arm **142** that cooperate to couple the first and second anchors **112, 114** and the external anchor **116** together. The first and second arms **140, 142** are movable with respect to each other in such a manner that the relative positions of the first and second anchors **112, 114** can be changed in three dimensions. A locking mechanism **144** enables the relative positions of the anchors **112, 114** to be simultaneously locked in all three dimensions. The manner in which the bridging structure **118** permits relative movement and locking of the arms **140, 142** will be described in greater detail subsequently.

The first arm **140** has a first end **154** coupled to the locking mechanism **144** and to the external anchor **116**. Additionally, the first arm **140** has a second end **156** attached to the first anchor **112**. The first end **156** has an alcove **158** with a generally rectangular shape. A hole **160** passes through one wall of the alcove **158** such that a fastener such as a screw **162**

may be inserted through the hole 160 to engage the corresponding aperture 126 of the first anchor 112. The screw 162 and the aperture 126 may each be threaded so that the screw 162 threadably engages the aperture 126. The generally rectangular end of the main body 120 of the first anchor 112 fits into the alcove 158 in such a manner that relative rotation between the first anchor 112 and the second end 156 is unable to occur.

The first end 154 includes a first rod 164 along which relative sliding motion between the arms 140, 142 can occur to provide relative translation along one axis, or one dimension. The first end 154 also has a stop feature 166 that limits motion along the first rod 164. The stop feature 166 may include a flexible flange 168 that extends away from, and then back toward, the first rod 164 along a generally U-shaped path. The flange 168 terminates in a stopper 170 that protrudes outward from the flange 168 and the aligned surface of the first rod 164.

When a slider slides over the stop feature 166 and onto the first rod 164, the relatively small thickness of the flexible flange 168 enables it to bend inward to remove the stopper 170 from the pathway of the slider. However, when the slider slides back toward the stop feature 166, the flexible flange 168 is only able to spring outward such that the stopper 170 further impedes removal of the slider from the first rod 164. The stopper 170 may be ramped on one side, and not on the other, to permit one-way passage of the slider as outlined above.

Like the first arm 140, the second arm 142 has a first end 174 coupled to the locking mechanism 144 and to the external anchor 116. Additionally, the second arm 142 has a second end 176 attached to the first anchor 112. The second end 176 has an alcove 178 that is a substantial mirror image of the alcove 158 of the first arm 140. Thus, a second fastener such as a screw 162 may be inserted through a hole 160 formed in one wall of the alcove 178 and threaded into engagement with the aperture 126 of the second anchor 114. As with the alcove 158, the generally rectangular end of the main body 120 of the second anchor 114 fits into the alcove 178 in such a manner that relative rotation between the first anchor 114 and the second end 176 is unable to occur.

The first end 174 of the second arm 142 has a second rod 184 that permits relative sliding motion between the arms 140, 142 along a second axis perpendicular to the first rod 164. The first end 174 also has a stop feature 166 that limits motion along the second rod 164 in a manner similar to that of the stop feature 166 of the first end 154 of the first arm 140.

The locking mechanism 144 includes a variety of components that permit tri-axial relative translation between the first ends 154, 174 of the arms 140, 142. More precisely, the locking mechanism 144 includes a first retention member 190, a first slider member 192, a second slider member 194, a compression member 196, a second retention member 198, two fasteners such as screws 200, and a handle 202. The interaction of these components to provide relative motion and locking will be described in greater detail as follows.

The first retention member 190 has a base plate 204 and a pair of receiving posts 206 that extend from the base plate 204, toward the handle 202. Each of the receiving posts 206 has a hole 208 that may be threaded to enable threadable engagement with the screws 200.

The first slider member 192 may have a third rod 210 that enables relative motion between the first and second arms 140, 142 along a third axis orthogonal to the first and second rods 164, 184. Additionally, the first slider member 192 has a first slider 212 that captures and slides along the first rod 164. The first slider 212 has a bore 214 with a generally rectangular

shape sized to receive the first rod 164 with clearance so that the first rod 164 is able to slide through the bore 214.

The first slider member 192 also has a slot 216 that bisects the third rod 210 and substantially bisects the first slider 212. The slot 216 has a certain width that can be compressed by pressing the two halves of the third rod 210 together, thereby deforming the walls of the first slider 212 to bend the bore 214 from its normally straight shape. Due to the close fit between the first slider 212 and the first rod 164, bending of the bore 214 causes frictional contact between the first slider 212 and the first rod 164. Thus, compression on the third rod 210 arrests motion of the first slider 212 along the first rod 164.

The second slider member 194 has a second slider 220 and a third slider 222, which are oriented orthogonally to each other and to the first slider 212. The second slider 220 has a bore 224 with a generally rectangular shape, with one unbounded side. Similarly, the third slider 222 has a bore 226 with a generally rectangular shape, with one unbounded side. The bores 224 and 226 of the second and third sliders 220, 222 are generally sized and shaped to slide along the corresponding second and third rods 184, 210, respectively.

Thus, the first, second, and third rods 164, 184, 210 cooperate with the first, second, and third sliders 212, 220, 222 to provide three linear joints that enable relative motion between the first and second arms 140, 142 along three orthogonal axes. In alternative embodiments, motion along only one or two axes may be desired. In other alternative embodiments, one or more joints with non-translational motion, such as rotary joints, may be used in place of any of the linear joints of the frame 110. However, use of the linear joints is advantageous because the guide posts 124 can be kept in a substantially fixed orientation relative to each other when the joints are adjusted. Thus, the frame 110 accounts for three-dimensional variation in the relative positions of the saddle points 42 of the first vertebra 24, while still maintaining the desired coordination between operations that are to be keyed to the guide posts 124.

Returning to the embodiment of FIG. 4, the compression member 196 may have a plate 230 with a generally rectangular shape. A central plateau 232 protrudes from the center of one side of the plate 230, toward the handle 202. The central plateau 232 has an alcove 234 with a generally circular cross section. The compression member 196 may be pressed toward the second slider 220 to cause locking of all three linear joints in a manner that will be described subsequently.

The second retention member 198 has a trough 236 within which the compression member 196 may be generally positioned. The second retention member 198 also has two holes 238 through which the screws 200 may pass to anchor in the holes 208 of the receiving posts 206 of the first retention member 190. Additionally, the second retention member 198 has a central plateau 240 in which an aperture 242 is formed. The aperture 242 may be threaded. The second retention member 198 also has an attachment projection that protrudes and has a bore (not shown) sized to receive the attachment post 132 of the external anchor 116.

The handle 202 has a threaded stud 246 sized to threadably engage the aperture 242 of the central plateau 240 of the second retention member 198. Furthermore, the handle 202 has wings 248 that facilitate gripping and rotation of the handle 202 by hand. The handle 202 may be used to move the locking mechanism 144 between a locked configuration, in which the three linear joints are relatively freely movable to enable tri-axial relative translation between the anchors 112, 114, and an unlocked configuration in which the anchors 112, 114 are fixed with respect to each other.

The first retention member 190, first slider member 192, second slider member 194, compression member 196, second retention member 198, screws 200, and handle 202 may be relatively easily assembled to form the bridging structure 118. According to one method of assembly, the compression member 196 may first be positioned in the trough 236 of the second retention member 198. The second slider member 194 may be positioned to rest on the base plate 204 of the first retention member 190, between the receiving posts 206 of the first retention member 190.

The screws 200 may be inserted through the holes 238 of the second retention member 198 and rotated into threaded engagement with the holes 208 of the receiving posts 206. The screws 200 may be tightened such that the receiving posts 206 abut the second retention member 198. The threaded stud 246 of the handle 202 may be inserted through the aperture 242 of the central plateau 240 of the second retention member 198 and rotated into threaded engagement with the aperture until the end of the threaded stud 246 enters the alcove 234 of the central plateau 232 of the compression member 196.

With the handle 202 positioned so as to allow the compression member 196 to remain in a retracted position, the first rod 164 may be inserted into the first slider 212, the second rod 184 may be inserted into the second slider 220, and the third rod 210 may be inserted into the third slider 222. The first and second sliders 212, 220 may be translated to slide past the stop features 166 at the ends of the first and second rods 164, 184, respectively. Assembly of the locking mechanism 144 is then complete.

Next, the external anchor 116 may be attached to the locking mechanism 144. More precisely, the attachment post 132 of the external anchor 116 may be inserted into the attachment projection 244 of the second retention member 198 and retained via interference fitting, welding, or the like. The anchors 112, 114 may be attached to the second ends 156, 176 of the first and second arms 140, 142 via the screws 162 in the manner indicated previously to complete assembly of the bridging structure 118.

Referring to FIG. 5, a perspective view illustrates the frame 110 in a fully assembled state. The anchoring features 122 of the anchors 112, 114 are ready to be attached to the saddle points 42 of the first vertebra 24. With the locking mechanism 144 in the unlocked configuration, the rods 164, 184, 210 are able to slide relatively freely through the sliders 212, 220, 222, respectively to permit tri-axial adjustment of the relative positions of the first and second anchors 112, 114. This permits the frame 110 to be easily adapted to a variety of spinal morphologies, including bone structures that are asymmetrical across the sagittal plane 22.

After the anchors 112, 114 have been relatively positioned as desired, the handle 202 may be rotated by hand to press the compression member 196 against the adjacent side of the second rod 184. As a result, the opposite side of the second rod 184 is pressed against the bore 224 of the second slider 220, thereby pressing the bore 226 of the third slider 222 against the third rod 210 to sandwich the third rod 210 between the third slider 222 and the base plate 204 of the first retention member 190. Consequently, the second and third sliders 220, 222 are unable to slide along the second and third rods 184, 210 due to transverse pressure acting transversely to compress the sliders 220, 222 against the rods 184, 210, respectively.

Compression of the third rod 210 also compresses the slot 216 of the first slider member 192, thereby compressing the sides of the first slider 212 against the first rod 164. Accordingly, the first slider 212 is also unable to slide along the first rod 164. Relative motion between the anchors 112, 114 is thus

substantially prevented along all three joints, or all three orthogonal axes. This is accomplished by actuating only one user control, i.e., the handle 202. Separate controls need not be actuated to lock each of the joints of the bridging structure 118.

Referring to FIG. 6, a perspective view illustrates a stationary external support 260 according to one embodiment of the invention. The stationary external support 260 may be coupled to a stationary object such as an operating table, wall, or the like, and to the external anchor 116 of the frame 110 to keep the frame 110 substantially stationary.

As shown in FIG. 6, the stationary external support 260 may have a fixed end 262 designed to be attached to the stationary object via a clamp (not shown), permanent welded attachment, or the like. The stationary external support 260 also has a grip 264 that can be used to grip the external anchor 116 of the frame 110 in a manner that will be described subsequently. The grip 264 and the first end 262 are movably coupled together via an adjustment structure 266.

The adjustment structure 266 may include a first rod 270, a second rod 272, and a third rod 274 that are coupled together via three joints, or more precisely, a first joint 276, a second joint 278, and a third joint 280. The rods 270, 272, 274 may be formed of a sturdy material such as steel, aluminum, or the like, and may be solid or hollow. Each of the joints 276, 278, 280 may provide at least rotary motion, and possibly linear motion, and may be securely lockable to enable the stationary external support 260 to provide stiff support to the frame 110.

The first joint 276 may have a main body 282 and a rod coupler 284 that is attached to the first rod 270 and is rotatably attached to the main body 282. Additionally, the first joint 276 has a handle 286 that can be rotated to control locking of the relative orientations of the main body 282 and the rod coupler 284. The rod coupler 284 has a slot 288 with a large portion through which the corresponding end of the first rod 270 passes.

The handle 286 has a plurality of ridges 290 that facilitate rotation of the handle 286 by hand, or through the use of a corresponding tool having an indentation that matches the shape of the handle 286. Clockwise rotation, or tightening, of the handle 286 substantially prevents further relative rotation between the rod coupler 284 and the main body 282 to keep the rod coupler 284 at a pre-established orientation with respect to the main body 282.

Additionally, if the first joint 276 also enables relative translation, tightening of the handle 286 may compress the rod coupler 284 to compress the slot 288 to grip the corresponding end of the first rod 270 to restrict relative translation between the rod coupler 284 and the first rod 270. Alternatively, the end of the first rod 270 may have a groove or other feature that cooperates with a corresponding feature within the rod coupler 284 to prevent relative translation. Gripping the end of the first rod 270 may also restrict rotation of the end of the first rod 270 within the rod coupler 284.

The second joint 278 may be configured somewhat similarly to the first joint 276, and may thus have a main body 292, a rod coupler 294, and a handle 296. The main body 292 is integrally formed with the main body 282 of the first joint 278. The rod coupler 294 is rotatably coupled to the main body 292 and retains the second rod 272 in a manner that may permit relative translation between the rod coupler 294 and the second rod 272. The handle 296 has wings 300 that facilitate gripping for manual rotation of the handle 296.

Tightening of the handle 286 of the first joint 276 substantially prevents relative rotation between the main body 292 and the rod coupler 294. Accordingly, the handle 286 is able to lock relative rotation between the first and second rods 270,

272 along three orthogonal axes. The handle 296 of the second joint 278 optionally also prevents relative translation and rotation between the rod coupler 294 and the second rod 272. Thus, the handle 296 of the second joint 278 may be capable of locking relative rotation and translation between the first and second rods 270, 272 along or about a single axis.

The third joint 280 is configured similarly to the first and second joints 276, 278. Thus, the third joint 280 has a main body 302, a rod coupler 304, and a handle 296. The main body 302 is rigidly attached to the end of the second rod 272. The main rod coupler 304 is rotatably coupled to the main body 302 and retains the third rod 274 in a manner that may permit relative translation between the rod coupler 304 and the third rod 274. The handle 296 has the same configuration as the handle 296 of the second joint 278. Tightening of the handle 296 substantially prevents relative rotation between the main body 302 and the rod coupler 304, and optionally also prevents relative translation between the rod coupler 304 and the third rod 274.

Furthermore, tightening the handle 296 prevents rotation of the end of the third rod 274 within the rod coupler 304. Thus, the handle 296 of the third joint 280 may be capable of locking relative rotation between the second and third rods 272, 274 about two orthogonal axes, and of locking relative translation between the second and third rods 272, 274 along one of the axes of rotation.

Each of the second and third rods 272, 274 has a stop 310 in the form of an outwardly-extending flange. The stops 310 prevent the second and third rods 272, 274 from being withdrawn from the rod couplers 294, 304 of the second and third joints 278, 280, respectively. Furthermore, each of the joints 276, 278, 280 may have a plurality of clocking features, such as internal ridges (not shown), which may restrict relative rotation of each of the joints 276, 278, 280 to a number of discrete positions, thereby enhancing the stability of the joints 276, 278, 280.

The grip 264 has a first gripping member 312, a second gripping member 314, and a handle 296. The first gripping member 312 may be integrally formed with the third rod 274, and the second gripping member 314 may be separate from the first gripping member 312 so as to permit relative motion between the first and second gripping members 312, 314. The handle 296 has the same configuration as the handles 296 of the second joint 278 and the third joint 280. The handle 296 has a threaded stud 316 that passes through a hole (not shown) of the first gripping member 312 and threadably engages a threaded hole 318 of the second gripping member 314.

Clockwise rotation, or tightening, of the handle 296 of the grip 264 may draw the first and second gripping members 312, 314 together. The first and second gripping members 312, 314 may cooperate to define a semispherical surface 320 with a concave configuration sized to receive the generally spherical surface 136 of the external anchor 116. The generally spherical surface 136 of the external anchor 116 may be inserted into the semispherical surface 320 of the grip 264 prior to tightening of the handle 296 so that the generally spherical surface 136 is unable to be drawn free of the semispherical surface 320 without loosening of the handle 296. The ridges 138 of the generally spherical surface 136 enhance locking and help to prevent relative rotation between the external anchor 116 and the grip 264.

Referring to FIG. 7, an exploded, perspective view illustrates a facet measurement tool 330 according to one embodiment of the invention. The facet measurement tool 330 may be designed to register on the frame 110 to measure a bony landmark such as the most medial and anterior surface of a superior facet, otherwise denoted "P1."

As shown, the facet measurement tool 330 may have a registration member 332, a handle member 334, a fastener such as a screw 336, a slider member 338, and a contact member 340. The registration member 332 has a registration interface 342, a first slider 344, and an arm 346 that couples the registration interface 342 and the first slider 344 together. The registration interface 342 has a bore 348 with a generally rectangular shape sized to receive the guide post 124 of the first anchor 112 of the frame 110. The first slider 344 also has a bore 350 with a generally rectangular cross sectional shape suitable for receiving a rod having a corresponding rectangular cross section.

Additionally, the first slider 344 has an aperture 352 that may be threaded to permit threaded engagement of the screw 336 with the aperture 352. The first slider 344 also has an indicator 354 that indicates the identity and proper use of the registration member 332 to help prevent improper assembly or use of the registration member 332. As shown in FIG. 7, the indicator 354 indicates that the registration member 332 is to be used for measurement of P1, or the most medial and anterior surface of a superior facet, on the left-hand side of a vertebra.

The handle member 334 has a handle 358 shaped to be grasped by a hand of a user, and an attachment end 360 attachable to the first slider 344 of the registration member 332. The attachment end 360 has an alcove 362 designed to conform to the shape of the first slider 344 to prevent relative rotation between the handle member 334 and the first slider 344. The alcove 362 has a hole (not shown) that permits passage of the screw 336 therethrough to attach the attachment end 360 to the first slider 344.

The slider member 338 has a first rod 364 slidable within the first slider 344 and a second slider 366 shaped to slidably receive the contact member 340. The first rod 364 is bounded by a generally rectangular cross sectional shape, and has markings 368 arranged in two separate groupings along its length. The second slider 366 has a bore 370 with a generally rectangular cross sectional shape similar to the bore 350 of the first slider 344. A stop feature 166 like those of the frame 110 is positioned on the opposite end of the first rod 364 from the second slider 366 to prevent unintended withdrawal the first rod 364 from the bore 350 of the first slider 344.

The contact member 340 has a second rod 374, a contact extension 376 extending from the second rod 374, and a grip 378 that extends from the opposite end of the second rod 374. The second rod 374 is bounded by a generally rectangular cross section and has a plurality of markings 380 distributed along one end, adjacent to the grip 378. The contact extension 376 has a contact feature 382 shaped to contact P1 to permit measurement of the position of P1 with the facet measurement tool 330.

According to one method of assembling the facet measurement tool 330, the attachment end 360 of the handle member 334 may first be attached to the first slider 344 by inserting the screw 336 through the hole (not shown) of the alcove 362 and then threadably anchoring the screw 336 in the aperture 352 of the first slider 344. Then, the first rod 364 may be inserted into the bore 350 of the first slider 344 until the first slider 344 has moved past the stop feature 166. The contact member 340 may then be inserted into the bore 370 of the second slider 366 so that the second rod 374 is positioned within the bore 370 to complete assembly of the facet measurement tool 330.

Referring to FIG. 8, a perspective view illustrates the facet measurement tool 330 in a fully assembled state. Once assembled, the registration member 332, slider member 338, and contact member 340 all combine to form a displacement structure 384 capable of permitting bi-axial variation in the

15

relative positions of the registration interface **342** and the contact feature **382**. More precisely, the first slider **344** and the first rod **364** cooperate to permit relative translation along one axis, and the second slider **366** and the second rod **374** cooperate to permit relative translation along an axis perpendicular to that of the first slider **344** and the first rod **364**.

The registration member **332** is particular to the left-hand side, and a mirror image of the registration member **332** would be required for right-side measurement operations. However, the slider member **338** and the contact member **340** may be used for either left-hand side or right-hand side measurement, and simply be rotated 180° and assembled with a right-hand registration member, handle member, and screw (not shown) to provide a facet measurement tool for the right-hand side.

Referring to FIG. 9, a plan view illustrates the facet measurement tool **330** in the fully assembled state. As shown, each of the first and second sliders **344**, **366** has a plurality of recesses **386** positioned to facilitate reading of the markings **368**, **380** of the first and second rods **364**, **374**, respectively. Each of the sliders **344**, **366** also has measurement edges **388** that align with the tic marks adjacent to the numbers of the markings **368**, **380** so that a clear and unambiguous measurement reading may be obtained.

As depicted in FIG. 9, the markings **368** are positioned on either side of the first slider **344**. Additionally, the recesses **386** and measurement edges **388** are positioned on either end of the first slider **344** so that readings can be taken from either side. With respect to the orientation of FIG. 9, the markings **368** above the first slider **344** include numerals that fall in between the numerals of the markings **368** below the first slider **344**. The appropriate measurement may be acquired from either set of the markings **368**, depending on which set of the markings **368** has a tic mark closest to the corresponding measurement edge **388**.

For example, in FIG. 9, the tic marks on either side of the number "16" are aligned with the measurement edges **388** on the adjacent end of the first slider **344**. The markings **368** below the first slider **344** do not have a tic mark aligned with the corresponding measurement edges **388**. Accordingly, "16" is the appropriate measurement. By permitting measurement readings to be taken on either side of the slider **344**, the resolution of the facet measurement tool **330** along the axis of the first rod **364** can be effectively doubled.

The same principle is applied to the second slider **366**. However, the markings **380** are not read from either side of the second slider **366**. Rather, the markings **380** are offset on each pair of adjacent surfaces of the generally square cross section of the second rod **374**, as shown in FIG. 9. Thus, the appropriate measurement for the second slider **366** and the second rod **374** is "10." In alternative embodiments, different offsets between all four sides may be used to further increase the resolution of the measurement provided by the second slider **366** and the second rod **374**.

Referring to FIG. 10, an exploded, perspective view illustrates a pedicle measurement tool **430** according to one embodiment of the invention. The pedicle measurement tool **430** may be designed to register on the frame **110** to measure the three-dimensional position of a bony landmark such as one of the saddle points **62** of a pedicle **50** of the second vertebra **26**.

As shown, the pedicle measurement tool **430** has a registration member **432**, a handle member **334**, a slider member **434**, a screw **336**, a pin **436**, a rod member **438**, and a contact member **440**. The registration member **432** may be similar or even identical to the registration member **332** of the facet measurement tool **330**, except that the registration member

16

**432** has a first slider **444** with an indicator **454** that indicates that registration member **432** is for saddle point, or pedicle, measurement rather than facet measurement. The handle member **334** and the screw **336** may be identical to those of the previous embodiment.

The rod member **438** has a first rod **464** and a second rod **466** integrally formed with the first rod **464** and separated from the first rod **464** by a ninety-degree bend **468**. The first rod **464** is designed to slide within the first slider **444**, and the second rod **466** is designed to slide within a second slider. The first rod **464** has a plurality of markings **470** used to indicate measurements, and the second rod **466** has markings **472** that indicate measurements along an axis orthogonal to that of the first rod **464**.

A stop feature **166** like those of the frame **110** is positioned at the end of the first rod **464** opposite to the bend **468** to prevent withdrawal of the first rod **464** from within the first slider **444**. The second rod **466** has an aperture **474** positioned at the end of the second rod **466** opposite to the bend **468** to receive the pin **436**. Once in place within the aperture **474**, the pin **436** protrudes from the aperture **474** to act as a stop feature to prevent withdrawal of the second rod **466** from the second slider.

As shown, the slider member **434** has a second slider **476** and a third slider **478**. The second slider **434** has a bore **480** with a generally rectangular cross section shaped to slidably receive the second rod **466**. Similarly, the third slider **478** has a bore **482** with a generally rectangular cross section shaped to slidably receive the contact member **440**. The second slider **476** has an indicator **484** that indicates the identity and intended use of the slider member **434**, i.e., use on the pedicle measurement tool **430** for the left-hand side of the spine.

The contact member **440** has a third rod **494**, a contact extension **496** extending from one end of the third rod **494**, and a grip **378** extending from the opposite end of the third rod **494**. The third rod **494** has a series of markings **500** distributed along its length. The third rod **494** is also bounded by a generally rectangular cross section so that the third rod **494** is slidably receivable within the bore **482** of the third slider **478**. The contact extension **496** has a contact feature **502** shaped to contact the saddle point **62** of the left-hand side of the second vertebra **26** for accurate positional measurement.

The registration member **432**, handle member **334**, slider member **434**, screw **336**, pin **436**, rod member **438**, and contact member **440** may all be assembled in a variety of ways to provide the pedicle measurement tool **430**. According to one method, the attachment end **360** of the handle member **334** is first attached to the first slider **444** via the screw **336** by inserting the screw **336** through the hole (not shown) of the alcove **362** and threadably anchoring the screw **336** in the aperture **352** of the first slider **444**.

The first rod **464** is then inserted through the bore **350** of the first slider **444** until the first slider **444** has passed beyond the stop feature **166** at the end of the first rod **464**. The second rod **466** is then inserted through the bore **480** of the second slider **476** until the second slider **476** has passed beyond the aperture **474** at the end of the second rod **466**. Then, the pin **436** is inserted into the aperture **474** to prevent passage of the second slider **476** back over the aperture **474**. The contact member **440** is then inserted through the bore **482** of the third slider **478** until the third rod **494** is positioned within the bore **482** to complete assembly of the pedicle measurement tool **430**.

Referring to FIG. 11, a perspective view illustrates the pedicle measurement tool **430** in a fully assembled state. Once assembled, the registration member **432**, slider member **434**, rod member **438**, and contact member **440** all combine to form a displacement structure **504** capable of permitting tri-

axial variation in the relative positions of the registration interface **342** and the contact feature **502**. More precisely, the first slider **444** and the first rod **464** cooperate to permit relative translation along one axis. The second slider **476** and the second rod **466** cooperate to permit relative translation along an axis perpendicular to that of the first slider **444** and the first rod **464**. The third slider **478** and the third rod **494** cooperate to permit relative translation along an axis perpendicular to those of the first slider **444** and the first rod **464**, and the second slider **476** and the second rod **466**.

The registration member **432** is particular to the left-hand side, and a mirror image of the registration member **432** would be required for right-side measurement operations. However, the slider member **434**, pin **436**, rod member **438**, and contact member **440** may be used for either left-hand side or right-hand side measurement. The slider member **434**, pin **436**, and rod member **438** may simply be rotated 180°, and the contact member **440** may be rotated 180° about a different axis, and then the slider member **434**, pin **436**, rod member **438**, and contact member **440** may be reassembled to each other and to a right-hand registration member, handle member, and screw (not shown) to provide a pedicle measurement tool for the right-hand side.

Referring to FIG. 12, a plan view illustrates the pedicle measurement tool **430** in a fully assembled state. As shown, each of the first, second, and third sliders **444**, **476**, **478** has a plurality of recesses **386** positioned to facilitate reading of the markings **470**, **472**, **500** of the first, second, and third rods **464**, **466**, **494**, respectively. Each of the sliders **444**, **476**, **478** also has measurement edges **388** that align with the tic marks adjacent to the numbers of the markings **470**, **472**, **500** so that a clear and unambiguous measurement reading may be obtained.

The recesses **386** and measurement edges **388** operate in the manner described previously, in connection with FIG. 9, to facilitate measurement. Furthermore, like the markings **368** of FIG. 9, each set of markings **470**, **472** of the first and second rods **464**, **466** of FIG. 12 is separated into two groupings to double the resolution of measurement along their respective axes by permitting measurements to be read from either end of the first and second sliders **444**, **476**. As more clearly illustrated in FIG. 11, the markings **500** of the third rod **494** may also be staggered between adjacent, perpendicular facets of the third rod **494** to provide a similar increase in resolution, as on the second rod **374** the facet measurement tool **330** of FIG. 8.

Referring to FIG. 13, a perspective view illustrates a kit **510** of cutting tools designed to resect the superior facets **38** of the first vertebra **24**. The kit **510** includes a short cutting tool **512**, a long cutting tool **514**, a curved cutting tool **516**, and a seat cutting tool **518**. Each of the cutting tools **512**, **514**, **516**, **518** is registrable to the spine **10** via a post or guide wire (not shown in FIG. 13) to guide rotation of the cutting tools **512**, **514**, **516**, **518** to a fixed axis. The short cutting tool **512**, the long cutting tool **514**, and the curved cutting tool **516** cooperate to resect bone tissue from the superior facet **38** of the left-hand side of the first vertebra **24** to provide a substantially continuous, planar surface. The seat cutting tool **518** is usable to provide a planar surface relatively nearer the saddle point **42** of the pedicle **30** of the left-hand side of the first vertebra **24**. The manner in which the kit **510** is used will be shown and described in greater detail subsequently.

As illustrated in FIG. 13, the short cutting tool **512** has a shaft **520** and a resection feature **522** protruding asymmetrically from the shaft **520**. The shaft **520** receives oscillating torque, which is then transmitted to the resection feature **522** to remove bone tissue as the resection feature **522** oscillates

against the bone tissue. The shaft **520** has a central portion **524**, a torque receiver **526**, and a distal cap **528**. In alternative embodiments, a shaft **520** of a superior cutting tool (not shown) need not have a circular cross section, and need not be used for rotation. Rather, such a shaft may be used to drive linear motion to provide resection of a bony landmark. Such translational superior cutting tools are envisioned by the present invention.

The central portion **524** has an indicator **530** that indicates the identity and intended use of the short cutting tool **512**, i.e., resection of the superior facet **38** of the left-hand side of the first vertebra **24**. The torque receiver **526** is shaped to receive a torque transmitting implement such as a manually grippable handle or a coupling driven by a motor. The torque receiver **526** may have a hexagonal cross section or the like to permit transmission of torque when inserted into a corresponding hexagonal cavity of a driver (not shown in FIG. 13). Manual rotation of the cutting tools **512**, **514**, **516**, **518** may provide greater control for purposes of superior facet resection. The shaft **520** further has a registration feature **532** that facilitates rotation about the desired stationary axis. The registration feature **532** will be shown and described in greater detail subsequently.

As illustrated in FIG. 13, the resection feature **522** is integrally formed with the distal cap **528** of the shaft **520**. The resection feature **522** includes an arm **534** generally parallel to the shaft **520** and a cutting surface **536** that extends substantially perpendicular to the arm **534**. The cutting surface **536** is shaped to form a substantially planar resection surface in response to oscillatory rotation about an axis of rotation **538** of the shaft **520**. As shown, the resection feature **522** protrudes non-collinear to the axis of rotation **538**. Thus, the resection feature **522** is not symmetrical about the axis of rotation **538**. The resection feature **522** and the registration feature **532** will be shown and described in greater detail subsequently.

The long cutting tool **514** similarly has a shaft **540** and a resection feature **542** protruding from the shaft **540**. The shaft **540** has a central portion **544**, a torque receiver **526**, and a distal cap **548**. The central portion **544** has an indicator **550** that indicates the identity and intended use of the long cutting tool **514**. The shaft **540** has a registration interface **532** that facilitates rotation about the desired stationary axis, i.e., the axis of rotation **538** of the shaft **540**. The resection feature **542** is integrally formed with the distal cap **548** and has an arm **534** and a cutting surface **556** that extends substantially perpendicular to the arm **534**. The cutting surface **556** is shaped to cooperate with the cutting surface **536** of the short cutting tool **512** to form the substantially planar resection surface.

The curved cutting tool **516** similarly has a shaft **560** and a resection feature **562** protruding from the shaft **560**. The shaft **560** has a central portion **564**, a torque receiver **526**, and a distal cap **568**. The central portion **564** has an indicator **570** that indicates the identity and intended use of the curved cutting tool **516**. The shaft **560** has a registration interface **532** that facilitates rotation about the desired stationary axis, i.e., the axis of rotation **538** of the shaft **560**. The resection feature **562** is integrally formed with the distal cap **568** and has an arm **534** and a cutting surface **576** that extends substantially perpendicular to the arm **534**.

The cutting surface **576** is shaped to cooperate with the cutting surfaces **536**, **556** of the short cutting tool **512** and the long cutting tool **514** to form the substantially planar resection surface. However, unlike the cutting surfaces **536**, **556**, the cutting surface **576** is generally arcuate in shape. The configuration of the cutting surface **576** will be shown and described in greater detail subsequently.



The seat cutting tool **518** also has a shaft **580** and a resection feature **582** protruding from the shaft **580**. The shaft **580** has a central portion **584**, a torque receiver **526**, and a distal cap **588**. The central portion **584** has an indicator **590** that indicates the identity and intended use of the seat cutting tool **518**. The shaft **580** has a registration interface **592** that facilitates rotation about the desired stationary axis, i.e., the axis of rotation **538** of the shaft **580**. The resection feature **582** is integrally formed with the distal cap **588** and has a cutting surface **596** that extends substantially perpendicular to the shaft **580**. The seat cutting tool **518** may be registered differently from the cutting tools **512**, **514**, **516**; therefore, the resection feature **582** does not require an arm **534** to displace the cutting surface **596** from the distal cap **588**.

Referring to FIG. **14**, an enlarged, perspective view illustrates the resection feature **522** and the corresponding end of the shaft **520** of the short cutting tool **512** in greater detail. As shown, the registration interface **532** has a bore **600** that passes through the distal cap **528** and into the remainder of the shaft **520** via an aperture **602** formed in the distal cap **528**. Accordingly, the registration interface **532** is able to receive a stationary registration feature such as a cylindrical member to constrain rotation of the short cutting tool **512** to the axis of rotation **538** of the shaft **520**.

As illustrated in FIG. **14**, the cutting surface **536** has a leading edge **604** and a rasp portion **606** that trails behind the leading edge **604** when the cutting surface **536** moves clockwise about the axis of rotation **538**, as viewed from the torque receiver **526**. The leading edge **604** has a wedge **608** with an acute angle that enables the wedge **608** to split off and pry up bits of bone tissue. The rasp portion **606** has a plurality of abrasive features in the form of teeth **610** that abrade the bone surface to further remove bone tissue. The teeth **610** may also have sharpened edges that scrape against the bone as the rasp portion **606** follows the leading edge **604**. If desired, the teeth **610** may vary slightly in length so that each tooth removes progressively more bone.

The teeth **610** advantageously are oriented to cut substantially along only one direction of rotation of the short cutting tool **512**, i.e., the direction moving away from the foramenal space of the first vertebra **24**. Thus, the sensitive nerve roots that extend through the foramenal space are protected from abrasion by the relatively blunt, trailing edges of the teeth **610**. In alternative embodiments, a rasp portion of a superior facet cutting tool may have teeth with various shapes to provide straight teeth, angled teeth, diamond-shaped teeth, or any other desirable tooth configuration.

The leading edge **604** and the rasp portion **606** provide two different types of cutting action that cooperate to enhance the efficiency of resection, as well as provide a relatively smooth resection surface. The short cutting tool **512** may be rotated by hand in an oscillatory manner about the axis of rotation **538** to form a portion of a resection surface that is generally bounded by a sector of a circle.

Referring to FIG. **15**, an enlarged, perspective view illustrates the resection feature **562** and the corresponding end of the shaft **560** of the curved cutting tool **516** in greater detail. The registration interface **532** of the curved cutting tool **516** is not shown in detail in FIG. **15**, but is substantially the same as that of the short cutting tool **512**, as described in connection with FIG. **14**. The curved, or generally arcuate, shape of the cutting surface **576** is more clearly illustrated in FIG. **15**.

As in the short cutting tool **512**, the cutting surface **576** of the curved cutting tool **516** has a leading edge **614** and a rasp portion **616** that trails behind the leading edge **614** when the cutting surface **576** moves clockwise about the axis of rotation **538**, as viewed from the torque receiver **526**. The leading

edge **614** has a wedge **618** with an acute angle that enables the wedge **618** to split off and pry up bits of bone tissue. The rasp portion **616** has a plurality of abrasive features in the form of teeth **620** that abrade the bone surface to further remove bone tissue.

As in the cutting surface **536**, the leading edge **614** and the rasp portion **616** of the cutting surface **576** provide two different types of cutting action that cooperate to enhance the efficiency of resection, as well as provide a relatively smooth resection surface. The curved cutting tool **516** may be rotated by hand in an oscillatory manner about the axis of rotation **538** to form a portion of a resection surface that is generally bounded by a skewed sector of a circle. The long cutting tool **514** and the curved cutting tool **516** may form progressively larger resections than the short cutting tool **512**, and may thus be used in progressive combination to split the superior facet resection procedure into a plurality of relatively simple steps.

Referring to FIG. **16**, a perspective view illustrates one embodiment of a cutting guide **630** usable to couple the short cutting tool **512**, the long cutting tool **514**, and the curved cutting tool **516** of FIG. **13** to the frame **110** of FIG. **4**. As shown, the cutting guide **630** has a main body **632**, a registration interface **634** designed to be registered on the frame **110**, and a registration feature **636** designed to guide motion of the cutting tools **512**, **514**, **516**.

The main body **632** may have a plurality of bends, including a first bend **640**, a second bend **642**, and a third bend **644** that provide the appropriate orientation of the registration feature **636** relative to the registration interface **634**. The main body **632** also has a shoulder **646** adjoining the registration feature **636** to support the cutting tools **512**, **514**, **516**, thereby controlling the depth of resection.

Further, the main body **632** has an indicator **648** that indicates the identity and intended use of the cutting guide **630**, i.e., resection of the superior facet **38** on the left-hand side of the first vertebra **24**. The indicator **648** further indicates that the cutting guide **630** corresponds to a specific implant, i.e., superior implant **#1**, which may be selected from a kit of several superior prostheses based on measurements made with the facet measurement tool **330** and/or the pedicle measurement tool **430**. Generally, each prosthesis is selected based on which prosthesis of the kit most nearly resembles the natural facet to be replaced.

The registration interface **634** has a bore **650** with a generally rectangular shape selected to slide onto the guide post **124** of the first anchor **112** of the frame **110**. The rectangular shape of the bore **650** and the guide post **124** then prevents relative rotation between the frame **110** and the cutting guide **630**. The registration feature **636** has a post **652** with a generally circular cross section sized to slide into the bore **600** of any of the cutting tools **512**, **514**, **516**. The post **652** may slide into the corresponding bore **600** until the corresponding distal cap **528**, **548**, **568** abuts the shoulder **646** of the main body **632**. The shoulder **646** thus controls the depth of resection by determining the plane within which resection occurs.

Referring to FIG. **17**, an exploded, perspective view illustrates an inferior resection tool **660** according to one embodiment of the invention. The inferior resection tool **660** may be used to resect the inferior facet **60** of the left-hand side of the second vertebra **26**. As will be described in greater detail subsequently, the inferior resection tool **660** remotely simulates the tangential contact between members of a ball-and-rough joint such as the facet joints **64** of the spine **10**, or a replacement facet joint designed to mimic the articulation of the facet joints **64**.

As shown, the inferior resection tool **660** has a registration member **662**, an anchoring member **664**, and a pivot member

666. A guide wire 668, a pedicle screw 670, and a castle nut 672 may be used in conjunction with the registration member 662 and the anchoring member 664, and are therefore depicted in FIG. 17, in addition to the first anchor 112 illustrated previously in FIGS. 4 and 5.

The registration member 662 has a registration interface 680 designed to register the inferior resection tool 660 on the frame 110 of FIG. 4. Additionally, the registration member 662 has a first arm 682 coupled to the registration interface 680 at a bend 684. The registration interface 680 has a bore 686 with a generally rectangular cross section shaped to receive the guide post 124 of the first anchor 112 of the frame 110 in such a manner that the registration member 662 is unable to rotate with respect to the frame 110. The bend 684 positions the first arm 682 at a desired orientation with respect to the registration interface 680. The first arm 682 has an extension 688 with a relatively narrower cross section and a shoulder 690 that controls the depth of insertion of the extension 688 into the pivot member 666.

As shown, the anchoring member 664 has an anchoring feature 700, a guide feature 702, a second arm 704, and an arcuate extension 706. The anchoring feature 700 is shaped to abut the left-side saddle point 62 of the second vertebra 26 in such a manner that the anchoring member 664 is able to rotate against the second vertebra 26 until locked in place via the castle nut 672. The anchoring feature 700 has a semispherical surface that permits relative rotation between the anchoring member 664 and the second vertebra 26 along three orthogonal axes. The anchoring feature also has a bore 712 through which the pedicle 670 may extend. The semispherical surface 700 corresponds to a semispherical surface of an inferior prosthesis so that motion of the anchoring feature 700 against the bone mimics positioning of the corresponding inferior prosthesis.

The guide feature 702 has a slot 714 positioned to guide a cutting tool, such as a blade of an oscillating saw designed for cutting bone. The second arm 704 has a first portion 716 and a second portion 718 extending from the first portion 716 at an angle. The second arm 704 also has an indicator 720 that indicates the identity and intended use of the second arm 704, i.e., resection of the left-side facet 60 of the second vertebra 24.

The indicator 720 further indicates that the anchoring member 664 corresponds to a specific implant, i.e., inferior implant #4 "long," which may be selected from a kit of several inferior implants based on measurements made with the facet measurement tool 330 and/or the pedicle measurement tool 430. The registration member 662 may similarly correspond to a specific superior implant, and may have an indicator (not shown) that indicates which implant of a kit of multiple implants the registration member 662 corresponds to.

The arcuate extension 706 has a generally arcuate shape designed to cooperate with the pivot member 666 to provide a rotary joint. The arcuate extension 706 has a groove 722 that extends along its length to interface with the pivot member 666.

The pivot member 666 has a main body 730, a retention interface 732, a lever 734, a plate 736, and an engagement interface 738. The main body 730 has a generally U-shaped configuration with a first pair of apertures 740 and a second pair of apertures 742. The first pair of apertures 742 pivotably engages the lever 734. The second pair of apertures 742 pivotably engages the plate 736. The main body 730 also has a plateau 744 that pivotably engages the engagement interface 738.

The plate 736 has a pair of pins 746 that extend into the second pair of apertures 742 of the main body 730 such that

the plate 736 is rotatable relative to the main body 730 about an axis passing through the pins 746. The retention interface 732 has a first bracket 748 with a generally U-shaped configuration and a second bracket 750 that also has a generally U-shaped configuration and is positioned in opposition to the first bracket 748 so that the extension 688 of the first arm 682 can be retained between the brackets 748, 750. The first and second brackets 748, 750 are positioned within a slot 752 defined by the shape of the main body 730. The retention interface 732 is able to slide along the slot 752 until the lever 734 is actuated to lock the extension 688 and the retention interface 732 in place.

The lever 734 has a grip plate 754 and a detent plate 756 that are positioned at near-ninety degree angles to each other. The grip plate 754 is positioned to be grasped and manually moved by a user to move the lever 734 between locked and unlocked positions. The detent plate 756 is positioned to abut the main body 730 to limit rotation of the lever 734. A pivot extension 758 extends from the detent plate 756 and includes a pair of flanges 760, only one of which is visible in FIG. 17. The flanges 760 are pivotably attached to the first pair of apertures 740 such that the lever 734 rotates about an axis passing through the first pair of apertures 740. The flanges 760 are also pivotably coupled to the plate 736 at a point-of-attachment that is not visible in FIG. 17, but is proximate the juncture of the grip plate 754 to the detent plate 756.

In FIG. 17, the lever 734 is in an unlocked position, in which the main body 730 is not compressed and therefore, the first and second brackets 748, 750 of the retention interface 732 are movable along the slot 752 and may be separated sufficiently to permit insertion of the extension 688 of the first arm 682 into the space between the first and second brackets 748, 750. When the lever 734 is pivoted such that the detent plate 756 abuts the end of the main body 730, the plate 736 is drawn by the flanges 760 such that the second pair of apertures 742 of the main body 730 is drawn toward the first pair of apertures 740. As a result, the slot 752 is compressed and the brackets 748, 750 of the retention interface 732 are pressed against each other. The brackets 748, 750 are then unable to slide along the slot 752 and the extension 688 of the first arm 682 is unable to slide within the compressed space between the brackets 748, 750.

The location of the pivotable coupling of the plate 736 to the flanges 760 provides an over-center geometry that makes the lever 734 "bi-stable." This over-center geometry is present because the point-of-attachment of the plate 736 to the flanges 760 passes through a plane extending through the first and second pairs of apertures 740, 742 in the course of motion of the lever 734 between the locked and unlocked positions. Thus, the lever 734 is able to rest in either of the locked and unlocked positions until actuated by a user. The lever 734 therefore provides a quick-release and quick-locking mechanism by which the first arm 682 can be locked in engagement with the pivot member 666.

The engagement interface 738 has a first plate 764 and a second plate 766, each of which has a generally arcuate shape with a radius substantially the same as that of the arcuate extension 706 of the anchoring member 664. The plates 764, 766 are positioned substantially parallel to each other such that a trough 768 is defined between them. The trough 768 is sized such that the arcuate extension 706 is able to slide along the trough 768 with clearance.

The second plate 766 has a pair of pins 770 that extend into the trough 768 to protrude into the groove 722 of the arcuate extension 706 to restrict motion of the engagement interface 738 perpendicular to the arcuate extension 706. Thus, the engagement interface 738 is constrained to follow the arcuate

pathway of the arcuate extension 706. The engagement interface 738 also has a collar 772 that is rotatably coupled to the plateau 744 of the main body 730 to permit rotation of the engagement interface 738 with respect to the main body 730.

The registration member 662, the anchoring member 664, and the pivot member 666 may be coupled together to define a linking structure 774 that couples the registration interface 680 of the registration member 662 with the anchoring feature 700 of the anchoring member 664. The linking structure 774 facilitates proper positioning of the slot 714 of the guide feature 702 of the anchoring member 664 in a manner that will be described subsequently.

As also shown in FIG. 17, the guide wire 668 has a central portion 776, a leading end 778, and a trailing interface 780. The leading end 778 is sharpened to facilitate bone penetration, and the trailing interface 780 may have a hexagonal or other cross sectional shape selected to permit connection of the trailing interface 780 with a driver (not shown in FIG. 17). The central portion 776 has a roughened portion 782 proximate the leading end 778, and a pair of markings 784 positioned near the center of the central portion 776.

The roughened portion 782, when exposed, may indicate that the guide wire 668 has not been driven sufficiently far into the pedicle (for example, one of the pedicles 30 of the first vertebra 24 or one of the pedicles 50 of the second vertebra 26). The markings 784 indicate proper implantation of the guide wire 668 into a pedicle when only one of the markings 784 is visible, and the other is beneath the surface of the bone.

As depicted in FIG. 17, the pedicle screw 670 has a shank 788, which may have machine threads (not shown) designed to receive the castle nut 672, and a threaded end 790 with threads shaped to retain the pedicle screw 670 firmly in bone. The pedicle screw 670 also has a torque receiver 792 designed to receive torque from a manual or motorized driver. The torque receiver 792 has a cavity with a generally hexagonal cross sectional shape selected to receive the end of a driver with a corresponding hexagonal shape.

The castle nut 672 has a semispherical surface 796 designed to rest against the concave semispherical surface within the anchoring feature 700. The castle nut 672 also has a bore 798 through which the shank 788 of the pedicle screw 670 may pass, and a plurality of radial grooves 800 that facilitate transmission of torque to the castle nut 672 from a manual or motorized driver. The semispherical surface 796 permits rotation of the anchoring feature 700 against the bone until the castle nut 672 is tightened to sandwich the anchoring feature 700 between the bone and the castle nut 672.

As mentioned previously, the inferior resection tool 660, or more precisely, the linking structure 774, remotely mimics the tangential contact between articulating surfaces of a natural facet joint, and the articulation of a corresponding prosthetic facet joint, by providing ball-in-trough motion. More precisely, the linking structure 774 provides a first joint 802, a second joint 804, and a third joint 806. The first joint 802 is a linear joint, and the second and third joints 804, 806 are rotary joints. The configuration and operation of the joints 802, 804, 806 will be described in greater detail in connection with FIG. 18.

The registration feature 662, the anchoring member 664, and the pivot member 666 may easily be assembled to provide the inferior resection tool 660. According to one method of assembly, the anchoring member 664 and the pivot member 666 may first be coupled together by inserting the arcuate extension 706 through the trough 768 of the engagement interface 738 such that the pins 770 extend into the groove 722. Then, with the lever 734 in the unlocked position, as shown in FIG. 17, the extension 688 of the first arm 682 may

be inserted into the space between the first and second brackets 748, 750 of the retention interface 732 until the shoulder 690 of the first arm 682 abuts the brackets 748, 750.

As mentioned previously, moving the lever 734 to the locked position locks the extension 688 in place between the first and second brackets 748, 750 and also prevents further translation of the retention interface 732 along the slot 752 of the main body 730. Motion of the retention interface 732 along the slot 752 may be required in order to couple the registration member 662 and the anchoring member 664 to the first vertebra 24 and the second vertebra 26, respectively, at their proper relative orientations. Accordingly, the lever 734 may be left in the unlocked position until attachment of the inferior resection tool 660 to the spine 10, or may be moved to the locked position during assembly and then moved back to the unlocked position prior to attachment to the spine 10.

Referring to FIG. 18, a perspective view illustrates the inferior cutting tool 660 in a fully assembled configuration. The first anchor 112, the guide wire 668, the pedicle screw 670, and the castle nut 672 are also shown in their proper positions to couple the inferior cutting tool 660 to the spine 10 (not shown in FIG. 18).

More precisely, the guide wire 668 is positioned as though implanted in the left-side pedicle 30 of the first vertebra 24, and the first anchor 112 is positioned such that the guide wire 668 passes through the bore 130 of the anchoring feature 122 of the first anchor 112 to keep the first anchor 112 properly positioned with respect to the pedicle 30. The guide post 124 of the first anchor 112 is inserted through the bore 686 of the registration interface 680 such that the registration interface 680 is registered on the first anchor 112. The pedicle screw 670 is positioned as though implanted in the left-side pedicle 50 of the second vertebra 26, and the anchoring feature 700 is placed such that the shank 788 of the pedicle screw 670 passes through the bore 712 of the anchoring feature 700. The castle nut 672 is threaded into engagement with the threaded end 690 of the pedicle screw 670 to keep the anchoring feature 700 in place against the pedicle 50.

The first, second, and third joints 802, 804, 806 of the inferior resection tool 660 enable adjustment of the relative positions and orientations of the anchoring feature 700 and the registration interface 680. As the relative orientations are adjusted, the anchoring member 664 will pivot about the center of the semispherical surface 710 of the anchoring feature 700 to the proper orientation to position the slot 714 at the desired orientation for proper resection of the inferior facet 60 of the left-hand side of the second vertebra 26.

The first joint 802 includes the main body 730 and the retention interface 732 of the pivot member 666. The first joint 802 simulates sliding of a ball within a trough by enabling linear motion of the registration interface 680 with respect to the anchoring feature 700 via translation of the retention interface 732 within the slot 752 of the main body 730. The first joint 802 permits adjustment to account for variations in the spacing between the pedicles 30, 50 of the first and second vertebrae 24, 26, respectively, generally along the cephalad and caudal directions 12, 14.

The second joint 804 includes the main body 730 and the engagement interface 738 of the pivot member 666. Rotation of the engagement interface 738 with respect to the main body 730 simulates rolling of a ball across a trough by enabling rotation of the registration interface 680 with respect to the anchoring feature 700. The second joint 804 permits adjustment to account for variations in the spacing between the pedicles 30, 50 of the first and second vertebrae 24, 26, respectively, generally along the medial/lateral axis 20.

The third joint **806** includes the engagement interface **738** of the pivot member **666** and the arcuate extension **706** of the anchoring member **664**. The third joint **806** simulates rolling of a ball along a trough by enabling rotation of the registration interface **680** with respect to the anchoring feature **700** via rotation of the engagement interface **738** as it moves along the arcuate path of the arcuate extension **706**. The third joint **806** permits adjustment to account for variations in the spacing between the pedicles **30**, **50** of the first and second vertebrae **24**, **26**, respectively, generally along the anterior and posterior directions **16**, **18**.

As stated above, motion of the first, second, and third joints **802**, **804**, **806** accounts for positional variation generally along the cephalad and caudal directions **12**, **14**, the medial/lateral axis **20**, and the anterior and posterior directions **16**, **18**, respectively. However, the joints **802**, **804**, **806** do not correspond directly to the various directions and axes **12**, **14**, **16**, **18**, **20** because the inferior resection tool **660** is positioned with respect to a coordinate system aligned with the axis of the pedicle **50** of the left-hand side of the second vertebra **26**, and not necessarily with the sagittal plane **22**. In any case, the joints **802**, **804**, **806** cooperate to adjust for a wide range of relative prosthesis positions and anatomical variations.

The first joint **802** remotely replicates the tangential contact between articulating surfaces of a facet joint because the retention interface **732** slides along an axis generally parallel to the trough defined by the superior facet **38** on the left-hand side of the first vertebra **24**. The second and third joints **804**, **806** remotely replicate the tangential contact between articulating surfaces of a facet joint because the second and third joints **804**, **806** provide for relative rotation about axes that pass through the center of a semispherical surface (not shown in FIG. **17**) of an inferior facet, such as the inferior facet **60** on the left-hand side of the second vertebra **26**. Thus, the joints **802**, **804**, **806** cooperate to position the slot **714** of the guide feature **702** at the proper orientation to guide resection of the inferior facet **60** of the left-hand side of the second vertebra **26** so that the selected inferior prosthesis (not shown in FIG. **18**) can be attached to the second vertebra **26** to replace the inferior facet **60**.

In alternative embodiments, a fourth joint (not shown) may be added to the configuration of FIG. **18**. More precisely, in place of the generally straight extension **688** of the first arm **682** more clearly illustrated in FIG. **16**, a second arcuate extension (not shown) may be provided. Like the arcuate extension **706**, the second arcuate extension may be centered about an axis passing through the center of curvature of the articulation surface of an inferior implant to be coupled to the saddle point **62** of the left-hand side of the second vertebra **26**. The second arcuate extension may be insertable into the retention interface **732** such that the retention interface **732** is positionable at a plurality of locations along the length of the second arcuate extension to provide one more rotational degree of freedom. Moving the lever **734** to the locked position then locks the position of the retention interface **732** along the second arcuate extension.

Referring to FIG. **19**, a perspective view illustrates a clamping tool **810** according to one embodiment of the invention. The clamping tool **810** is used to hold the prostheses that replace the inferior facets **60** of the second vertebra **26** in place as they are securely attached. The manner in which the clamping tool **810** accomplishes this function will be described in greater detail subsequently.

As shown, the clamping tool **810** has a first clamping member **812**, a second clamping member **814**, a threaded post **816**, and a knob **818**. The first clamping member **812** has a main body **822**, a handle portion **824** extending from one end

of the main body **822**, and a grip portion **826** extending from the other end of the main body **822**. The grip portion **826** has a recess **828** proximate a free end of the grip portion **826** to receive and exert clamping force on a projection extending from an inferior facet prosthesis (not shown).

The second clamping member **814** is shaped to be a substantial mirror image of the first clamping member **812**. Accordingly, the second clamping member **814** has a main body **832**, a handle portion **824** extending from one end of the main body **832**, and a grip portion **826** extending from the other end of the main body **832**. Like the grip portion **826** of the first clamping member **812**, the grip portion **826** of the second clamping member **814** has a recess **828** proximate a free end thereof to receive and exert clamping force on projection extending from an inferior facet prosthesis.

The threaded post **816** is integrally formed with or securely attached to the main body **822** of the first clamping member **812**, and extends through the main body **832** of the second clamping member **814**. The threaded post **816** further passes through and engages a threaded hole **840** of the knob **818**. The knob **818** has a plurality of ridges **842** that facilitate gripping and rotation of the knob **818** by hand. The threaded post **816** has threads **844** that engage the threaded hole **840** and enable the knob **818** to advance along the threaded post **816** to press the first and second clamping members **812**, **814** together in response to rotation of the knob **818**. The operation of the clamping tool **810** will be shown and described in greater detail subsequently.

The various implements described in connection with FIGS. **1-19** may be used to facilitate measurement and resection of spinal bony landmarks and replacement of facets such as the superior facets **38** of the first vertebra **24** and the inferior facets **60** of the second vertebra **26**. FIGS. **20-48** set forth one exemplary method for carrying out facet joint replacement according to the invention. However, a wide variety of methods may be used, and the structures of the present invention are not limited to use in any one method. Similarly, methods according to the invention may be carried out using structures different from those of FIGS. **1-19**.

The method of FIGS. **20-48** will be set forth in connection with a bi-lateral facet joint replacement, or an operation in which both of the superior facets **38** of the first vertebra **24** and both of the inferior facets **60** of the second vertebra **26** are replaced. Those of skill in the art will recognize that the systems and methods of the present invention are also applicable to unilateral facet replacements, and operations in which only one facet of a facet joint is replaced such that the facet prosthesis articulates against a natural facet.

Some of the implements of FIGS. **1-19**, including the reamers **70**, **72**, the frame **110**, the stationary external support **260**, and the clamping tool **810**, may be usable to carry out operations on either side of the sagittal plane **22**, i.e., on either of the left and right sides of the spine **10**. However, some of the implements of FIGS. **1-19**, including the facet measurement tool **330**, the pedicle measurement tool **430**, the kit **510** of superior cutting tools, the cutting guide **630**, and the inferior resection tool **660**, are specific to the left-hand side of the spine **10**. The corresponding surgical instruments for the right-hand side may be substantial mirror images of the foregoing.

The method outlined below will generally describe procedures to be carried out with respect to the left-hand side of the spine **10**, with the understanding that those of the right-hand side may be performed in a similar manner using the appropriate surgical instruments for the right-hand side. In some of FIGS. **20-48**, the operations described in connection with the left-hand side have already been carried out on the right-hand

side, so that the manner in which the operation is performed is shown in on the left-hand side, and the results of the operation are illustrated on the right-hand side.

The method may commence with performance of a CT scan of the patient to get the best possible mapping of the morphology of the spine **10**. From the mapping, various dimensions may be obtained and used to preliminarily determine the appropriate prostheses to replace the superior facets **38** of the first vertebra **24** and the inferior facets **60** of the second vertebra **26**. The prostheses may be selected from a kit of superior implant prostheses and a kit of inferior implant prostheses, each of which includes a plurality of prostheses varied in shape and size to provide compatibility with the vast majority of spinal morphologies.

Once the appropriate superior and inferior implant prostheses have been selected, blunt dissection and retraction of the tissues surrounding the first and second vertebrae **24**, **26** may be carried out. The tissues are retracted to expose the vertebrae **24**, **26**, and also a portion of a third vertebra (not shown) adjacent to the second vertebra **26** and a portion of the sacrum (also not shown), which is adjacent to the first vertebra **24**. The facet joints **64**, pedicles **30**, **50**, and transverse processes **34**, **54** of the first and second vertebrae **24**, **26** are then identified. If needed, the facet joints **64** may be exposed by removing hypertrophic bone. The capsules that normally encase the facet joints **64** are then removed to expose the bony surfaces of the facet joints **64**.

Referring to FIG. **20**, a perspective view illustrates the first and second vertebrae **24**, **26** of the spine **10** with a joint flag **850** that serves as a reference for rotation of various instruments about the medial/lateral axis **20**. The joint flag **850** has a shaft **852**, an insertion plate **854**, and a handle **856**. The insertion plate **854** is generally flat and is coupled to the shaft **852** at a pre-established angle, which may be at or near a statistical average of the angle between the anterior surface of the facet joint **64** and the major axis of the associated pedicle **30**. The handle **856** extends from the opposite end of the shaft **852** at a ninety degree angle, coplanar with the shaft **852** and the insertion plate **854**.

After exposure of the facet joints **64**, the insertion plate **854** is inserted into the "joint space," i.e., the space between the superior facet **38** of the left-hand side of the first vertebra **24** and the inferior facet **60** of the left-hand side of the second vertebra **26**. The insertion plate **854** is inserted into the caudal edge of the joint space, and is then pressed generally along the cephalad direction **12** to provide thorough contact between the insertion plate **854** and the adjacent surfaces of the facets **38**, **60**. Since the handle **856** is coplanar with the shaft **852** and the insertion plate **854**, the handle **856** provides visual confirmation that the insertion plate **854** is properly aligned.

Referring to FIG. **21**, an enlarged, perspective view illustrates the first and second vertebrae **24**, **26** with the joint flag **850** in place. After insertion of the insertion plate **854** into the joint space, the shaft **852** extends outward from the spine **10** at an angle that enables the shaft **852** to serve as a reference for other surgical instruments. Thus, surgical instruments may be coupled to the spine **10** based on the angle at which the facets **38**, **60** contact each other.

When the joint flag **850** has been properly positioned, the saddle point **42** of the pedicle **30** of the left-hand side of the first vertebra **24** may be identified. A pin, chisel, or the like may be used to nick the saddle point **42** to indicate where the corresponding guide wire **668** should be implanted. The saddle point **42** is then prepared for implantation of the guide wire **668**.

Referring to FIG. **22**, a perspective view illustrates the first and second vertebrae **24**, **26**, with a guide wire inserter **860**

positioned to implant the guide wire **668** into the saddle point **42** of the left-hand side of the first vertebra **24**. As shown, the guide wire inserter **860** has a main body **862**, a grip member **864**, a handle member **866**, and an angular reference member **868**.

The main body **862** has a central portion **872** and an insertion portion **874**. The central portion **872** has a generally cylindrical shape, and is coupled to the handle member **866** and the angular reference member **868**. The central portion **872** receives a shaft **876** via a bore **878** passing through the central portion **872**. The shaft **876** serves to couple the grip member **864** to the central portion **872**. The central portion **872** also has a handle coupling **880** to which the handle member **866** is attached, and a slot **882** that receives the angular reference member **868**.

The insertion portion **874** has a tapered end **884** that abuts the surface of the bone, i.e., the saddle point **42** of the pedicle **30** of the left-hand side of the first vertebra **24**, to facilitate accurate implantation. The insertion portion **874** also has a guide extension **886** that protrudes from the tapered end **884**. The guide extension **886** has two pairs of aligned notches that can be used to visually confirm that the saddle point **42** has been properly placed and that the anatomy of the spine **10** is within acceptable limits prior to implantation of the guide wire **668**. The guide wire **668** may be positioned within the insertion portion **874** such that the leading end **778** of the guide wire **668** is able to exit the insertion portion **874** through the tapered end **884**.

The grip member **864** has a coupling **890**, a grip **892**, and a strike plate **894**. The grip member **864** may be a standardized, universal grip that is attachable to a wide variety of instruments to provide manual torque and/or linear force. Thus, the coupling **890** is removably attachable to the shaft **876**, and to a variety of other surgical tools. The grip **892** is shaped to be comfortably grasped and rotated by hand. The strike plate **894** may be formed of a metal, and may be coupled to the coupling **890** via a metal support (not shown) extending through the interior of the grip **892** so that impact can be nondestructively transmitted from the strike plate **894** to the coupling **890**.

The handle member **866** includes a handle **898**, a body coupling **900**, and a lever **902**. The handle **898** is shaped to be easily grasped by a hand of a user. The body coupling **900** is shaped to facilitate attachment of the handle member **866** to the central portion **872** of the main body **862**. The handle **898** and the body coupling **900** may be shaped similarly to the handle **358** and the attachment end **360** of the handle member **334** of the facet measurement tool **330** and the pedicle measurement tool **430**. Accordingly, the body coupling **900** may be attached to the central portion **872** through the use of a screw (not shown) such as the screw **336** of the facet measurement tool **330** and the pedicle measurement tool **430**.

The lever **902** of the handle member **866** may be pivotably coupled to the central portion **872**. The lever **902** may be subject to resilient force provided by a spring (not shown) or the like such that, in the absence of actuation by a user, the lever **902** restricts motion of the angular reference member **868** through the slot **882** of the central portion **872**. However, when the lever **902** is actuated toward the handle **898** by a user, the lever **902** permits motion of the angular reference member **868** through the slot **882**. This permits rotational adjustment about the cephalad and caudal directions **12**, **14** of the angle along which the guide wire **668** enters the saddle point **42**.

As shown, the angular reference member **868** has an arcuate rod **904**, a guide plate **906** attached to the arcuate rod **904**, and a plurality of markings **908** arranged along the length of the arcuate rod **904**. The guide plate **906** is generally square in

shape, and is generally perpendicular to the end of the arcuate rod **904** to which it is attached. The markings **908** specify angles, and when the lever **902** is actuated to permit adjustment of the angular reference member **868**, any of the markings **908** may be aligned with a marking (not shown) on the central portion **872** of the main body **862** to set the angle of rotation about the cephalad and caudal directions **12**, **14** along which the guide wire **668** will be inserted.

The guide wire inserter **860** may be used in the following manner to implant the guide wire **668** into the saddle point **42** of the left-hand side of the first vertebra **24**. A surgeon may first measure the angle at which the pedicle **30** of the left-hand side of the first vertebra **24** extends with respect to the sagittal plane **20**. This may be accomplished by using the spinal morphology mapping from the CT scan performed previously. Then, the lever **902** may be actuated to release the angular reference member **868**, and the arcuate rod **904** may be moved through the slot **862** until the markings **908** indicate that the angular reference member **868** is set at the proper angle. The lever **902** may then be released to keep the angular reference member **868** at the proper angle.

Then, the tapered end **884** of the insertion portion **874** of the main body **862** is placed on the saddle point **42**. The guide wire inserter **860** is pivoted about the saddle point **42** until the guide plate **906** is parallel to the sagittal plane **22** and the shaft **876** is substantially coplanar with the shaft **852** of the joint flag **850**. This form of alignment is more clearly illustrated in FIG. **23**.

Referring to FIG. **23**, a lateral view illustrates the first and second vertebrae **24**, **26**, with the joint flag **850** and the guide wire inserter **860** in position. As shown, the guide plate **906** of the angular reference member **868** is generally parallel to the sagittal plane **22** (shown in FIG. **1**). Furthermore, the shaft **876** of the guide wire inserter **860** is oriented substantially coplanar with the shaft **852** of the joint flag **850**. Thus, the guide wire inserter **860** has been rotated about the medial/lateral axis **20** to substantially the same angle as the joint flag **850**.

As set forth above, alignment of the guide plate **906** with the sagittal plane **22** controls the medial/lateral angulation of the guide wire inserter **860**, i.e., orientation via rotation about the cephalad and caudal directions **12**, **14**. Alignment of the shaft **876** with the shaft **852** of the joint flag **850** controls the cephalad/caudal angulation of the guide wire inserter **860**, i.e., orientation via rotation about the medial/lateral axis **20**. These two modes of alignment are used to ensure that the guide wire **668** permits the necessary range of multiaxial rotation of a semispherical bone apposition surface of a superior facet prosthesis (not shown in FIG. **23**) against the saddle point **42** to permit proper alignment of the prosthesis. However, it has been found that a relatively wide range of implantation angles is acceptable for the guide wire **668**. Accordingly, the above-described procedures for cephalad/caudal and medial/lateral alignment of the guide wire inserter **860** may be omitted in favor of expedited implantation of the guide wire **668**.

After the guide wire inserter **860** has been oriented as desired, the surgeon may use the guide extension **866** to verify that the insertion portion **874** is properly positioned and that the anatomy of the spine **10** is within necessary boundaries. More precisely, when the surgeon looks down the length of the guide wire inserter **860**, the joint space of the facet joint **64** should appear to cross the guide extension **866** between the pairs of notches. If this is not the case, the insertion portion **874** may be moved slightly to a location more suitable for implantation.

Then, a hammer or the like may be impacted against the strike plate **894** of the grip member **864**. The impact is transferred through the coupling **890**, through the shaft **876**, and to the guide wire **668** within the insertion portion **874** of the guide wire inserter **860**. The guide wire **668** is driven generally along the axis of the pedicle **30**, or along the length of the pedicle **30**. Once the guide wire **668** has been driven into the bone a sufficient distance, the guide wire inserter **860** may be removed. The guide wire inserter **860** may control the depth to which the guide wire **668** is implanted in the first vertebra **24**. The guide wire **668** is driven into the bone until only one of the markings **784** of the central portion **776** of the guide wire **668** is showing above the surface of the bone.

After the guide wires **668** have been implanted in both pedicles **42** of the first vertebra **24**, the superior facets **38** of the first vertebra **24** may be preliminarily resected. The preliminary resection may not need to be accurately guided or measured. Rather, a minimal amount of bone tissue, i.e., only the superior articular process, is removed from the superior facets **38** to enhance access to the joint space of the facet joints **64** and to further expose the inferior facets **60** of the second vertebra **26** for resection. Further, more precise resection of the superior facets **38** of the first vertebra **24** will be performed subsequently to prepare the first vertebra **24** to receive superior facet prostheses.

Referring to FIG. **24**, a perspective view illustrates the first and second vertebrae **24**, **26**, with the joint flag **850** and the guide wires **668** in place. The superior facets **38** of the first vertebra **24** have been preliminarily resected to form preliminary resection surfaces **912** on the first vertebra **24**. Such preliminary resection may be carried out with a reciprocating bone saw or the like. As mentioned previously, further resection of the superior facets **38** of the first vertebra **24** will be carried out subsequently. After preliminary resection has been carried out, the saddle points **42** of the first vertebra **24** may be reamed to enable attachment of the frame **110**.

Referring to FIG. **25**, a perspective view illustrates the first and second vertebrae **24**, **26** with the right-hand saddle point **42** of the first vertebra **24** partially reamed, and with the primary reamer **70** positioned to ream the left-hand saddle point **42**. As shown, the primary reamer **70** has been registered on the guide wire **668** of the left-hand saddle point **42**. More precisely, the portion of the guide wire **668** exposed outside the bone of the first vertebra **24** is inserted into the bore **88** of the primary reamer **70** to register the primary reamer **70** with respect to the saddle point **42**. Thus, motion of the primary reamer **70** is constrained to rotation about the axis of the guide wire **668** and motion along the guide wire **668**.

The primary reamer **70** is coupled at the torque interface **76** to a handle, motor, or the like (not shown). The primary reamer **70** may operate most effectively when driven by a motor. The primary reamer **70** rotates along a direction **914** such that the cutting flanges **92** scrape away bone tissue from around the saddle point **42**. The primary reamer **70** is advanced into the pedicle **30** until the flat surface **90** abuts the bone immediately surrounding the guide wire **668**. The primary reamer **70** is then unable to advance further into the bone, and is withdrawn to leave a roughened semispherical surface **916**, as shown on the right-hand side of the first vertebra **24**. The roughened semispherical surface **916** has a plateau **918** immediately surrounding the guide wire **668**, where the primary reamer **70** was unable to remove the bone tissue.

Referring to FIG. **26**, a perspective view illustrates the first and second vertebrae **24**, **26** with the right-hand saddle point **42** of the first vertebra **24** partially reamed, and with the primary reamer **70** positioned to ream the left-hand saddle

point 42, as in FIG. 25. The plateau 918 of the roughened semispherical surface 916 is more clearly shown. The plateau 918 will be removed via the secondary reamer 72.

Referring to FIG. 27, a perspective view illustrates the first and second vertebrae 24, 26 with the right-hand saddle point 42 of the first vertebra 24 fully reamed, and with the secondary reamer 72 positioned to complete reaming of the left-hand saddle point 42. As described previously, the dome 102 of the secondary reamer 72 is advanced into the roughened semispherical surface 916. However, the dome 102 does not remove bone tissue, and thus, the roughened semispherical surface 916 remains at its proper depth. The central teeth 100 remove the plateau 918 to leave a semispherical interface 920 at the saddle point 42.

Referring to FIG. 28, a perspective view illustrates the first and second vertebrae 24, 26 with the right-hand saddle point 42 of the first vertebra 24 fully reamed, and with the secondary reamer 72 positioned to complete reaming of the left-hand saddle point 42, as in FIG. 27. The semispherical interface 920 on the right-hand side of the first vertebra 24 is more clearly visible. The effect of the progressive use of the primary and secondary reamers 70, 72 is to accurately control the depth of the semispherical interface 920 so that, at its deepest, the semispherical interface 920 is, for example, two millimeters below the former bone surface of the saddle point 42.

If a deeper ream is desired, the procedure illustrated in FIGS. 25, 26, 27, and 28 may be repeated by using the primary reamer 70 to add limited depth to the ream, and then using the secondary reamer 72 to complete reaming to the additional depth. Thus, the depth of a reamed indentation may be increased by discrete quantities, such as two millimeters.

After the saddle points 42 of the first vertebra 24 have been reamed to provide the semispherical interfaces 920, the frame 11 may be anchored to the spine 10. In this application, “anchoring” refers to contacting one part with another to limit relative motion between the two parts. “Coupling” refers to contacting one part with another, either directly or through a third part, to limit relative motion between the first two parts.

The frame 110 may easily be anchored on the first vertebra 24. The locking mechanism 144 may first be moved to the unlocked configuration by rotating the handle 202 counterclockwise, as viewed from above, to permit the first, second, and third rods 164, 184, 210 to slide relatively freely within the first, second, and third sliders 212, 220, 222. The first and second anchors 112, 114 may thus be repositioned along three orthogonal axes to slide the bore 130 of the anchoring feature 122 of the first anchor 112 over the guide wire 668 of the left-hand side of the first vertebra 24, and to slide the bore 130 of the anchoring feature 122 of the second anchor 114 over the guide wire 668 of the right-hand side of the first vertebra 24.

Each of the semispherical surfaces 128 of the anchoring features 122 is then seated in the corresponding semispherical interface 920 of the first vertebra 24. With the semispherical surfaces 128 seated against the semispherical interfaces 920, the frame 110 is pivotable only about the medial/lateral axis 20, or about an axis angularly displaced slightly therefrom. Since the semispherical surfaces 128 permit pivotal motion with respect to the first vertebra 24, they are “pivot features” within the meaning of this application. The frame 110 is pivoted about the medial/lateral axis 20 until the frame 110 is oriented generally parallel to the shaft 852 of the joint flag 850.

The stationary external support 260 is then attached to the frame 110. More precisely, the fixed end 262 of the stationary external support 260 is attached to a stationary object such as an operating table, wall, or the like. The first, second, and

third joints 276, 278, 280 of the stationary external support 260 are all unlocked by rotating the corresponding handles 286, 296 counterclockwise, thereby permitting relative rotation and/or translation of the first, second, and third rods 270, 272, 274. The handle 296 of the grip 264 is also actuated to permit the first and second gripping members 312, 314 to move apart from each other.

The first, second, and third joints 276, 278, 280 are moved to position the grip 264 proximate the external anchor 116 of the frame 110, and the generally spherical surface 136 of the external anchor 116 is then inserted into the space between the gripping members 312, 314. Then, the handles 286, 296 of the joints 276, 278, 280 are moved clockwise to lock the joints 276, 278, 280. The handle 296 of the grip 264 is also moved clockwise to draw the first and second gripping members 312, 314 closer together to grip the generally spherical surface 136 of the external anchor 116.

Attachment of the stationary external support 260 to the frame 110, in combination with coupling of the frame 110 to the first vertebra 24, makes the frame 110 a stable platform for surgical instrument registration. However, external attachment is optional, and in alternative embodiments, the stationary external support 260 need not be used. Furthermore, attachment to the first vertebra 24 is optional, as a frame (not shown) coupled only to the stationary external support 260 may still be stable enough to guide spinal measurement and resection operations. Indeed, if desired, surgical instruments could be made to register directly on the grip 264 of the stationary external support 260. The remainder of this disclosure assumes that both anchoring to the vertebra 24 and attachment to the stationary external support 260 are used.

Referring to FIG. 29, a perspective view illustrates the first and second vertebrae 24, 26 with the guide wires 668 and joint flag 850 in place, and with the frame 110 anchored to the first vertebra 24 and coupled to the stationary external support 260. The stationary external support 260 is substantially rigid and securely grips the external anchor 116 to stabilize the frame 110, and especially, fix the orientation of the frame 110 about the medial/lateral axis 20 to be substantially parallel to the shaft 852 of the joint flag 850.

Referring to FIG. 30, a lateral view illustrates the first and second vertebrae 24, 26 with the guide wires 668 and joint flag 850 in place, and with the frame 110 anchored to the first vertebra 24 and coupled to the stationary external support 260. As shown, the frame 110 is oriented substantially parallel to the shaft 852 of the joint flag 850. The frame 110 is then ready to receive registration of surgical instruments to facilitate additional measurement and resection operations. The joint flag 850 may be removed and set aside. Holes (not shown in FIG. 30) may then be drilled or burred through the inferior facets 60 of the second vertebra 26 to expose or the most medial and anterior surface, of each of the superior facets 38 of the first vertebra 24 in preparation for measurement of the location of P1.

The facet measurement tool 330 may then be used to measure the location of P1. More precisely, the registration interface 342 of the facet measurement tool 330 may be registered on the first anchor 112 by sliding the bore 348 of the registration interface 342 over the guide post 124 of the first anchor 112. The user then grasps the grip 378 of the contact member 340 and moves it to slide the first and second rods 364, 374 within the first and second sliders 344, 366 until the contact feature 382 is positioned to contact P1.

Referring to FIG. 31, a perspective view illustrates the first and second vertebrae 24, 26 with the guide wires 668, frame 110, and stationary external support 260 in place, and with the facet measurement tool 330 registered to the frame 110 to

measure P1. Once the contact feature 382 is in contact with P1, measurements corresponding to the location of P1 may be acquired from the first and second rods 364, 374, with respect to the saddle point 38 of the left-hand side of the first vertebra 24. The measurements may be read as indicated previously, in connection with the description of FIG. 9.

Referring to FIG. 32, a cephalad section view illustrates the first and second vertebrae 24, 26 with the guide wires 668, frame 110, and stationary external support 260 in place, and with the facet measurement tool 330 registered to the frame 110 to measure P1. The section view more clearly illustrates the position of the contact feature 382 when measurement is conducted, and the manner in which the inferior facets 60 of the second vertebra 26 have been drilled or burred through to expose P1 for each of the superior facets 38 of the first vertebra 24. The contact extension 376 of the contact member 340 extends through the opening formed by drilling or burring to enable the contact the feature 38 to contact P1.

When the position of P1 has been measured, the facet measurement tool 330 may be removed. The pedicle measurement tool 430 may then be used to measure the position of the saddle point 62 of the left-hand side of the second vertebra 26, with respect to the saddle point 42 of the left-hand side of the first vertebra 24. More precisely, the registration interface 342 of the pedicle measurement tool 430 may be registered on the first anchor 112 by sliding the bore 348 of the registration interface 342 over the guide post 124 of the first anchor 112. The user then grasps the grip 378 of the contact member 440 and moves it to slide the first, second, and third rods 464, 466, 494 within the first, second, and third sliders 444, 476, 478 until the contact feature 502 is positioned to contact the saddle point 62 of the left-hand side of the second vertebra 26.

Referring to FIG. 33, a perspective view illustrates the first and second vertebrae 24, 26 with the guide wires 668, frame 110, and stationary external support 260 in place, and with the pedicle measurement tool 430 registered to the frame 110 to measure the saddle point 62. Once the contact feature 502 is in contact with the saddle point 62, measurements corresponding to the location of the saddle point 62 may be acquired from the first, second, and third rods 464, 466, 494, with respect to the saddle point 38 of the left-hand side of the first vertebra 24. The measurements may be read as indicated previously, in connection with the description of FIG. 12.

Referring to FIG. 34, a cephalad section view illustrates the first and second vertebrae 24, 26 with the guide wires 668, frame 110, and stationary external support 260 in place, and with the pedicle measurement tool 430 registered to the frame 110 to measure the saddle point 62. The section view more clearly illustrates the position of the contact feature 502 when measurement is conducted. When the position of the saddle point 62 has been measured, the pedicle measurement tool 430 may be removed. The measurements obtained from the facet measurement tool 330 and the pedicle measurement tool 430 may be used to verify or change the selection of inferior and superior prostheses made previously to ensure that the selected prostheses match the shapes of the superior and inferior facets 38, 60 as closely as possible.

After measurement has been carried out with the measurement tools 330, 430, guide wires 668 may then be inserted into the saddle points 62 of the second vertebra 26. Guide wire implantation into the saddle points 62 of the second vertebra 26 may be carried out in a manner very similar to that of implantation into the saddle points 42 of the first vertebra 24.

Referring to FIG. 35, a perspective view illustrates the first and second vertebrae 24, 26 with the guide wires 668, frame 110, and stationary external support 260 in place, and with the guide wire inserter 860 positioned to insert a guide wire (not

visible in FIG. 35) into the saddle point 62 of the left-hand side of the second vertebra 26. The lever 902 may be actuated to enable the arcuate rod 904 of the angular reference member 868 to slide through the slot 882 of the central portion 872 of the main body 862. The arcuate rod 904 may then be moved to indicate the proper angle, and the lever 902 may be released to keep the angular reference member 868 at the angle.

The guide plate 906 is then aligned with the sagittal plane 22 (shown in FIG. 1), and the guide wire inserter 860 is rotated into alignment with the major axis of the corresponding pedicle 50 of the second vertebra 26, as viewed from a lateral viewpoint. The strike plate 894 may then be tapped to insert the guide wire 668 into the saddle point 62 of the left-hand side of the second vertebra 26. Accurate guidance of the implantation angle of the guide wire 668 into the saddle point 62 of the left-hand side of the second vertebra 26 may be somewhat less important than in the corresponding saddle point 42 of the first vertebra 24.

After the guide wires 668 have been implanted into the saddle points 62 of the second vertebra 26, the saddle points 62 may be reamed in a manner similar to that of the saddle points 42 of the first vertebra 42. As with the saddle points 42, the primary and secondary reamers 70, 72 may be used.

Referring to FIG. 36, a perspective view illustrates the first and second vertebrae 24, 26 with the guide wires 668, frame 110, and stationary external support 260 in place, and with the primary reamer 70 positioned to ream the left-hand saddle point 62 of the second vertebra 26. As shown, the primary reamer 70 has been registered on the guide wire 668 of the left-hand saddle point 62 by inserting the guide wire 668 into the bore 88 of the primary reamer 70, thereby registering the primary reamer 70 with respect to the saddle point 62. Thus, motion of the primary reamer 70 is constrained to rotation about the axis of the guide wire 668 and motion along the guide wire 668.

The primary reamer 70 is coupled at the torque interface 76 to a handle, motor, or the like (not shown). The primary reamer 70 rotates along the direction 914 such that the cutting flanges 92 scrape away bone tissue from around the saddle point 62. The primary reamer 70 is advanced into the pedicle 50 until the flat surface 90 abuts the bone immediately surrounding the guide wire 668. The primary reamer 70 is then unable to advance further into the bone, and is withdrawn to leave a roughened semispherical surface 926, as shown on the right-hand side of the second vertebra 26. The roughened semispherical surface 926 has a plateau (not visible in FIG. 36) immediately surrounding the guide wire 668, where the primary reamer 70 was unable to remove the bone tissue.

Referring to FIG. 37, a perspective view illustrates the first and second vertebrae 24, 26 with the guide wires 668, frame 110, and stationary external support 260 in place, and with the secondary reamer 72 positioned to complete reaming of the left-hand saddle point 62. As described previously, the dome 102 of the secondary reamer 72 is advanced into the roughened semispherical surface 926. The dome 102 does not remove bone tissue, but the central teeth 100 remove the plateau (not visible) to leave a semispherical interface 930 at the saddle point 62.

After the semispherical interfaces 930 have been formed at the saddle points 62 of the second vertebra 26, The guide wires 668 implanted in the saddle points 62 are no longer needed and may be removed. The pedicles 50 of the second vertebra 26 may then be tapped and the pedicle screws 670 may be inserted into the resulting tapped holes.

Referring to FIG. 38, a perspective view illustrates the first and second vertebrae 24, 26 with the guide wires 668, frame 110, and stationary external support 260 in place, and with



tools positioned to tap and drive a pedicle screw **670** into the pedicles **50** of the second vertebra **26**. More precisely, a pedicle tapping tool **934** is positioned to tap the pedicle **50** of the left-hand side of the second vertebra **26**.

The pedicle tapping tool **934** may have any of a variety of configurations, some of which may be known in the art of spinal fusion. According to one example, the pedicle tapping tool **934** has a shaft **936**, a tapping head **938** at one end of the shaft **936**, and a grip member **864** on the opposite end of the shaft **936**. The grip member **864** may be substantially the same as the grip member **864** of the guide wire inserter **860** of FIGS. **22** and **35**, and may thus be used to manually impart torque to the shaft **936**. The tapping head **938** has a plurality of threads (not visible in FIG. **38**). The shaft **936** has a coupling end **940** retained within the coupling **890** of the grip member **864**, and a working end **942** either permanently or removably coupled to the tapping head **938**.

The end (not shown) of the tapping head **938** is inserted into the canal left by removal of the guide wire **668**. Then, the tapping head **938** is rotated clockwise to cause the threads of the tapping head **938** to cut a threaded path into the wall of the canal. The tapping head **938** may be rotated counterclockwise to withdraw the threads from the canal, thereby leaving a tapped hole in the pedicle **50** of the second vertebra **26**. The tapped hole may also be sounded through the use of a sounder (not shown) having any of a variety of known configurations, if desired.

A screw insertion tool **944** is positioned to drive the pedicle screw **670** into the pedicle **50** of the right-hand side of the second vertebra **26**. The right-hand side pedicle **50** has already been tapped and sounded, and is therefore ready to receive the pedicle screw **670**. The screw insertion tool **944** has a shaft **946** and a grip **948** coupled to one end of the shaft **946**. The shaft **946** has a grip attachment end **950** coupled to the grip **948** and a working end **952**, which may have a hexagonal shape designed to be insertable into the torque receiver **792** of the pedicle screw **670**.

The end (not shown) of the pedicle screw **670** is inserted into the tapped hole of the pedicle **50**. Then, the grip **948** is rotated clockwise to cause the threaded end **790** of the pedicle screw **690** to engage the threads of the tapped hole. The working end **952** may then be drawn free of the torque receiver **792** of the pedicle screw **670**. The pedicle screw **670** may remain implanted in the pedicle **50**, with the shank **788** and a portion of the threaded end **790** exposed.

After the pedicle screws **670** have been implanted in the pedicles **50** of the second vertebra **26**, the inferior resection tool **660** may be used to guide resection of the inferior facet **60** of the left-hand side of the second vertebra **26**. The registration member **662** and the anchoring member **664** of the inferior resection tool **660** may be selected based on the selection of the superior and inferior prostheses. The inferior resection tool **660** may then be assembled and registered on the frame **110** by sliding the bore **686** of the registration interface **680** over the guide post **124** of the first anchor **112** of the frame **110**.

Simultaneously, the first, second, and third joints **802**, **804**, **806** may be actuated to move the anchoring feature **700** with respect to the registration interface **680** such that the anchoring feature **700** is able to slide into engagement with the semispherical interface **930** and the pedicle screw **670** of the left-hand side of the second vertebra **26**. The anchoring feature **700** may be attached to the semispherical interface **930** via the castle nuts **672** through the use of a nut tightening tool.

Referring to FIG. **39**, a perspective view illustrates the first and second vertebrae **24**, **26** with the guide wires **668**, pedicle screws **670**, frame **110**, and stationary external support **260** in

place, and with the inferior resection tool **660** registered to the frame **110** and anchored to the second vertebra **26**. The joints **802**, **804**, **806** of the inferior resection tool **660** have moved to positions in which the relative positions and orientations of the registration interface **680** and the anchoring feature **700** are adapted to the morphology of the spine **10**. Thus, the slot **714** of the guide feature **702** of the inferior resection tool **660** is positioned at the proper orientation to guide a reciprocating blade of a cutting tool (not shown) to resect the inferior facet **60** of the left-hand side of the second vertebra **26**. The cutting tool may be an oscillating saw or another cutting tool designed specifically for spinal applications.

Referring to FIG. **40**, a lateral view illustrates the first and second vertebrae **24**, **26** with the guide wires **668**, pedicle screws **670**, frame **110**, and stationary external support **260** in place, and with the inferior resection tool **660** registered to the frame **110** and anchored to the second vertebra **26**. Before the inferior facet **60** is resected, the lever **734** may be actuated into the locked position to lock the first joint **802** in place to stabilize the position and orientation of the slot **714**. In alternative embodiments, the second and third joints **804**, **806** may be lockable in addition to or in the alternative to the first joint **802** to stabilize the position and orientation of the slot **714**.

After the cutting tool has been used to resect the inferior facet **60**, the castle nuts **672** may then be removed, and the inferior resection tool **660** may be removed from the spine **10**. If the surgeon decides not to drive the oscillating saw completely through the facet **58**, to avoid entry into the central canal of the spine **10**, an osteotome or other similar tool may be used to complete resection of the inferior facets **60** of the second vertebra **26**. Manual tools may be required to complete resection of the medial margins of the inferior facets **58** of the second vertebra **26**. An inferior resection surface **956** has then been formed on each side of the second vertebra **26**, as shown in FIG. **40**.

After the inferior facets **60** of the second vertebra **26** have been resected, the superior facets **38** of the first vertebra **24** are relatively easily accessible. Thus, the superior facet **38** of the left-hand side of the first vertebra **24** may be resected through the use of the kit **510** of superior cutting tools.

The cutting guide **630** is selected from a kit of multiple cutting guides based on the selection of the superior facet prosthesis. The cutting guide **630** may be registered on the frame **110**, and the short, long, and curved cutting tools **512**, **514**, **516** may be sequentially registered on the cutting guide **630** to perform resection of the superior facet **38**. The short cutting tool **512** may be used first to commence forming a resection surface, then the curved cutting tool **516** may be used to broaden the resection surface, and then the long cutting tool **514** may be used to further broaden the resection surface.

Referring to FIG. **41**, a perspective view illustrates the first and second vertebrae **24**, **26** with the guide wires **668**, pedicle screws **670**, frame **110**, and stationary external support **260** in place, and with the cutting guide **630** registered on the frame **110** and the curved cutting tool **516** registered on the cutting guide **630** to carry out resection of the superior facet **38** of the left-hand side of the first vertebra **24**. The registration interface **634** of the cutting guide **630** is registered on the first anchor **112** of the frame **110** by sliding the bore **650** of the registration interface **634** over the guide post **124** of the first anchor **112**. The post **652** of the registration feature **636** of the cutting guide **630** then protrudes at an angle offset from that of the guide post **124**. The post **652** extends substantially perpendicular to the plane along which resection of the superior facet **38** is to be carried out.

The curved cutting tool **516** is registered on the cutting guide **630**, and thereby registered on the frame **110**, by sliding the bore **600** of the registration interface **532** of the curved cutting tool over the post **652**. Relative motion between the curved cutting tool **516** and the first vertebra **24** is then limited to translation along the post **652** and rotation about the axis of the post **652**. As shown, the grip member **864** may be coupled to the curved cutting tool **516** by inserting the torque receiver **526** of the shaft **560** of the curved cutting tool **516** into the coupling **890** of the grip member **864**.

The grip **892** may thus be grasped and rotated by hand in reciprocating fashion, while slight pressure is applied to urge the cutting surface **576** of the curved cutting tool **516** against the surface of the bone, to remove bone tissue from the superior facet **38**. As bone tissue is removed, the bore **600** progresses further along the post **652** until the distal cap **568** of the shaft **560** of the curved cutting tool **516** abuts the shoulder **646** of the main body **632** of the cutting guide **630**.

At the time the curved cutting tool **516** is used, the short cutting tool **512** has already been applied in a similar manner. The short cutting tool **512** has been rotated clockwise such that the cutting surface **536** of the short cutting tool **512** sweeps from the foraminal space until the arm **534** of the short cutting tool **512** contacts the first anchor **112** of the frame **110**. The curved cutting tool **516** is used in a similar manner to simply broaden the radius of the resection surface and to extend the resection surface around the semispherical surface **128** of the first anchor **112**. After the curved cutting tool **516** is applied, the long cutting tool **514** may be used in a similar manner to further broaden the resection surface. The resulting resection surface, which is a superior resection surface **958**, is substantially planar and continuous despite the use of multiple different cutting tools **512**, **514**, **516** to form it.

Referring to FIG. **42**, a cephalad view illustrates the first vertebra **24** with the guide wires **668**, pedicle screws **670**, frame **110**, and stationary external support **260** in place, and with the cutting guide **630** registered on the frame **110** and the curved cutting tool **516** registered on the cutting guide **630** to carry out resection of the superior facet **38** of the left-hand side of the first vertebra **24**. FIG. **42** provides an edge view of the superior resection surface **958** formed through the use of the cutting tools **512**, **514**, **516**. As in other drawings previously described, the same operation has already been performed on the right-hand side of the first vertebra **24**.

After the short, long, and curved cutting tools **512**, **514**, **516** have been applied and removed in sequence, the cutting guide **630** and the frame **110** may be removed, and the seat cutting tool **518** may be used. The seat cutting tool **518** does not register on the cutting guide **630** and is not designed to contribute to formation of the superior resection surface **958**. Rather, the seat cutting tool **518** provides a flat surface proximate the semispherical interfaces **920** of the saddle points **42** of the first vertebra **24**. The flat surface formed by the seat cutting tool **518** may correspond to a flat surface of the selected superior facet prosthesis, and may help prevent rotation of the selected superior facet prosthesis against the first vertebra **24** after the selected superior facet prosthesis has been attached to the first vertebra **24**.

Referring to FIG. **43**, a perspective view illustrates the first and second vertebrae **24**, **26** with the guide wires **668** and the pedicle screws **670** in place, and with the seat cutting tool **518** positioned to provide a flat surface proximate the semispherical interface **920** of the left-hand side of the first vertebra **24**. The seat cutting tool **518** is registered to the guide wire **668** extending from the saddle point **42** of the left-hand side of the first vertebra **24**.

More precisely, the registration interface **592** of the shaft **580** of the seat cutting tool **518** is registered on the guide wire **668** by sliding a bore (not visible in FIG. **43**) of the shaft **580** over the exposed portion of the guide wire **668**. Relative motion between the seat cutting tool **518** and the first vertebra **24** is thus constrained to translation along the guide wire **668**, or rotation about the axis of the guide wire **668**. The guide wire **668** is substantially collinear with an axis of the corresponding pedicle **30**; accordingly, the seat cutting tool **518** is registered to form a flat surface substantially perpendicular to the axis of the pedicle **30**.

Referring to FIG. **44**, a cephalad view illustrates the first vertebra **24** with the guide wires **668** and the pedicle screws **670** in place, and with the seat cutting tool **518** positioned to provide a flat surface proximate the semispherical interface **920** of the left-hand side of the first vertebra **24**. The size of the flat surface formed by the seat cutting tool **518** varies according to the selection of the superior facet prosthesis. In FIG. **44**, the seat cutting tool **518** has little bone to resect because the superior resection surface **958** extends substantially to the edge of the semispherical interface **920**. However, in alternative embodiments, the seat cutting tool **518** may resect away more bone tissue to provide a more distinct flat surface.

After resection of the superior facets **38** of the first vertebra **24** has been completed, the guide wires **668** may be removed from the pedicles **30** of the first vertebra **24**. The remaining canals may be tapped, and pedicle screws **670** may be inserted into the resulting tapped holes in preparation for attachment of facet joint prostheses to the vertebrae **24**, **26**.

Referring to FIG. **45**, a perspective view illustrates the first and second vertebrae **24**, **26** with the pedicle screws **670** of the second vertebra **26** in place. Furthermore, in FIG. **45**, the pedicle tapping tool **934** is positioned to tap the pedicle **30** of the left-hand side of the first vertebra **24**, and the screw insertion tool **944** is positioned to insert one of the pedicle screws **670** into the pedicle **30** of the right-hand side of the first vertebra **24**.

The end (not shown) of the tapping head **938** is inserted into the canal left by removal of the guide wire **668** from the left-hand pedicle **30** of the first vertebra **24**. Then, the tapping head **938** is rotated clockwise to cause the threads of the tapping head **938** to cut a threaded path into the wall of the canal. The tapping head **938** may be rotated counterclockwise to withdraw the threads from the canal, thereby leaving a tapped hole in the pedicle **30** of the first vertebra **24**. The tapped hole may also be sounded through the use of a sounder (not shown) having any of a variety of known configurations, if desired.

The right-hand side pedicle **30** has already been tapped and sounded, and is therefore ready to receive the pedicle screw **670**. The end (not shown) of the pedicle screw **670** is inserted into the tapped hole of the pedicle **30**. Then, the grip **948** is rotated clockwise to cause the threaded end **790** of the pedicle screw **690** to engage the threads of the tapped hole. The working end **952** may then be drawn free of the torque receiver **792** of the pedicle screw **670**. The pedicle screw **670** may remain implanted in the pedicle **30**, with the shank **788** and a portion of the threaded end **790** exposed.

After the pedicle screws **670** have been implanted in the pedicles **30** of the first vertebra **24**, trial facet prostheses may be coupled to the vertebrae **24**, **26** and checked for proper fit. If the fit is not proper, different prostheses may be selected and/or additional resections may be carried out on the first and second vertebrae **24**, **26** to obtain the desired fit. Then, the selected facet prostheses may be coupled to the vertebrae **24**, **26**. The facet prostheses may be secured to the vertebrae **24**, **26** via the castle nuts **672**.

Referring to FIG. 46, a perspective view illustrates the vertebrae 24, 26 with the pedicle screws 670 in place, with facet prostheses attached, with a nut tightening tool 964 positioned to secure the facet prostheses via the castle nuts 672. In FIG. 46, the clamping tool is used to clamp the inferior facet prostheses in place as they are secured to the second vertebra 26.

As shown, the nut tightening tool 964 is used in combination with the screw insertion tool 944 of FIG. 38. The nut tightening tool 964 has a shaft 966 and a grip 968, which may be shaped similarly to the grip 948 of the screw insertion tool 944, except that the grip 968 is cannulated to receive the shaft 946 of the screw insertion tool 944. The shaft 966 has a grip attachment end 970 attached to the grip 968 and a working end 972. The shaft 966 is hollow so that the shaft 946 of the screw insertion tool 944 is able to pass through the shaft 966 to reach the corresponding pedicle screw 670. Thus, a user may hold the grip 948 of the screw insertion tool 944 substantially stationary while rotating the grip 968 of the nut tightening tool 964 to tighten the corresponding castle nut 672 without significant rotation of the pedicle screw 670 about which the castle nut 672 is tightened. The castle nut 672 may engage exposed threads of the threaded end 790 of the pedicle screw 670.

In FIG. 46, a first superior prosthesis 974 and a second superior prosthesis 976 may be attached to the first vertebra 24, and a first inferior prosthesis 978 and a second inferior prosthesis 980 may be attached to the second vertebra 26. The prostheses 974, 976 replace the superior facets 38 of the first vertebra 24 that were resected away previously, while the prostheses 978, 980 replace the inferior facets 60 of the second vertebra 26 that were also resected away previously. Although FIG. 46 illustrates full, bi-lateral replacement of both of the facet joints 64 of the vertebrae 24, 26, the systems and methods of the present invention apply equally to unilateral replacement operations, or operations in which only superior or inferior facets are replaced.

The process of tightening the castle nuts 672 to secure the inferior prostheses 978, 980 transmits torque to the inferior prostheses 978, 980 that could potentially move them from their optimal positions. Accordingly, the clamping tool 810 may be used to hold the inferior prostheses 978, 980 in place while the corresponding castle nuts 672 are tightened using the nut tightening tool 964 and the screw insertion tool 944. More precisely, each of the inferior prostheses 978, 980 may have a projection 982 that extends posteriorly and terminates in a semispherical surface or the like. The projections 982 may be designed for use with a cross-link (not shown) that permanently stabilizes the inferior prostheses 978, 980.

As shown, the clamping tool 810 is positioned such that the grip portions 826 of the first and second clamping members 812, 814 are spread apart. The knob 818 has been rotated counterclockwise to retract the knob 818 along the threaded post 816, thereby permitting the clamping members 812, 814 to move apart. The projections 982 have been positioned in the recesses 828 of the grip portions 826, and the knob 818 has been rotated clockwise to draw the clamping members 812, 814 slightly together, thereby pressing the projections 982 snugly toward each other. As a result, the first and second inferior prostheses 978, 980 are held securely against the intervening bony body of the second vertebra 26. Thus, the clamping tool 810 prevents either of the inferior prostheses 978, 980 from rotating against the second vertebra 26.

Once the castle nuts 672 have all been tightened, the nut tightening tool 964 and the screw insertion tool 944 may be set aside, and the clamping tool may be removed by once again rotating the knob 818 counterclockwise to permit the

clamping members 812, 814 to move apart sufficiently to withdraw the projections 982 from the recesses 828 of the grip portions 826. Attachment of the prostheses 974, 976, 978, 980 is now complete.

Referring to FIG. 47, a perspective view illustrates the first and second vertebrae 24, 26, with the first and second superior prostheses 974, 976 attached to the first vertebra 24 and with the first and second inferior prostheses 978, 980 attached to the second vertebra 26. As illustrated in FIG. 47, each of the superior prostheses 974, 976 has an anchoring surface 984 with a generally semispherical shape that fits within the corresponding semispherical interface 920 of each saddle point 42 of the first vertebra 24. Similarly, each of the inferior prostheses 978, 980 has an anchoring surface 986 with a generally semispherical shape that fits within the corresponding semispherical interface 930 of each saddle point 62 of the second vertebra 26.

Additionally, each of the superior prostheses 974, 976 has an articulating surface 988 that faces generally medially (i.e., inward). The articulating surfaces 988 are generally trough-shaped to replicate the natural shapes of the superior facets 38 of the first vertebra 24. Each of the inferior prostheses 978, 980 has an articulating surface 990 that faces generally laterally (i.e., outward). The articulating surfaces 990 are generally semispherical to replicate the natural shapes of the inferior facets 60 of the second vertebra 26. Accordingly, the articulating surfaces 988, 990 may articulate against each other to provide ball-in-trough motion characteristic of the natural facet joints 64 of the vertebrae 24, 26.

Referring to FIG. 48, a posterior view illustrates the first and second vertebrae 24, 26, with the first and second superior prostheses 974, 976 attached to the first vertebra 24 and with the first and second inferior prostheses 978, 980 attached to the second vertebra 26. The articulating surfaces 988, 990 are more clearly visible in FIG. 48. If desired, a cross-link (not shown) may be attached to the projections 982 of the inferior prostheses 978, 980 to help keep them in place. Such a cross-link may, if desired, be attached to the spinous process 56 of the second vertebra 26, or separate linking structures may attach the projections 982 to the spinous process 56 to provide additional stability.

As a result of the manner in which the prostheses 974, 976, 978, 980 articulate against each other, the spine 10 maintains its natural kinematics in flexion/extension, lateral bending, and rotation, or twisting. Additionally, the loads on the vertebrae 24, 26 and on the surrounding bone structures, ligaments, and musculature will be substantially the same as before the facet joints 64 were replaced. Accordingly, the prostheses 974, 976, 978, 980 may correct facet joint problems without disrupting the normal functioning of the spine 10. Furthermore, through the use of the various surgical instruments and methods presented herein, prostheses 974, 976, 978, 980 may be accurately selected and safely attached to vertebrae of patients having a wide variety of spinal morphologies.

The present invention has particular relevance to surgery, and more particularly to facet joint replacement. However, the principles, structures, and methods of the present invention may also be extended to other fields including measurement and resection of bone for installation of other implants such as hip and knee implants.

The present invention may be embodied in other specific forms without departing from its spirit or essential characteristics. As such the described embodiments are to be considered in all respects only as illustrative and not restrictive. The scope of the invention is, therefore, indicated by the appended claims rather than by the foregoing description. All changes

41

which come within the meaning and range of equivalency of the claims are to be embraced within their scope.

The invention claimed is:

1. A method of conducting measurements on a spine of a patient through the use of a measurement tool comprising a registration interface, a contact feature, and a displacement structure that couples the contact feature to the registration interface, the method comprising:

attaching a frame directly to a first bone portion such that the frame abuts the first bone portion;

coupling the registration interface to the first bone portion, wherein the registration interface comprises a bore having a noncircular shape, wherein the first bone portion is part of the spine, wherein coupling the registration interface to the first bone portion comprises inserting a post of the frame into the bore to couple the registration interface to the first bone portion, wherein coupling the registration interface to the first bone portion comprises limiting relative translation between the registration interface and the first bone portion along three nonparallel directions;

restricting relative rotation between the registration interface and the first bone portion in response to coupling of the registration interface to the first bone portion;

moving the displacement structure to position the contact feature in contact with a bony landmark, wherein the bony landmark is part of the spine; and

acquiring data from the displacement structure to indicate a displacement of the bony landmark with respect to the registration interface in at least two dimensions.

2. The method of claim 1, wherein the displacement structure comprises three sliding joints, wherein moving the displacement structure comprises translating the contact feature with respect to the registration interface along three orthogonal axes via the three sliding joints.

3. The method of claim 2, wherein the displacement structure further comprises three rods, each of which is parallel to one of the three orthogonal axes, wherein each of the rods is slidably coupled to one of the sliding joints, wherein each of the rods comprises a plurality of markings, wherein acquiring the data comprises reading the markings on each of the rods to indicate the displacement along the axis parallel to it.

4. The method of claim 1, further comprising:

coupling a second measurement tool to a second bone portion generally symmetrical to the first bone portion across a sagittal plane of a patient; and

acquiring data with the second measurement tool such that the first and second measurement tools perform measurements substantially symmetrically across the sagittal plane.

5. The method of claim 1, wherein the first bone portion comprises a pedicle of a first vertebra of the spine and the bony landmark comprises a pedicle of a second vertebra of the spine, wherein the second vertebra is adjacent to the first vertebra, wherein moving the displacement structure comprises contacting the pedicle of the second vertebra with the contact feature.

6. The method of claim 1, wherein at least one of the first bone portion and the bony landmark is on a facet of the spine.

7. The method of claim 6, wherein the first bone portion comprises a pedicle of a first vertebra of the spine and the bony landmark comprises a most medial and anterior surface of a facet of the first vertebra, wherein moving the displacement structure comprises contacting the most medial and anterior surface of the facet with the contact feature.

42

8. The method of claim 1, further comprising replacing at least a portion of a facet of a vertebra of the spine with at least one prosthesis.

9. The method of claim 1, further comprising:

replacing two facets of a vertebra of the spine with two prostheses; and

attaching a cross-linking member to the prostheses to couple the prostheses together.

10. A method for measuring a location of a bony landmark through the use of a measurement tool comprising a registration interface, a contact feature, and a displacement structure that couples the contact feature to the registration interface, the method comprising:

attaching a frame directly to a first bone portion such that the frame abuts the first bone portion;

coupling the registration interface to the first bone portion such that relative translation between the registration interface and the first bone portion is limited along three nonparallel directions, wherein the registration interface comprises a bore having a noncircular shape, wherein the first bone portion is part of the spine, wherein coupling the registration interface to the first bone portion comprises inserting a post of the frame into the bore to couple the registration interface to the first bone portion;

restricting relative rotation between the registration interface and the first bone portion in response to coupling of the registration interface to the first bone portion;

moving the displacement structure to position the contact feature in contact with a bony landmark; and

acquiring data from the displacement structure to indicate a displacement of the bony landmark with respect to the registration interface.

11. The method of claim 10, wherein the displacement structure comprises three sliding joints, wherein moving the displacement structure comprises translating the contact feature with respect to the registration interface along three orthogonal axes via the three sliding joints, wherein the displacement structure further comprises three rods, each of which is parallel to one of the three orthogonal axes, wherein each of the rods is slidably coupled to one of the sliding joints, wherein each of the rods comprises a plurality of markings, wherein acquiring the data comprises reading the markings on each of the rods to indicate the displacement along the axis parallel to it.

12. The method of claim 10, wherein the first bone portion comprises a pedicle of a first vertebra of the spine and the bony landmark comprises a pedicle of a second vertebra of the spine, wherein the second vertebra is adjacent to the first vertebra, wherein moving the displacement structure comprises contacting the pedicle of the second vertebra with the contact feature.

13. The method of claim 10, wherein at least one of the first bone portion and the bony landmark is on a facet of the spine.

14. The method of claim 13, wherein the first bone portion comprises a pedicle of a first vertebra of the spine and the bony landmark comprises a most medial and anterior surface of a facet of the first vertebra, wherein moving the displacement structure to position the contact feature in contact with the bony landmark comprises contacting the most medial and anterior surface of the facet with the contact feature.

15. The method of claim 10, further comprising replacing at least a portion of a facet of a vertebra of the spine with at least one prosthesis.

16. A method comprising:

attaching a frame directly to a pedicle of the first vertebra such that the frame abuts the pedicle of the first vertebra;

43

coupling a first end of a measurement tool to the pedicle of the first vertebra, of a spine of a wherein the first end comprises a bore having a noncircular shape, wherein coupling the first end to the pedicle of the first vertebra comprises inserting a post of the frame into the bore to couple the first end to the pedicle of the first vertebra, wherein coupling the first end to the pedicle of the first vertebra comprises limiting relative translation between the first end and the pedicle of the first vertebra along three nonparallel directions;  
 restricting relative rotation between the first end and the pedicle of the first vertebra in response to coupling of the first end to the pedicle of the first vertebra;  
 coupling a second end of the measurement tool to a bony landmark selected from the group consisting of a most medial and anterior surface of a facet of the first vertebra, and a pedicle of a second vertebra; and  
 acquiring data from a displacement structure that couples the first and second ends together, wherein the data

44

indicates at least one of a position and an orientation of the bony landmark with respect to the pedicle of the first vertebra.

17. The method of claim 16, wherein the displacement structure comprises three sliding joints, the method further comprising translating the second end with respect to the first end along three orthogonal axes via the three sliding joints, wherein the displacement structure further comprises three rods, each of which is parallel to one of the three orthogonal axes, wherein each of the rods is slidably coupled to one of the sliding joints, wherein each of the rods comprises a plurality of markings, wherein acquiring the data comprises reading the markings on each of the rods to indicate the displacement along the axis parallel to it.

18. The method of claim 16, further comprising replacing at least a portion of a facet of a vertebra of the spine with at least one prosthesis.

\* \* \* \* \*