



US00D425201S

# United States Patent [19]

[11] Patent Number: Des. 425,201

Tetzlaff et al.

[45] Date of Patent: \*\* May 16, 2000

[54] **DISPOSABLE ELECTRODE ASSEMBLY**

[75] Inventors: **Philip Mark Tetzlaff**, Golden; **Dale Francis Schmaltz**, Fort Collins; **Steven Paul Buysse**, Longmont; **Kate Ryland Lawes**, Boulder, all of Colo.

5,324,289 6/1994 Eggers .  
 5,330,471 7/1994 Eggers .  
 5,342,359 8/1994 Rydell .  
 5,352,222 10/1994 Rydell .  
 5,356,408 10/1994 Rydell .  
 5,389,104 2/1995 Hahnen et al. .  
 5,391,166 2/1995 Eggers .  
 5,403,312 4/1995 Yates et al. .  
 5,431,674 7/1995 Basile et al. .  
 5,443,463 8/1995 Stern et al. .  
 5,443,464 8/1995 Russell et al. .  
 5,445,658 8/1995 Durrfeld et al. .  
 5,456,684 10/1995 Schmidt et al. .  
 5,462,546 10/1995 Rydell .

[73] Assignee: **Sherwood Services AG**, Schaffhausen, Switzerland

[\*\*] Term: **14 Years**

[21] Appl. No.: **29/095,493**

[22] Filed: **Oct. 23, 1998**

[51] **LOC (7) Cl.** ..... **24-02**

[52] **U.S. Cl.** ..... **D24/144**

[58] **Field of Search** ..... D24/143, 144, D24/148; 606/40, 41, 45, 51, 52, 50, 205-208

(List continued on next page.)

### FOREIGN PATENT DOCUMENTS

401367 11/1947 U.S.S.R. .

### OTHER PUBLICATIONS

International Search Report—PCT/US98/18640.  
 International Search Report—PCT/US98/23950.  
 Sigel et al., "The Mechanism of Blood Vessel Closure by High Frequency Electrocoagulation", *Surgery Gynecology & Obstetrics*, Oct. 1965 pp. 823-831.

(List continued on next page.)

*Primary Examiner*—Eric Watterson

### [57] CLAIM

We claim the ornamental design for a disposable electrode, as shown.

### DESCRIPTION


FIG. 1 is a perspective view of a disposable electrode showing our new design;  
 FIG. 2 is a left side view of the disposable electrode;  
 FIG. 3 is a rear view of the disposable electrode;  
 FIG. 4 is a right side view of the disposable electrode;  
 FIG. 5 is a front view of the disposable electrode;  
 FIG. 6 is a bottom view of the disposable electrode; and,  
 FIG. 7 is a top view of the disposable electrode.  
 The end portion shown broken away for ease of illustration.

1 Claim, 4 Drawing Sheets

### [56] References Cited

#### U.S. PATENT DOCUMENTS

371,664 10/1887 Brannan et al. .  
 702,472 6/1902 Pignolet .  
 728,883 5/1903 Downes .  
 1,586,645 6/1926 Bierman .  
 2,002,594 5/1935 Wappler et al. .  
 2,176,479 10/1939 Willis .  
 3,651,811 3/1972 Hildebrandt et al. .  
 3,920,021 11/1975 Hildebrandt .  
 3,938,527 2/1976 Rioux et al. .  
 3,952,749 4/1976 Fridolph et al. .  
 4,005,714 2/1977 Hildebrandt .  
 4,370,980 2/1983 Lottick .  
 4,552,143 11/1985 Lottick .  
 4,597,379 7/1986 Kihn et al. .  
 4,671,274 6/1987 Sorochenko .  
 4,685,459 8/1987 Koch et al. .  
 4,887,612 12/1989 Esser et al. .  
 4,938,761 7/1990 Ensslin .  
 5,026,370 6/1991 Lottick .  
 5,116,332 5/1992 Lottick .  
 5,151,102 9/1992 Kamiyama et al. .  
 5,217,458 6/1993 Parins .  
 5,250,047 10/1993 Rydell .  
 5,258,006 11/1993 Rydell et al. .  
 5,277,201 1/1994 Stern .

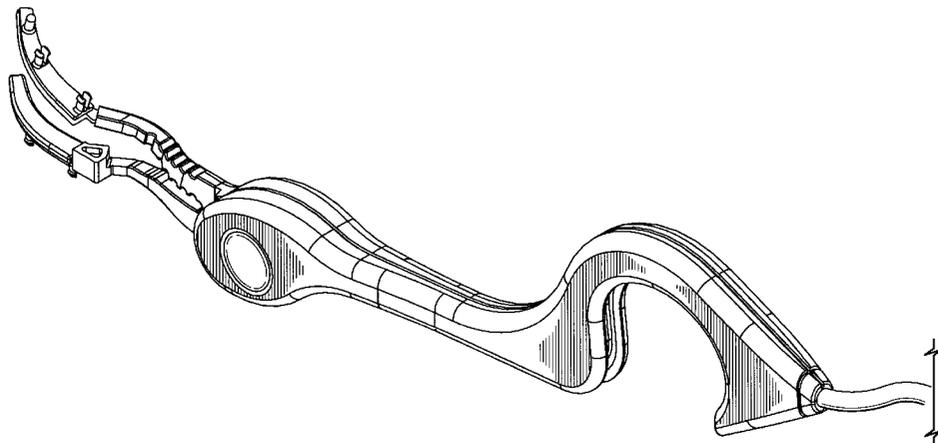

## U.S. PATENT DOCUMENTS

5,472,443	12/1995	Cordis et al. .	5,674,220	10/1997	Fox et al. .
5,478,351	12/1995	Meade et al. .	5,693,051	12/1997	Schulze et al. .
5,484,436	1/1996	Eggers et al. .	5,700,261	12/1997	Brinkerhoff .
5,509,922	4/1996	Aranyi et al. .	5,702,390	12/1997	Austin et al. .
5,527,313	6/1996	Scott et al. .	5,735,849	4/1998	Baden et al. .... 606/51
5,531,744	7/1996	Nardella et al. .	5,766,166	6/1998	Hooven .
5,540,684	7/1996	Hassler, Jr. .	5,769,849	6/1998	Eggers .
5,558,672	9/1996	Edwards et al. .	5,776,128	7/1998	Eggers .
5,569,241	10/1996	Edwards .	5,776,130	7/1998	Buysse et al. .
5,573,535	11/1996	Viklund .	5,817,128	10/1998	Storz ..... 606/205
5,626,578	5/1997	Tihon .	5,827,281	10/1998	Levin .
5,626,609	5/1997	Zvenyatsky et al. .... 606/208			
5,637,110	6/1997	Pennybacker et al. .			
5,658,281	8/1997	Heard .			
5,667,526	9/1997	Levin .			

## OTHER PUBLICATIONS

Bergdahl et al. "Studies on Coagulation and the Development of an Automatic Computerized Bipolar Coagulator", J. Neurosurg, vol. 75, Jul. 1991, pp. 148-151.

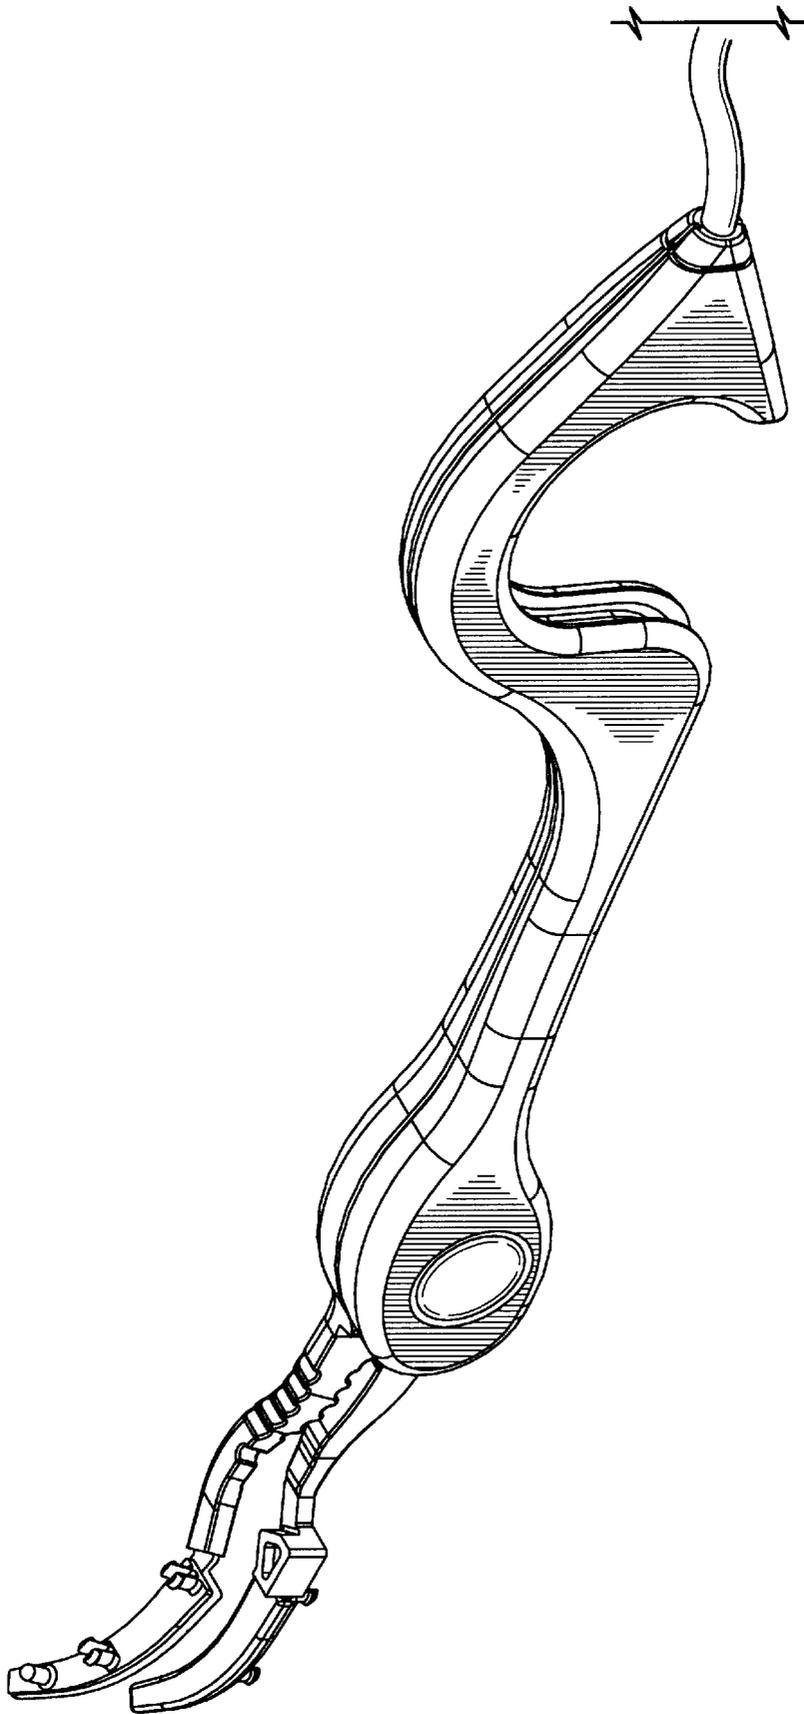


FIG. 1

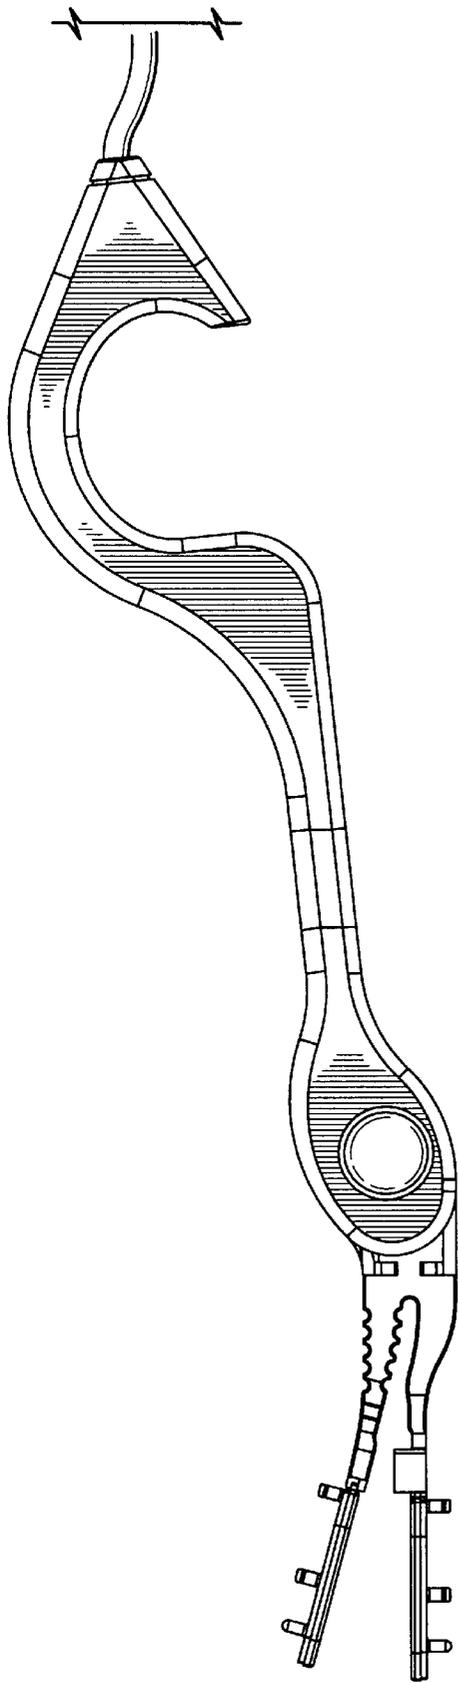


FIG. 2

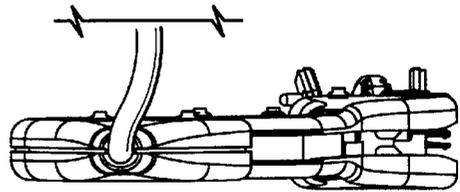


FIG. 3

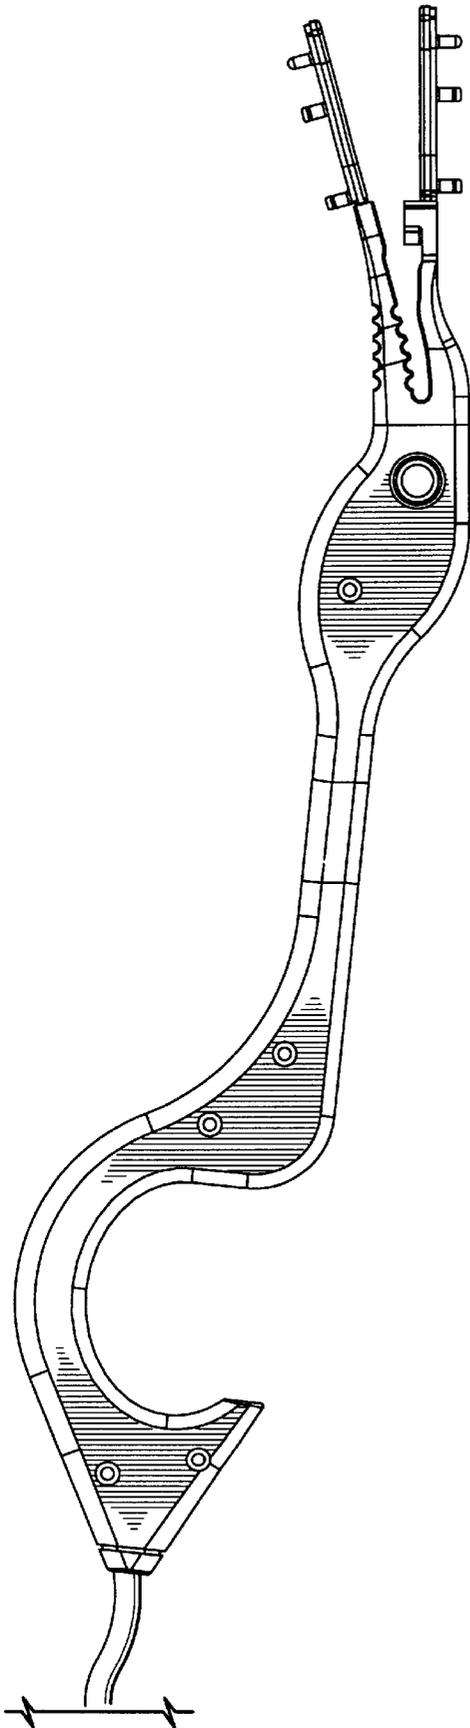


FIG. 4

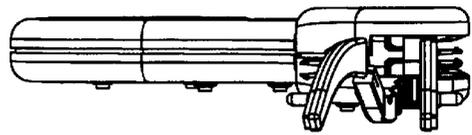


FIG. 5

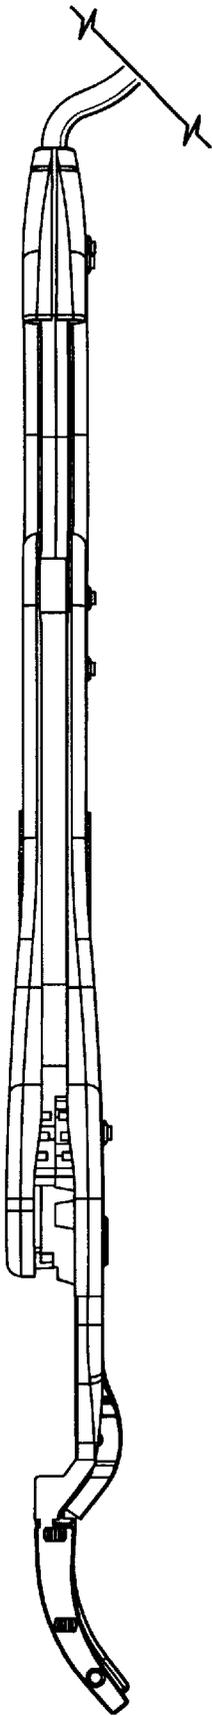


FIG. 6

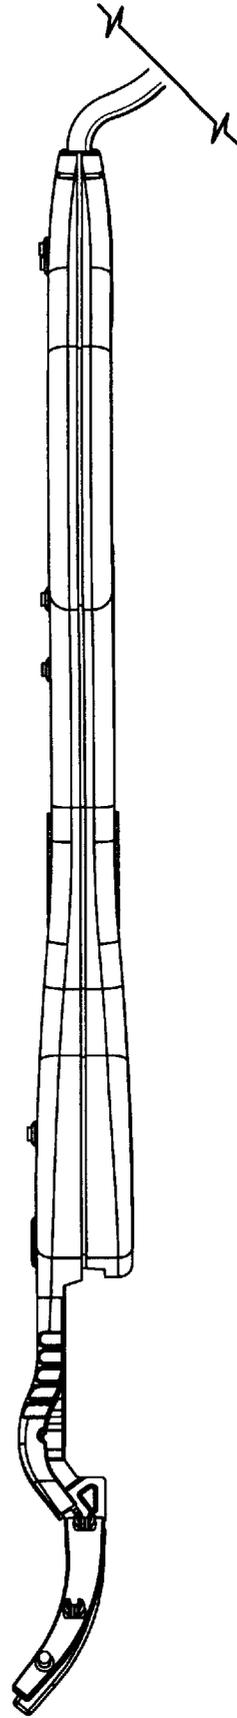


FIG. 7